



1,4-Dioxane

Response Ratio

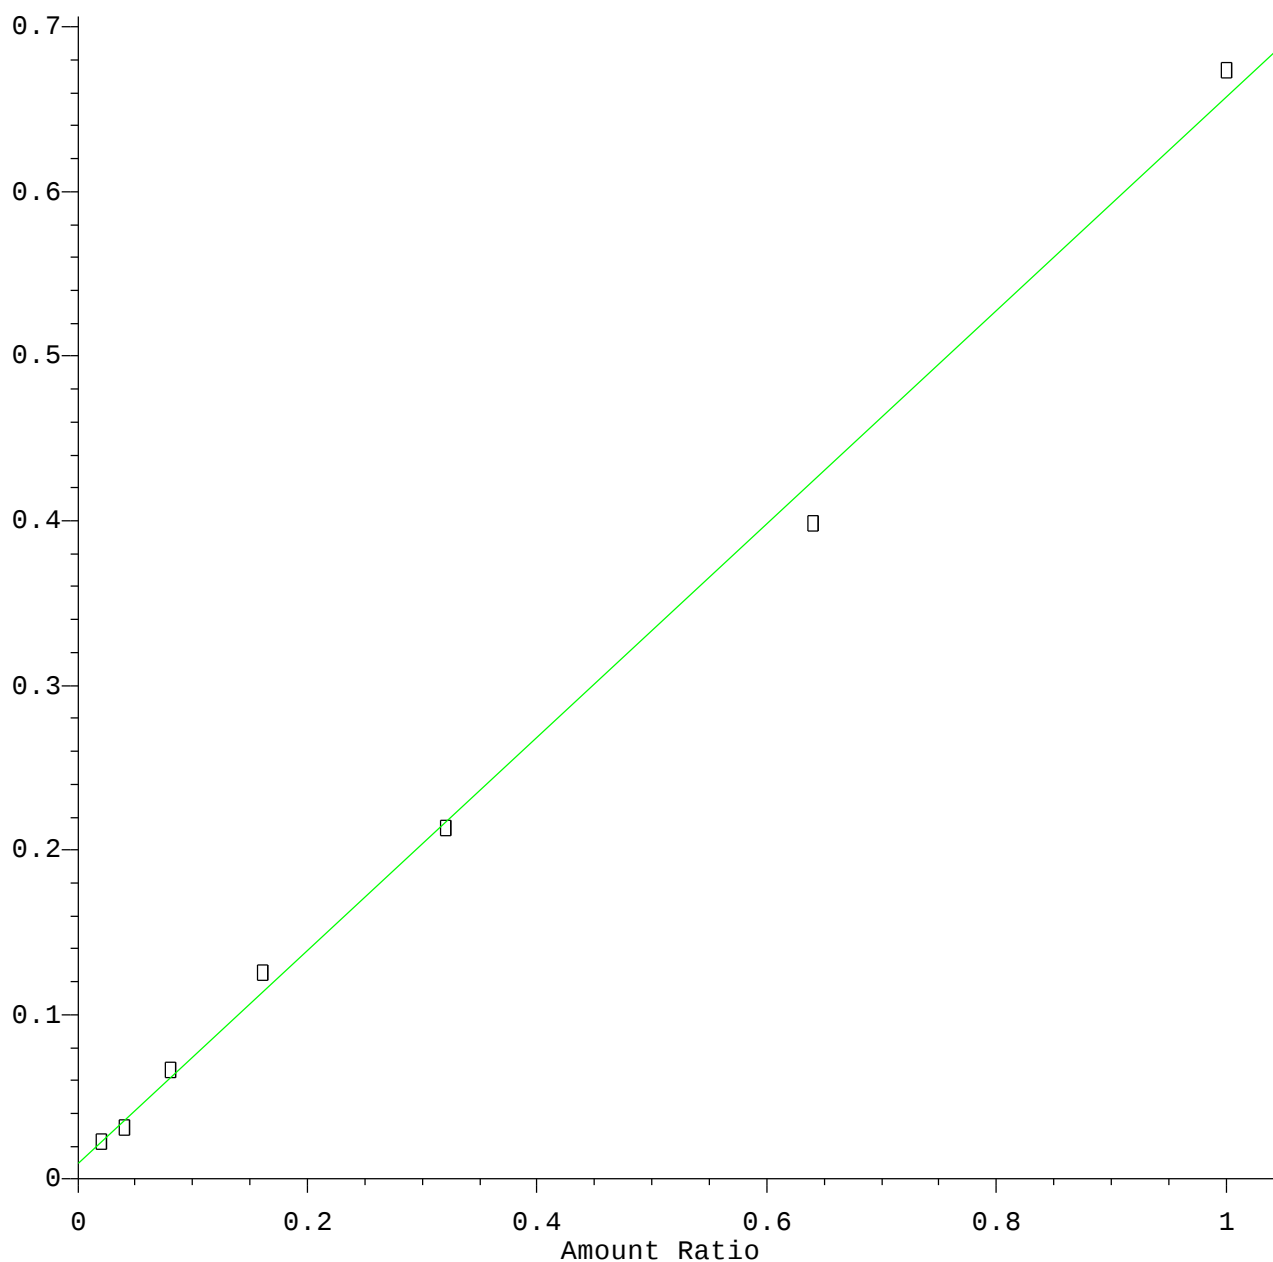


Resp Ratio = $6.49 \times 10^{-1} \times \text{Amt} + 8.99 \times 10^{-3}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

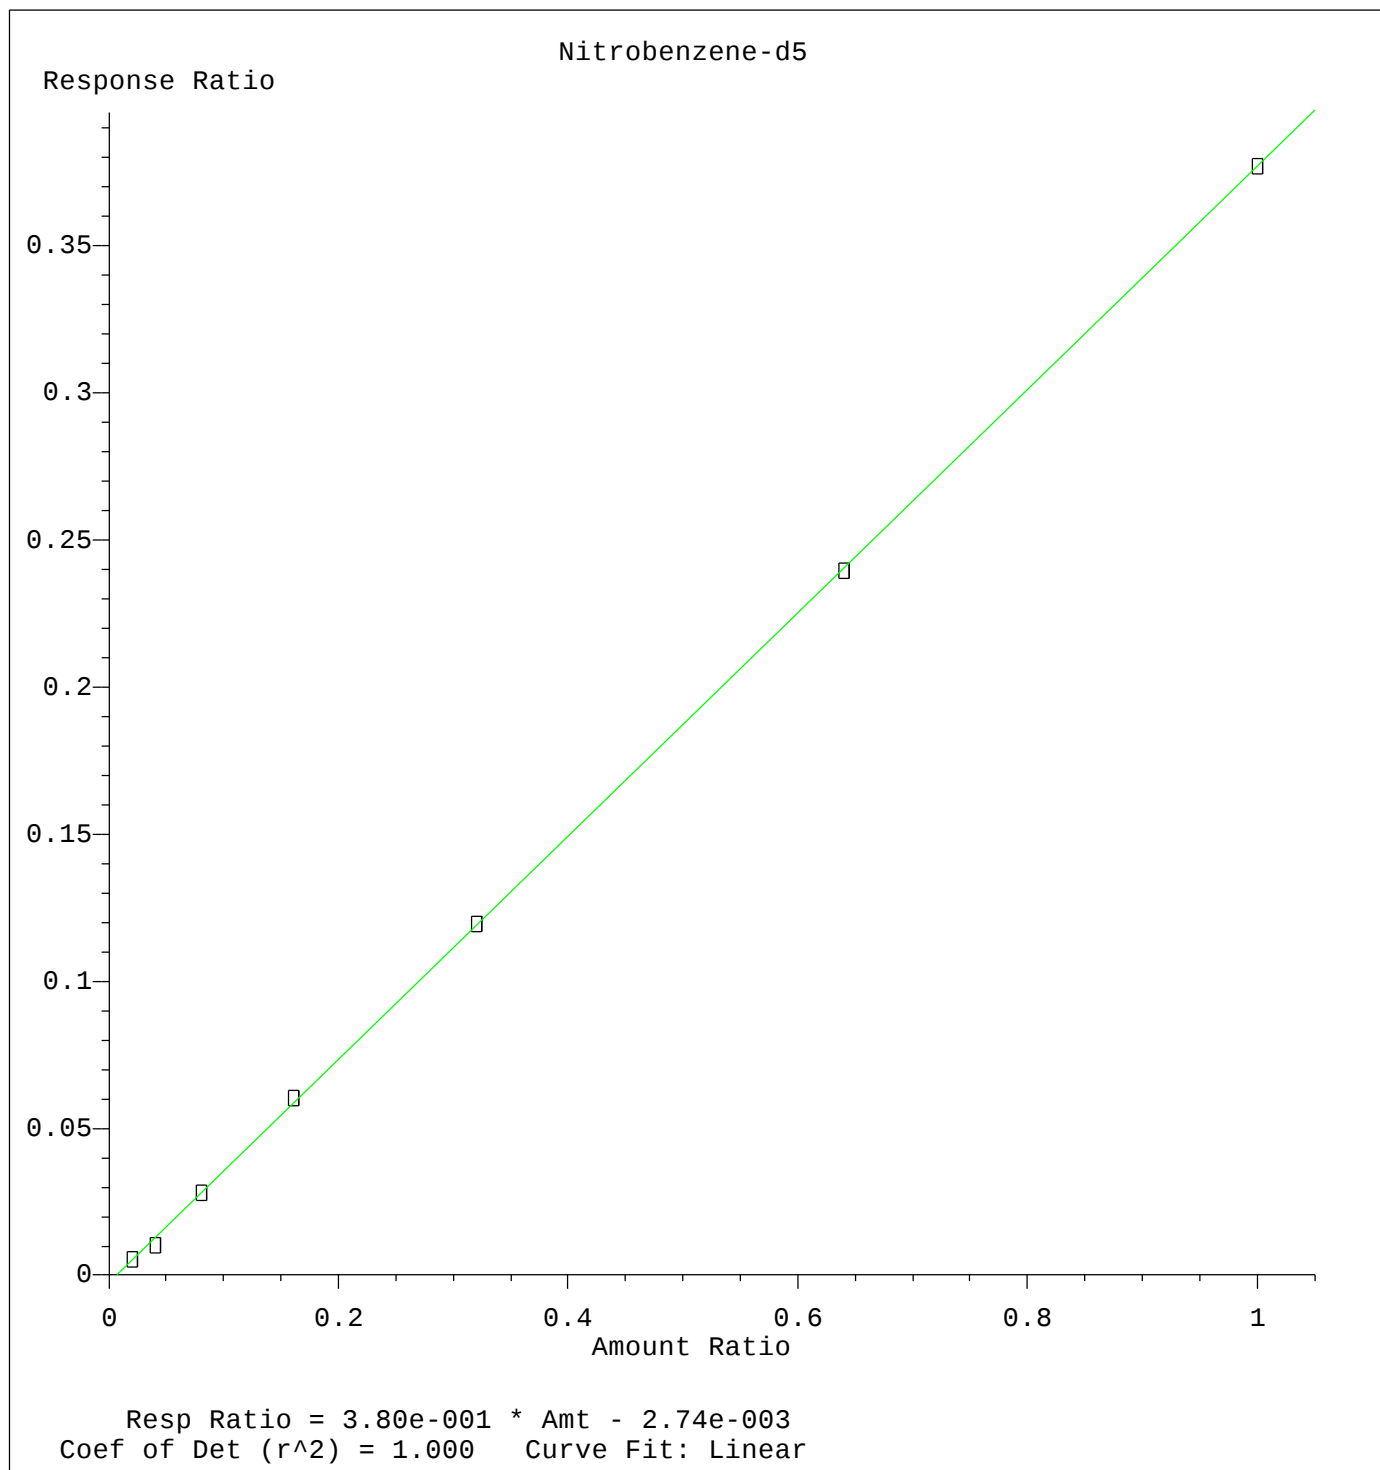

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

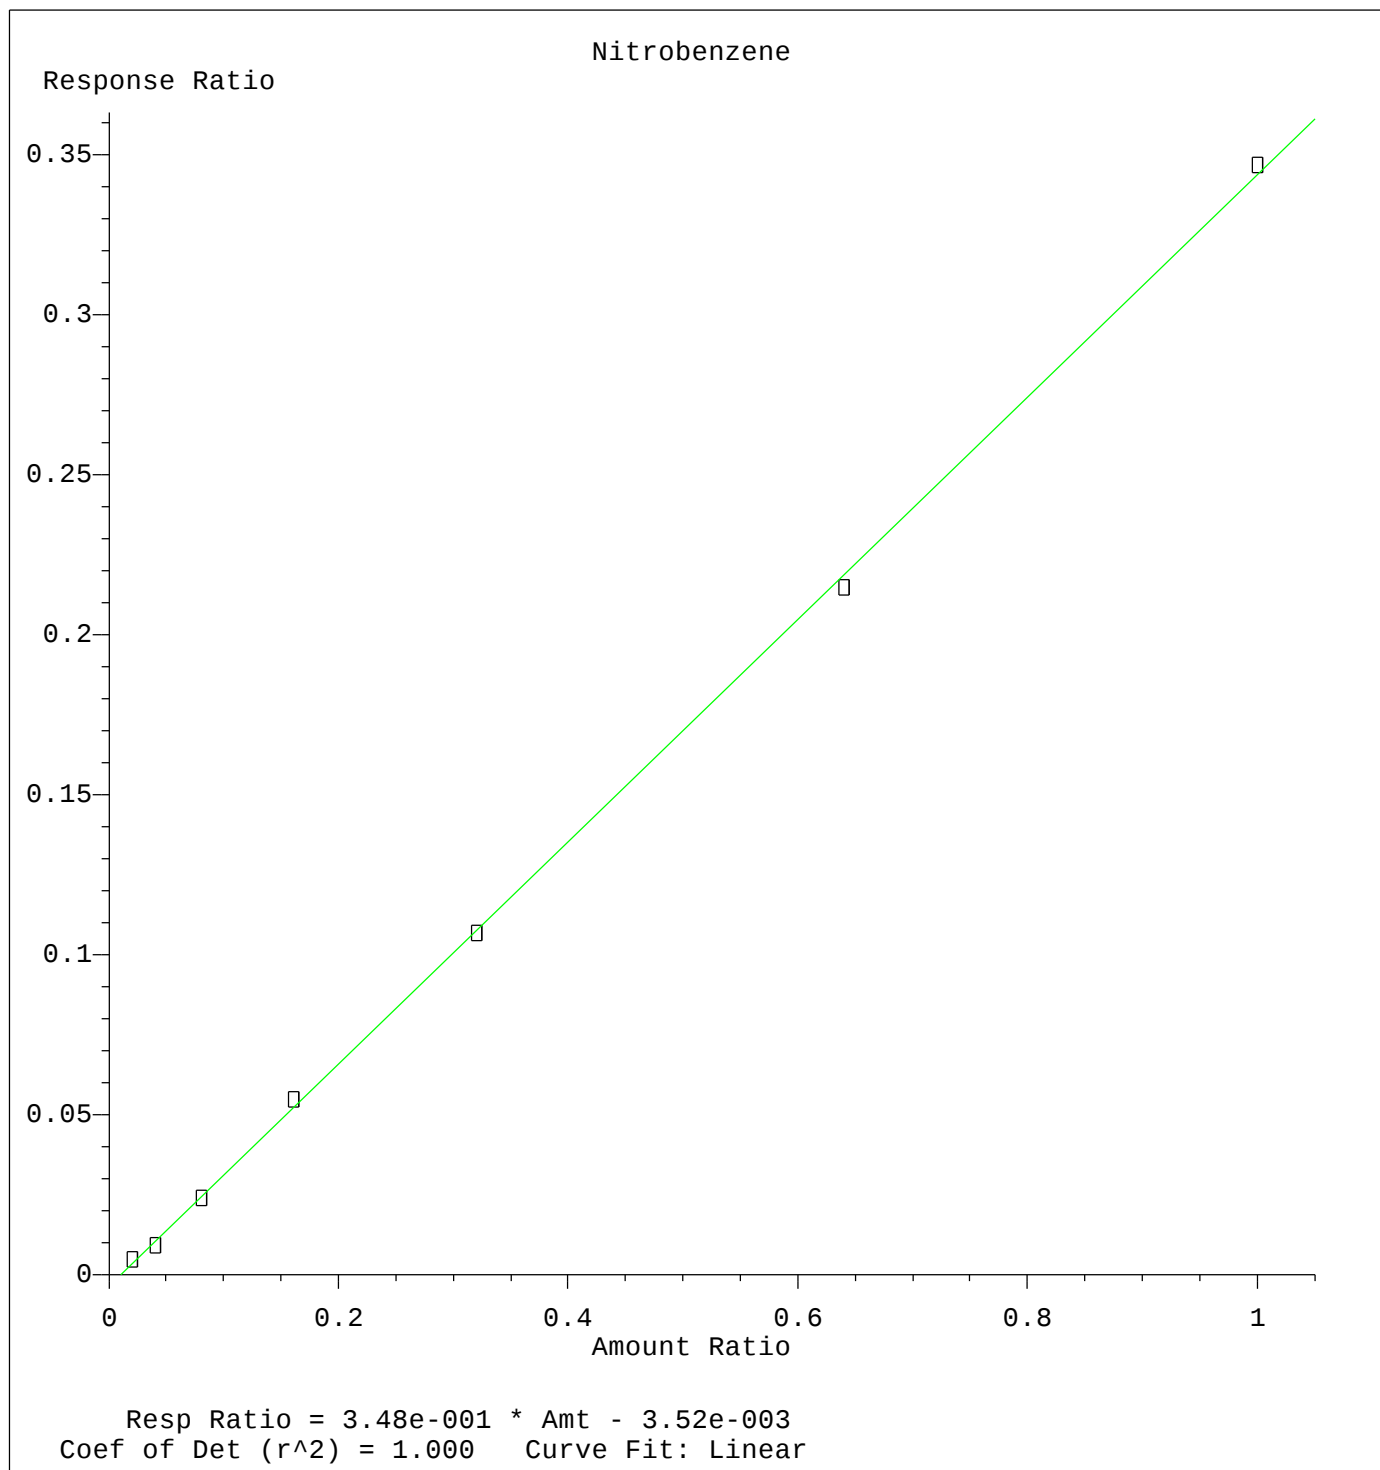


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

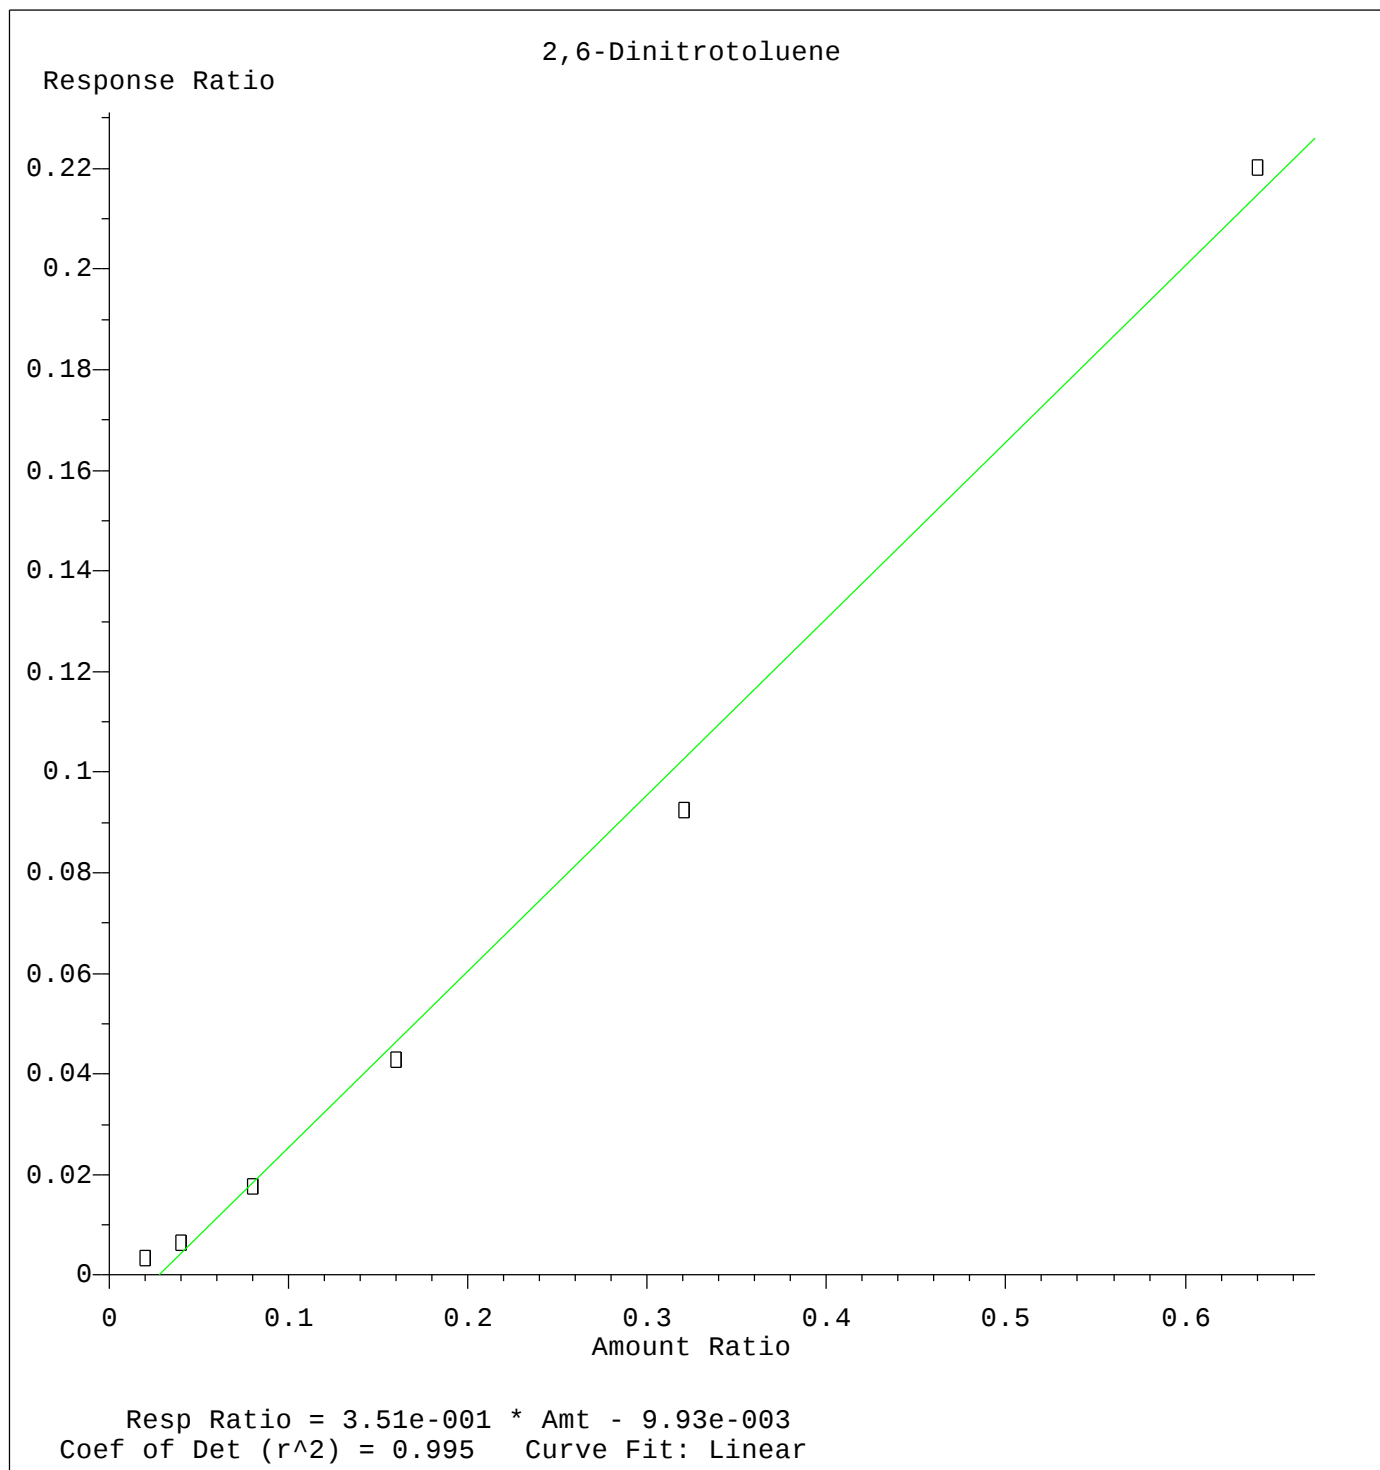


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

2,4-Dinitrotoluene

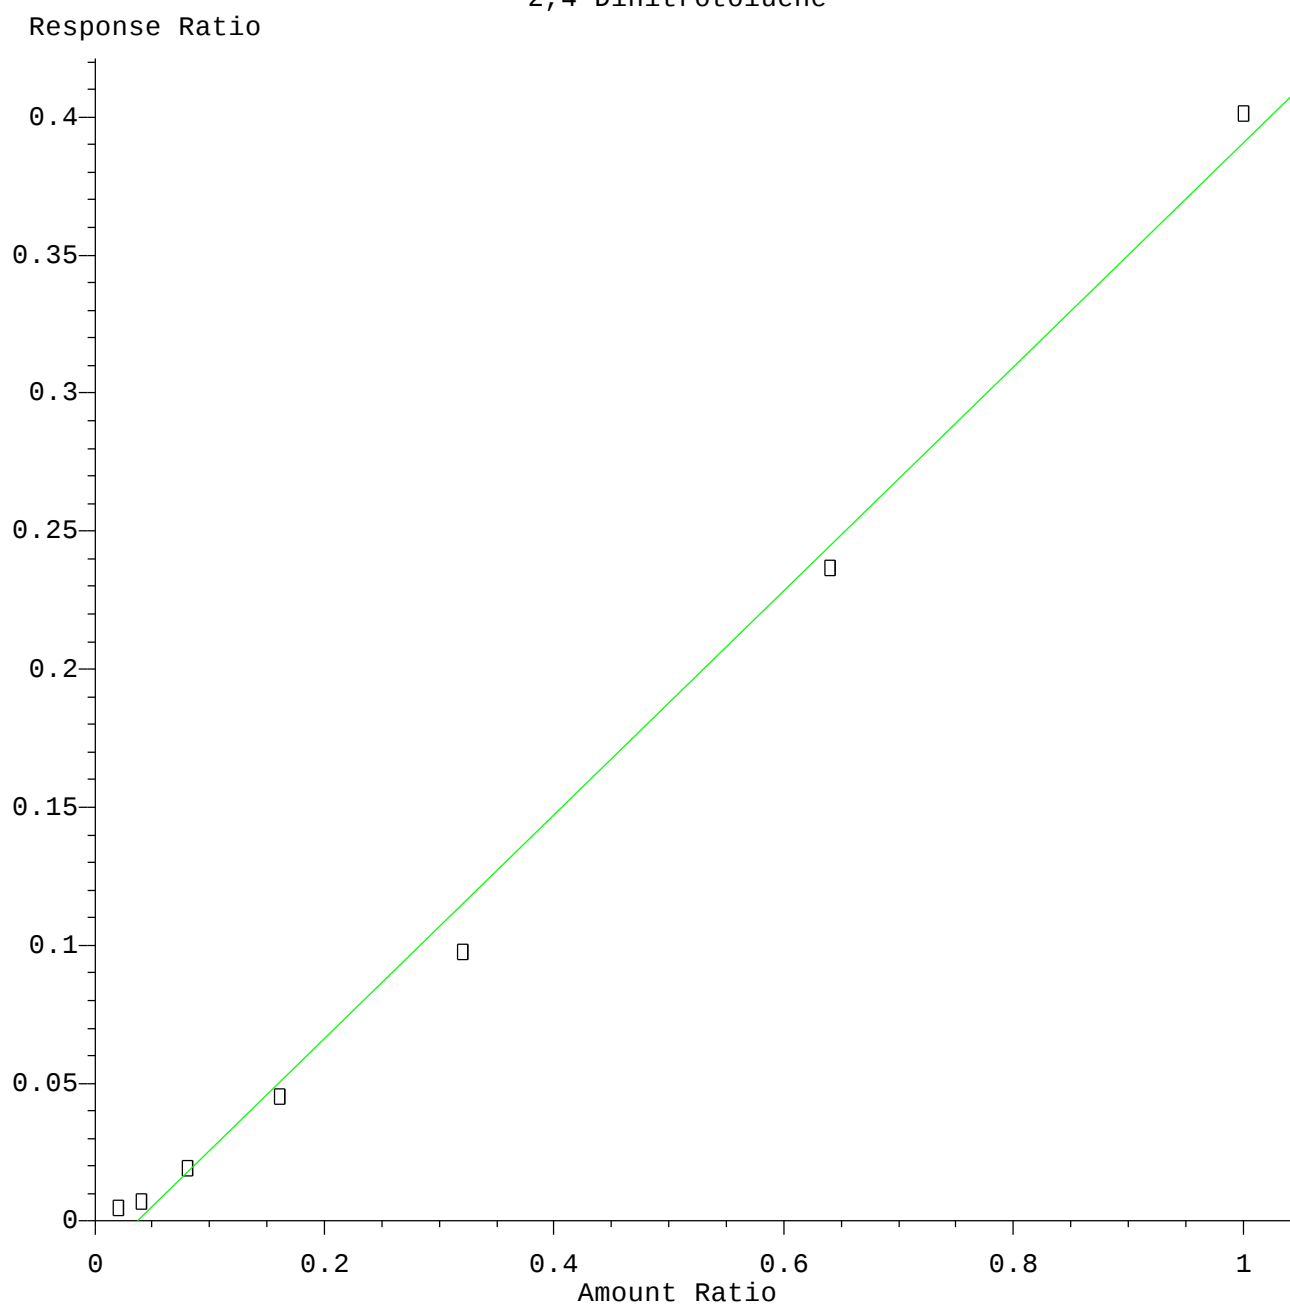


Resp Ratio = $4.05e-001 * \text{Amt} - 1.51e-002$
Coef of Det (r^2) = 0.995 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

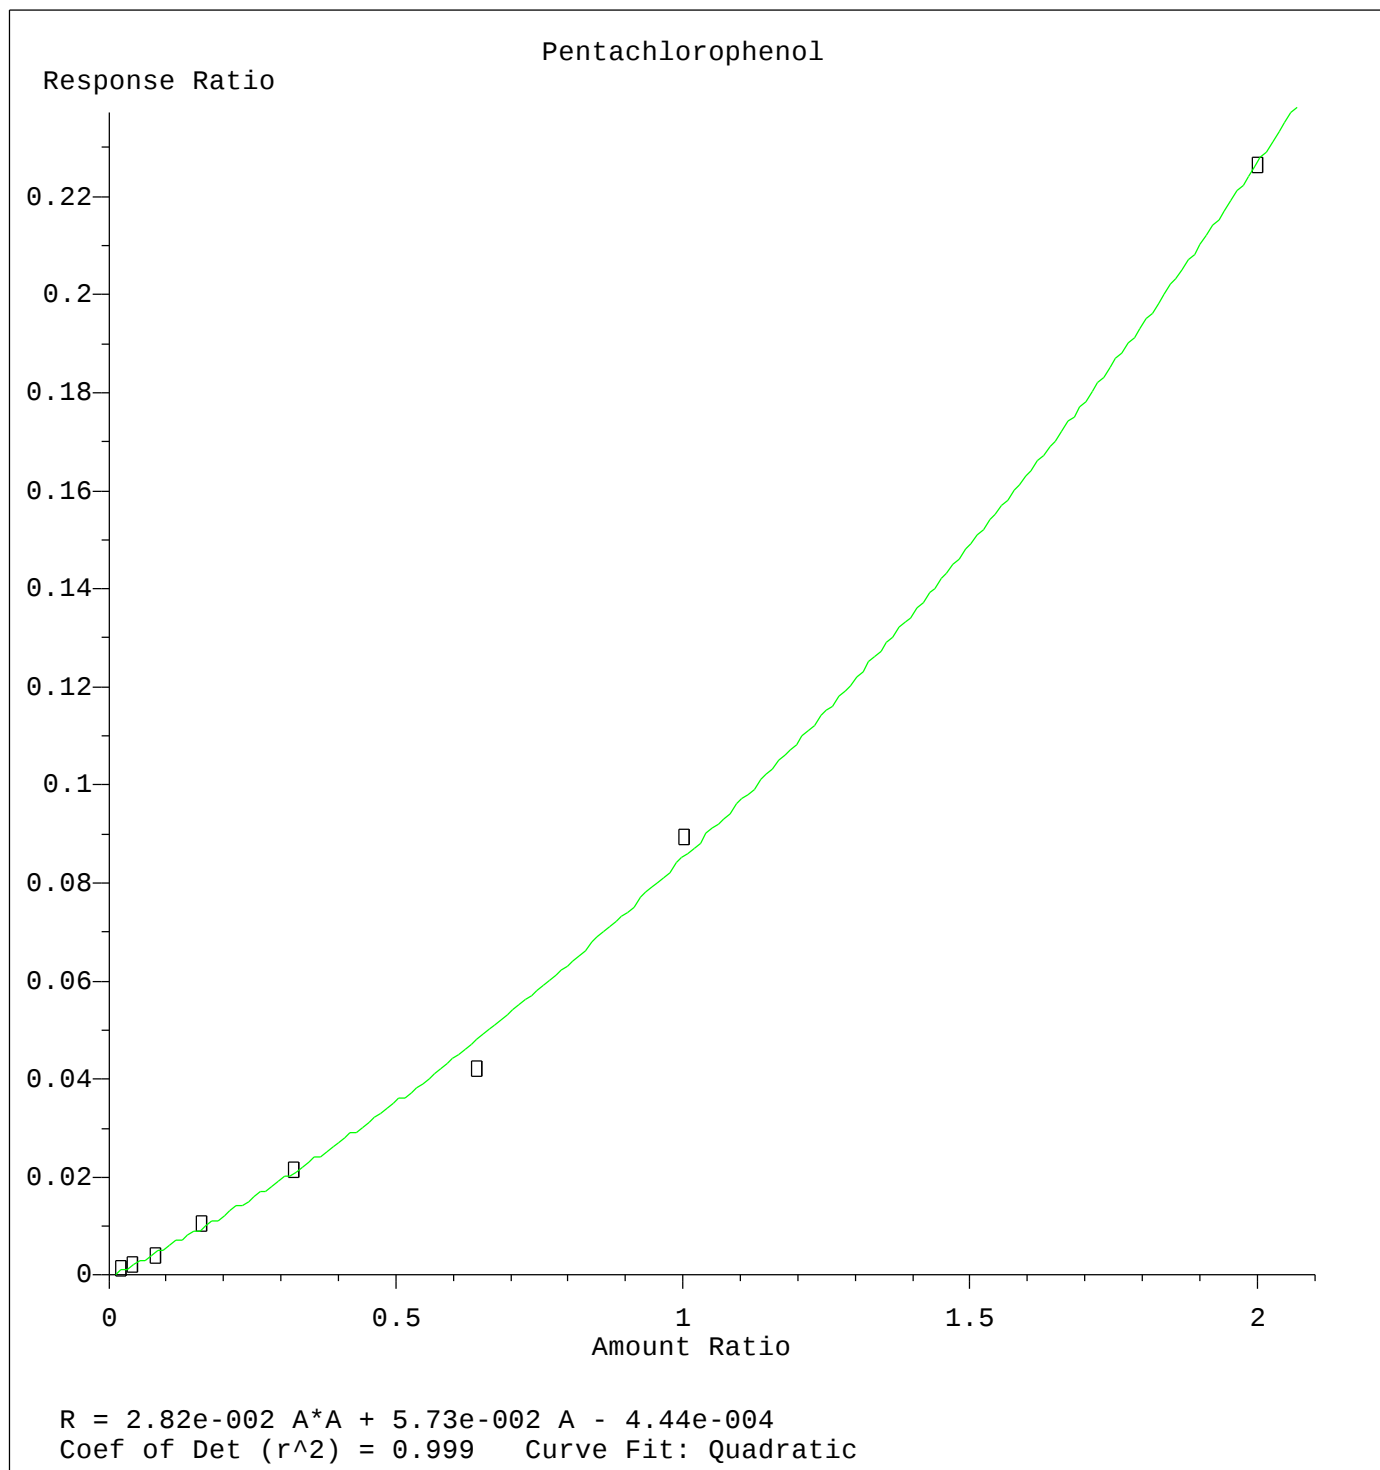

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

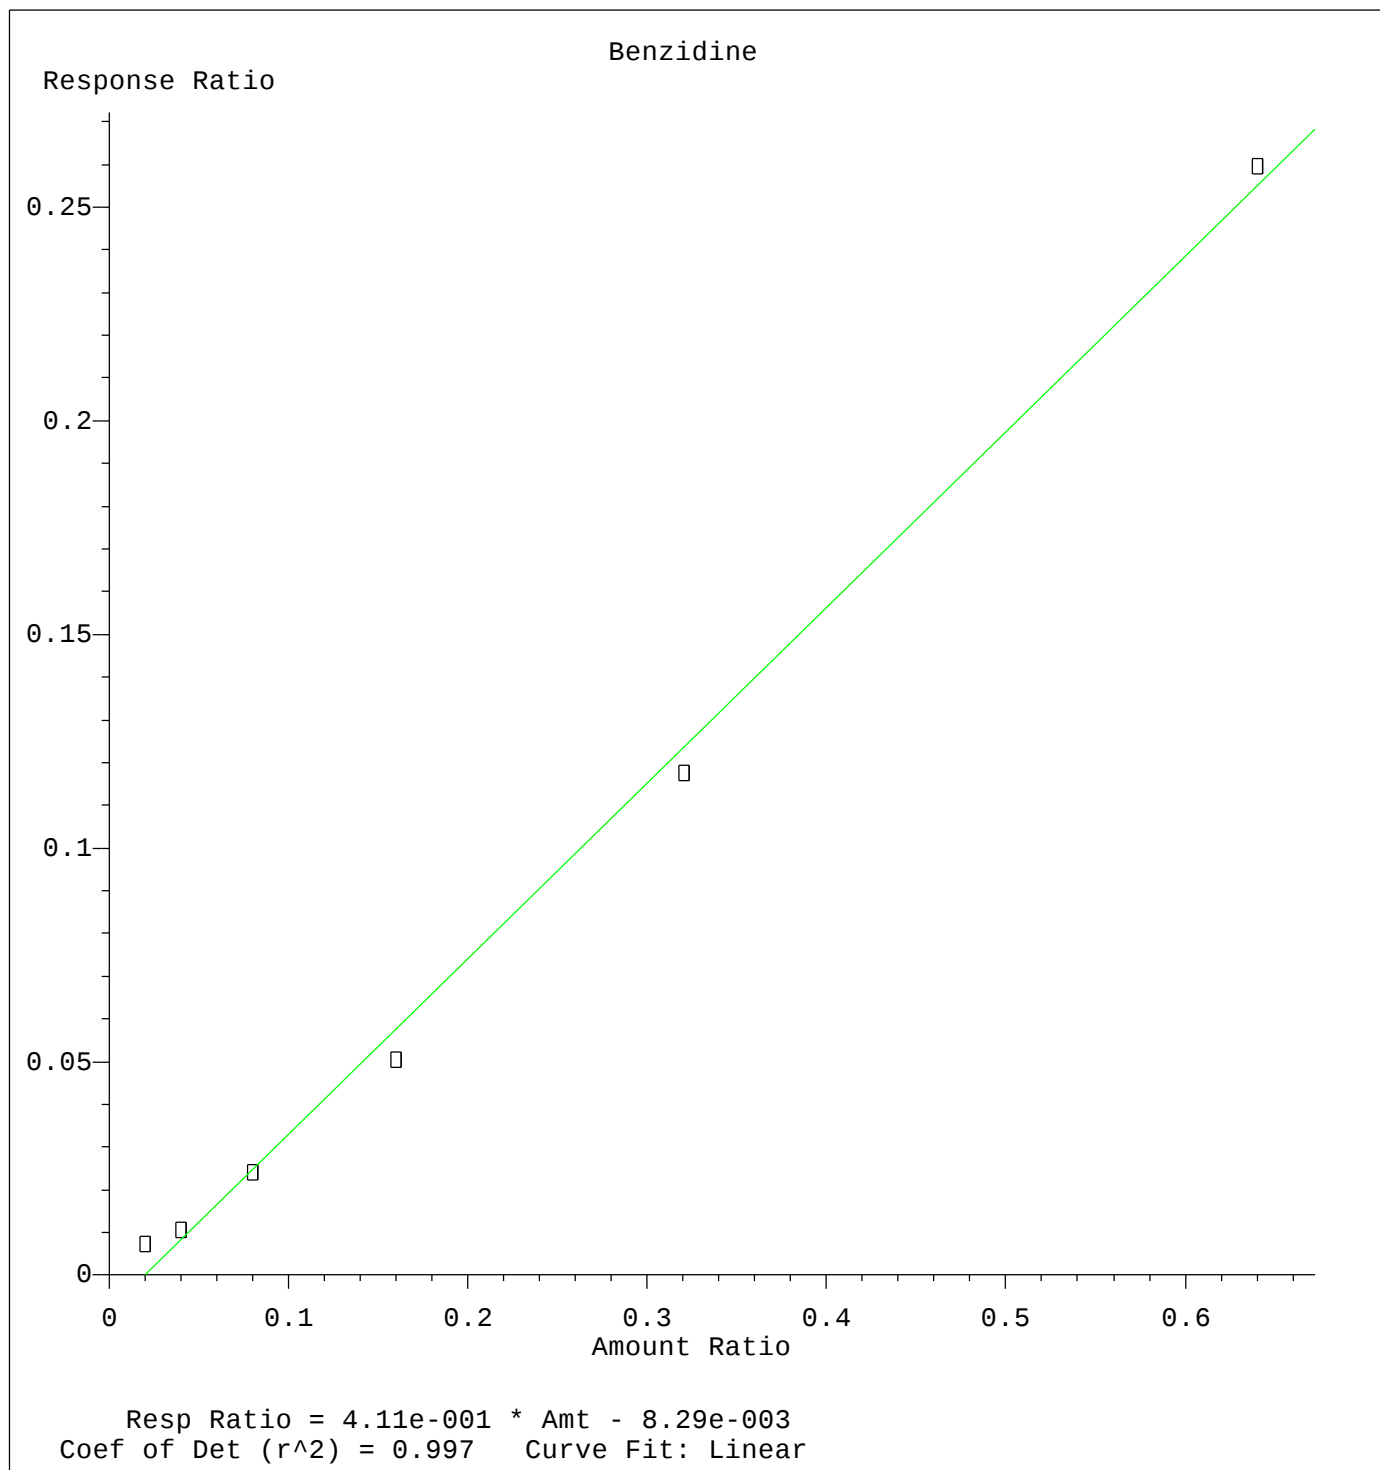


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

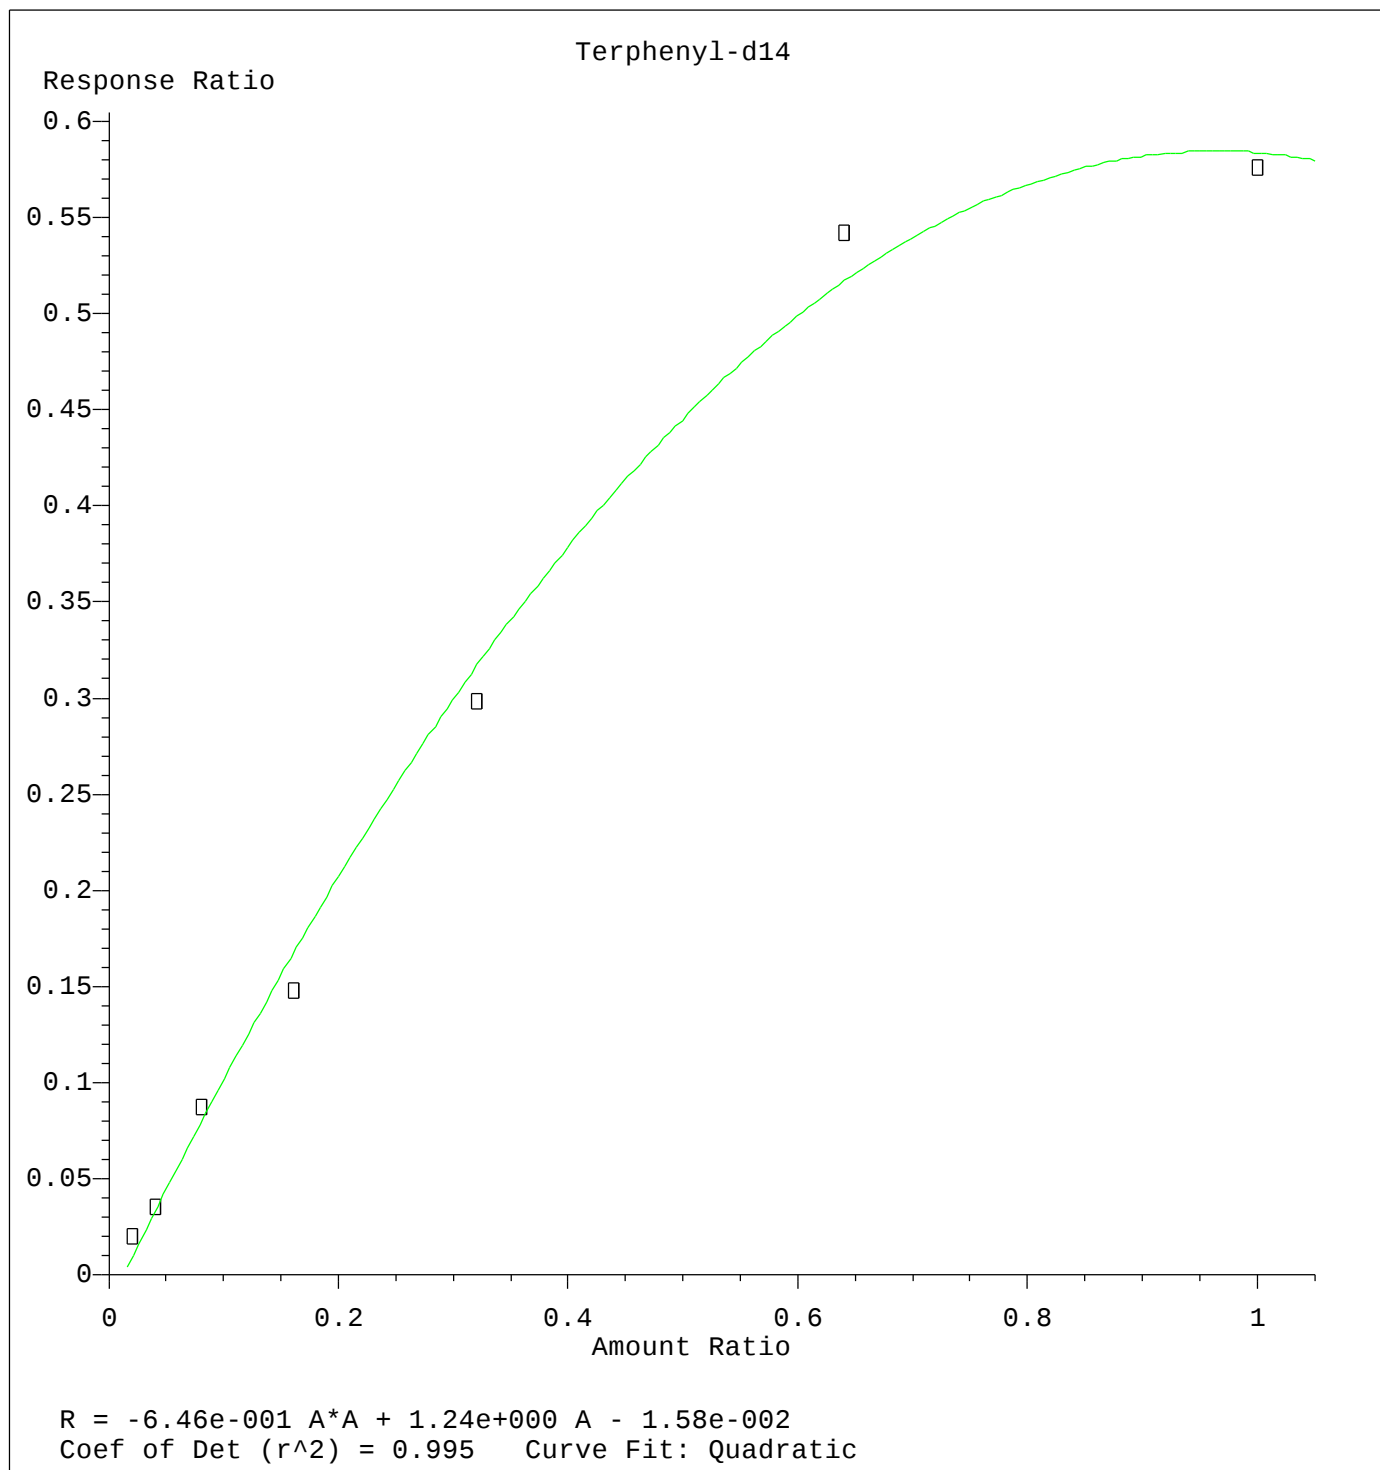

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

Benzo(a)anthracene


Response Ratio

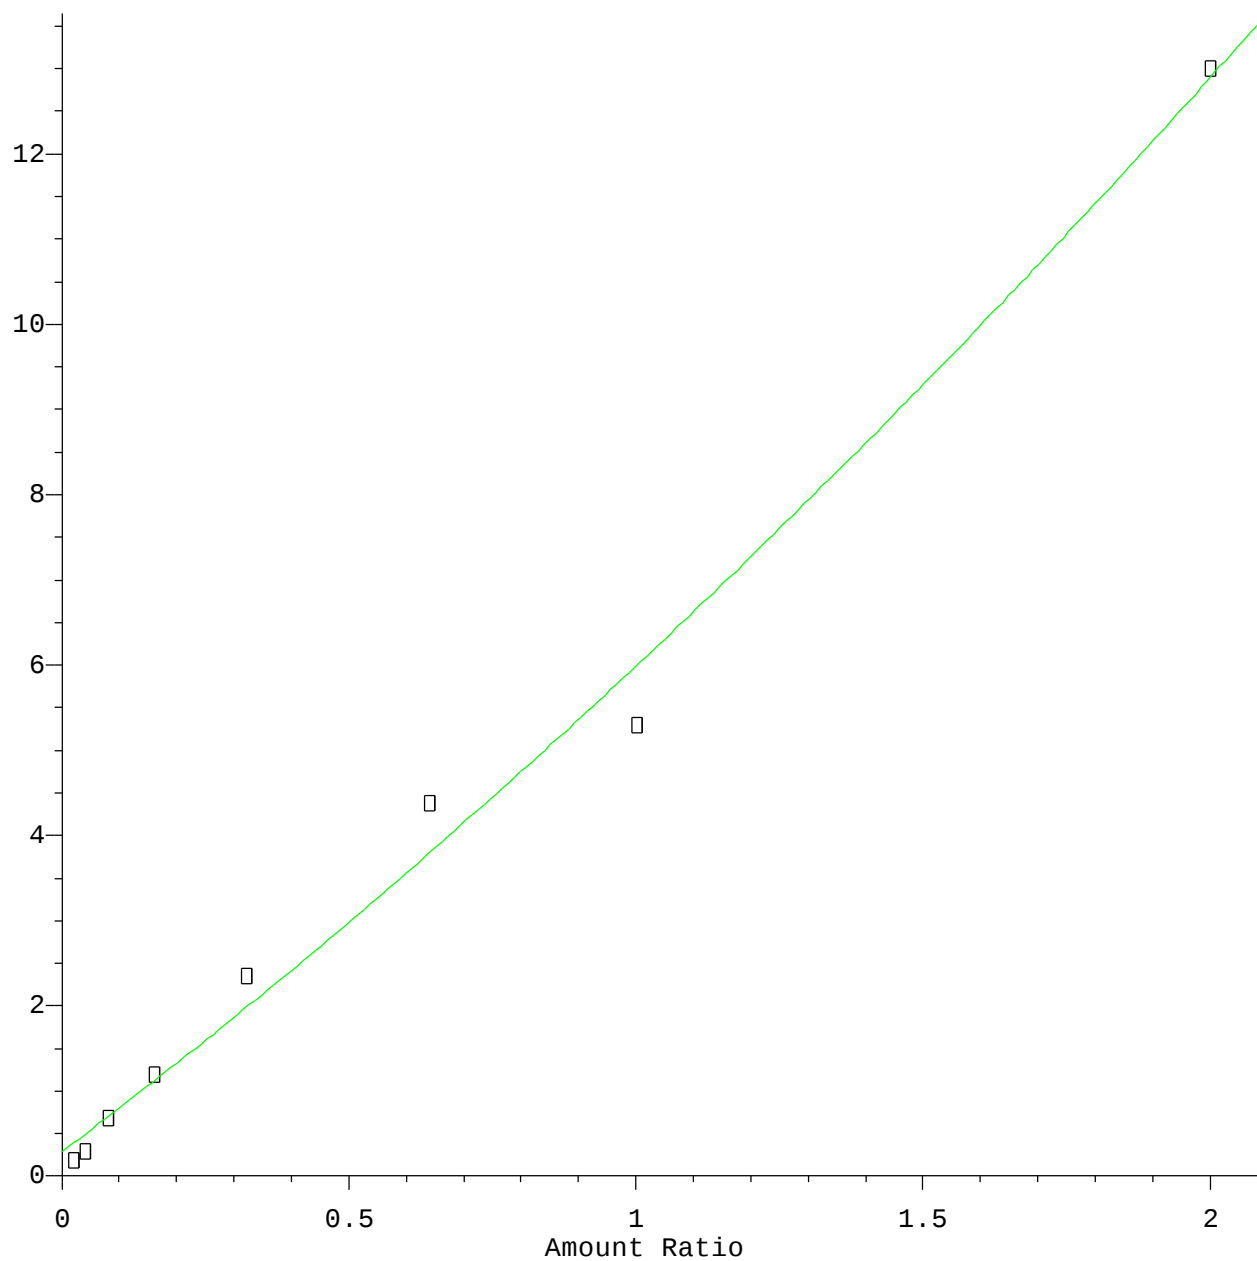

$R = 6.03e-001 A^2 + 5.10e+000 A + 2.83e-001$
Coef of Det (r^2) = 0.992 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016


3,3'-Dichlorobenzidine

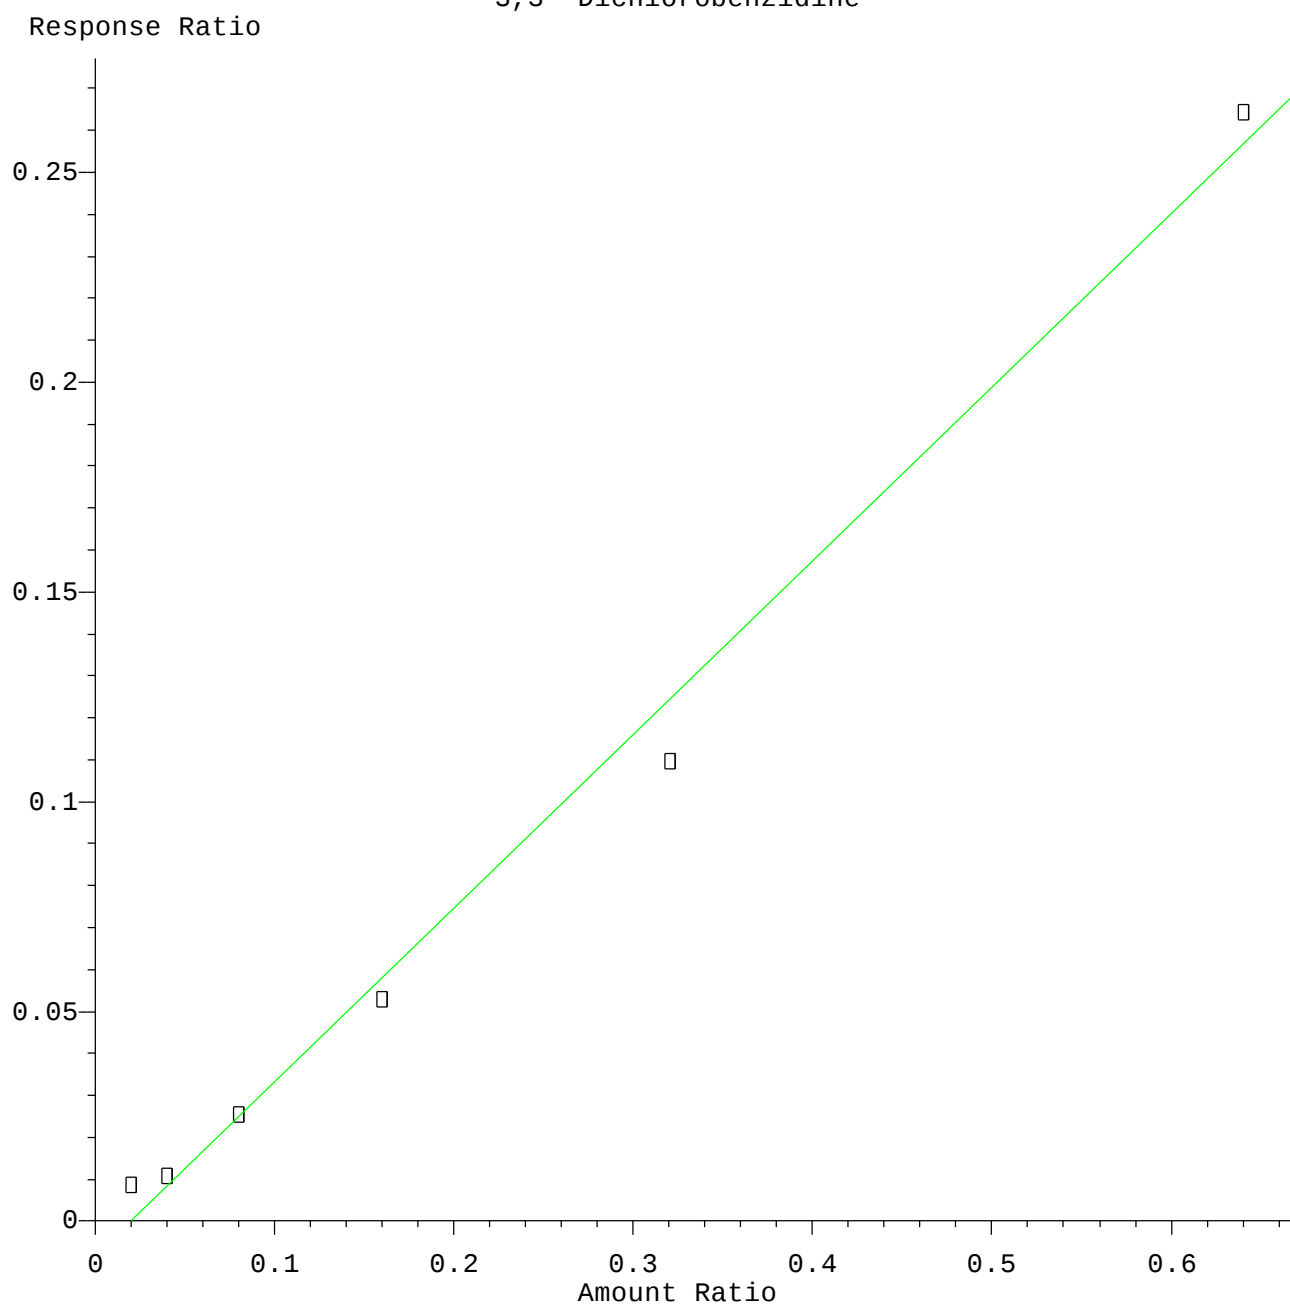

Resp Ratio = $4.13 \times 10^{-1} \times \text{Amt} - 8.32 \times 10^{-3}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

Bis(2-ethylhexyl)phthalate

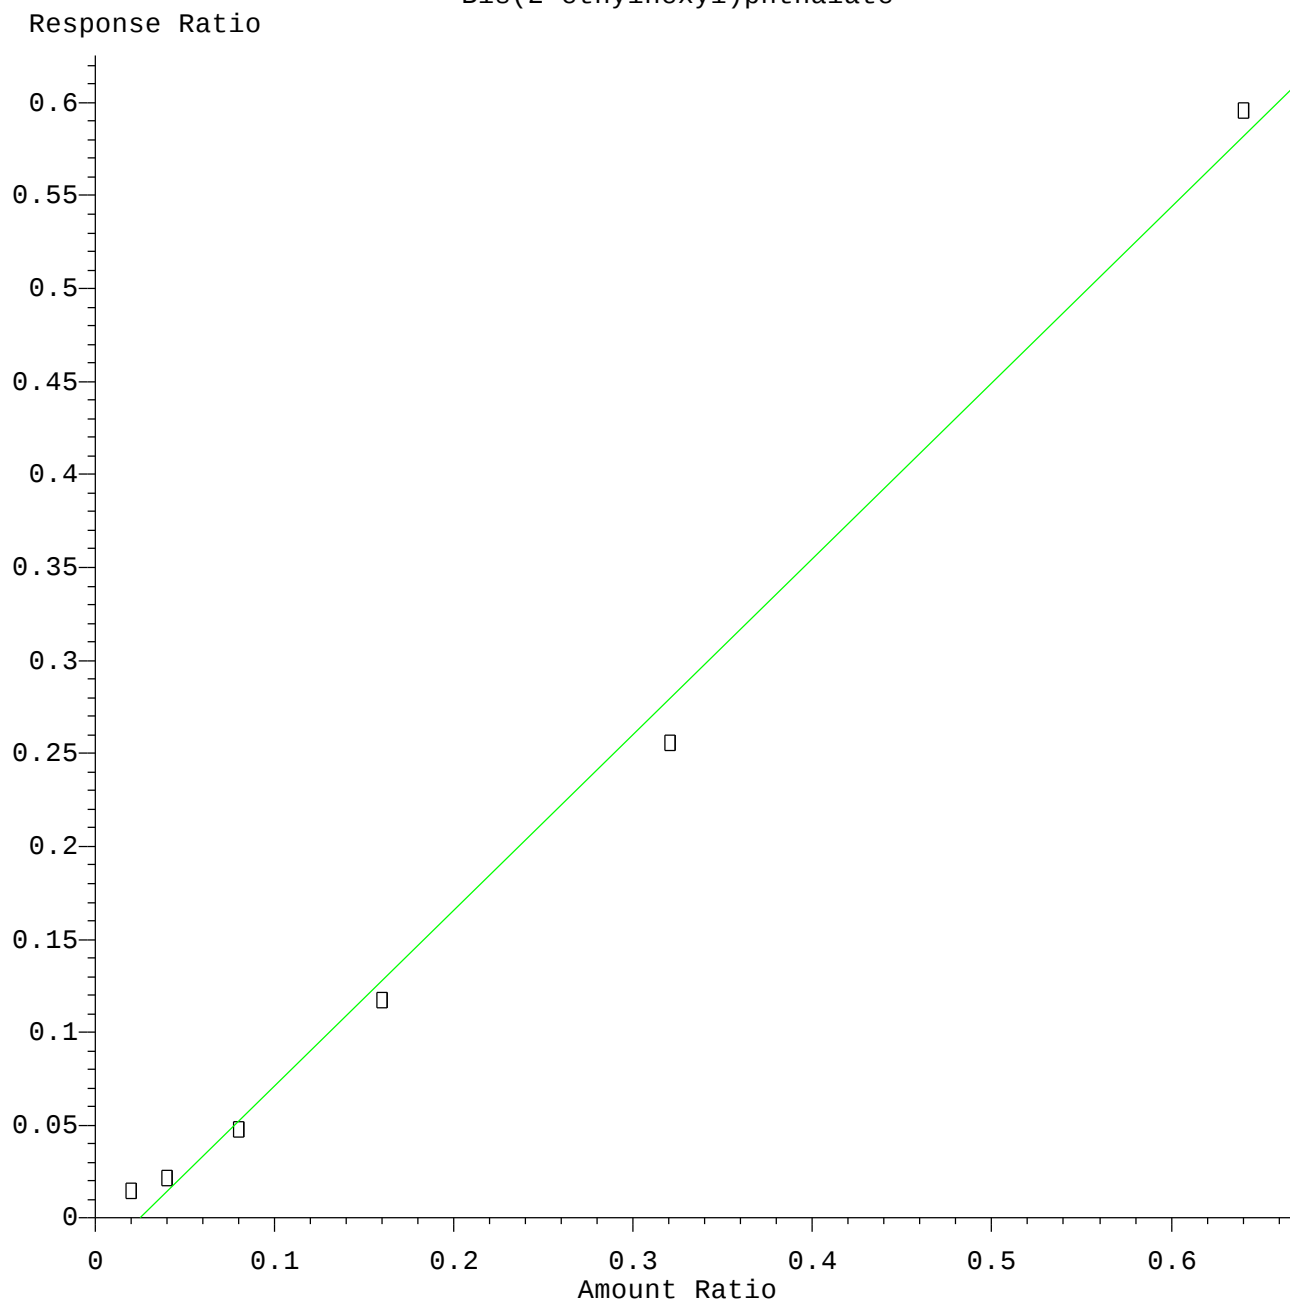


Resp Ratio = $9.45 \times 10^{-1} \times \text{Amt} - 2.32 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016

Indeno(1,2,3-cd)pyrene

Response Ratio

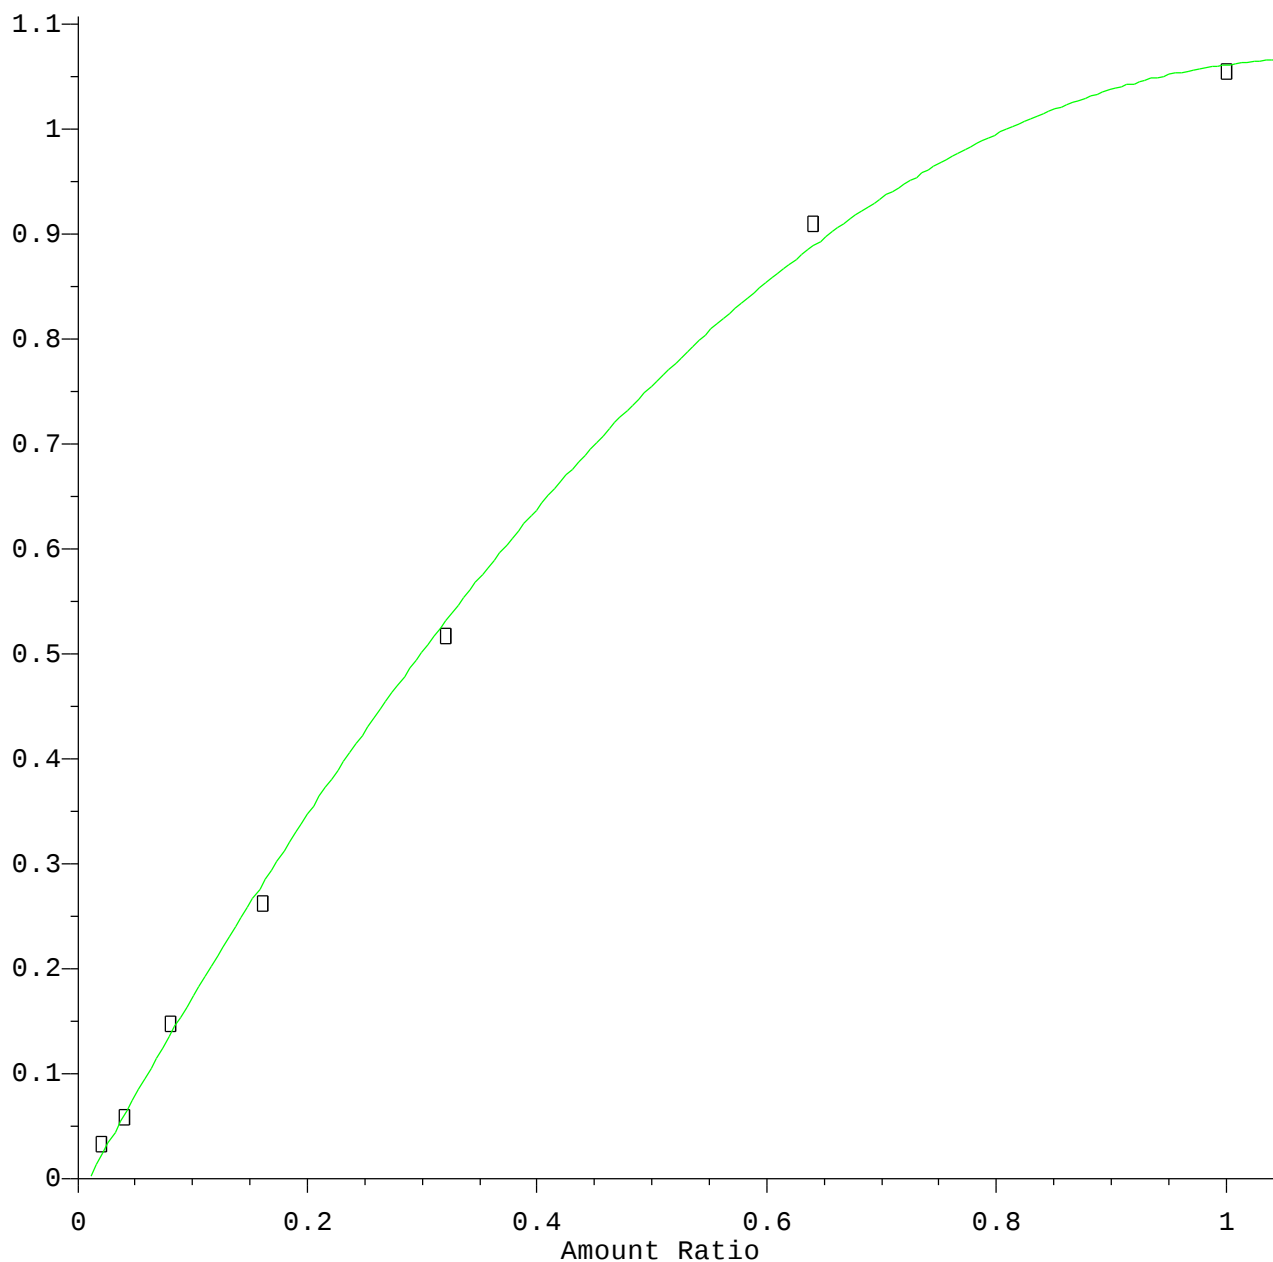

$R = -9.38e-001 A^2 + 2.02e+000 A - 1.82e-002$
Coef of Det (r^2) = 0.999 Curve Fit: Quadratic

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Calibration Table Last Updated: Wed Jun 08 16:11:34 2016