


Data Path : Z:\HPCHEM1\BNA E\DATA\BE060716\
 Data File : BE091875.D
 Acq On : 7 Jun 2016 9:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 08 16:11:34 2016

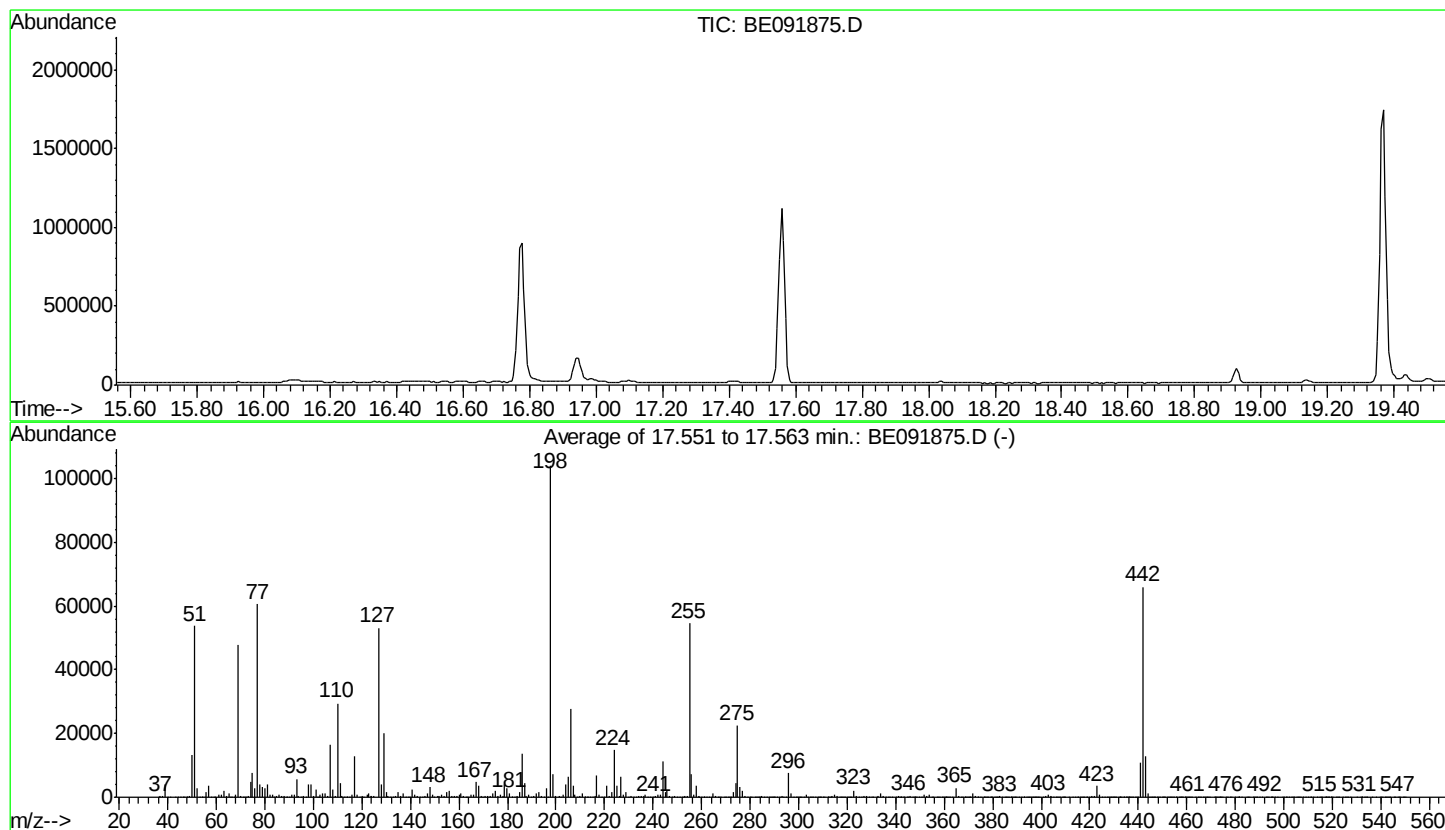

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	53789	PASS
68	69	0.00	2	1.5	738	PASS
69	198	0.00	100	46.0	47813	PASS
70	69	0.00	2	0.5	256	PASS
127	198	10	80	51.0	53098	PASS
197	198	0.00	2	0.2	204	PASS
198	198	100	100	100.0	104038	PASS
199	198	5	9	6.8	7056	PASS
275	198	10	60	21.5	22326	PASS
365	198	1	100	2.9	2980	PASS
441	442	0.01	24	16.3	10740	PASS
442	198	50	100	63.3	65903	PASS
443	442	15	24	19.3	12719	PASS