


Data Path : Z:\HPCHEM1\BNA E\DATA\BE060716\
Data File : BE091885.D
Acq On : 7 Jun 2016 17:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060716.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 08 16:11:34 2016

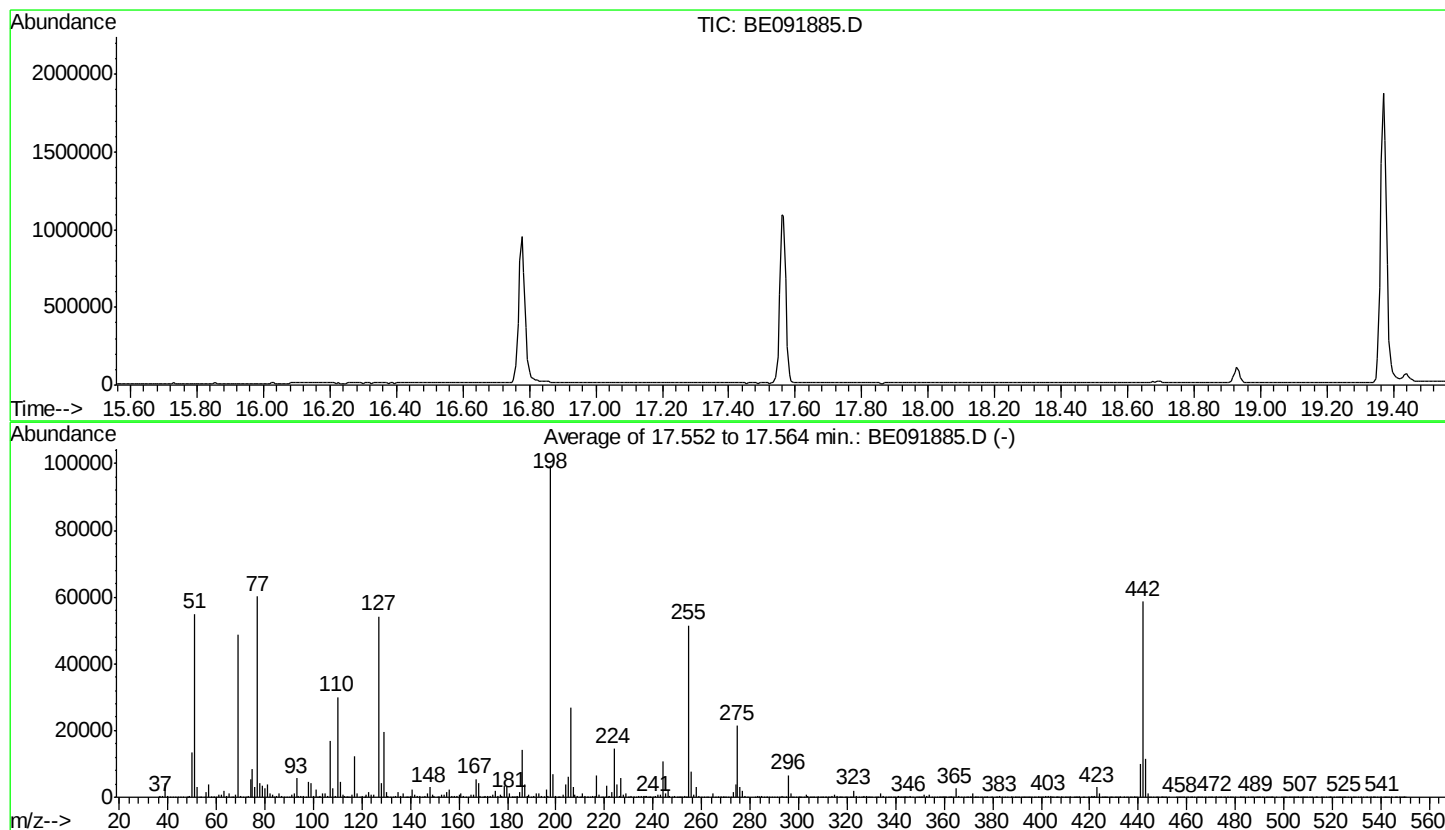

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	55022	PASS
68	69	0.00	2	1.7	811	PASS
69	198	0.00	100	49.1	48795	PASS
70	69	0.00	2	0.5	267	PASS
127	198	10	80	54.5	54128	PASS
197	198	0.00	2	0.2	224	PASS
198	198	100	100	100.0	99386	PASS
199	198	5	9	7.1	7102	PASS
275	198	10	60	21.6	21451	PASS
365	198	1	100	2.6	2585	PASS
441	442	0.01	24	16.9	9885	PASS
442	198	50	100	58.9	58520	PASS
443	442	15	24	20.0	11702	PASS