
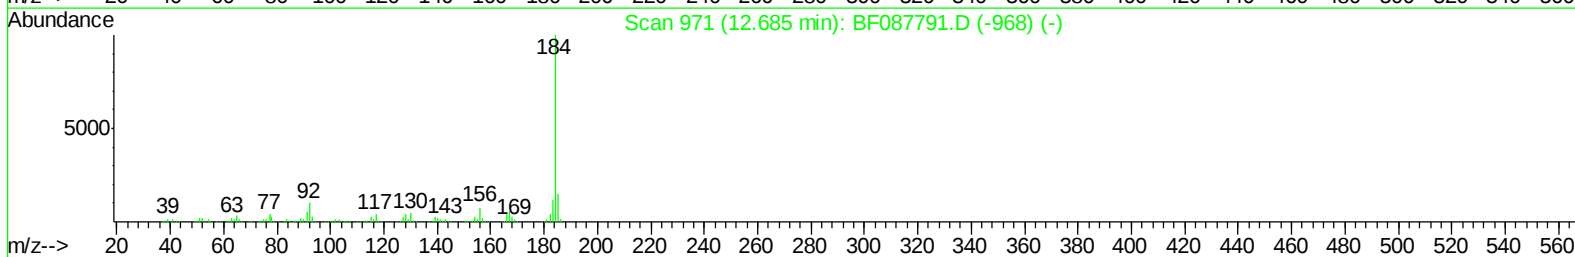
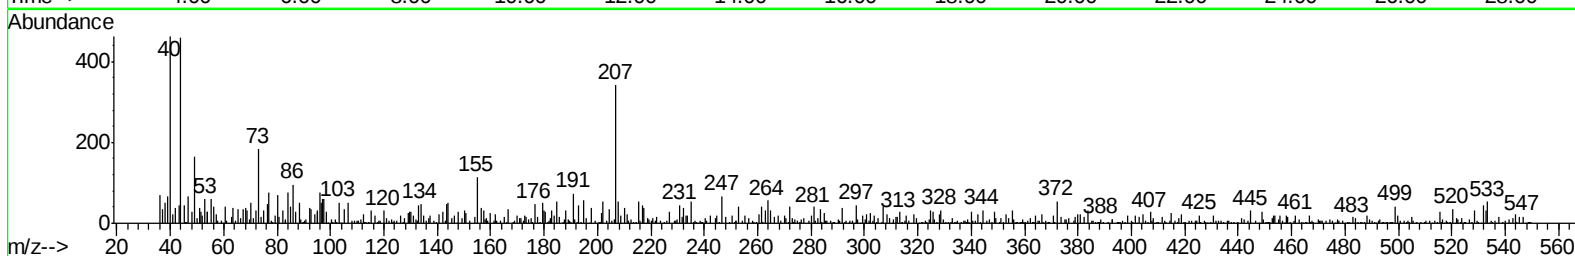


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE060816\
Data File : BE091899.D
Acq On : 8 Jun 2016 13:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:05:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

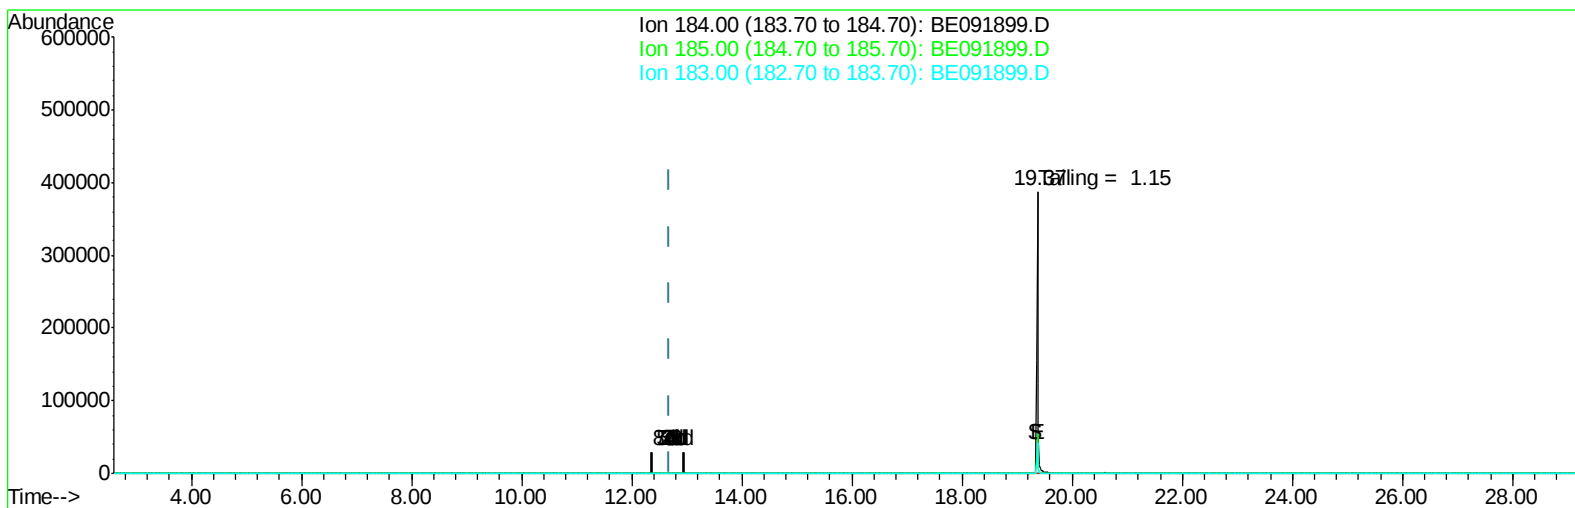

TIC: BE091899.D

(76) Benzidine




12.758min (+0.073) 131.33ng

response 40

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	21.62#
183.00	11.60	68.92#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE060816\
Data File : BE091899.D
Acq On : 8 Jun 2016 13:26
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 09 05:05:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 18:51:55 2016
Response via : Initial Calibration

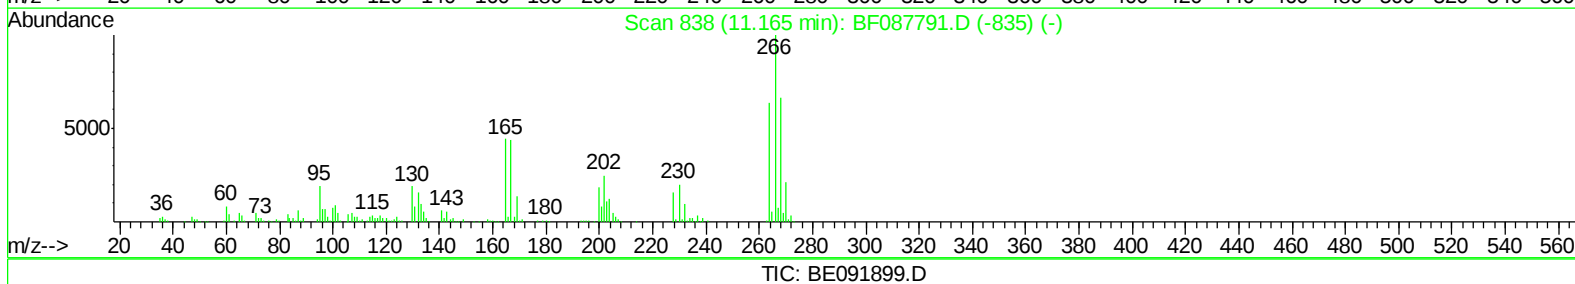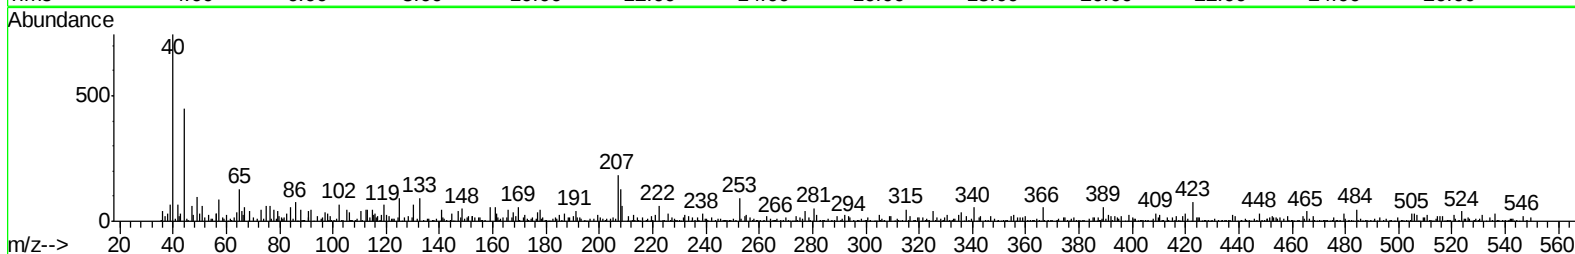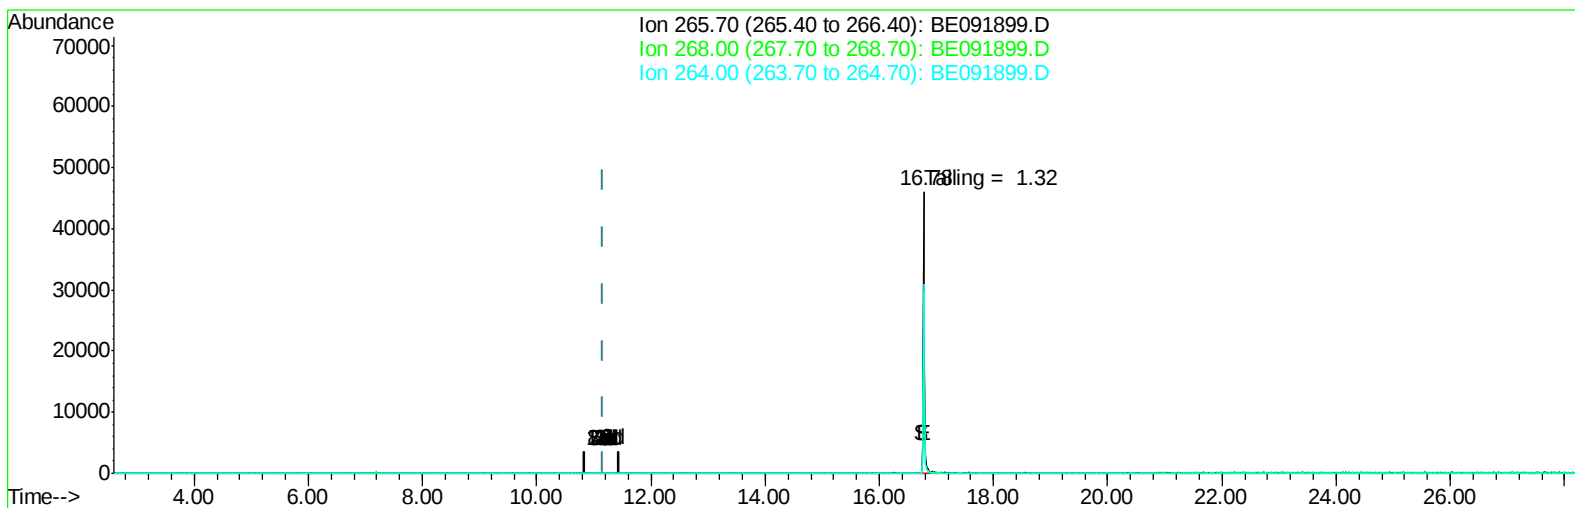

TIC: BE091899.D

(69) Pentachlorophenol (C)

10.989min (-0.176) 37.23ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	54.55
264.00	62.00	72.73
0.00	0.00	0.00