
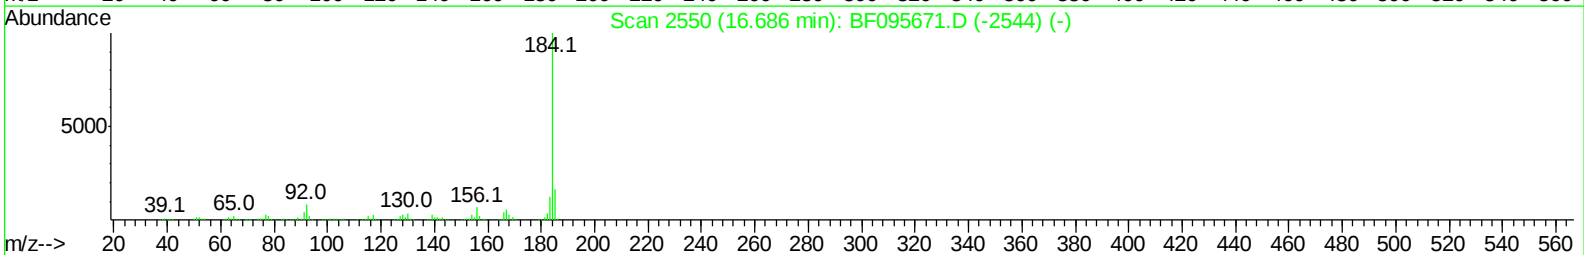
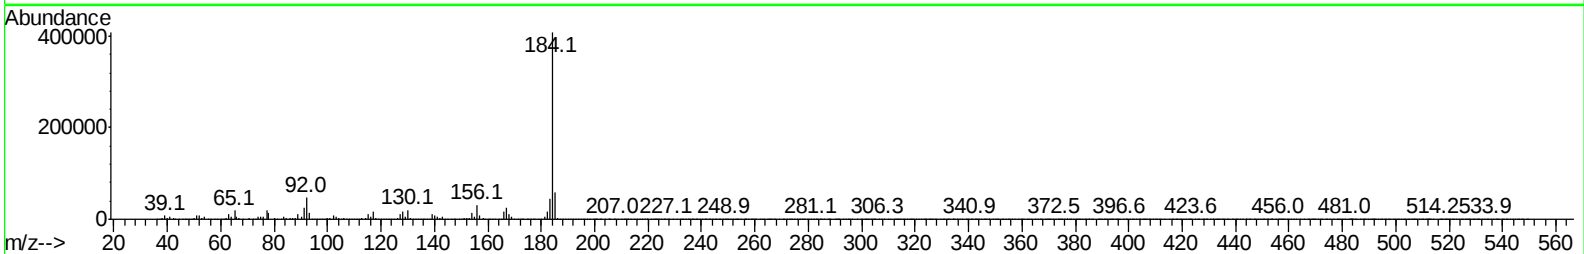


Data Path : Z:\HPCHEM1\BNA E\DATA\BE061217\
Data File : BE093105.D
Acq On : 12 Jun 2017 16:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 08:38:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

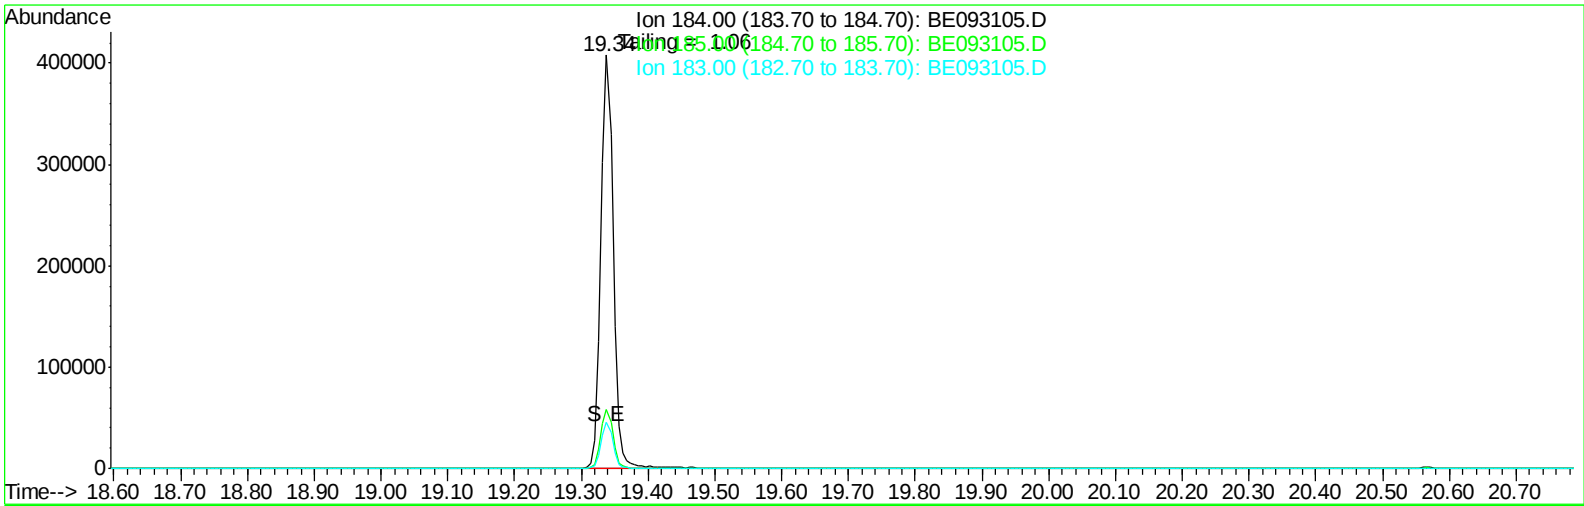

TIC: BE093105.D

(76) Benzidine




16.677min (-0.009) 27.45ng

response 39

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	40.35#
183.00	12.20	59.65#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061217\
Data File : BE093105.D
Acq On : 12 Jun 2017 16:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 13 08:38:54 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF060517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 05 16:15:31 2017
Response via : Initial Calibration

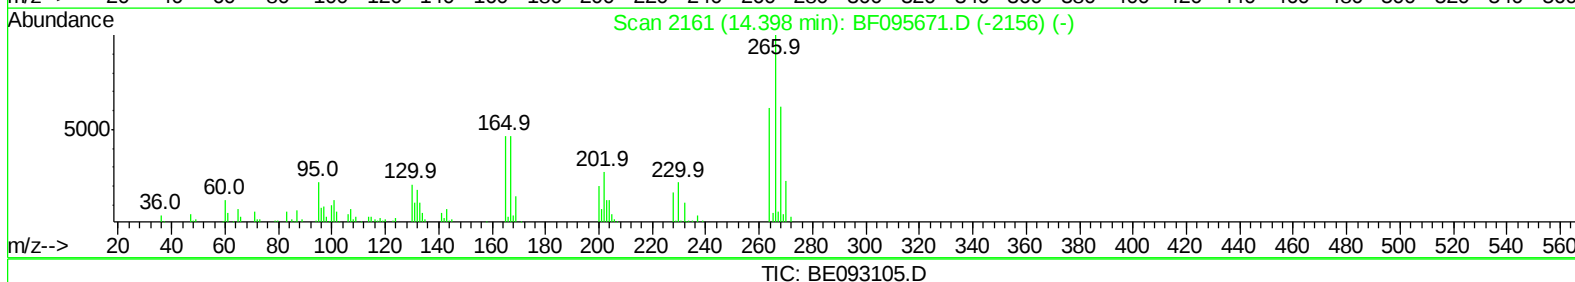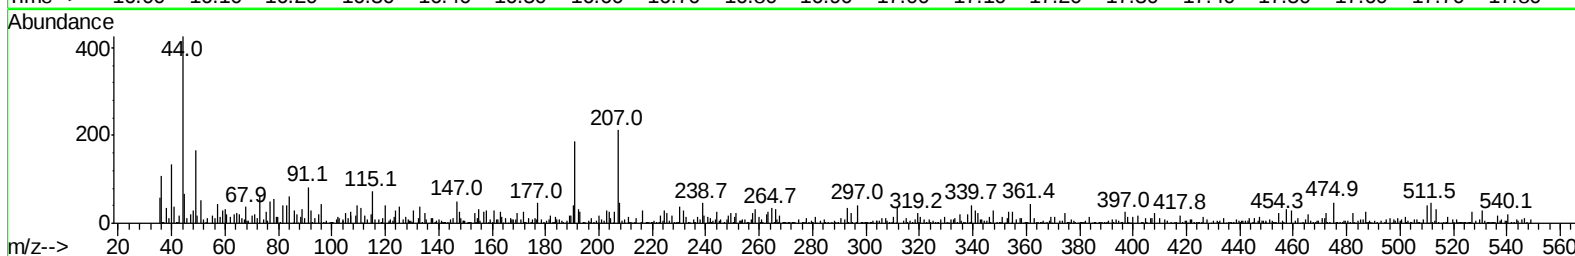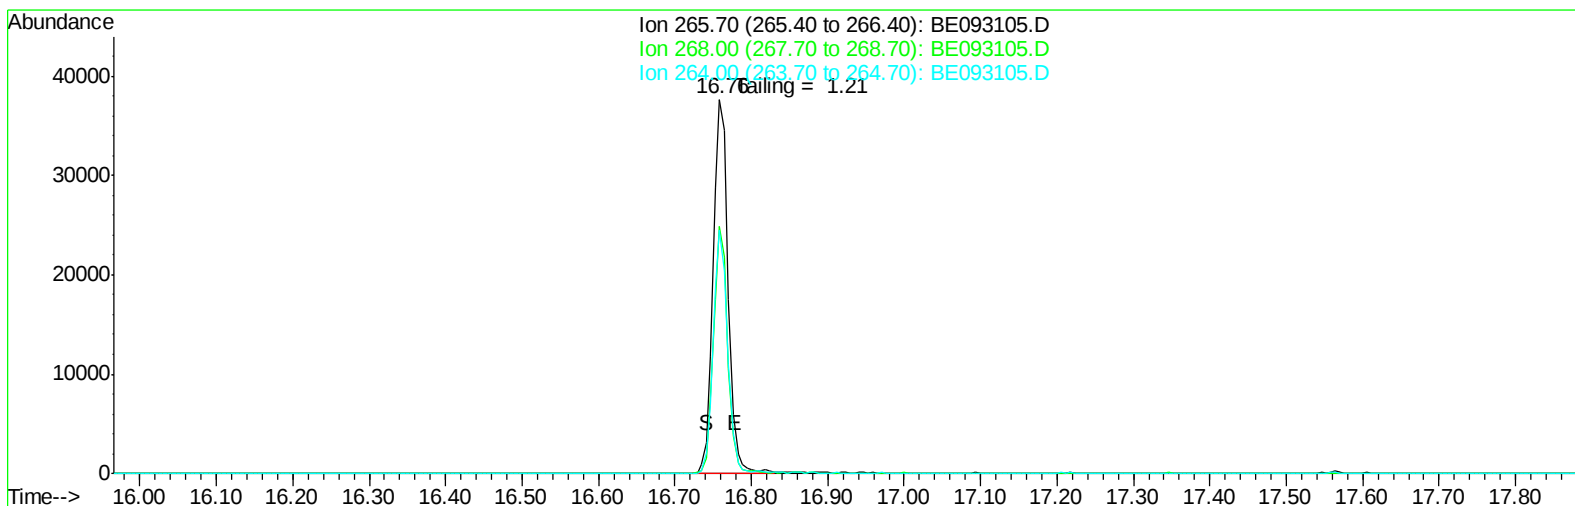

TIC: BE093105.D

(69) Pentachlorophenol (C)

14.368min (-0.029) 644.54ng

response 27

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	51.43
264.00	64.60	97.14#
0.00	0.00	0.00