


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061217\
Data File : BE093094.D
Acq On : 12 Jun 2017 8:32
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 12 14:07:54 2017

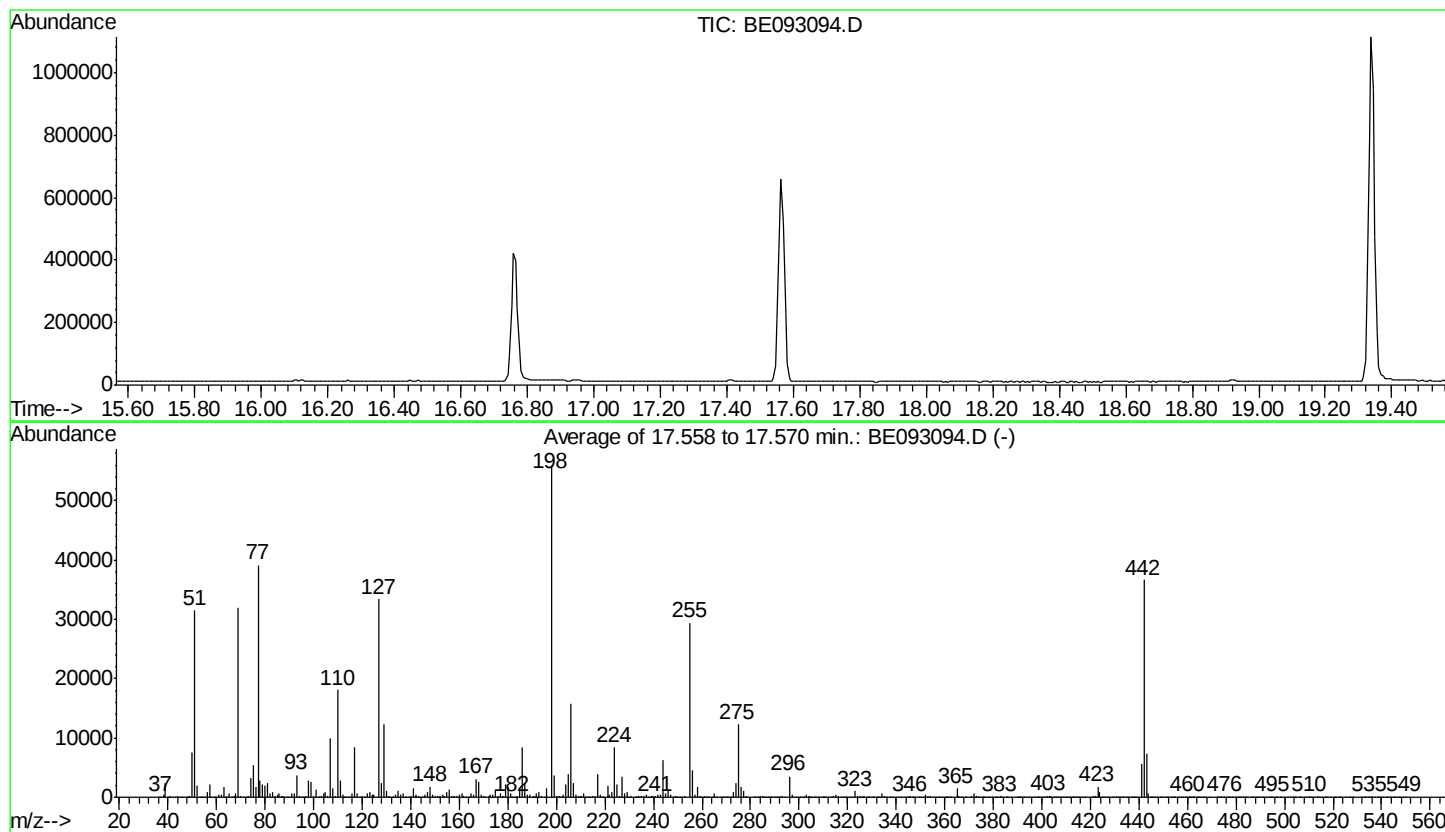

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	31482	PASS
68	69	0.00	2	1.8	563	PASS
69	198	0.00	100	57.2	31970	PASS
70	69	0.00	2	0.5	153	PASS
127	198	10	80	59.8	33421	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55903	PASS
199	198	5	9	6.5	3618	PASS
275	198	10	60	21.9	12235	PASS
365	198	1	100	2.5	1417	PASS
441	442	0.01	24	15.6	5720	PASS
442	198	50	100	65.6	36670	PASS
443	442	15	24	20.1	7374	PASS