


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061217\
 Data File : BE093105.D
 Acq On : 12 Jun 2017 16:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 12 14:07:54 2017

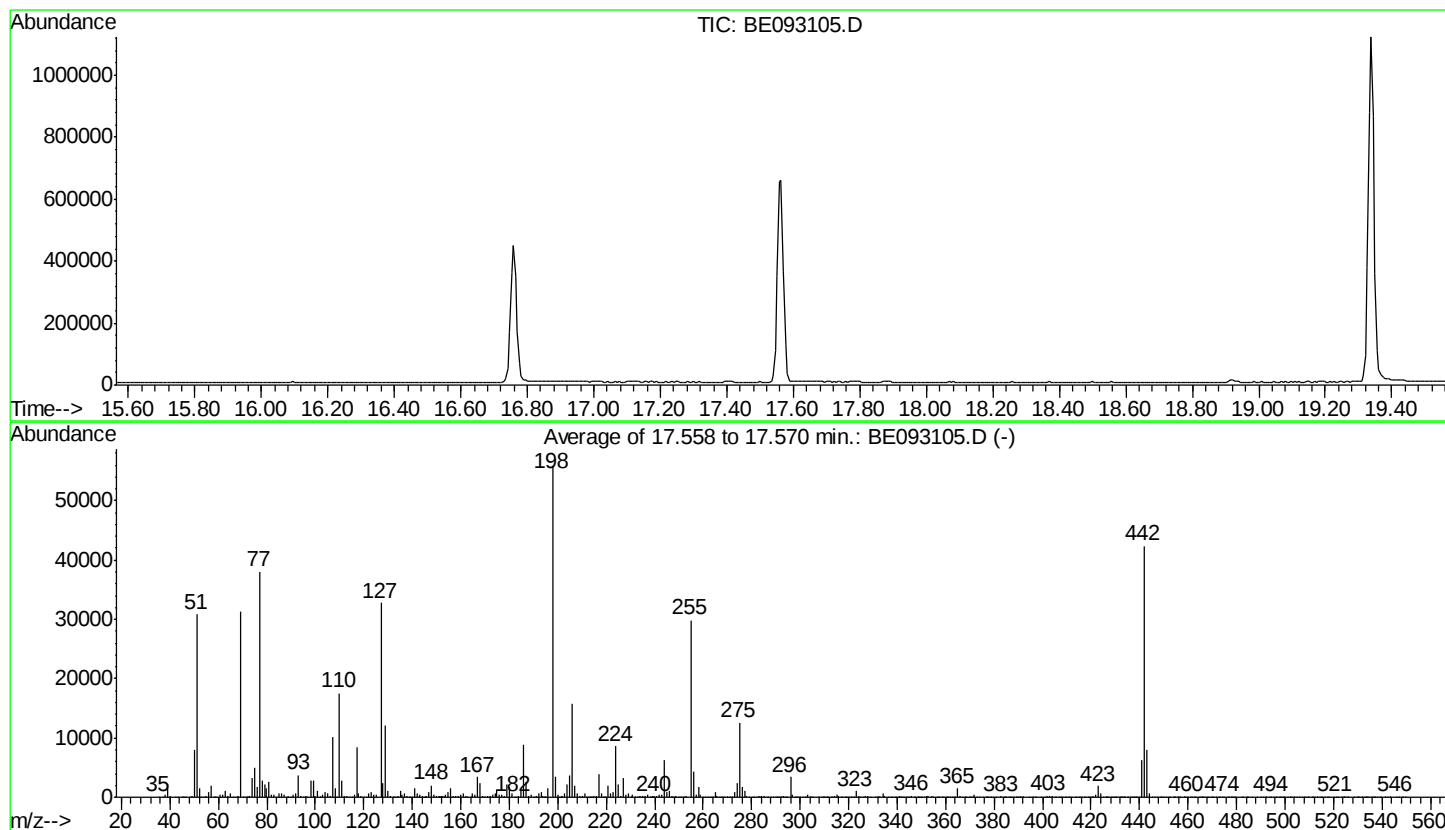

AutoFind: Scans 2548, 2549, 2550; Background Corrected with Scan 2541

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.0	30777	PASS
68	69	0.00	2	0.4	134	PASS
69	198	0.00	100	55.9	31270	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	58.5	32729	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55923	PASS
199	198	5	9	6.3	3534	PASS
275	198	10	60	22.5	12581	PASS
365	198	1	100	2.5	1426	PASS
441	442	0.01	24	15.0	6349	PASS
442	198	50	100	75.7	42350	PASS
443	442	15	24	18.8	7964	PASS