


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061217\
 Data File : BE093121.D
 Acq On : 13 Jun 2017 3:08
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 12 14:07:54 2017

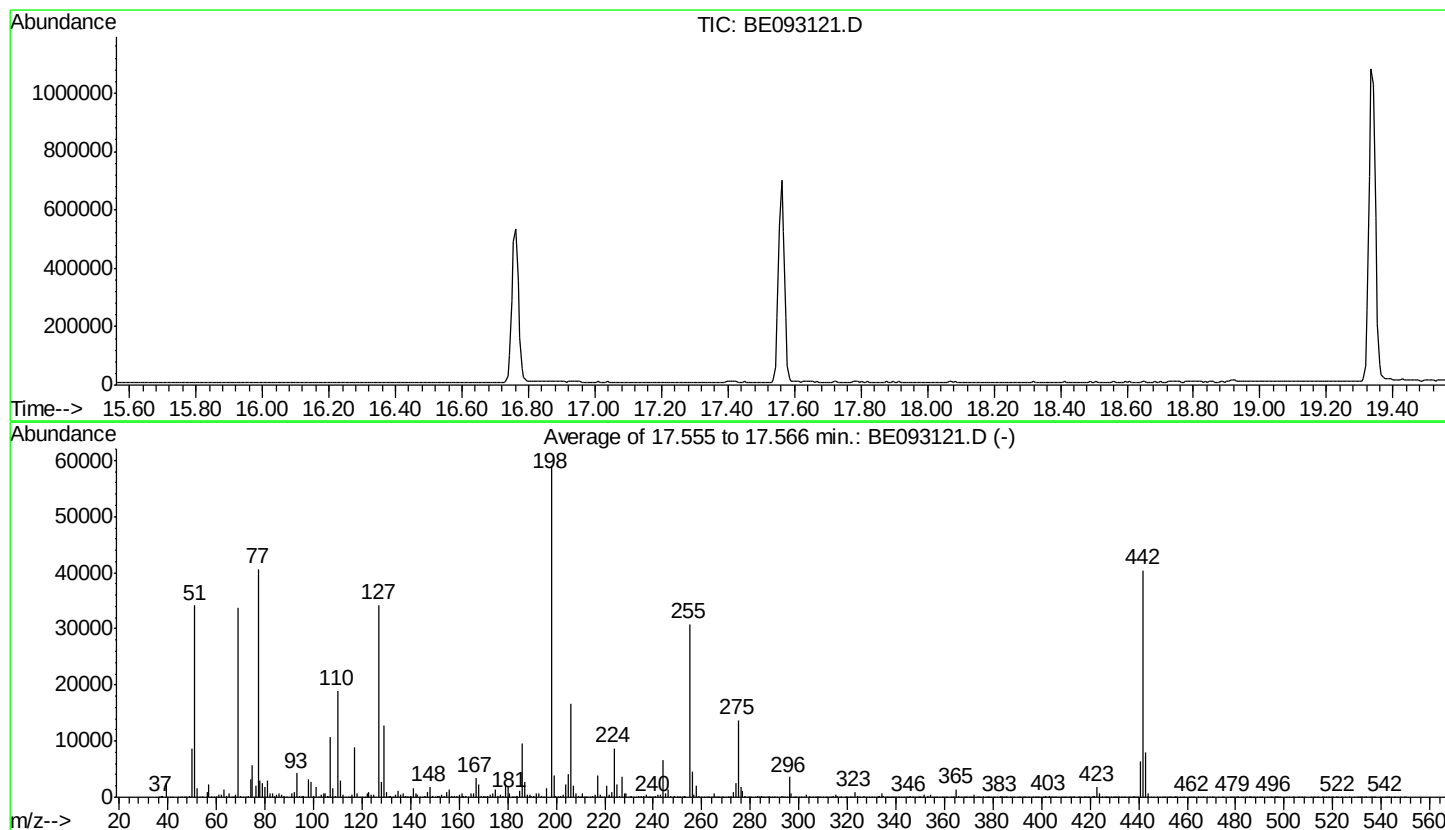

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.8	34136	PASS
68	69	0.00	2	1.3	450	PASS
69	198	0.00	100	57.2	33798	PASS
70	69	0.00	2	0.4	134	PASS
127	198	10	80	58.1	34311	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59071	PASS
199	198	5	9	6.6	3919	PASS
275	198	10	60	23.3	13740	PASS
365	198	1	100	2.4	1434	PASS
441	442	0.01	24	15.7	6355	PASS
442	198	50	100	68.4	40387	PASS
443	442	15	24	20.0	8073	PASS