

Data File : BE093129.D
Acq On : 13 Jun 2017 14:01
Operator : SJ/MA
Sample : PB99574BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK74

Quant Time: Jun 14 01:25:07 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 01:25:15 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4476	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	21891	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	13551	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	34743	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	2330582	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.12	152	9748	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	28921	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	3462	0.06	ng/ul#	21
17) Pyrene	19.49	202	4319	0.04	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093129.D

Acq On : 13 Jun 2017 14:01

Operator : SJ/MA

Sample : PB99574BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK74


Quant Time: Jun 14 01:25:07 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 14 01:25:15 2017

Response via : Initial Calibration

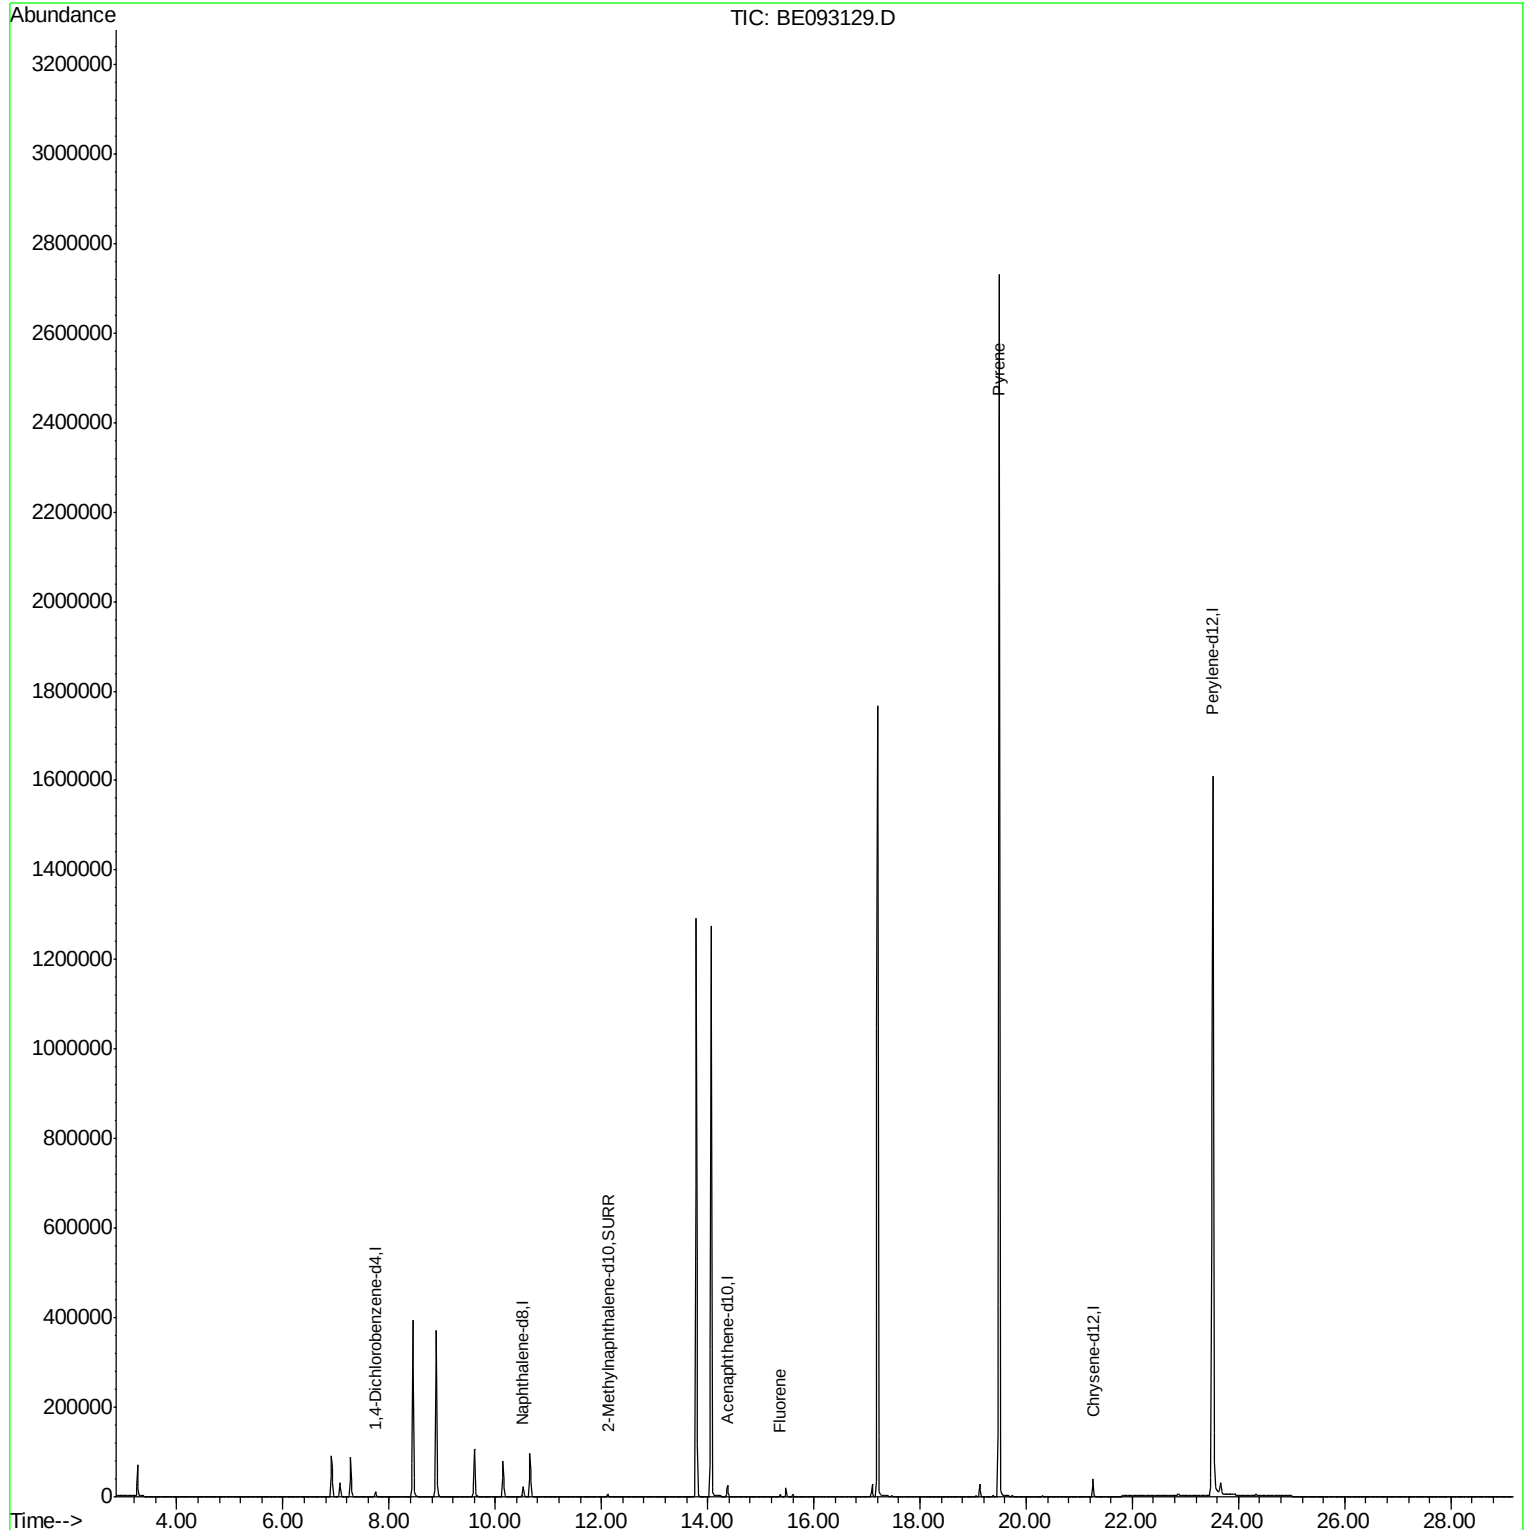

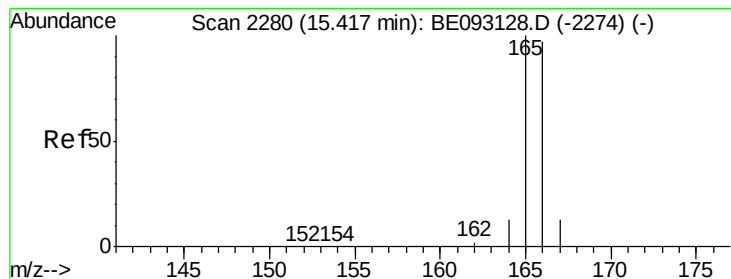

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.36 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BE093129.D

Acq: 13 Jun 2017 14:01

Instrument :

BNA_E

ClientSampleId :

SBLK74


Tgt Ion:166 Resp: 3462

Ion Ratio Lower Upper

166 100

165 7.8 73.4 110.2#




167 33.1 14.6 22.0#

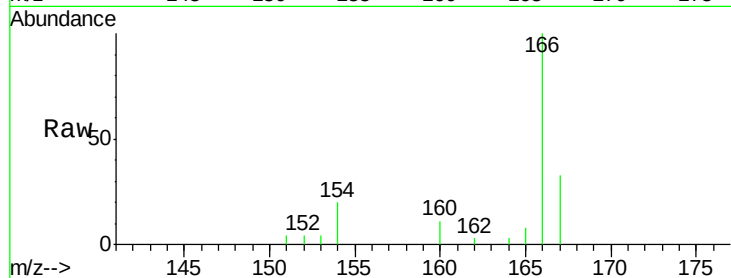

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

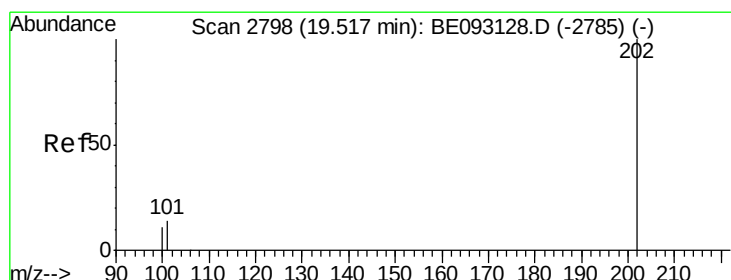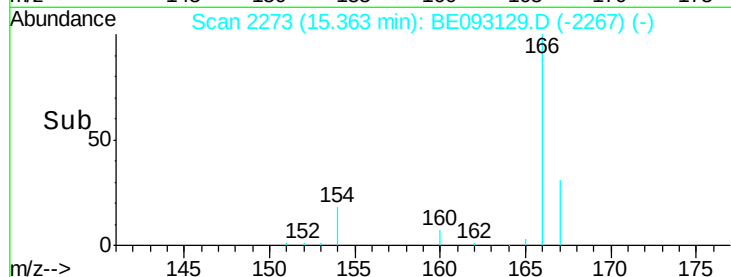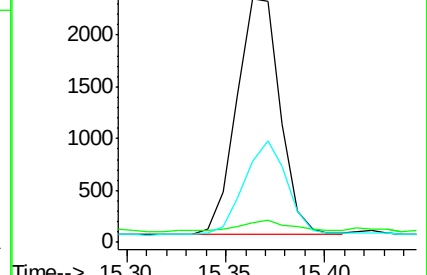

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.03 min

Lab File: BE093129.D

Acq: 13 Jun 2017 14:01


Tgt Ion:202 Resp: 4319

Ion Ratio Lower Upper

202 100

101 200.9 18.2 27.4#

100 1178.0 15.6 23.4#

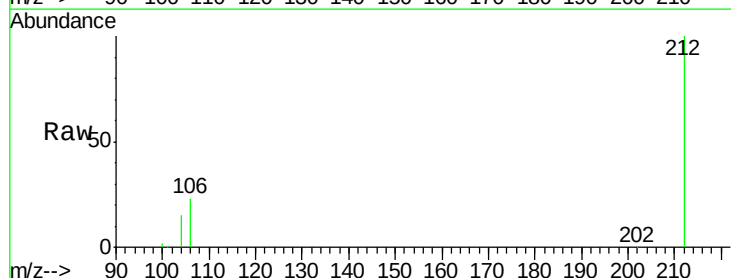

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

