

Data File : BE093130.D
Acq On : 13 Jun 2017 14:40
Operator : SJ/MA
Sample : PB99576BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK76

Quant Time: Jun 14 01:25:12 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 01:25:15 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4509	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	21987	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	13217	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	33724	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	2406277	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	9946	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	28700	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	3369	0.06	ng/ul#	19
17) Pyrene	19.49	202	4311	0.04	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093130.D

Acq On : 13 Jun 2017 14:40

Operator : SJ/MA

Sample : PB99576BL

Misc :

ALS Vial : 4 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK76


Quant Time: Jun 14 01:25:12 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 14 01:25:15 2017

Response via : Initial Calibration

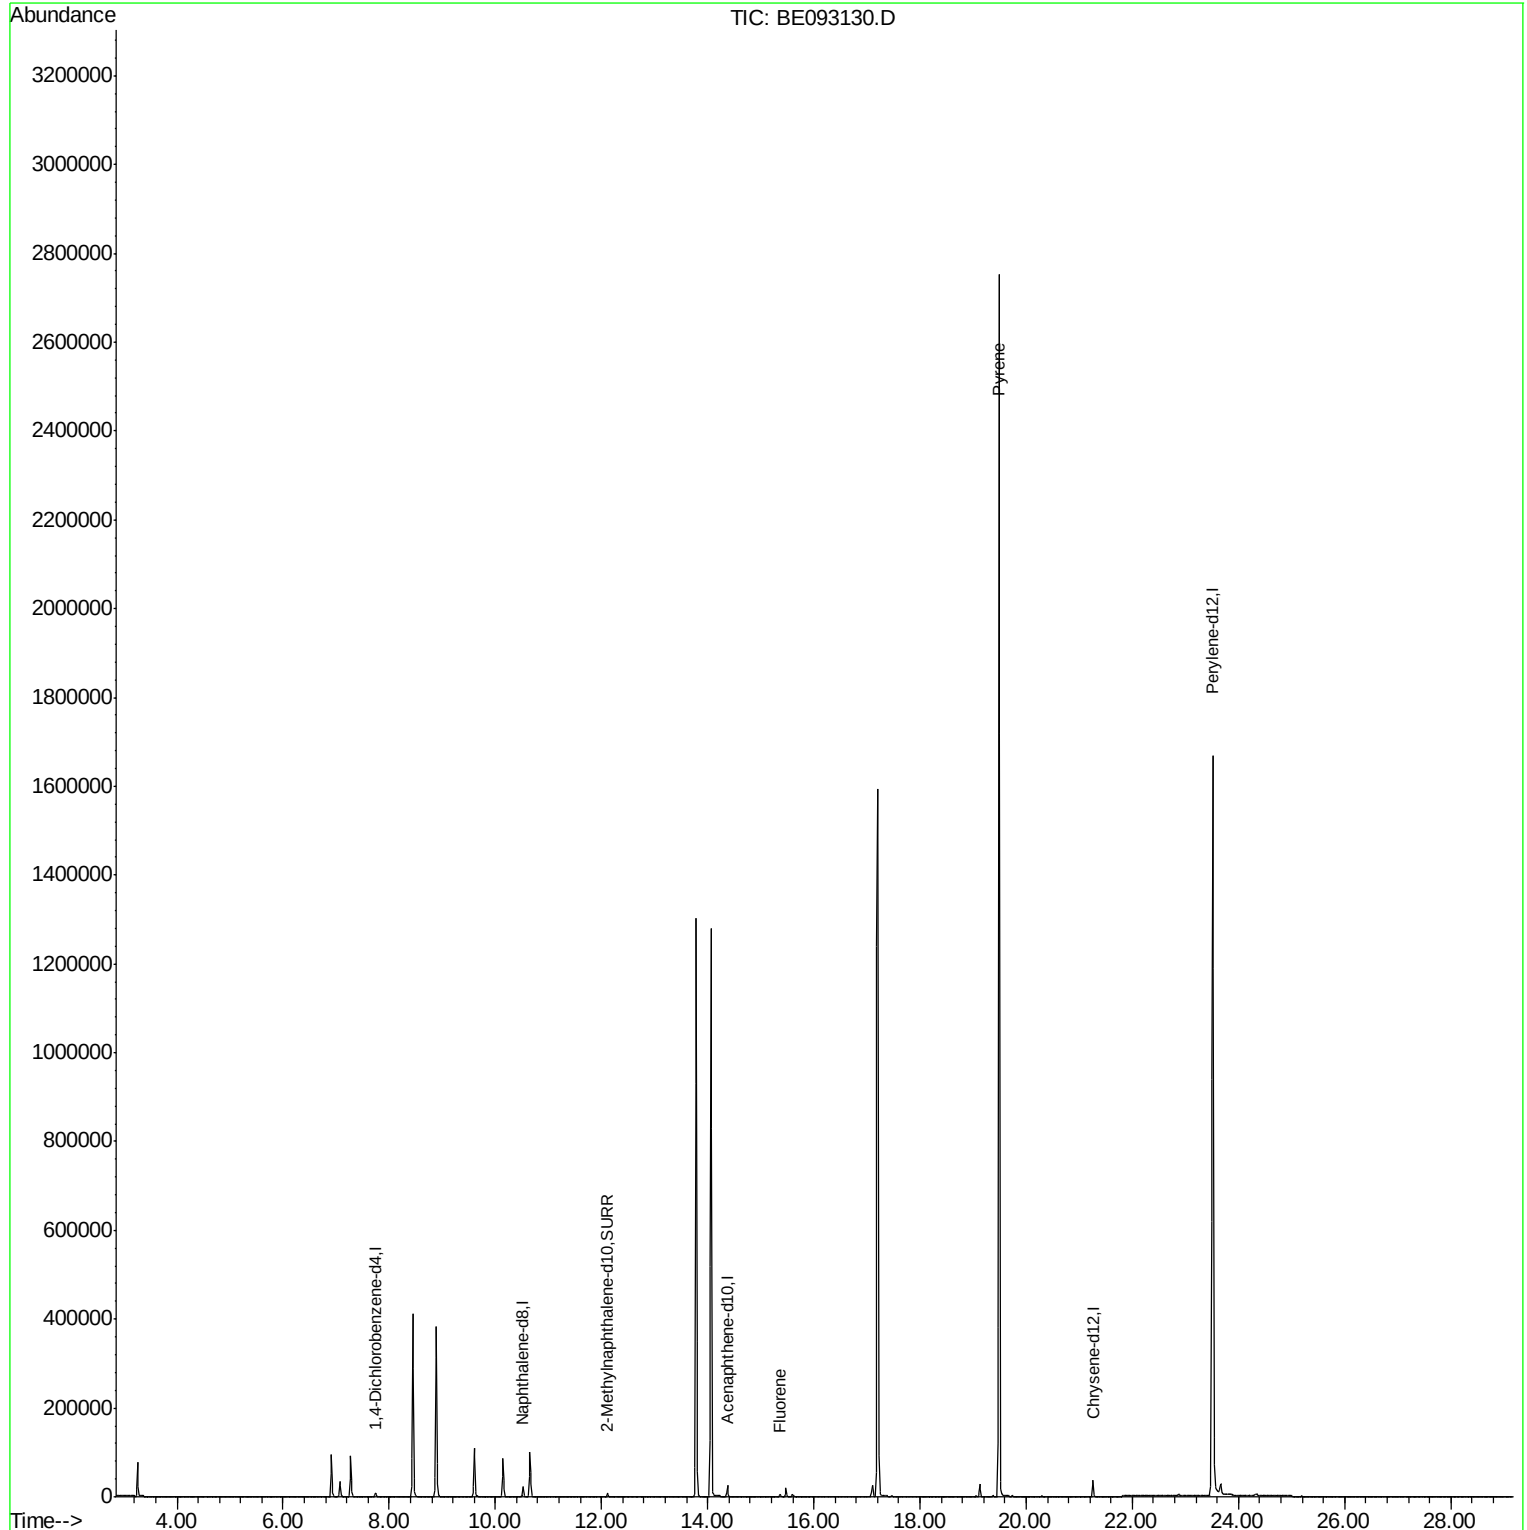

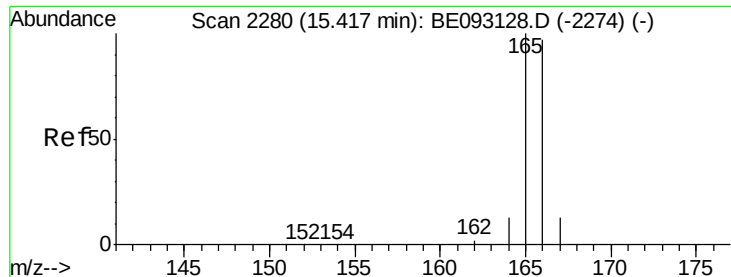

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.36 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BE093130.D

Acq: 13 Jun 2017 14:40

Instrument :

BNA_E

ClientSampleId :

SBLK76





Tgt Ion:166 Resp: 3369

Ion Ratio Lower Upper

166 100

165 7.8 73.4 110.2#

167 37.5 14.6 22.0#

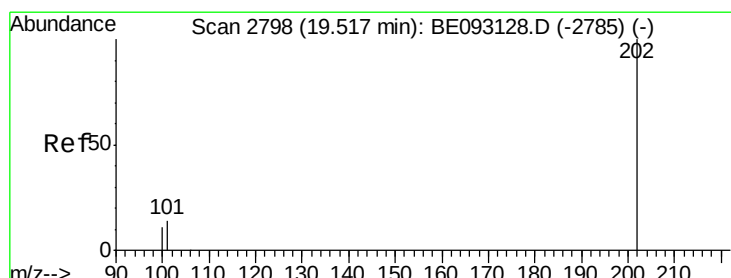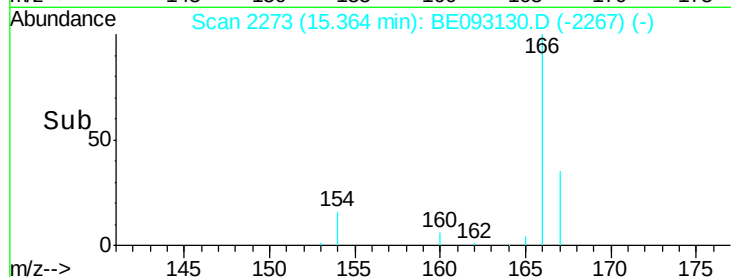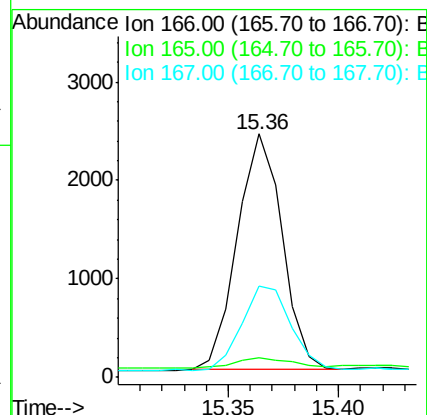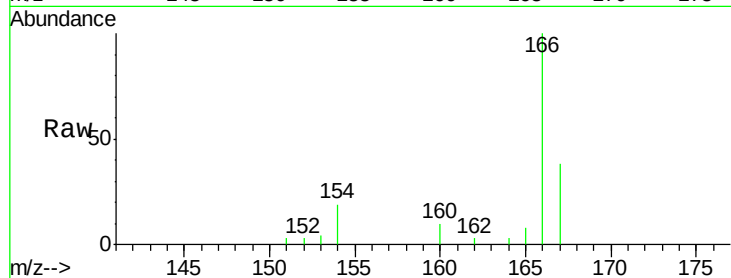

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.49 min Scan# 2792

Delta R.T. -0.03 min

Lab File: BE093130.D

Acq: 13 Jun 2017 14:40

Tgt Ion:202 Resp: 4311

Ion Ratio Lower Upper

202 100

101 200.6 18.2 27.4#

100 1200.6 15.6 23.4#

