

Data File : BE093131.D
Acq On : 13 Jun 2017 15:16
Operator : SJ/MA
Sample : PB99639BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK39

Quant Time: Jun 14 01:25:18 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 01:25:15 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4851	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	23750	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	14623	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	34159	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	2627647	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	12007	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	33705	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	4148	0.07	ng/ul#	19
17) Pyrene	19.49	202	5097	0.05	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093131.D

Acq On : 13 Jun 2017 15:16

Operator : SJ/MA

Sample : PB99639BL

Misc :

ALS Vial : 5 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK39


Quant Time: Jun 14 01:25:18 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 14 01:25:15 2017

Response via : Initial Calibration

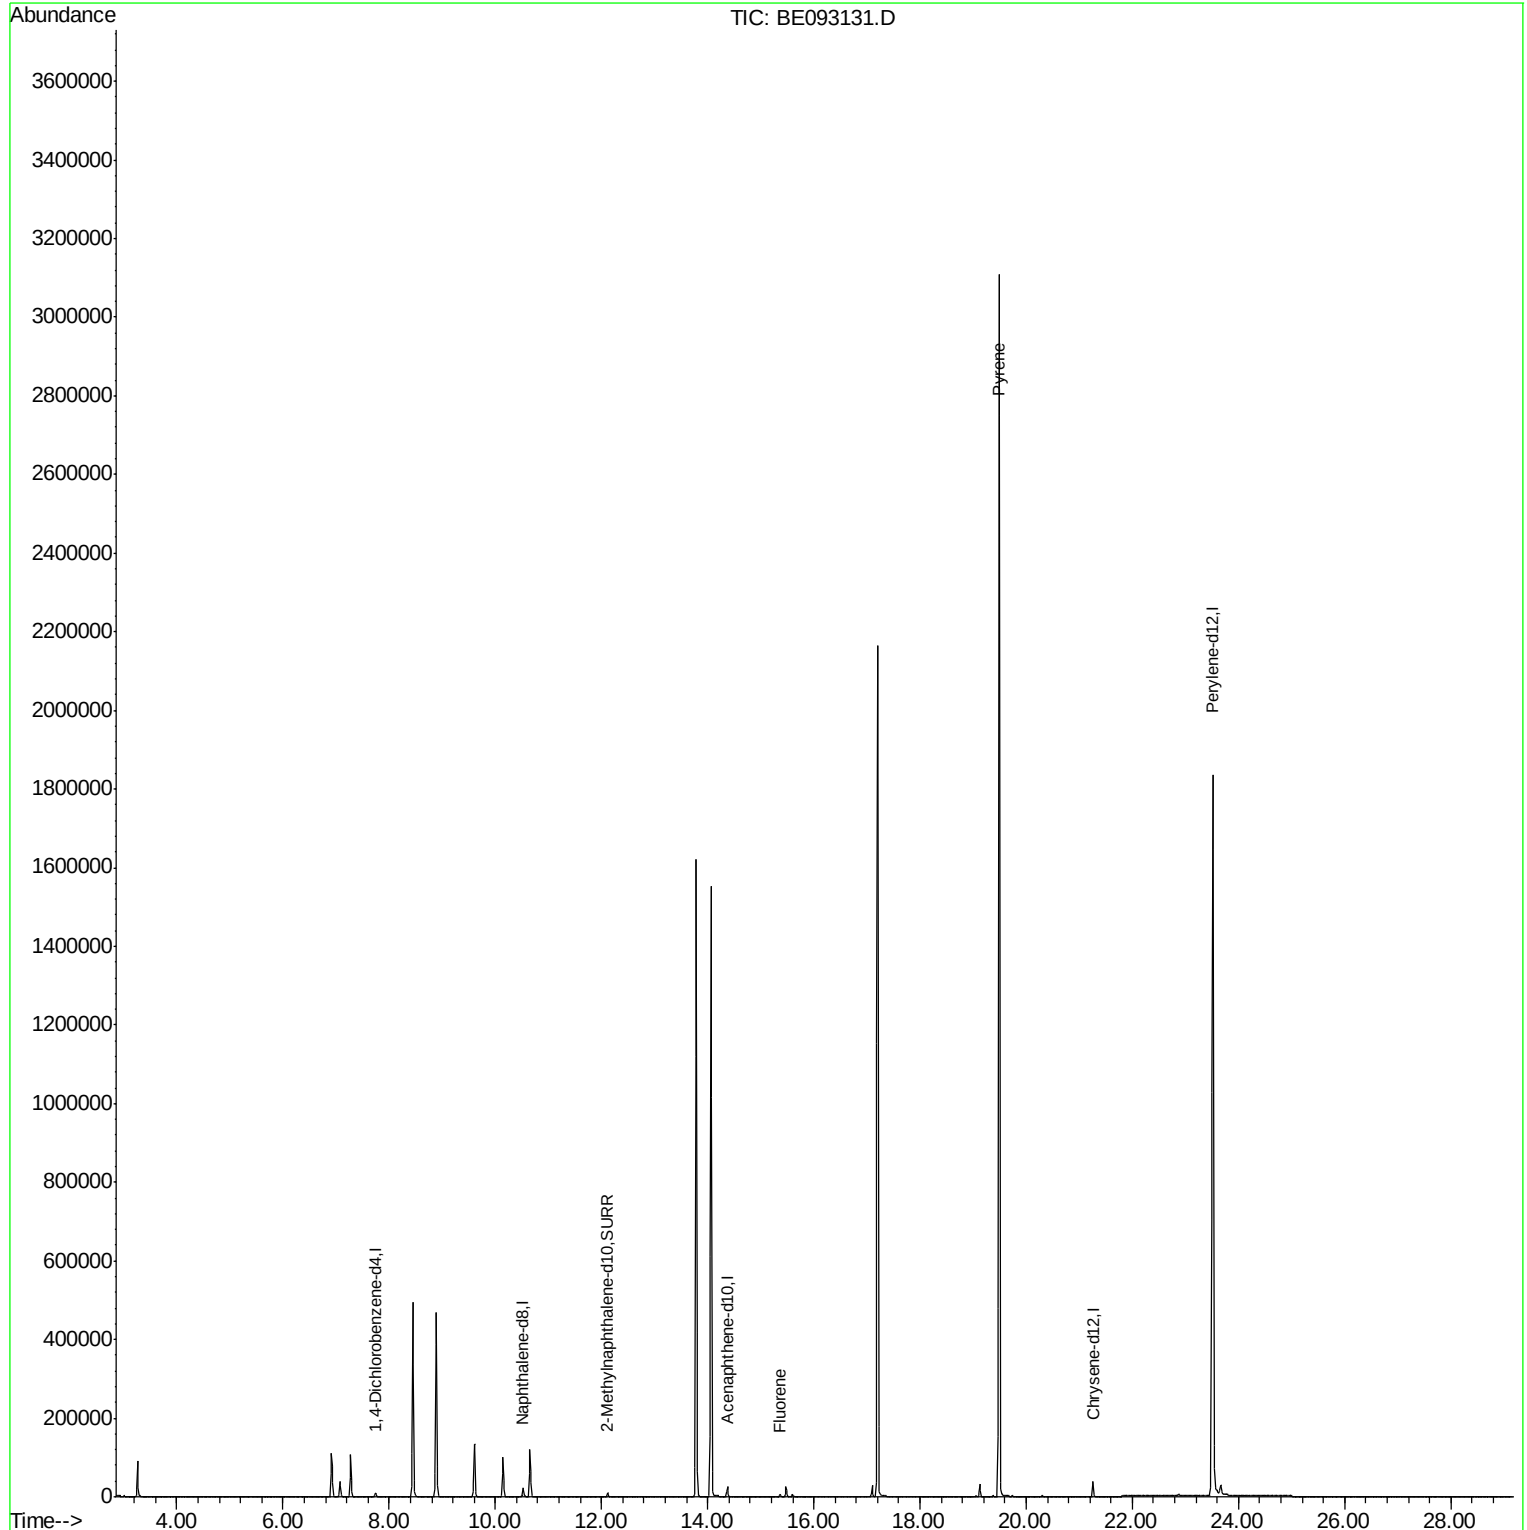

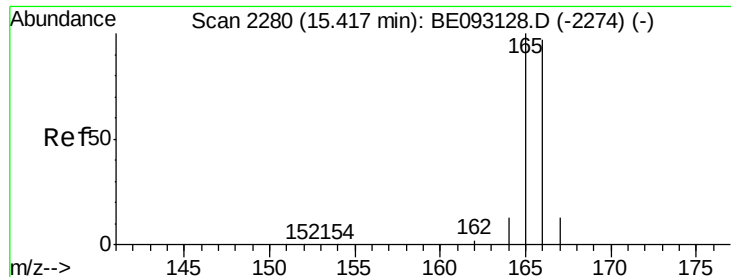

#9

Fluorene

Concen: 0.07 ng/ul

RT: 15.36 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BE093131.D

Acq: 13 Jun 2017 15:16

Instrument :

BNA_E

ClientSampleId :

SBLK39





Tgt Ion:166 Resp: 4148

Ion Ratio Lower Upper

166 100

165 6.6 73.4 110.2#

167 34.7 14.6 22.0#

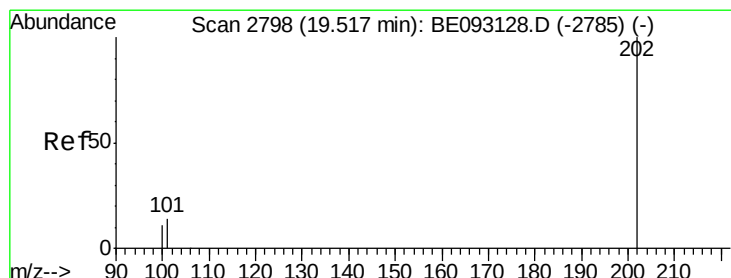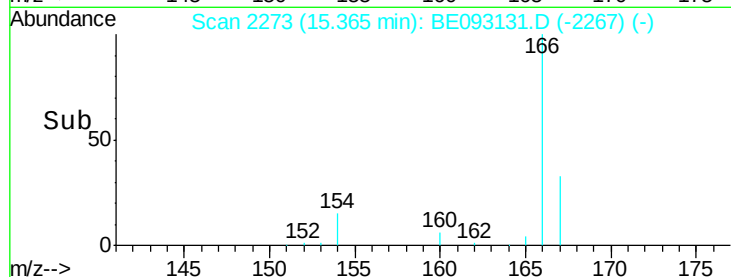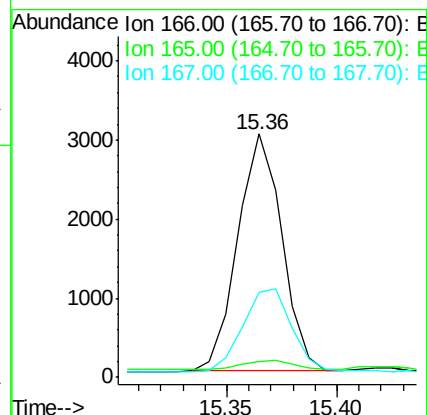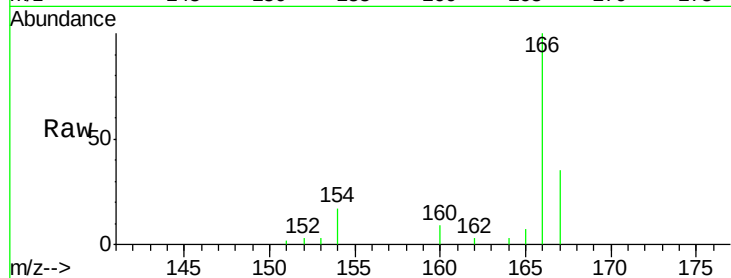

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.03 min

Lab File: BE093131.D

Acq: 13 Jun 2017 15:16

Tgt Ion:202 Resp: 5097

Ion Ratio Lower Upper

202 100

101 204.2 18.2 27.4#

100 1201.7 15.6 23.4#

