

Data File : BE093132.D
Acq On : 13 Jun 2017 15:55
Operator : SJ/MA
Sample : PB99647BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK47

Quant Time: Jun 14 01:25:24 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 01:25:15 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4709	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	22623	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	13692	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	34066	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	2607382	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	11176	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	31638	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	3858	0.07	ng/ul#	20
17) Pyrene	19.49	202	4891	0.05	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093132.D

Acq On : 13 Jun 2017 15:55

Operator : SJ/MA

Sample : PB99647BL

Misc :

ALS Vial : 6 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK47


Quant Time: Jun 14 01:25:24 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 14 01:25:15 2017

Response via : Initial Calibration

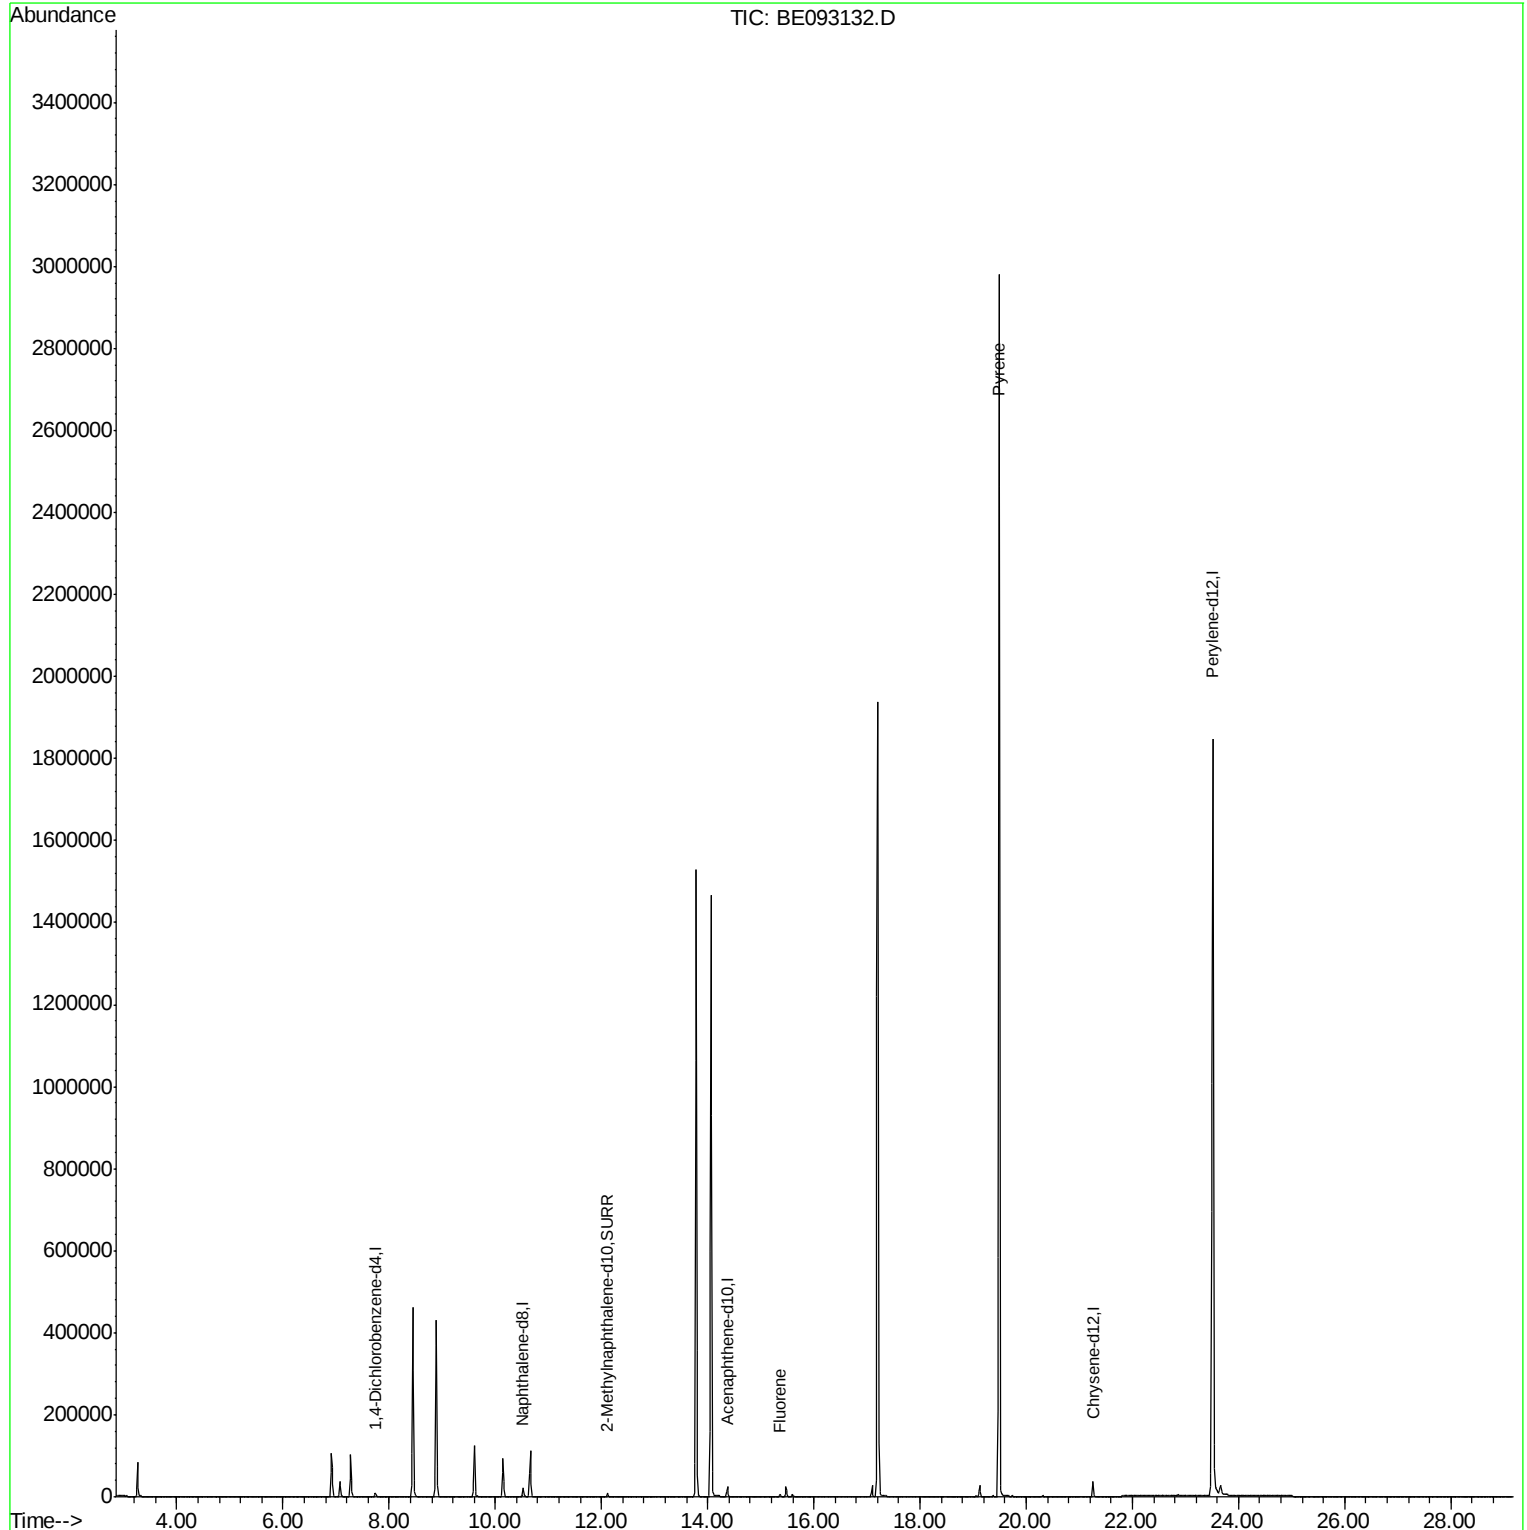

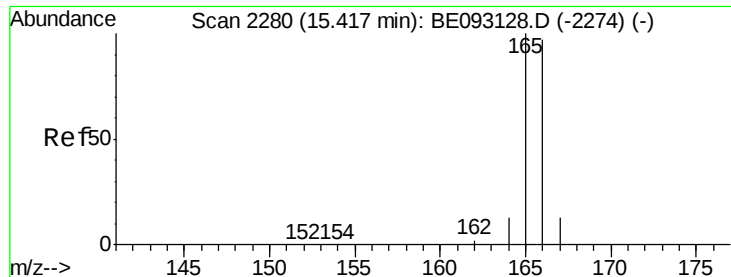

#9

Fluorene

Concen: 0.07 ng/ul

RT: 15.36 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BE093132.D

Acq: 13 Jun 2017 15:55

Instrument :

BNA_E

ClientSampleId :

SBLK47


Tgt Ion:166 Resp: 3858

Ion Ratio Lower Upper




166 100

165 7.4 73.4 110.2#

167 35.9 14.6 22.0#

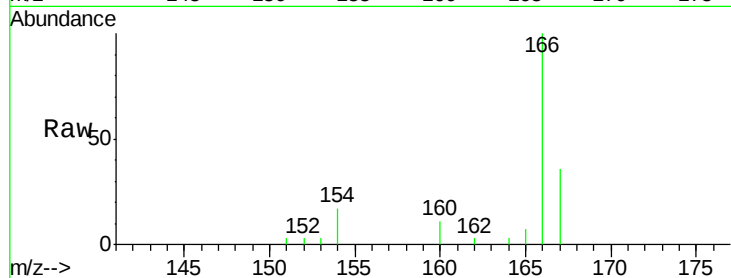

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

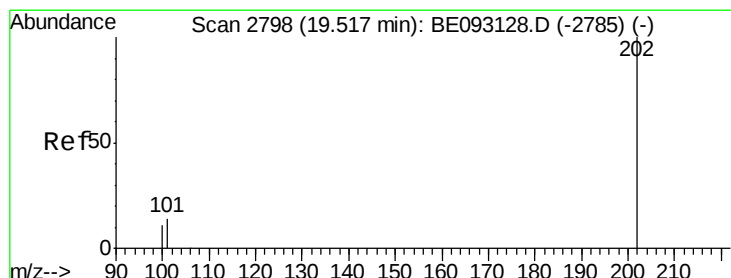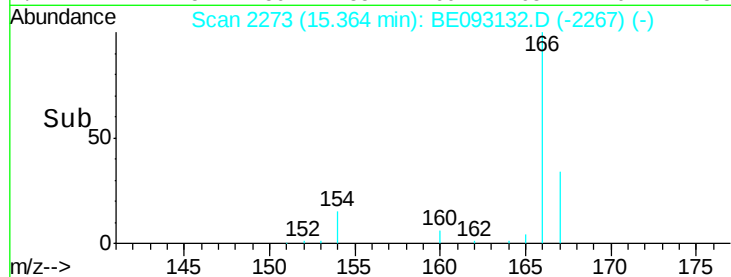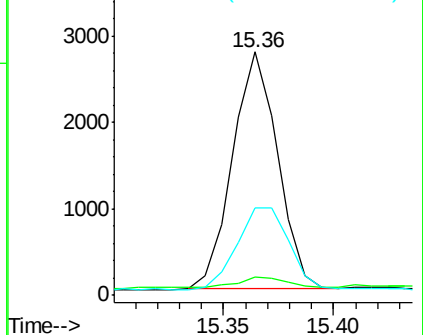

#17

Pyrene

Concen: 0.05 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.03 min

Lab File: BE093132.D

Acq: 13 Jun 2017 15:55


Tgt Ion:202 Resp: 4891

Ion Ratio Lower Upper

202 100

101 194.7 18.2 27.4#

100 1119.8 15.6 23.4#

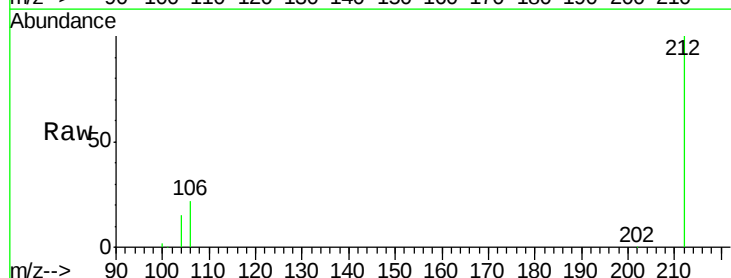

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

