


Data Path : Z:\HPCHEM1\BNA E\DATA\BE061317\
Data File : BE093146.D
Acq On : 14 Jun 2017 00:34
Operator : SJ/MA
Sample : I3558-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A59

Quant Time: Jun 28 19:01:31 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/14/2017 2:59:37 PM

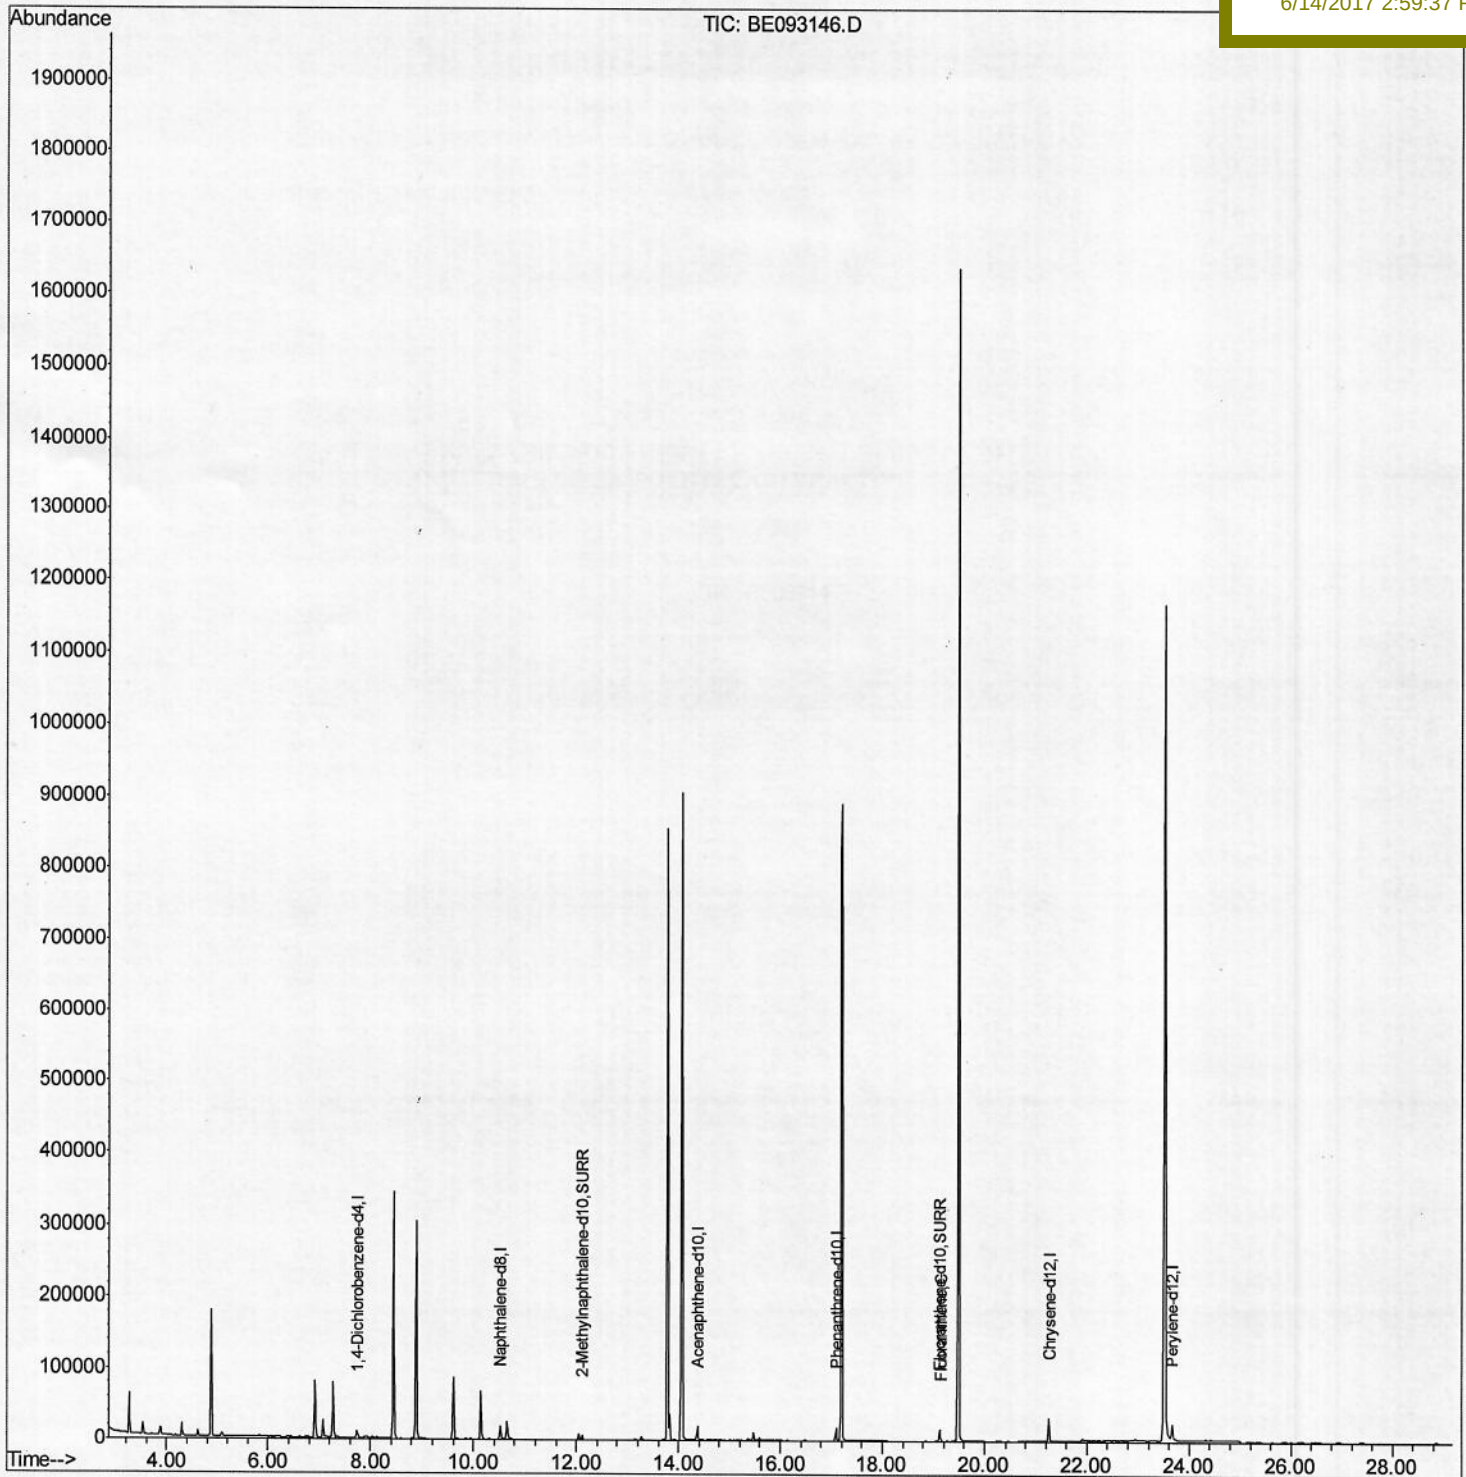

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
 Data File : BE093146.D
 Acq On : 14 Jun 2017 00:34
 Operator : SJ/MA
 Sample : I3558-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 14 11:05:10 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 14 08:39:04 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5A59

Manual Integrations
 APPROVED

mohammad
 6/14/2017 2:59:37 PM

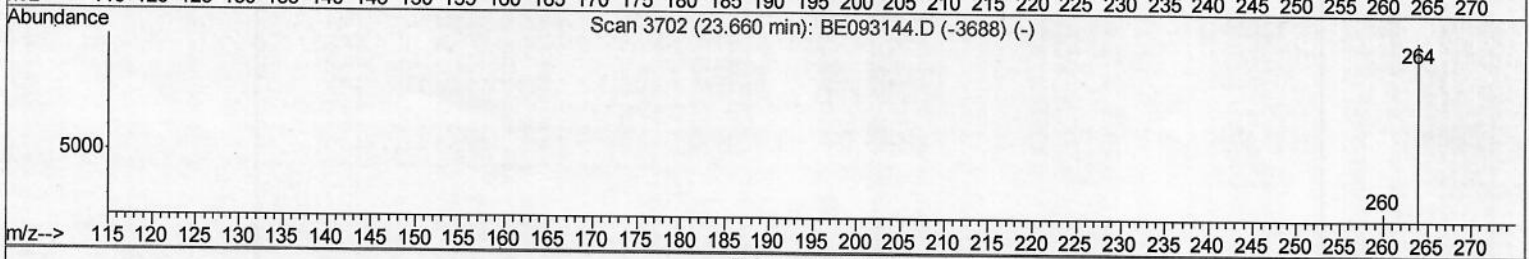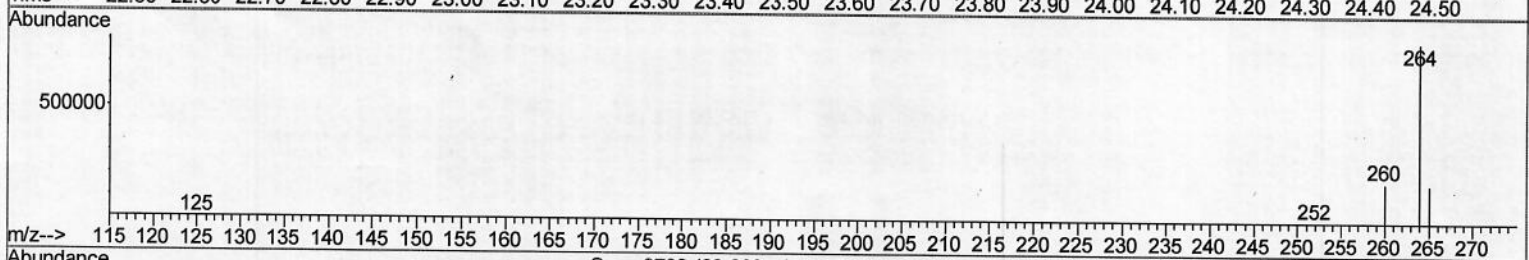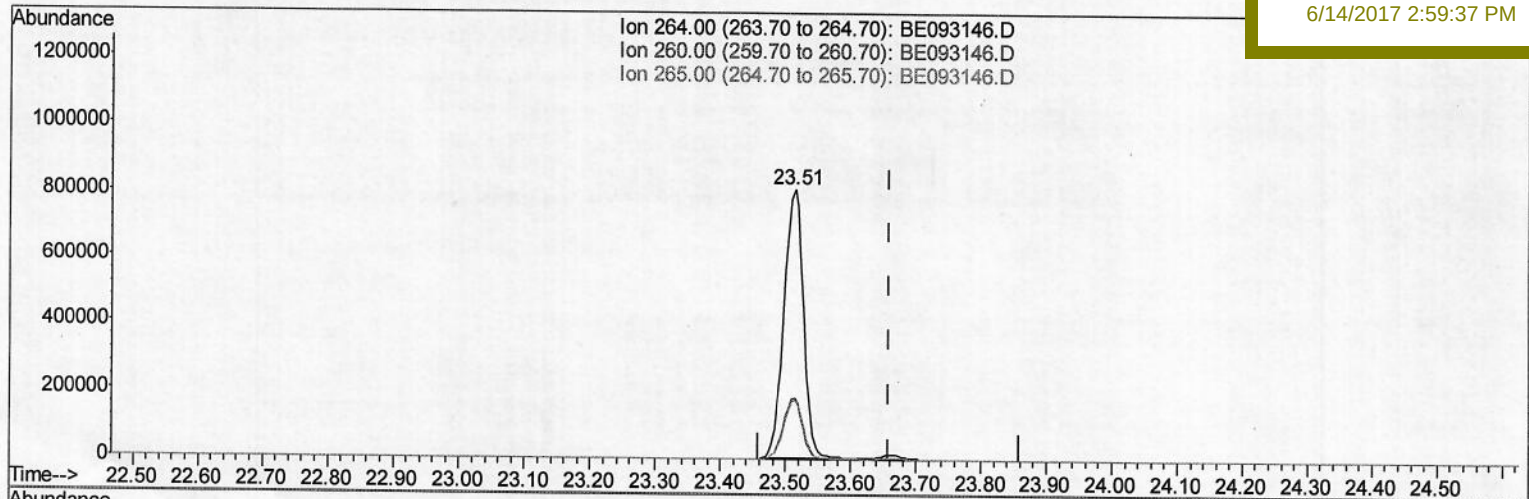

TIC: BE093146.D

(20) Perylene-d12 (I)

23.514min (-0.146) 0.40ng/ul

response 1671243

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.23#
265.00	103.50	21.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
 Data File : BE093146.D
 Acq On : 14 Jun 2017 00:34
 Operator : SJ/MA
 Sample : I3558-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Quant Time: Jun 14 11:05:10 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 14 08:39:04 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5A59

Manual Integrations
 APPROVED

mohammad
 6/14/2017 2:59:37 PM

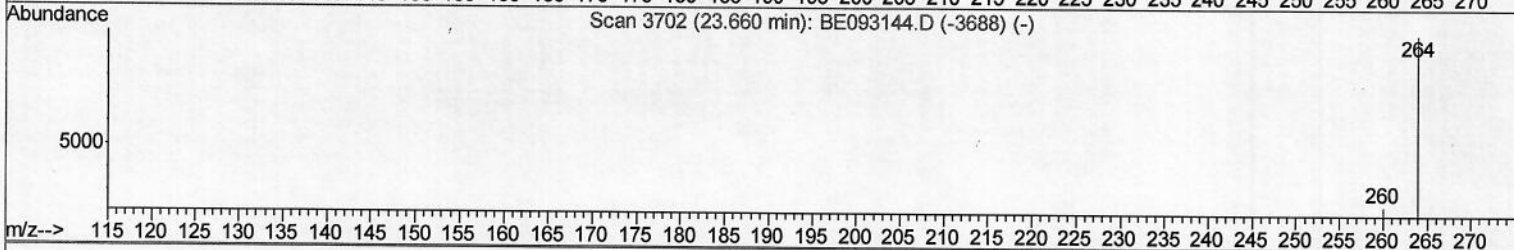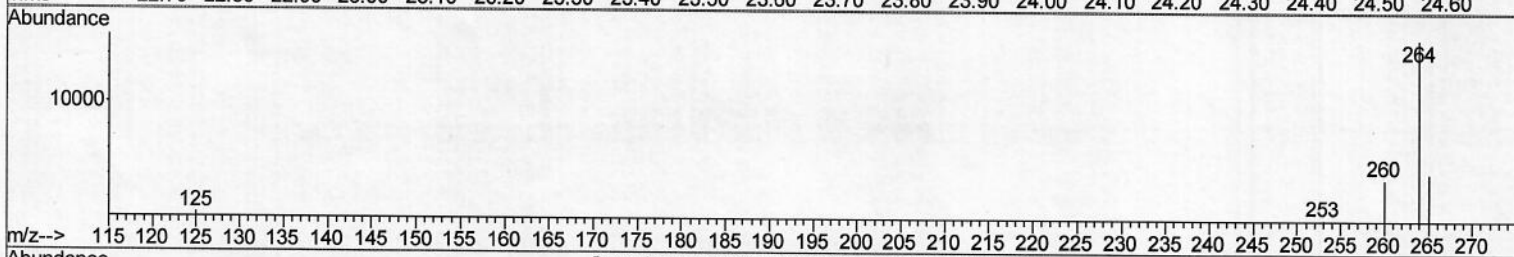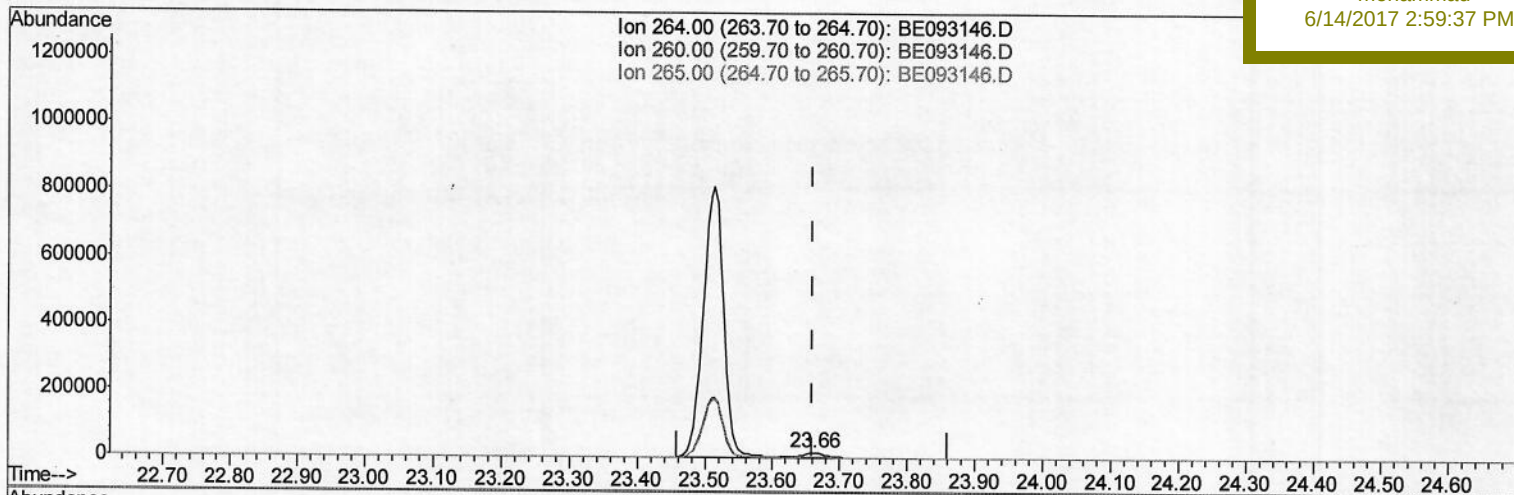

TIC: BE093146.D

(20) Perylene-d12 (I)

23.660min (+0.000) 0.40ng/ul m

response 26267

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.98
265.00	103.50	28.60#
0.00	0.00	0.00

SJ
06/21/17

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061317\
 Data File : BE093146.D
 Acq On : 14 Jun 2017 00:34
 Operator : SJ/MA
 Sample : I3558-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5A59

Quant Time: Jun 28 19:01:31 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 14 08:39:04 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/14/2017 2:59:37 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4416	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	19419	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	10552	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	23051	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	29040	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	26267m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	7750	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	17519	0.28	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.15	202	2084	0.03	ng/ul	Ovalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
 06/21/17