

Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Quantitation Report (QT Reviewed)


Data File : BE093158.D
Acq On : 14 Jun 2017 7:58
Operator : SJ/MA
Sample : I3520-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5A35

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:16 PM

Quant Time: Jun 14 11:53:27 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

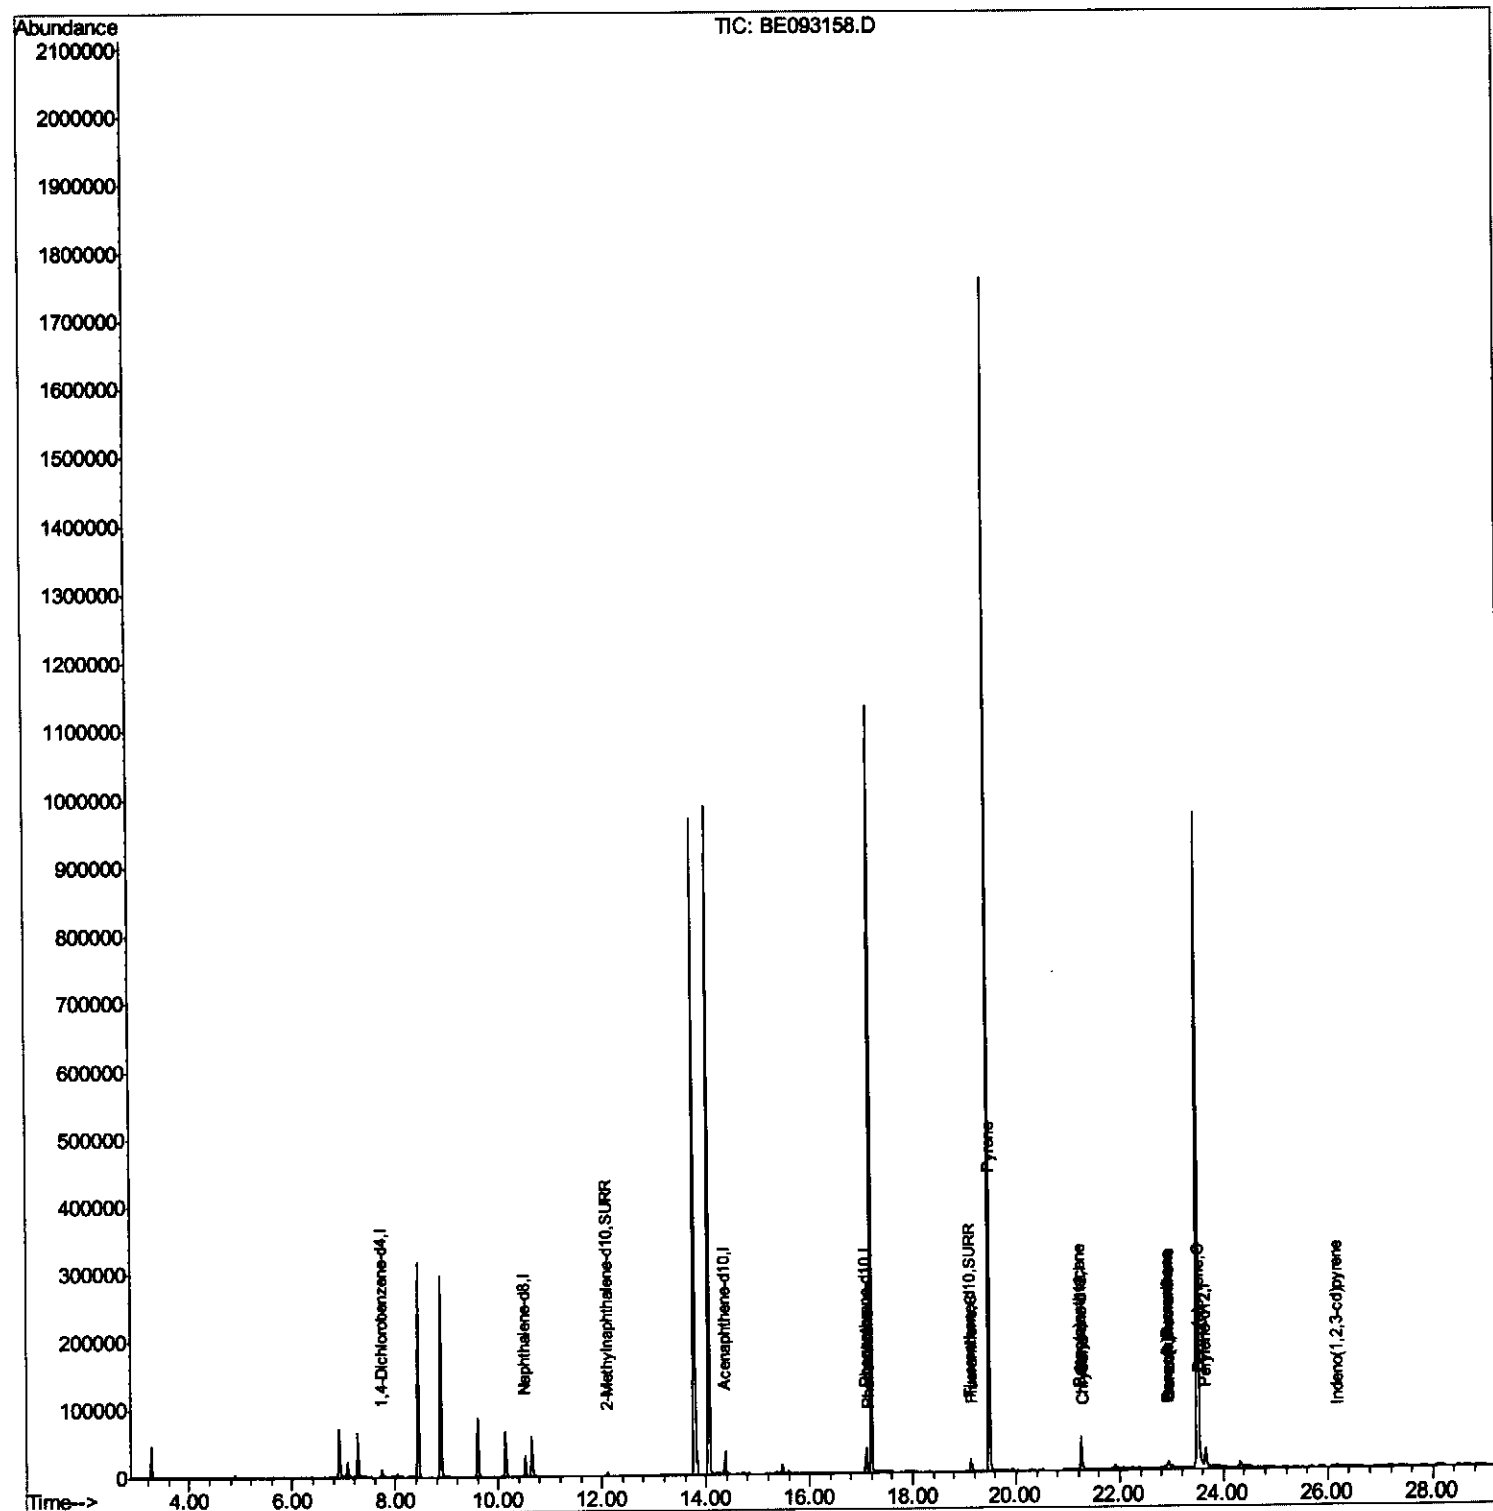


Data File : BE093158.D
Acq On : 14 Jun 2017 7:58
Operator : SJ/MA
Sample : I3520-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A35

Manual Integrations
APPROVED
mohammad
6/14/2017 3:00:16 PM

Quant Time: Jun 14 11:53:27 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

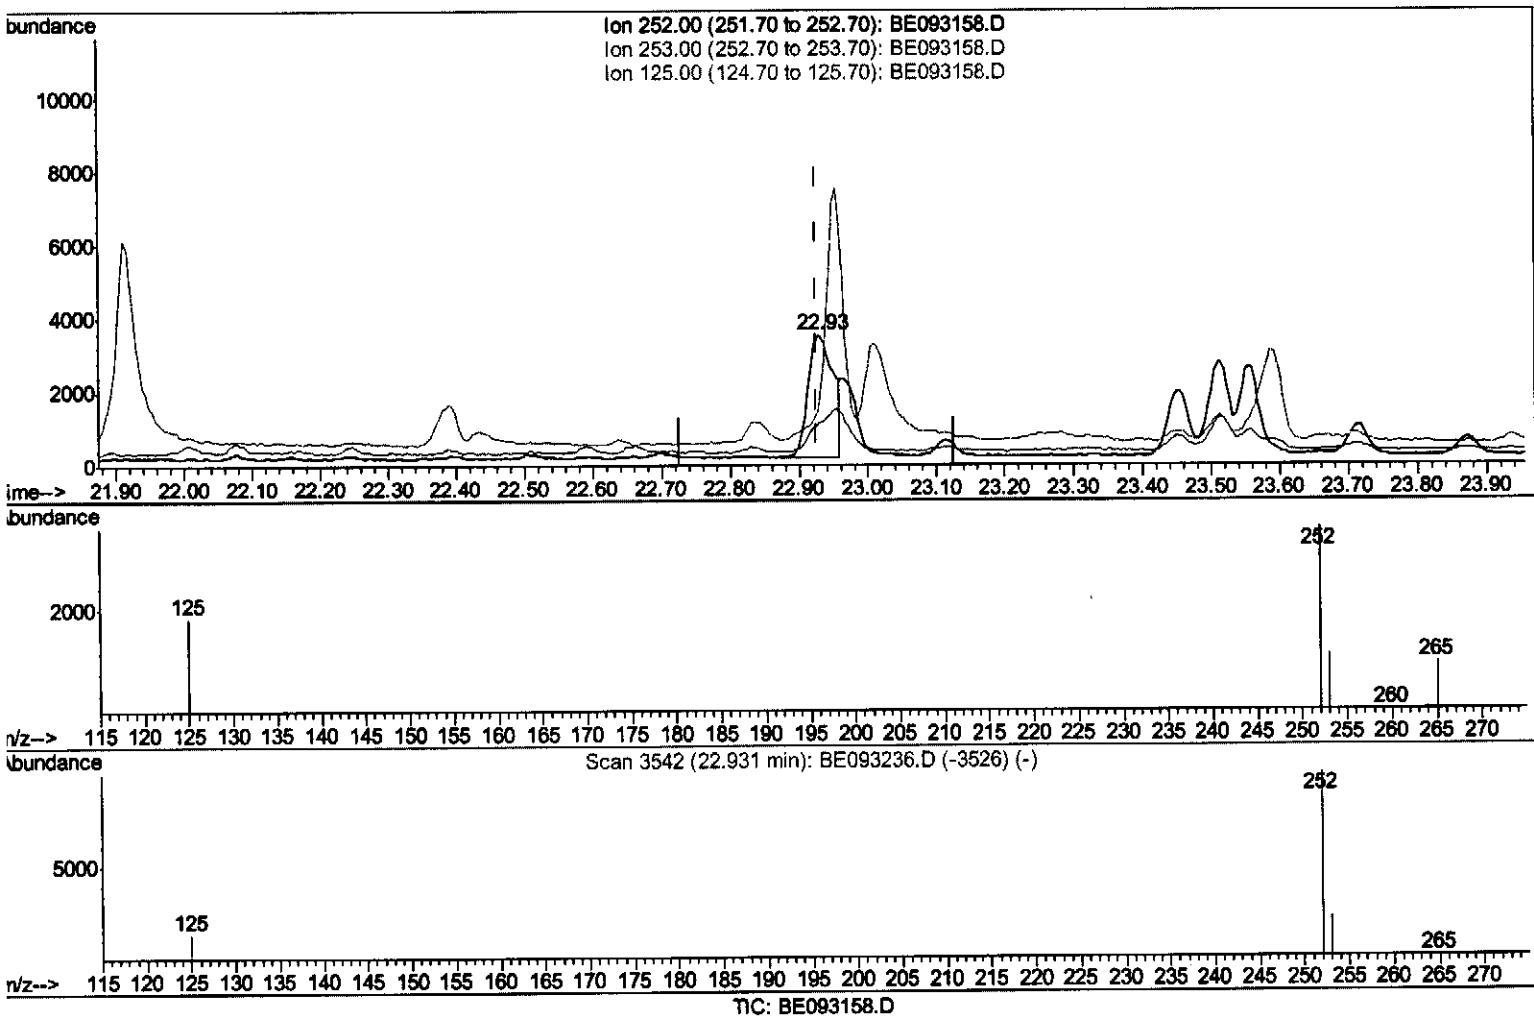

(21) Benzo(b)fluoranthene

22.930min (+0.004) 0.06ng/ul m

response 8467

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	32.99
125.00	17.50	52.12#
0.00	0.00	0.00

SJ
06/21/17


Data File : BE093158.D
Acq On : 14 Jun 2017 7:58
Operator : SJ/MA
Sample : I3520-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A35

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:16 PM

Quant Time: Jun 14 11:53:27 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

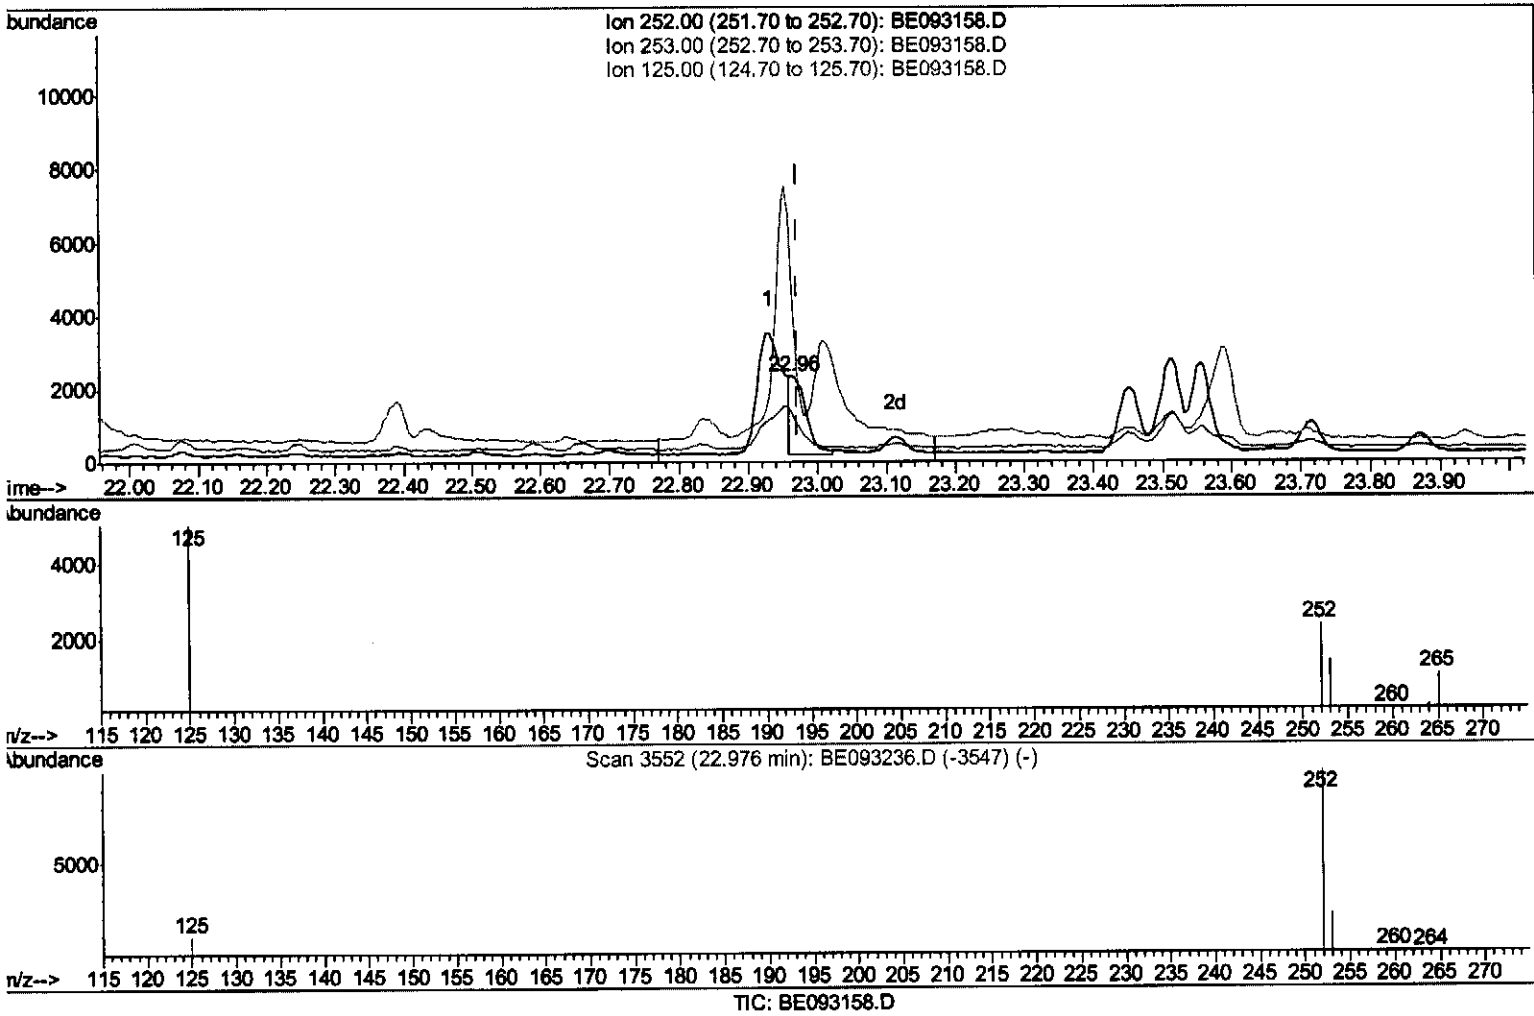

(22) Benzo(k)fluoranthene

22.962min (-0.010) 0.02ng/ul m

response 3393

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	59.03#
125.00	17.10	215.89#
0.00	0.00	0.00

SJ
06/21/17

Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Quantitation Report (QT Reviewed)

Data File : BE093158.D
Acq On : 14 Jun 2017 7:58
Operator : SJ/MA
Sample : I3520-03
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A35

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:16 PM

Quant Time: Jun 14 11:53:27 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	6094	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	30974	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	18319	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	43033	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	43533	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	45136	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	7886	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	19486	0.17	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
12) Phenanthrene	17.13	178	4698	0.04	ng/ul#	89
15) Fluoranthene	19.15	202	11131	0.08	ng/ul	83
17) Pyrene	19.51	202	13473	0.10	ng/ul#	92
18) Benzo(a)anthracene	21.24	228	4744	0.04	ng/ul#	86
19) Chrysene	21.29	228	5849	0.05	ng/ul	94
21) Benzo(b)fluoranthene	22.93	252	8467m	0.06	ng/ul	} JJ 06/21/17
22) Benzo(k)fluoranthene	22.96	252	3393m	0.02	ng/ul	
23) Benzo(a)pyrene	23.55	252	4631	0.04	ng/ul#	
24) Indeno(1,2,3-cd)pyrene	26.18	276	3467	0.02	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed