


Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Data File : BE093160.D
Acq On : 14 Jun 2017 9:13
Operator : SJ/MA
Sample : I3520-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5A40

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:22 PM

Quant Time: Jun 14 12:01:59 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

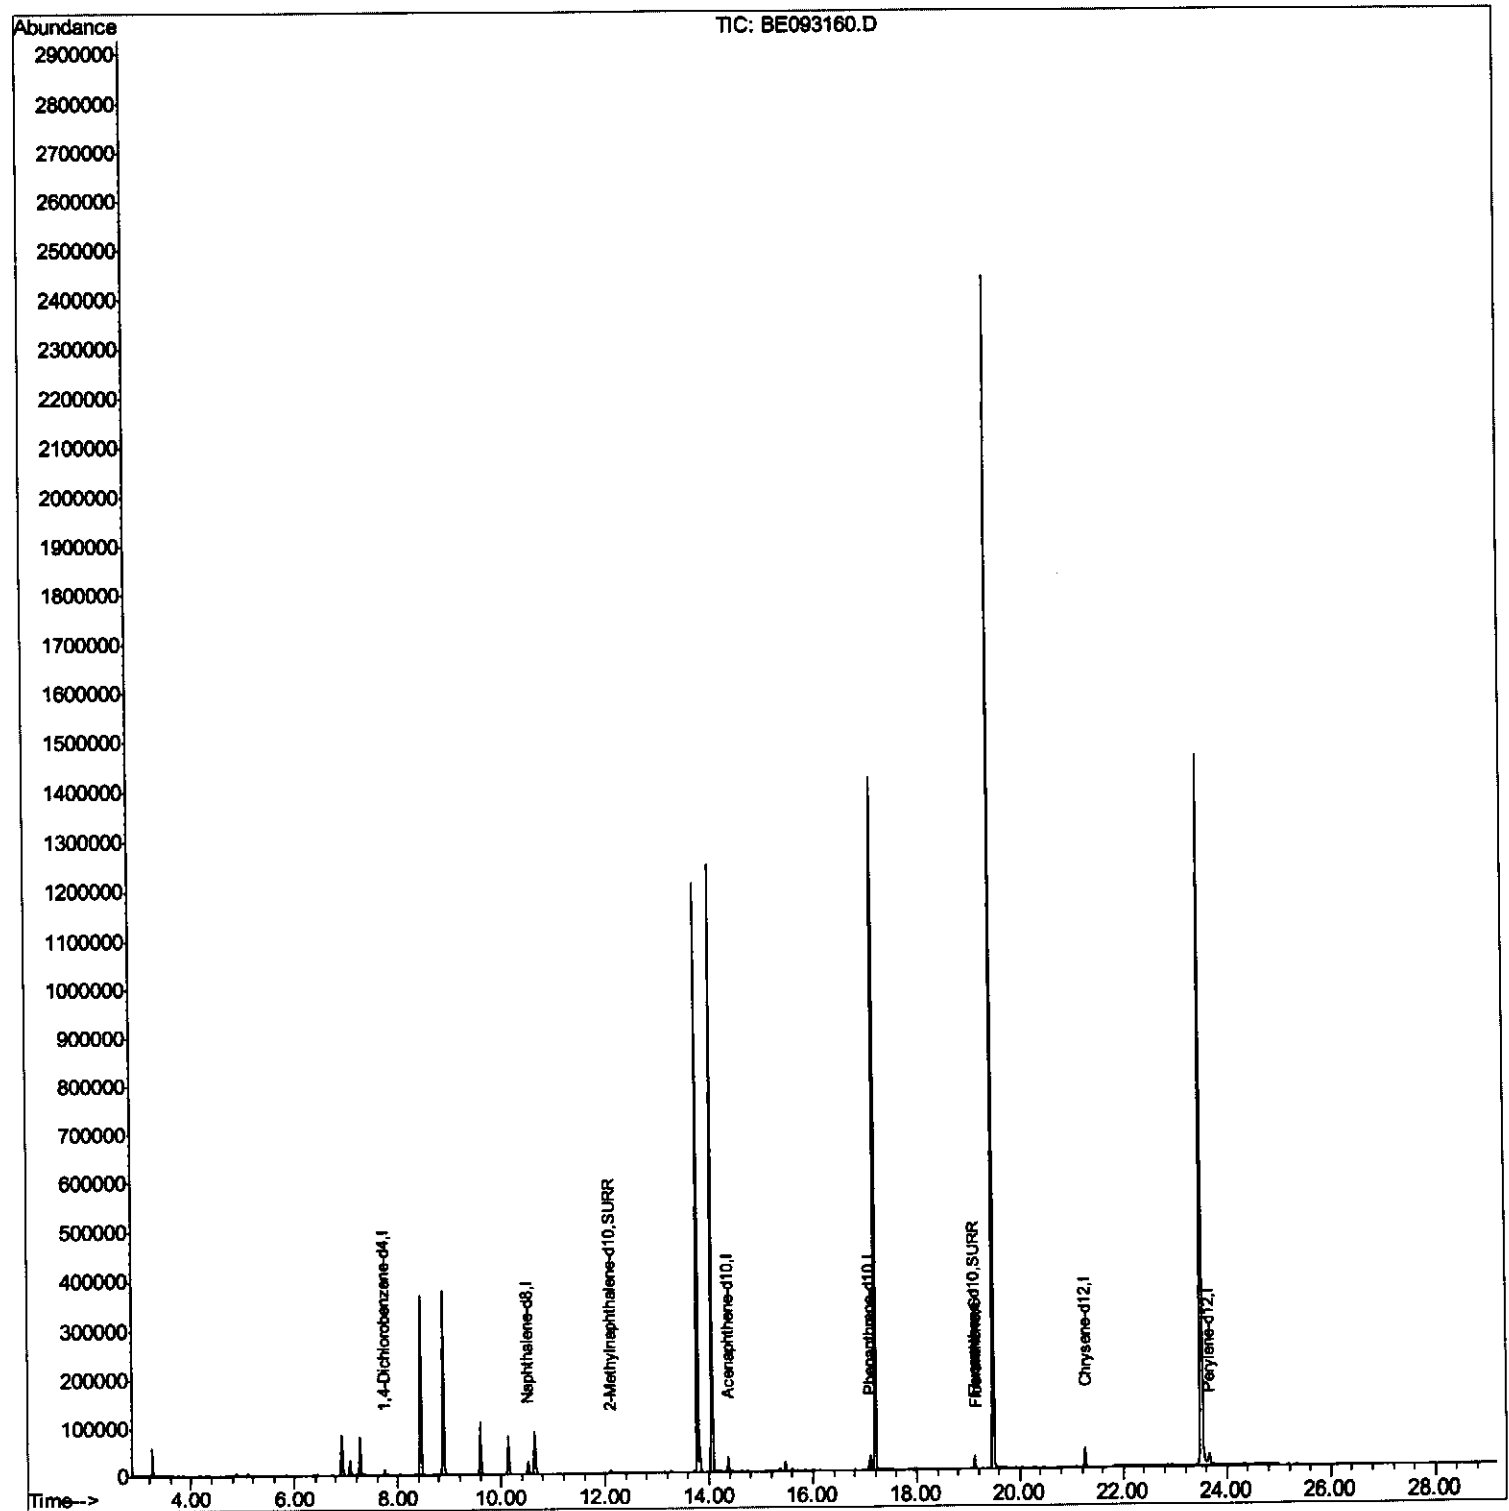


Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Data File : BE093160.D
Acq On : 14 Jun 2017 9:13
Operator : SJ/MA
Sample : I3520-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5A40

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:22 PM

Quant Time: Jun 14 11:58:51 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

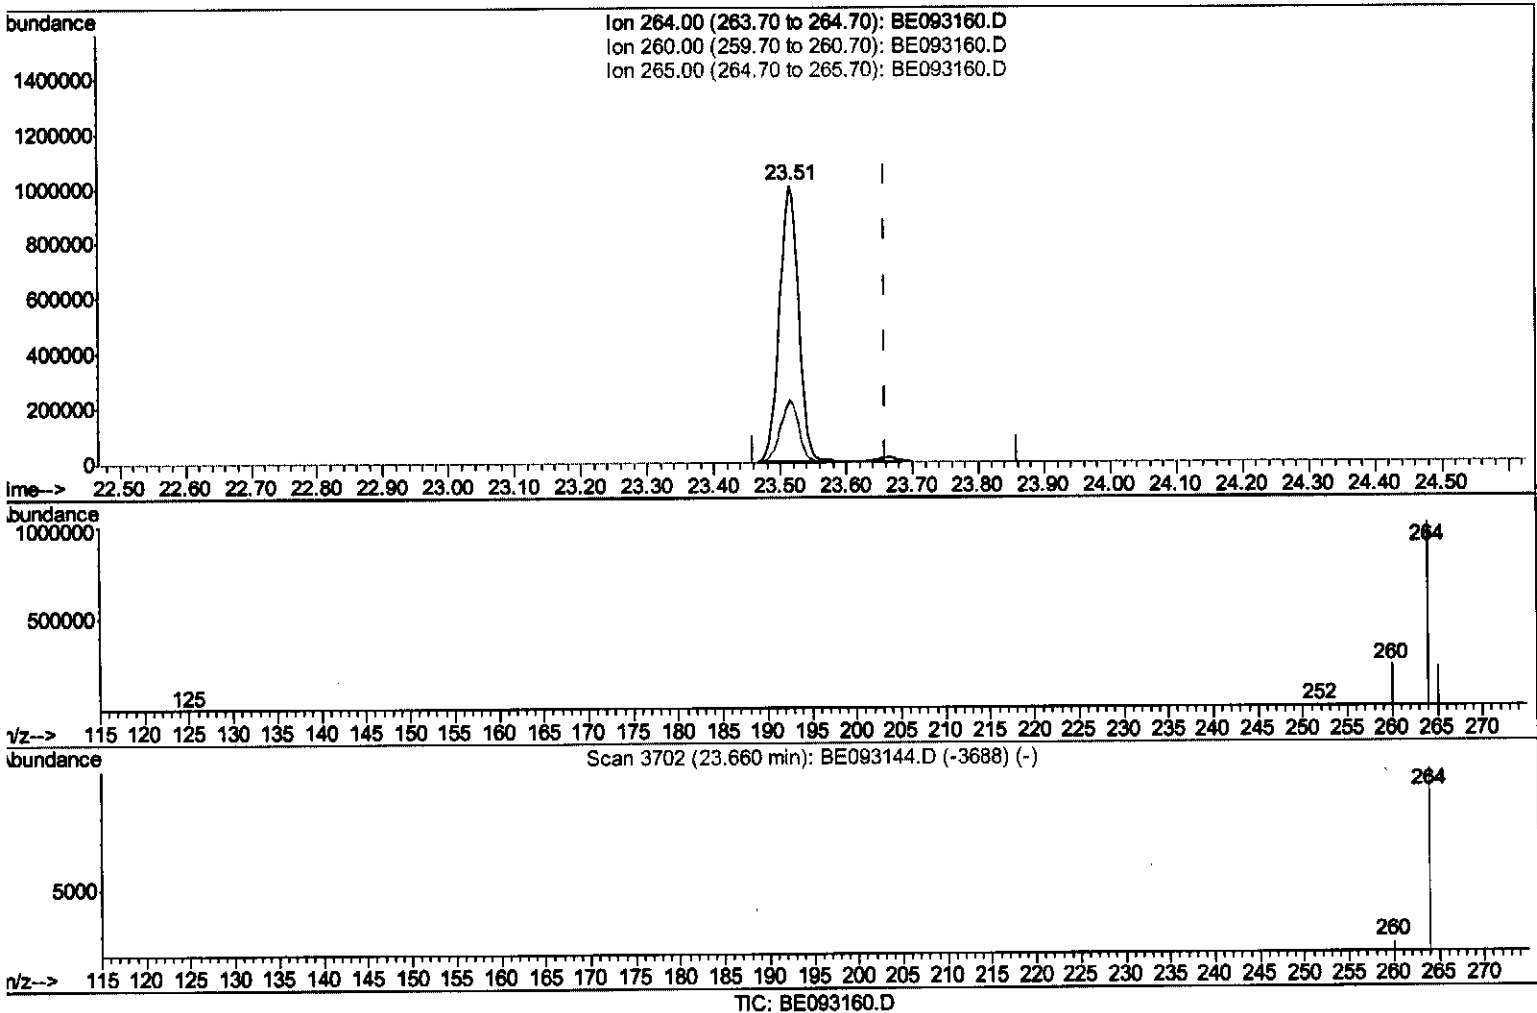

(20) Perylene-d12 (I)

23.514min (-0.145) 0.40ng/ul

response 2005509

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.71#
265.00	103.50	21.77#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Data File : BE093160.D
Acq On : 14 Jun 2017 9:13
Operator : SJ/MA
Sample : I3520-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5A40

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:22 PM

Quant Time: Jun 14 11:58:51 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

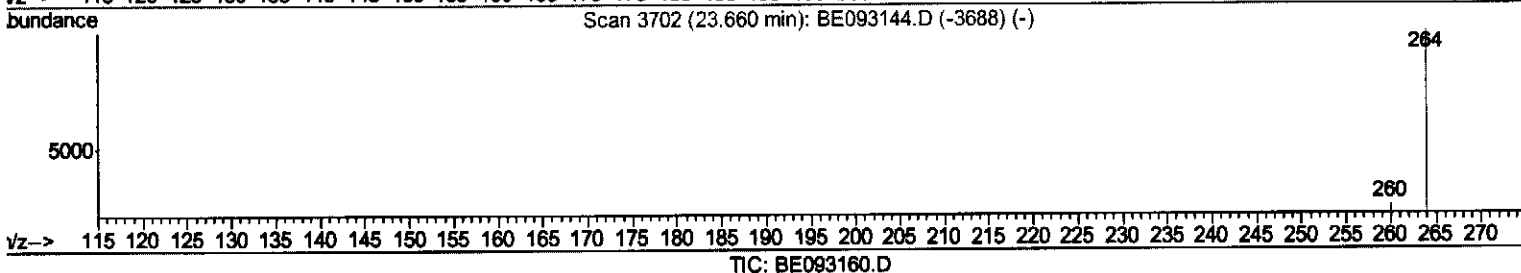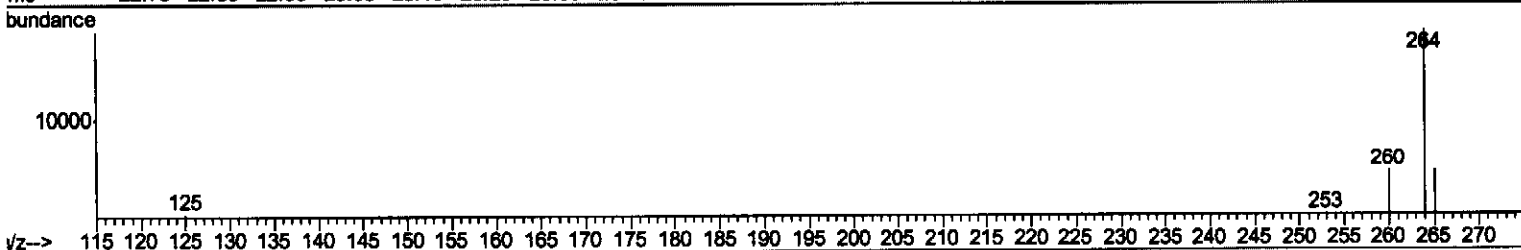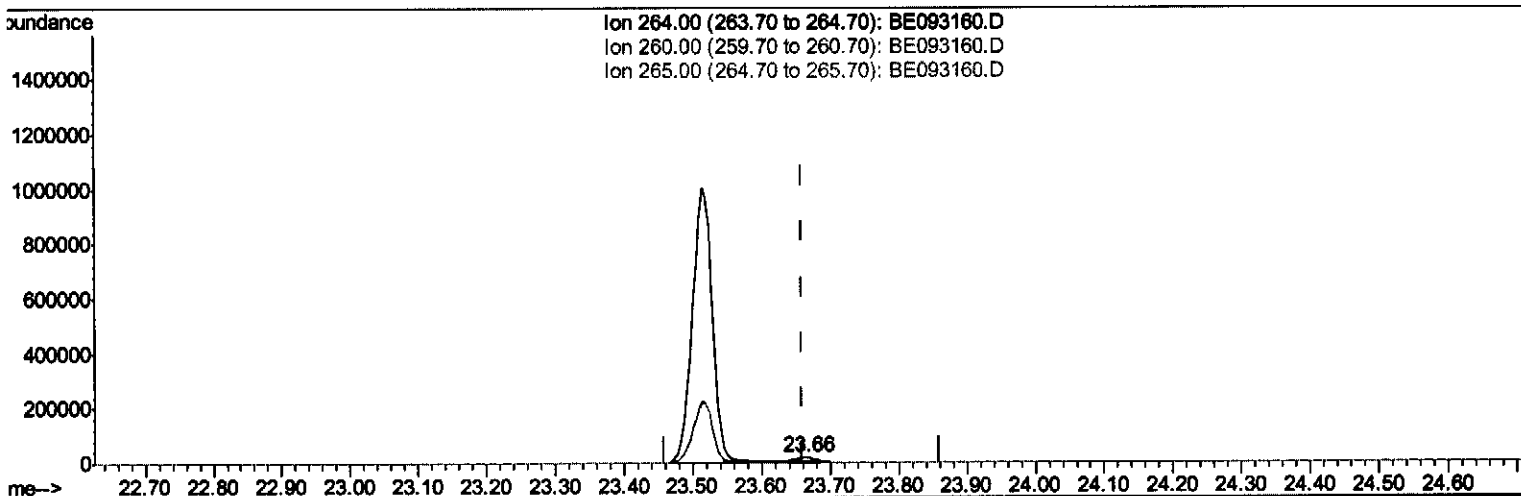

(20) Perylene-d12 (I)

23.664min (+0.005) 0.40ng/ul m

response 30771

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.95
265.00	103.50	25.50#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE061317\
Data File : BE093160.D
Acq On : 14 Jun 2017 9:13
Operator : SJ/MA
Sample : I3520-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5A40

Manual Integrations
APPROVED

mohammad
6/14/2017 3:00:22 PM

Quant Time: Jun 14 12:01:59 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 14 08:39:04 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	5201	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	25420	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	15599	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	36613	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	39314	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	30771m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	9806	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	28111	0.28	ng/ul	0.00
Target Compounds						Qvalue
15) Fluoranthene	19.15	202	3658	0.030	ng/ul	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed