
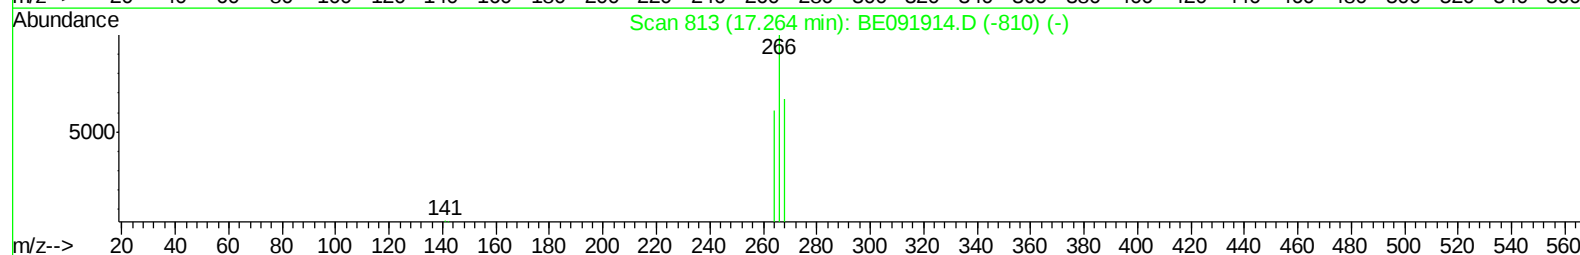
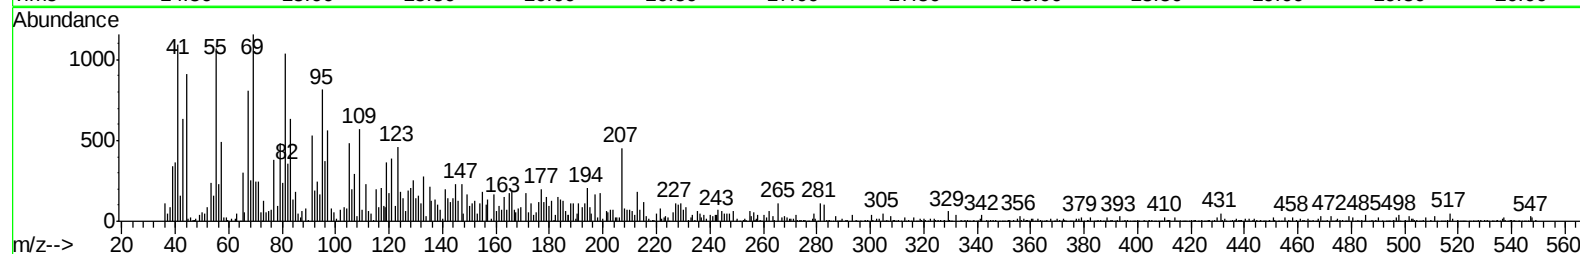


Data Path : Z:\HPCHEM1\BNA E\Data\BE061416\
 Data File : BE091908.D
 Acq On : 14 Jun 2016 9:58
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 19:45:12 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE061416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 15 12:00:38 2016
 Response via : Initial Calibration

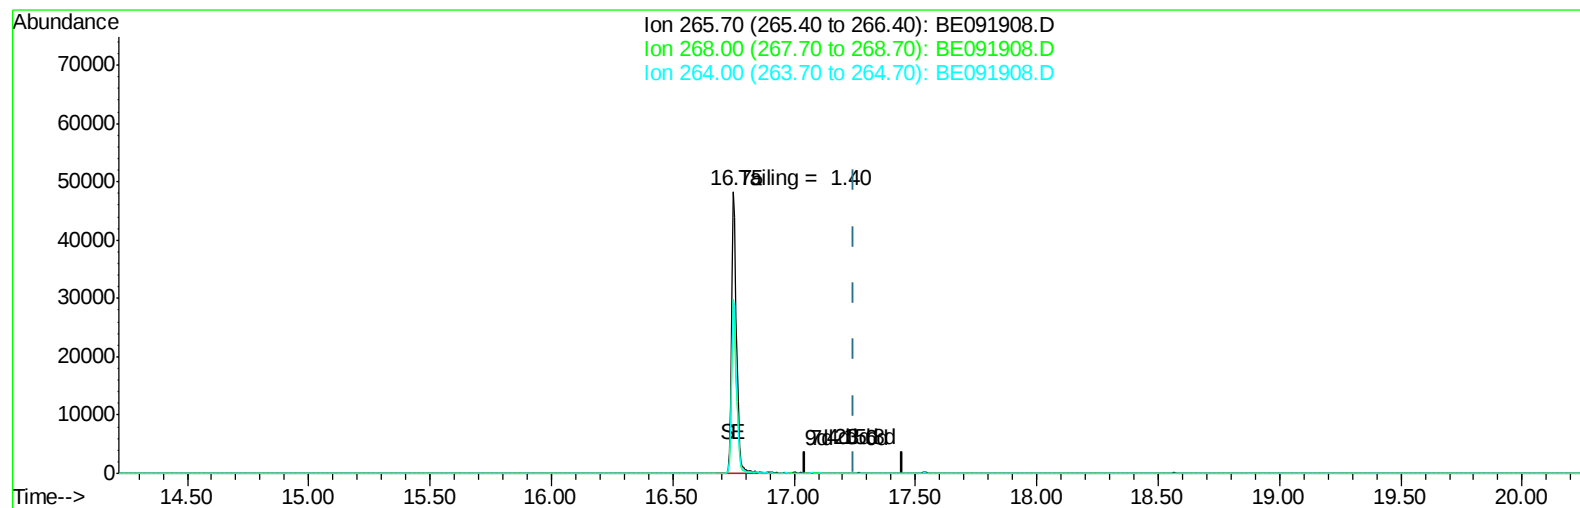

TIC: BE091908.D

(27) Pentachlorophenol




17.232min (-0.015) 28.35ng

response 86

Ion	Exp%	Act%
265.70	100	100
268.00	75.60	30.43#
264.00	63.70	8.70#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE061416\
Data File : BE091908.D
Acq On : 14 Jun 2016 9:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 15 19:45:12 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE061416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 15 12:00:38 2016
Response via : Initial Calibration

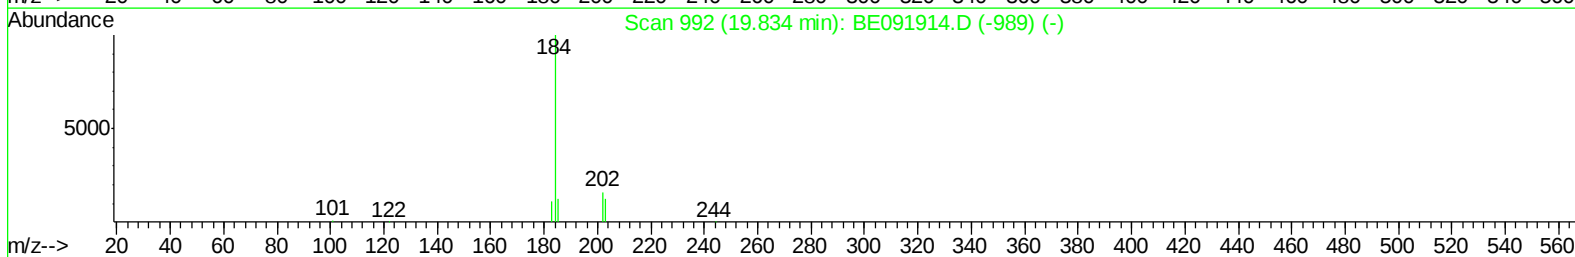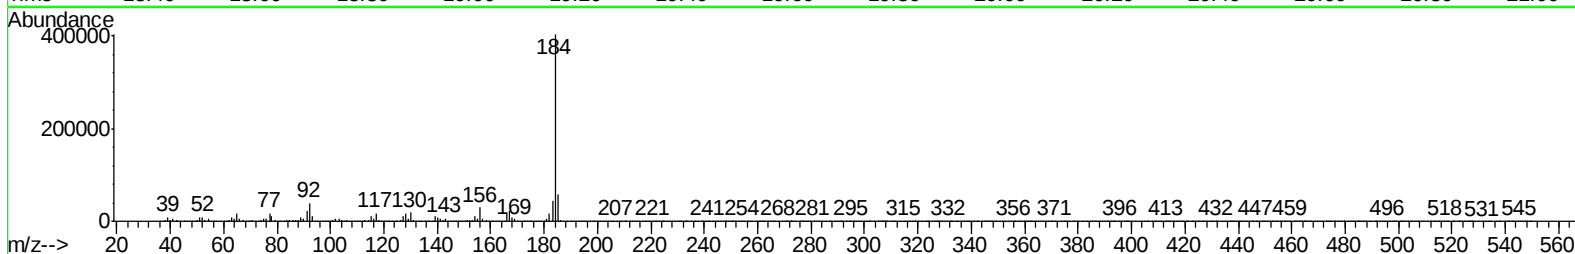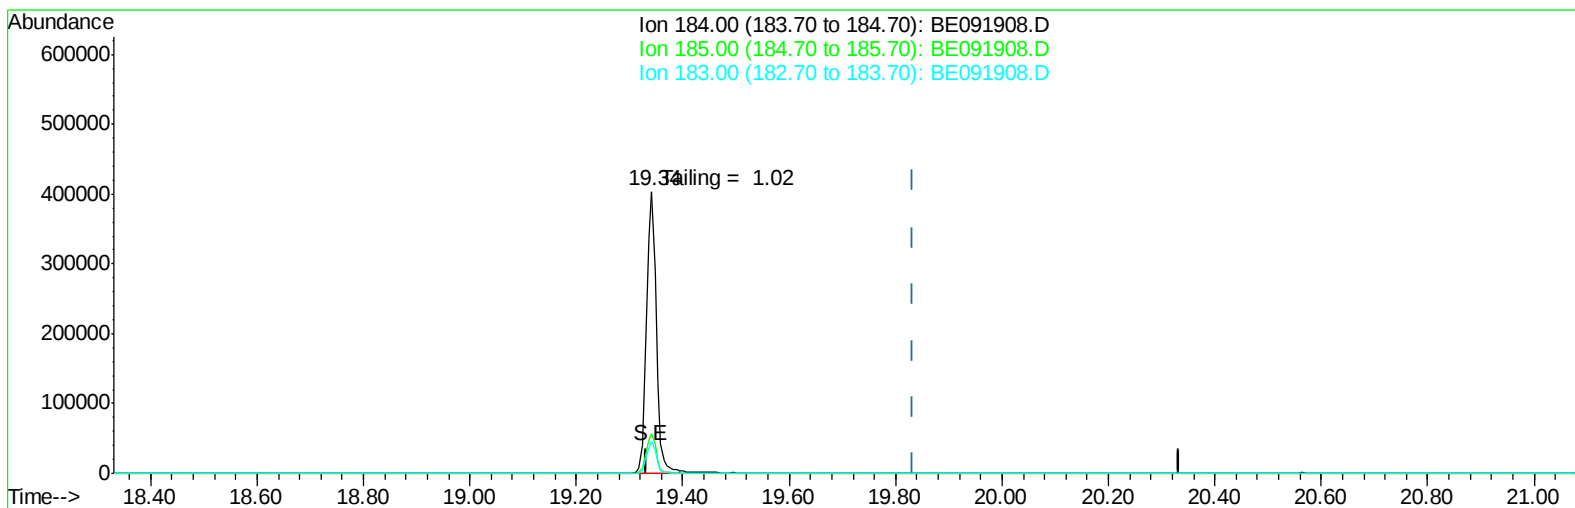

TIC: BE091908.D

(32) Benzidine

19.341min (-0.492) 1751.79ng

response 439520

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.22
183.00	14.70	11.22#
0.00	0.00	0.00