

Data File : BE093172.D
Acq On : 14 Jun 2017 16:41
Operator : SJ/MA
Sample : PB99752BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK52

Quant Time: Jun 15 02:28:14 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 02:27:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	3239	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	15799	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	9976	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	23820	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	1553248	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	7472	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20195	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	2544	0.06	ng/ul#	19
17) Pyrene	19.49	202	3044	0.04	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093172.D

Acq On : 14 Jun 2017 16:41

Operator : SJ/MA

Sample : PB99752BL

Misc :

ALS Vial : 10 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK52


Quant Time: Jun 15 02:28:14 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

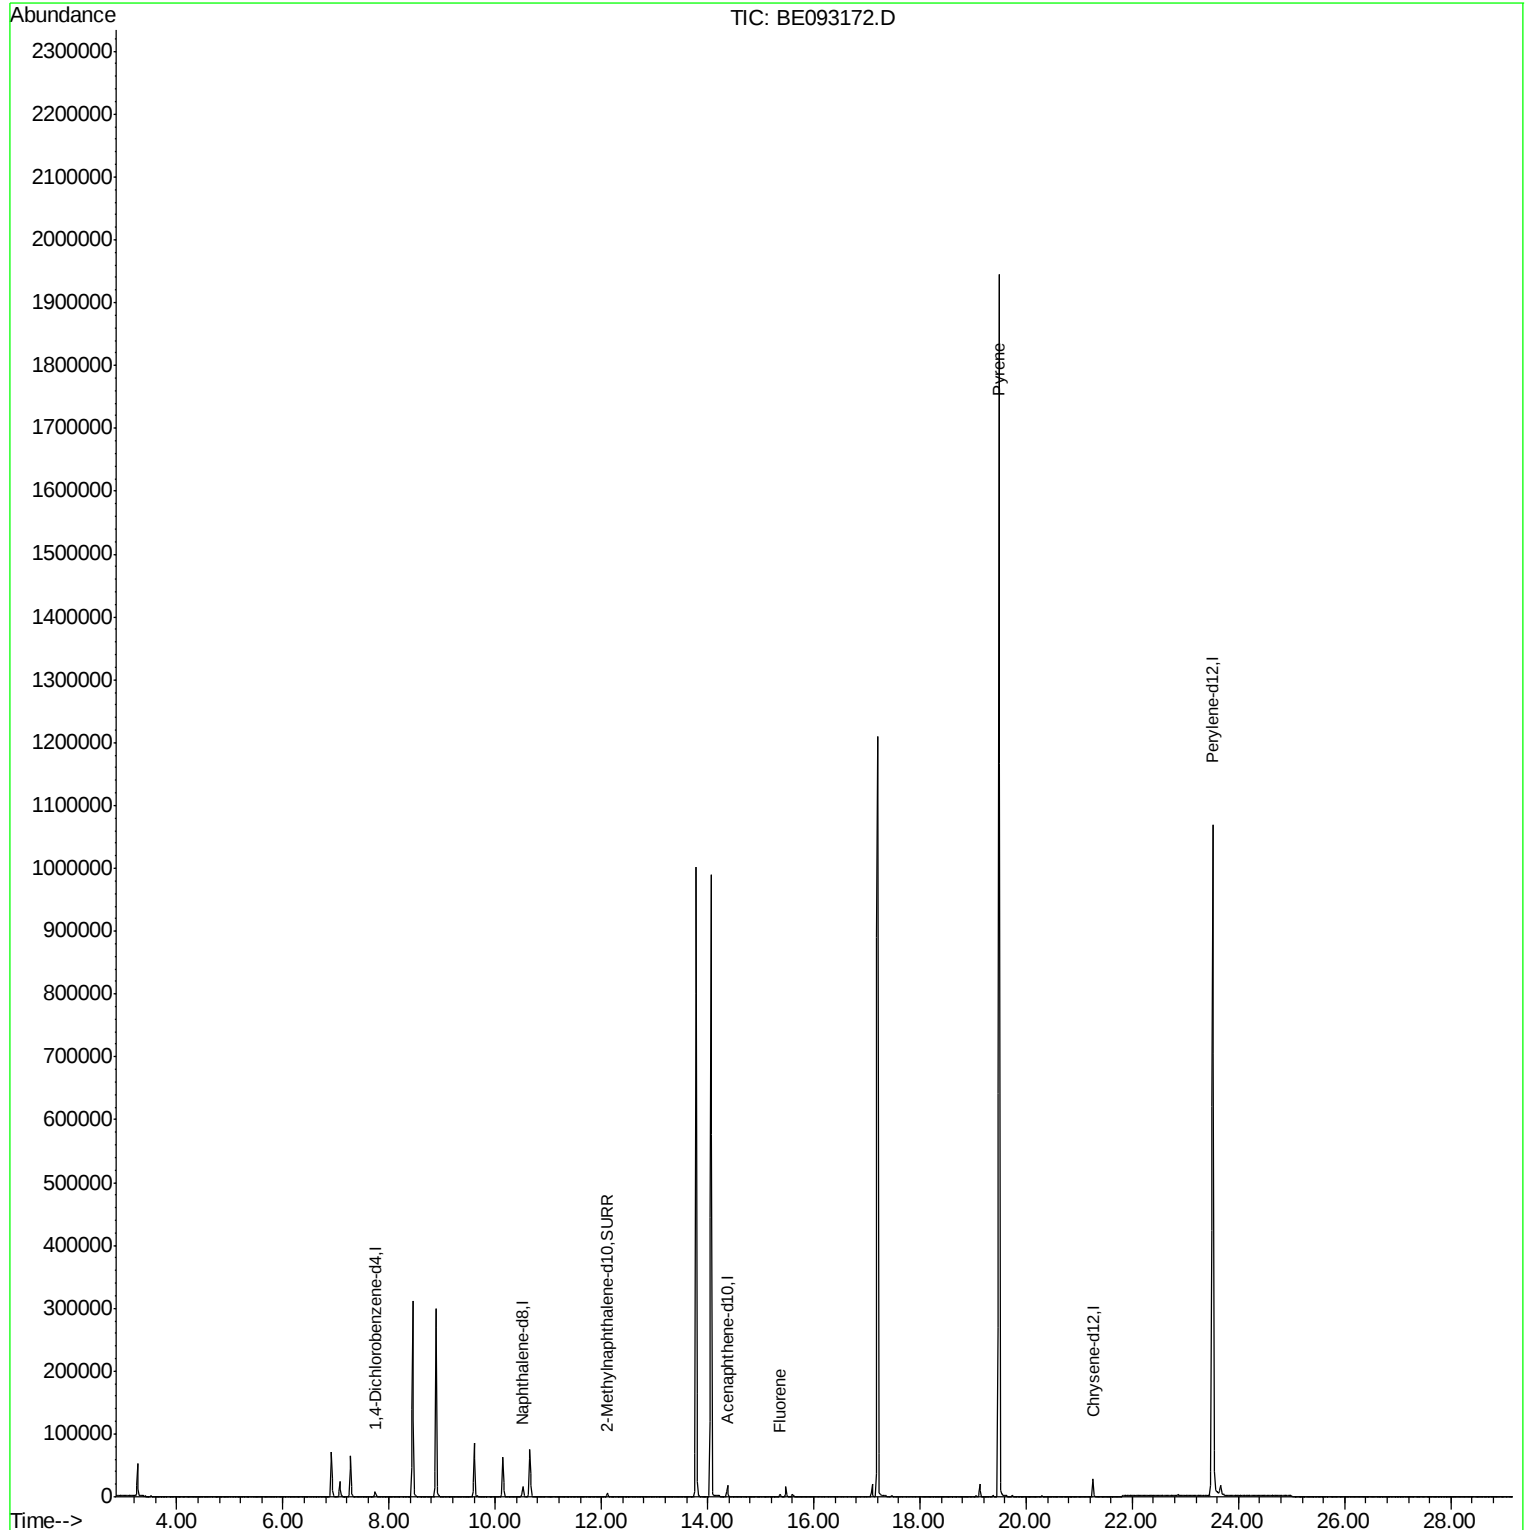

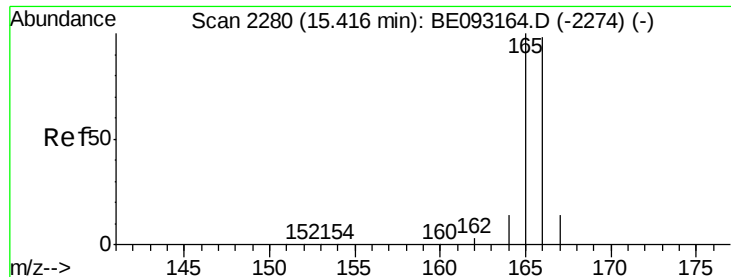

#9

Fluorene

Concen: 0.06 ng/ul

RT: 15.36 min Scan# 2274

Delta R.T. -0.05 min

Lab File: BE093172.D

Acq: 14 Jun 2017 16:41

Instrument :

BNA_E

ClientSampleId :

SBLK52


Tgt Ion:166 Resp: 2544

Ion Ratio Lower Upper




166 100

165 6.7 73.4 110.2#

167 36.2 14.6 22.0#

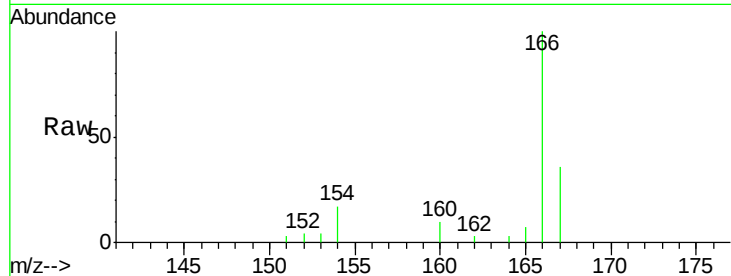

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

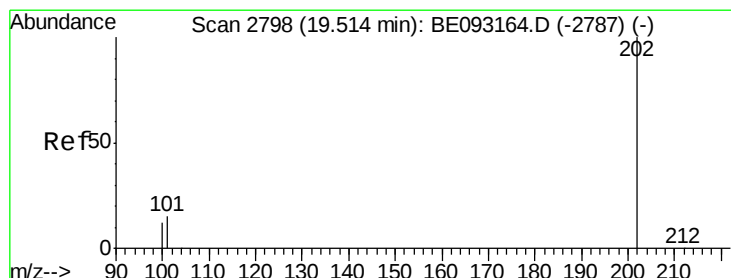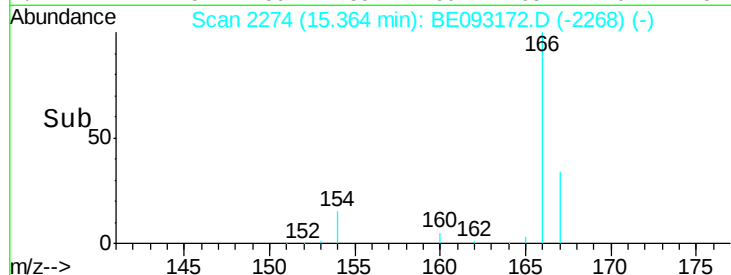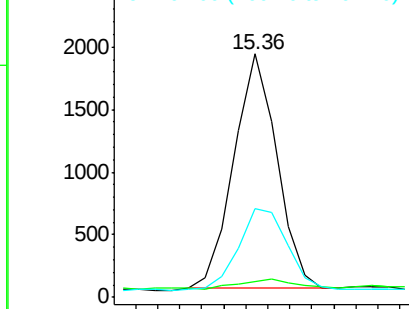

#17

Pyrene

Concen: 0.04 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.02 min

Lab File: BE093172.D

Acq: 14 Jun 2017 16:41


Tgt Ion:202 Resp: 3044

Ion Ratio Lower Upper

202 100

101 197.3 18.2 27.4#

100 1131.1 15.6 23.4#

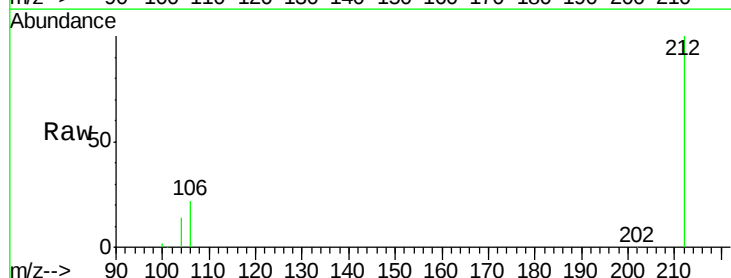

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

