


Data File : BE093173.D
Acq On : 14 Jun 2017 17:16
Operator : SJ/MA
Sample : I3646-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
B0AD0

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:09 PM

Quant Time: Jun 15 03:38:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 02:27:21 2017
Response via : Initial Calibration

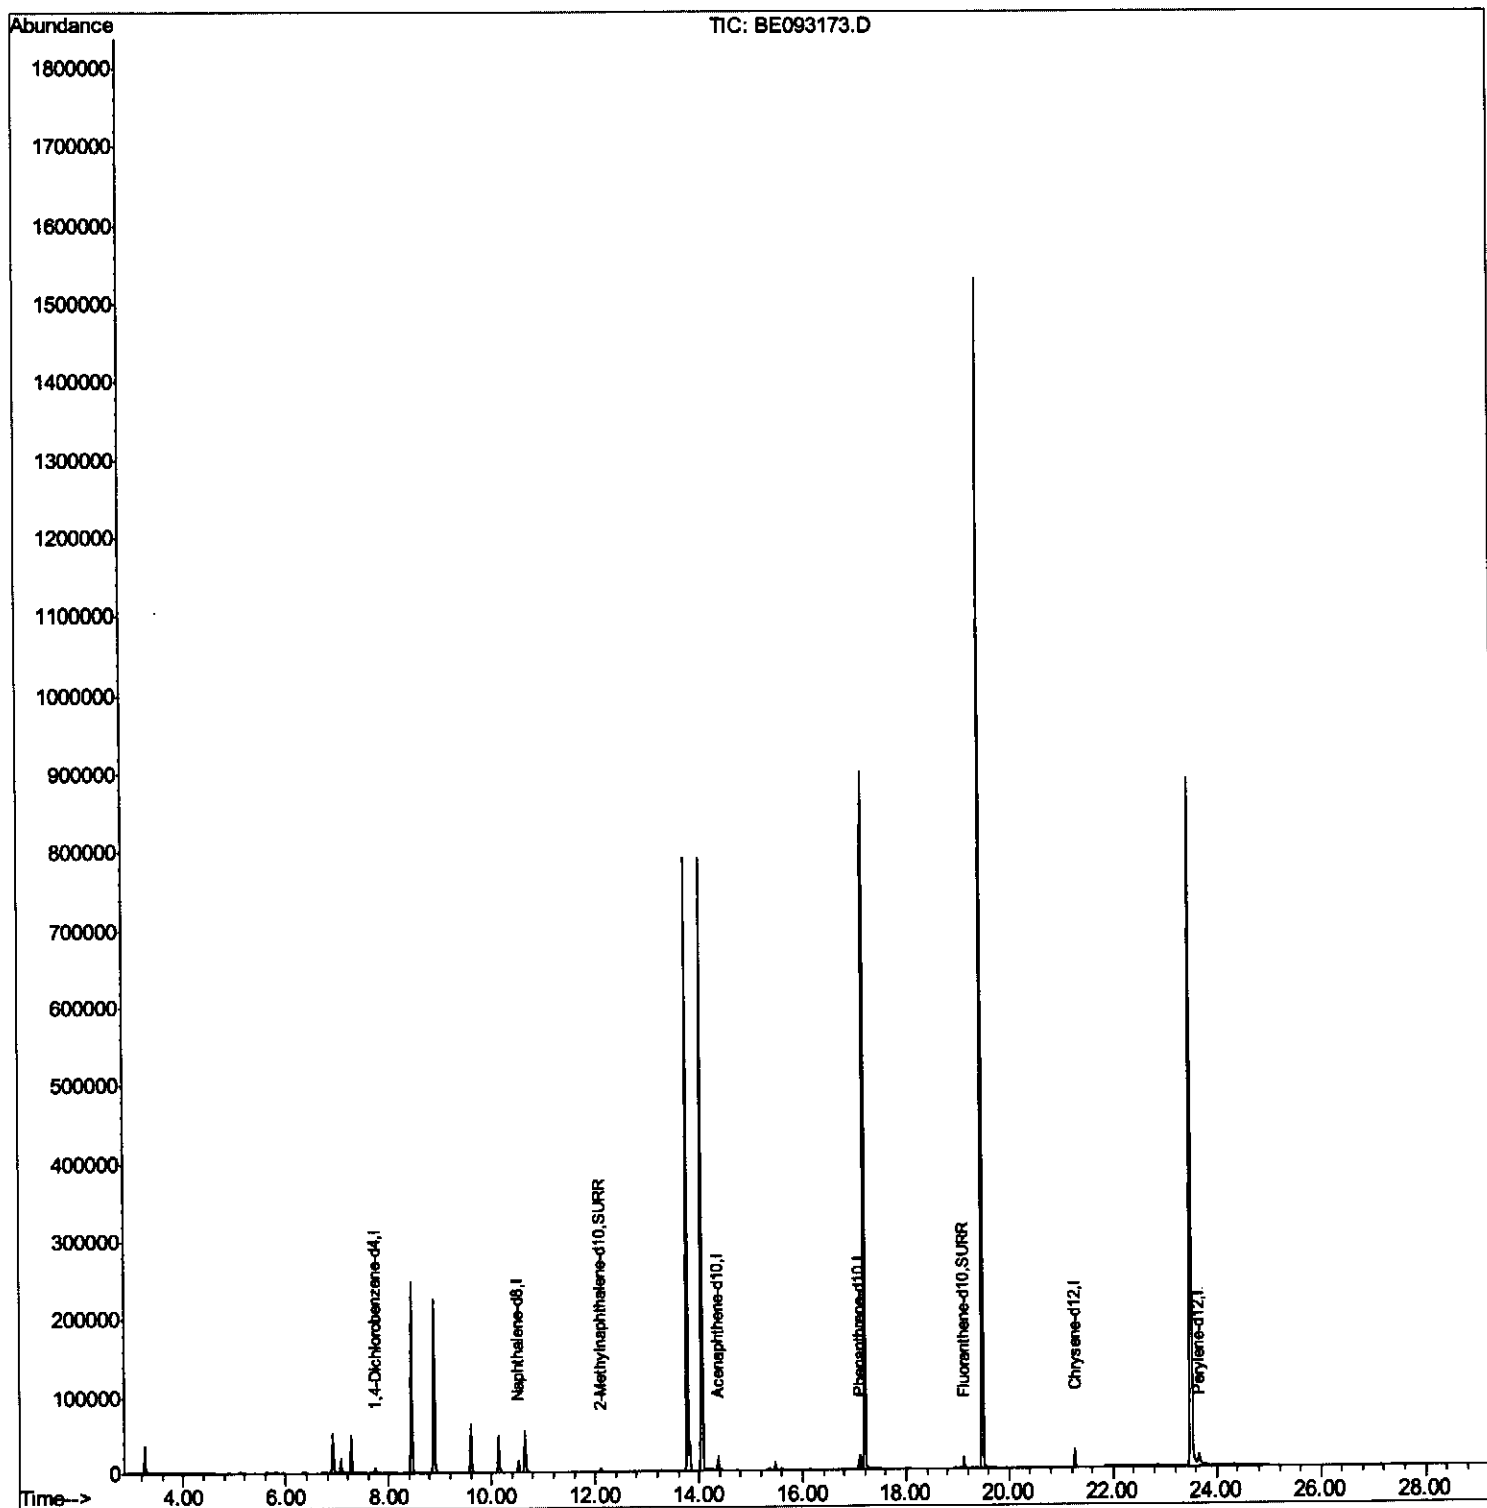

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093173.D

Acq On : 14 Jun 2017 17:16

Operator : SJ/MA

Sample : I3646-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

B0AD0

Manual Integrations

APPROVED

mohammad

6/15/2017 3:53:09 PM




Quant Time: Jun 15 02:28:20 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

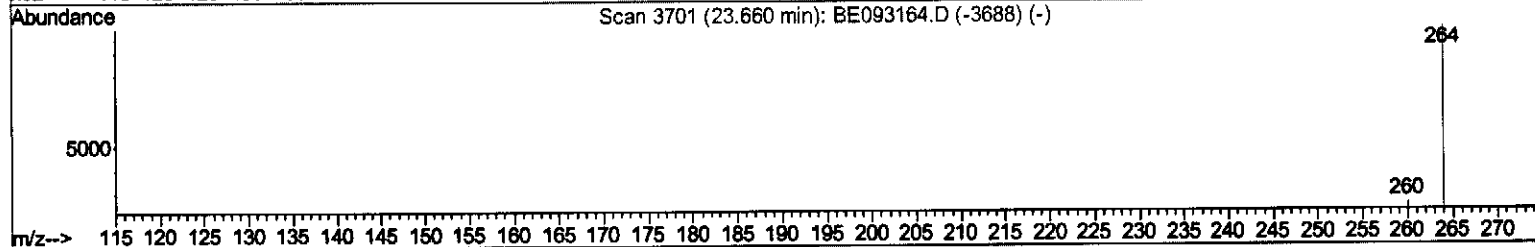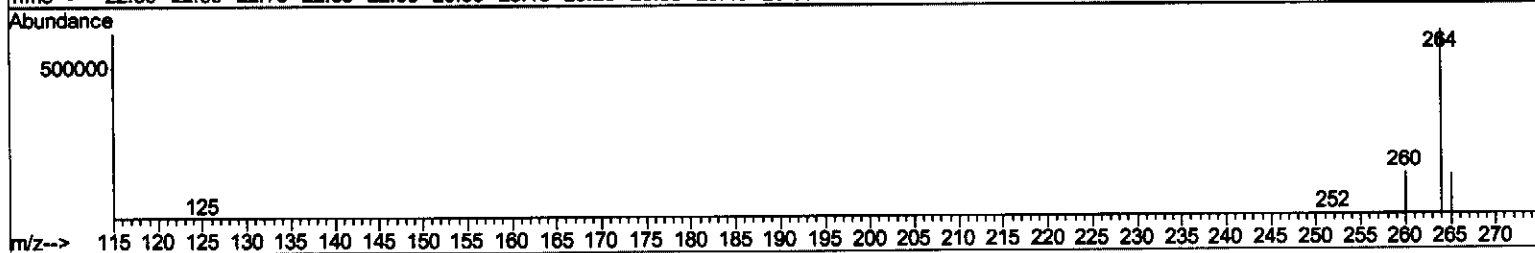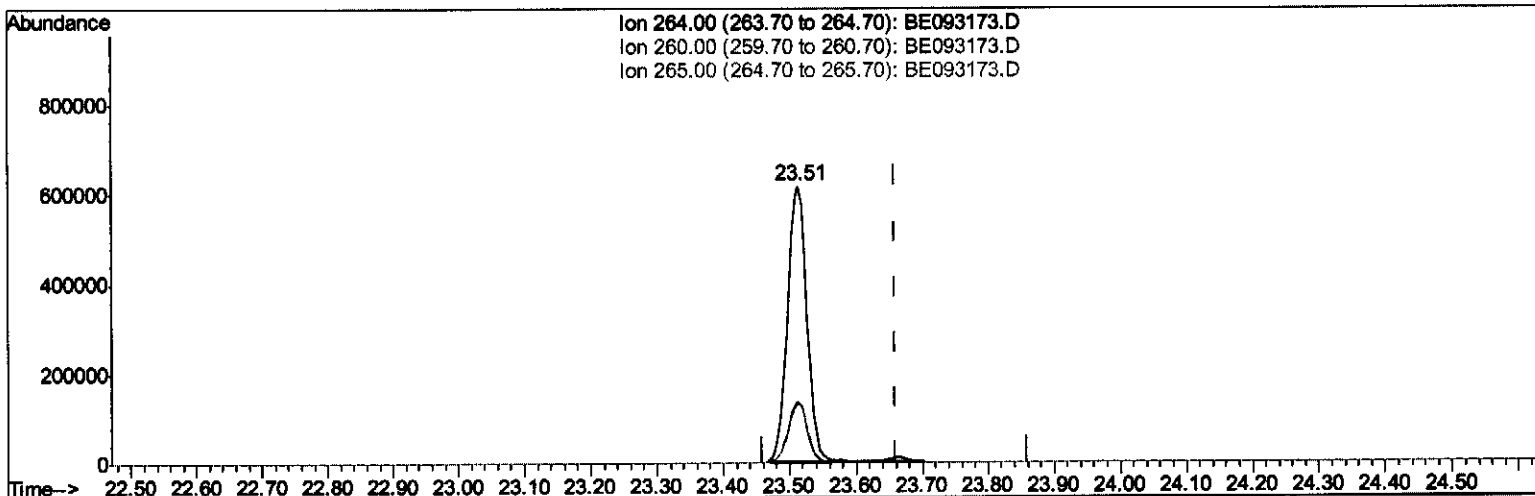

TIC: BE093173.D

(20) Perylene-d12 (I)

23.514min (-0.146) 0.40ng/ul

response 1240473

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.12#
265.00	103.50	21.59#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093173.D

Acq On : 14 Jun 2017 17:16

Operator : SJ/MA

Sample : I3646-01

Misc :

ALS Vial : 11 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

B0AD0

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:09 PM




Quant Time: Jun 15 02:28:20 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

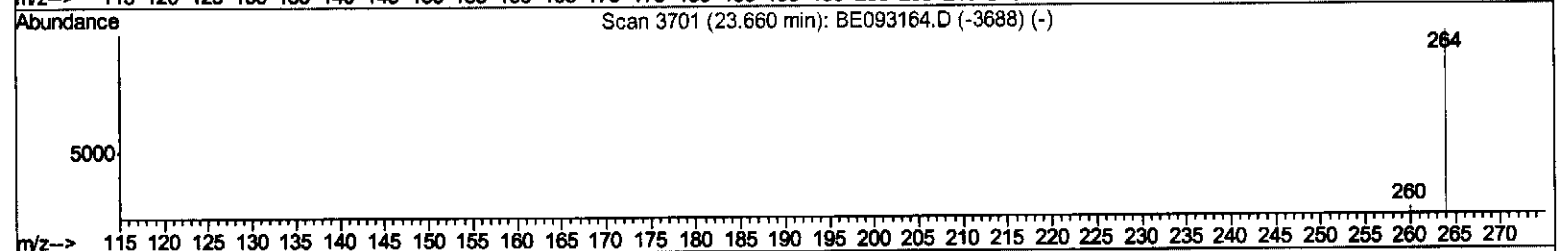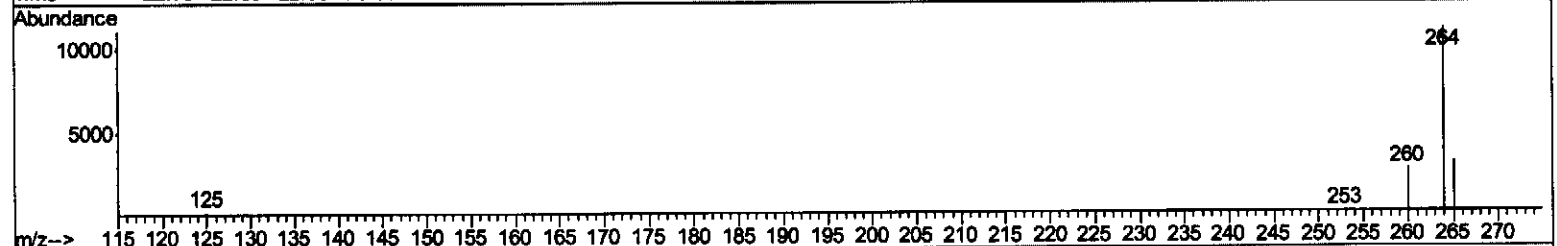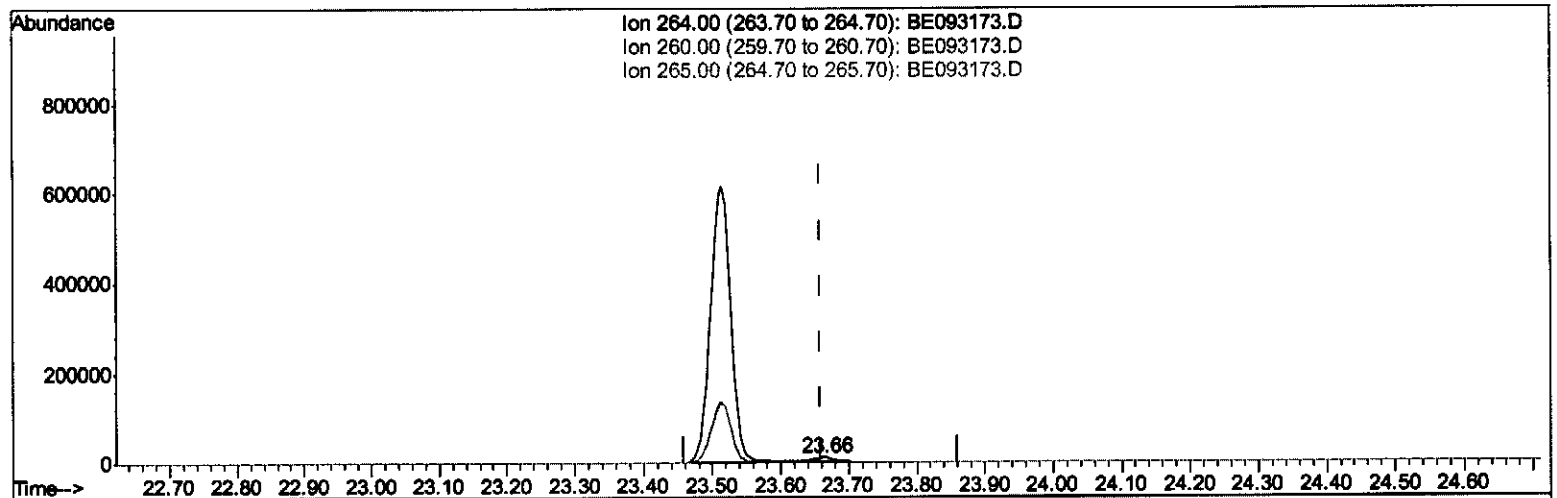

TIC: BE093173.D

(20) Perylene-d12 (I)

23.664min (+0.005) 0.40ng/ul m

response 18941

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.41
265.00	103.50	27.76#
0.00	0.00	0.00

SJ
06/21/17

Data File : BE093173.D
Acq On : 14 Jun 2017 17:16
Operator : SJ/MA
Sample : I3646-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
B0AD0

Manual Integrations
APPROVED
mohammad
6/15/2017 3:53:09 PM

Quant Time: Jun 15 03:38:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 02:27:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	3226	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	16360	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	10173	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	23618	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	23104	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	18941m >	0.40	ng/ul	0.00

SJ
06/21/17

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	6066	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	17014	0.26	ng/ul	0.00

Target Compounds	Qvalue
-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed