

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\
Quantitation Report (QT Reviewed)


Data File : BE093176.D
Acq On : 14 Jun 2017 19:10
Operator : SJ/MA
Sample : I3522-20DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F5D36DL

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:18 PM

Quant Time: Jun 15 03:49:31 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 02:27:21 2017
Response via : Initial Calibration

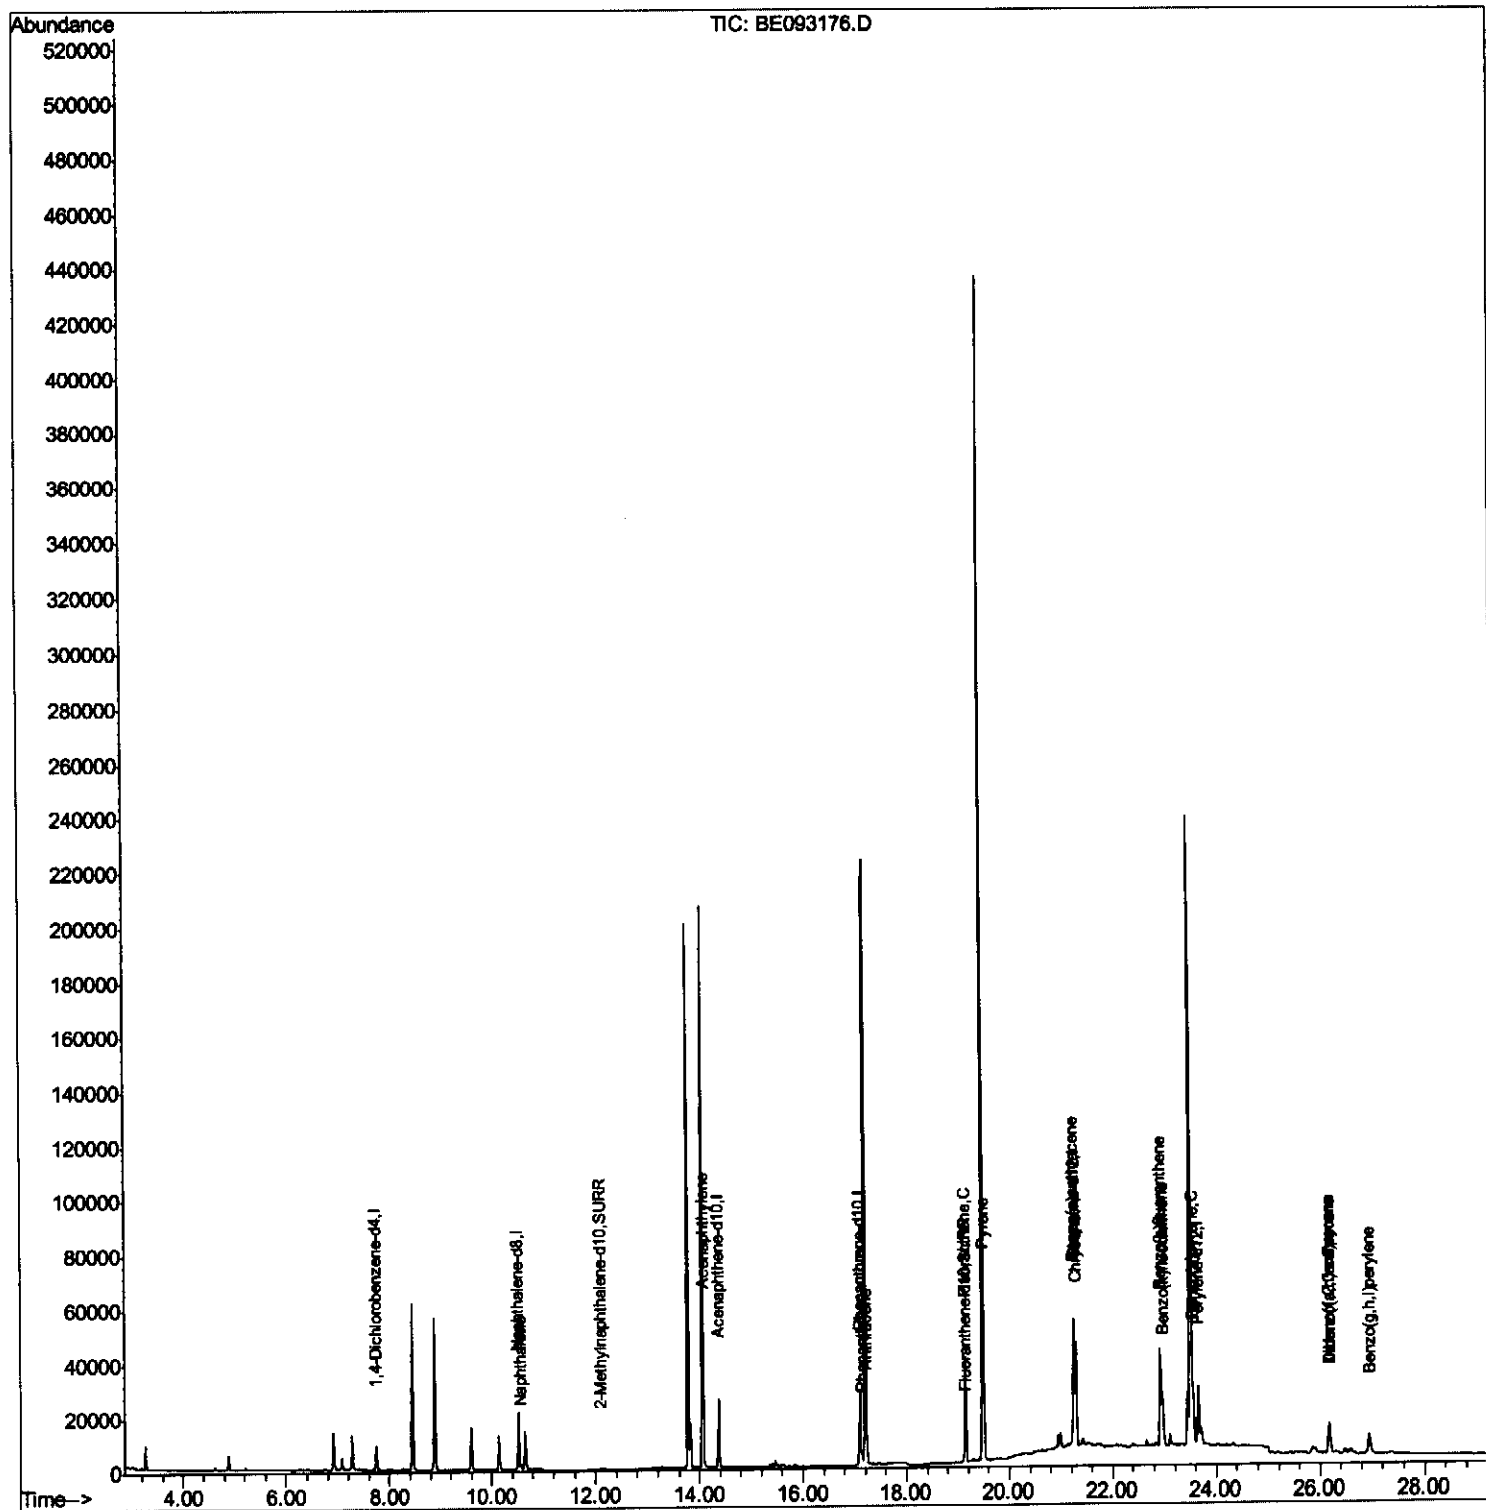

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093176.D

Acq On : 14 Jun 2017 19:10

Operator : SJ/MA

Sample : I3522-20DL 5X

Misc :

ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampled :

F5D36DL

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:18 PM




Quant Time: Jun 15 02:28:46 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

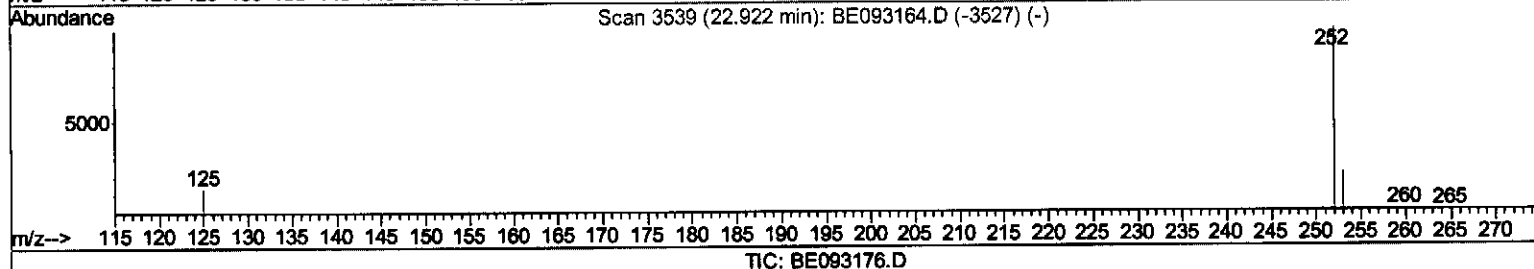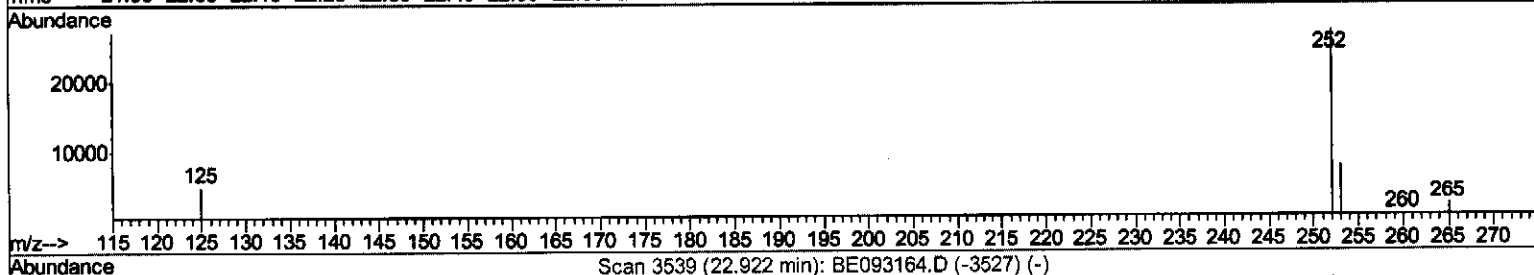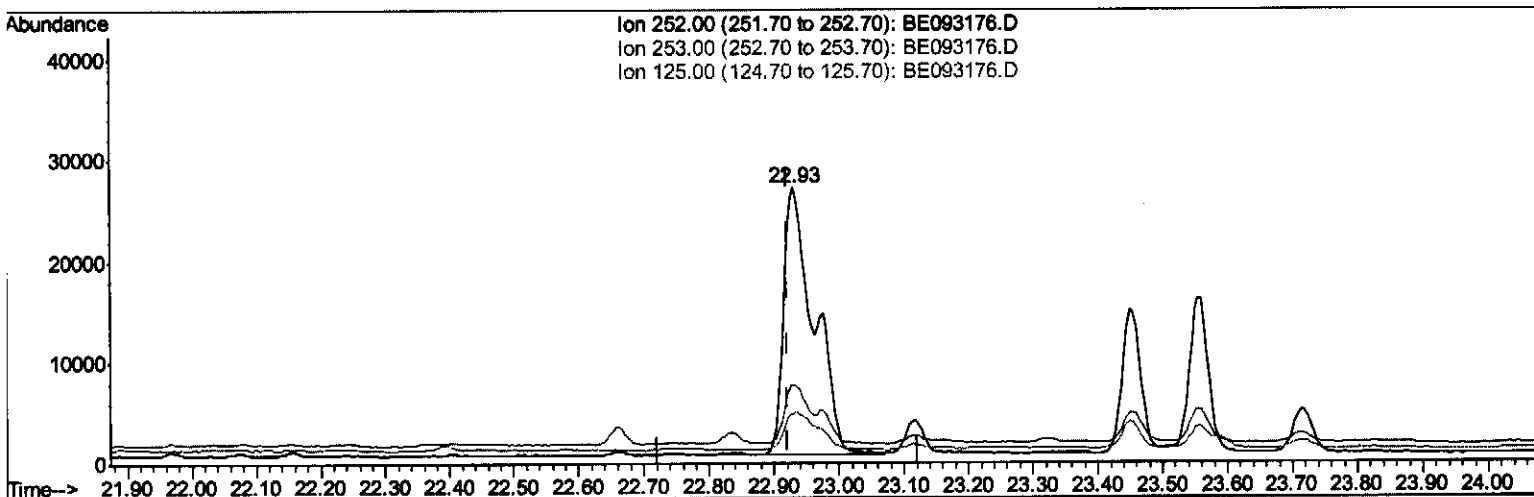

(21) Benzo(b)fluoranthene

22.930min (+0.008) 0.86ng/ul

response 85879

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.83
125.00	17.50	18.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093176.D

Acq On : 14 Jun 2017 19:10

Operator : SJ/MA

Sample : I3522-20DL 5X

Misc :

ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F5D36DL

Manual Integrations
APPROVED

mohammad

6/15/2017 3:53:18 PM




Quant Time: Jun 15 02:28:46 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

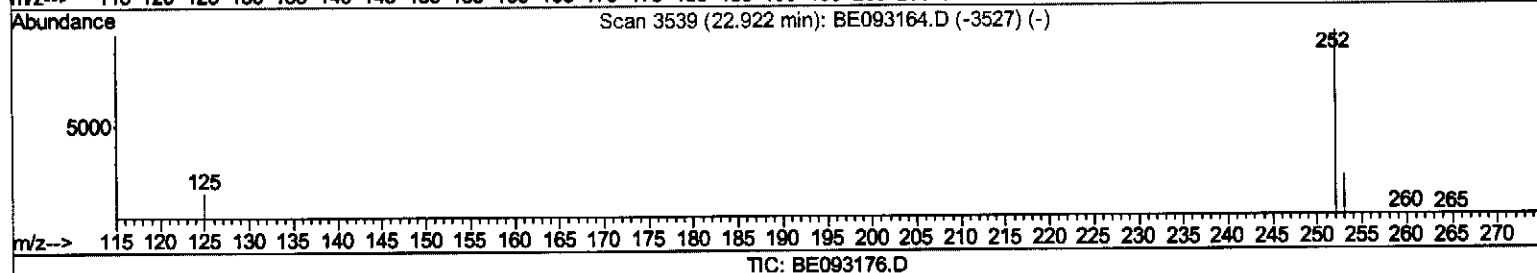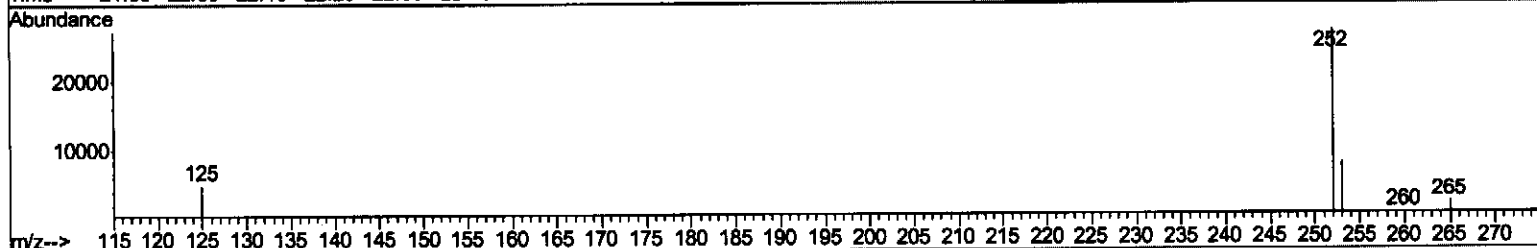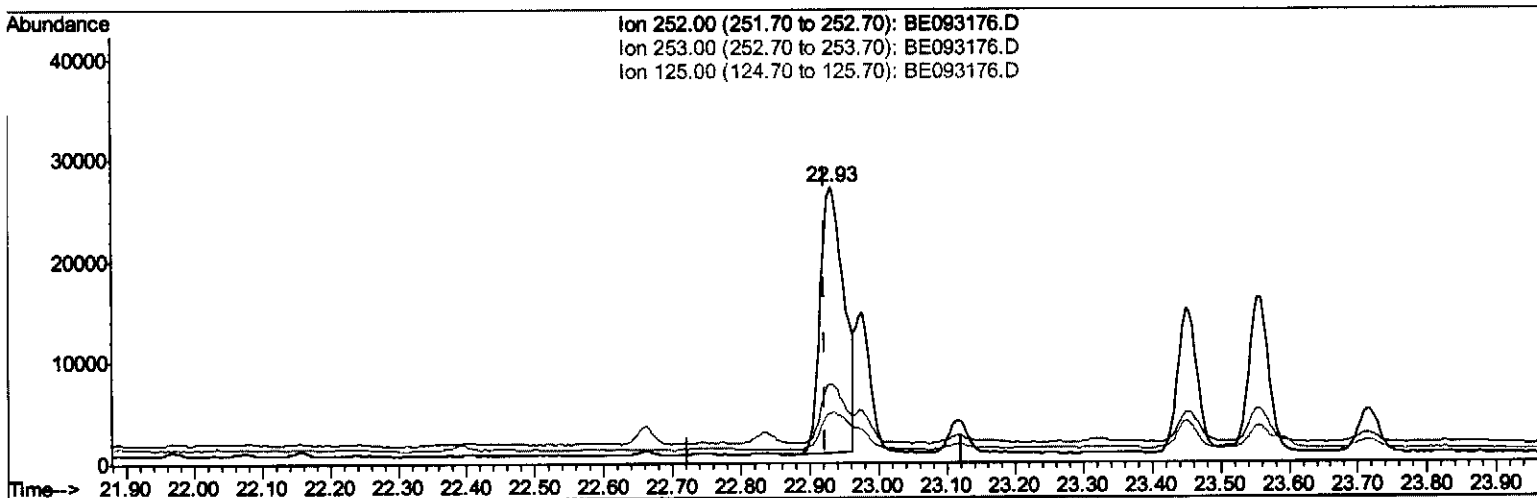

(21) Benzo(b)fluoranthene

22.930min (+0.008) 0.64ng/ul m

response 63409

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	28.83
125.00	17.50	18.14
0.00	0.00	0.00

SS
06/21/17

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093176.D

Acq On : 14 Jun 2017 19:10

Operator : SJ/MA

Sample : I3522-20DL 5X

Misc :

ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F5D36DL

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:18 PM




Quant Time: Jun 15 02:28:46 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

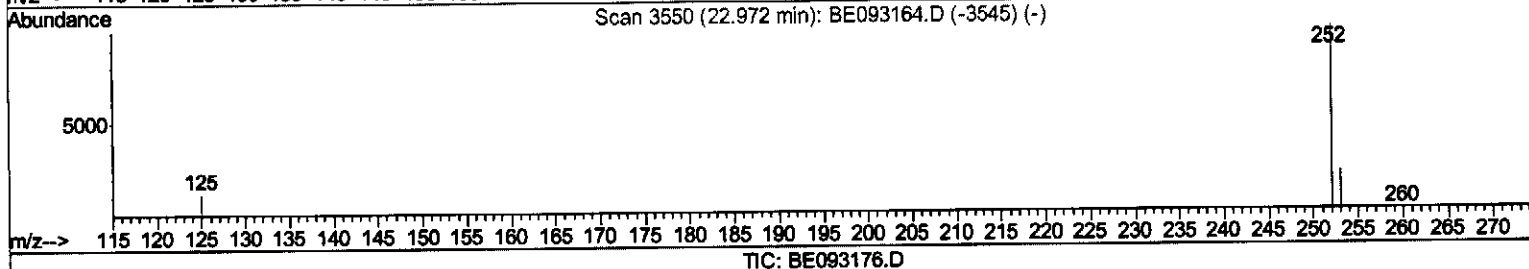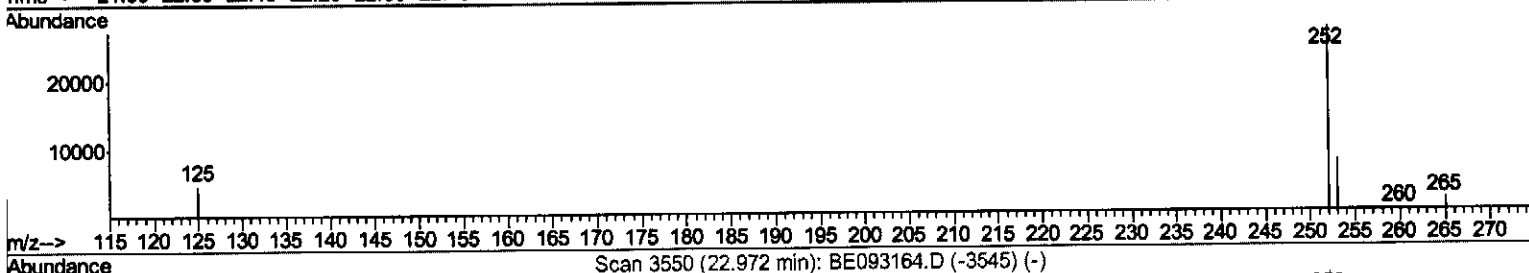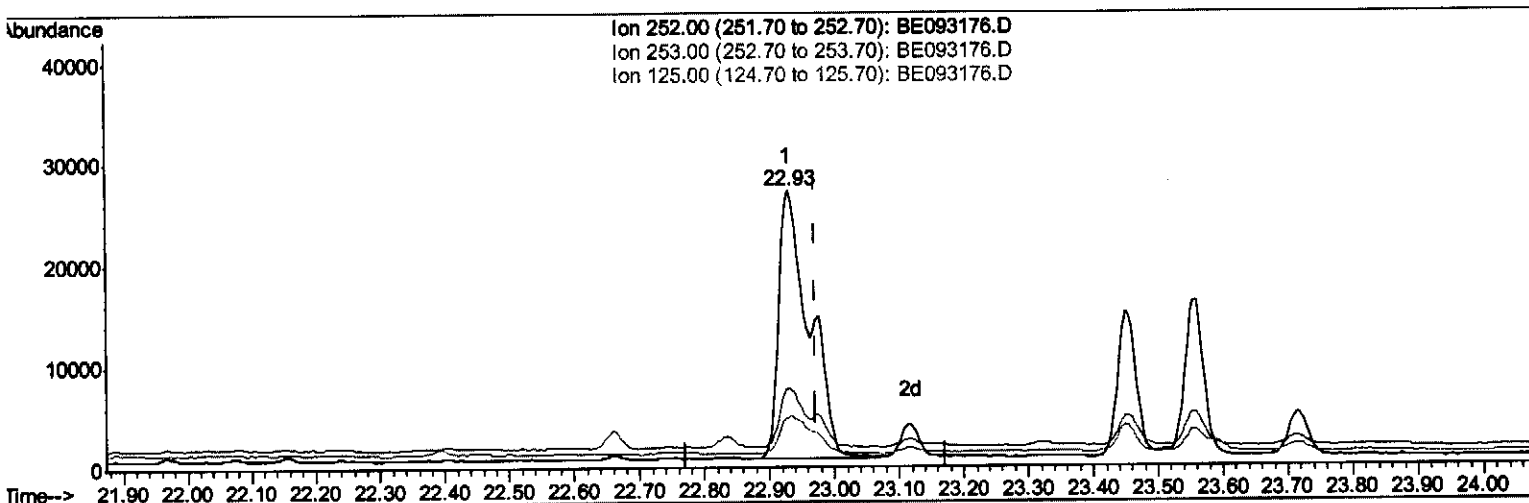

(22) Benzo(k)fluoranthene

22.930min (-0.042) 0.81ng/ul

response 85879

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	28.83
125.00	17.10	18.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061417\

Quantitation Report (Qedit)

Data File : BE093176.D

Acq On : 14 Jun 2017 19:10

Operator : SJ/MA

Sample : I3522-20DL 5X

Misc :

ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F5D36DL

Manual Integrations
APPROVED

mohammad

6/15/2017 3:53:18 PM




Quant Time: Jun 15 02:28:46 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Jun 15 02:27:21 2017

Response via : Initial Calibration

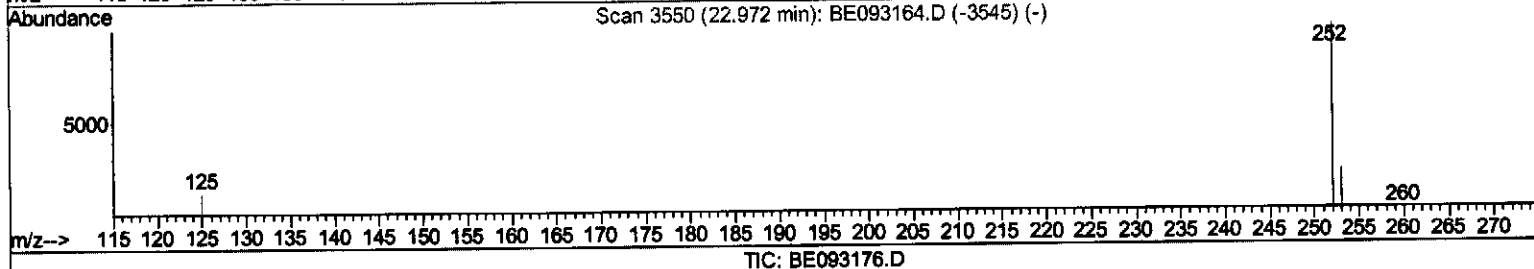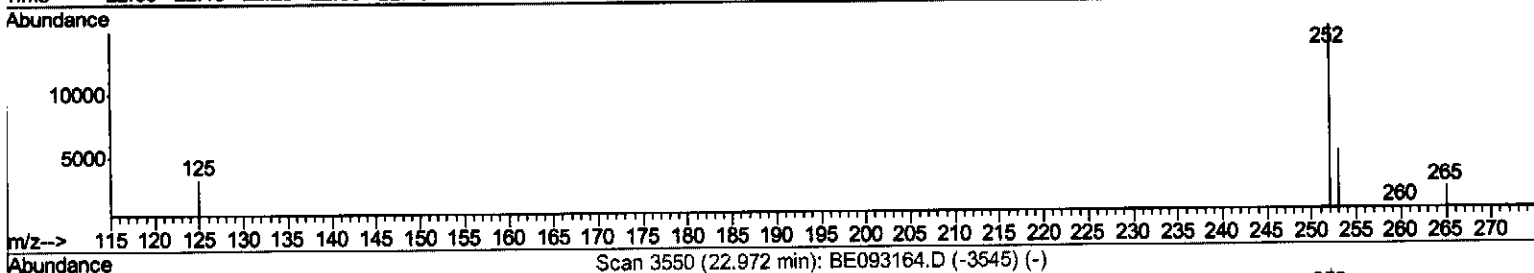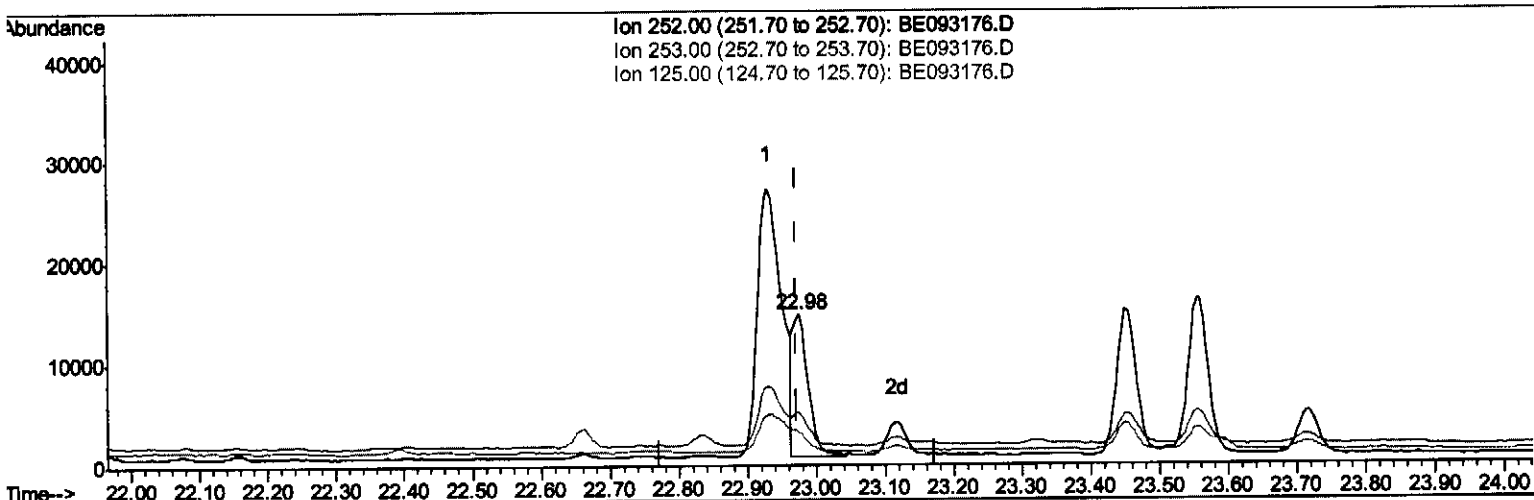

(22) Benzo(k)fluoranthene

22.976min (+0.004) 0.21ng/ul m

response 21800

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	34.83
125.00	17.10	22.00#
0.00	0.00	0.00

SJ
06/21/17

Data File : BE093176.D
Acq On : 14 Jun 2017 19:10
Operator : SJ/MA
Sample : I3522-20DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5D36DL

Manual Integrations
APPROVED

mohammad
6/15/2017 3:53:18 PM

Quant Time: Jun 15 03:49:31 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 15 02:27:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	4365	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	22001	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	13549	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	34250	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	34919	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	32865	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	1571	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	4782	0.05	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.57	128	2617	0.05	ng/ul#	90
7) Acenaphthylene	14.09	152	2714	0.05	ng/ul	96
12) Phenanthrene	17.14	178	5438	0.06	ng/ul#	90
13) Anthracene	17.22	178	4751	0.06	ng/ul#	93
15) Fluoranthene	19.16	202	42721	0.37	ng/ul	84
17) Pyrene	19.52	202	43454	0.42	ng/ul#	83
18) Benzo(a)anthracene	21.24	228	30670	0.33	ng/ul#	90
19) Chrysene	21.29	228	40753	0.42	ng/ul#	92
21) Benzo(b)fluoranthene	22.93	252	63409m	0.64	ng/ul	
22) Benzo(k)fluoranthene	22.98	252	21800m	0.21	ng/ul	
23) Benzo(a)pyrene	23.55	252	31437	0.33	ng/ul	96
24) Indeno(1,2,3-cd)pyrene	26.18	276	19798	0.18	ng/ul#	88
25) Dibenzo(a,h)anthracene	26.19	278	5757	0.06	ng/ul#	21
26) Benzo(g,h,i)perylene	26.95	276	16852	0.18	ng/ul#	81

SS
06/21/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed