

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061516\
 Data File : BE091927.D
 Acq On : 15 Jun 2016 16:28
 Operator : UM/SJ
 Sample : PB91035BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB91035BL

Quant Time: Jun 15 17:16:17 2016
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 15 12:00:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	23847	5.00	ng	0.00
8) Naphthalene-d8	11.02	136	101973	5.00	ng	0.03
15) Acenaphthene-d10	14.86	164	72982	5.00	ng	0.00
24) Phenanthrene-d10	17.61	188	158485	5.00	ng	0.00
31) Chrysene-d12	21.76	240	234345	5.00	ng	0.00
40) Perylene-d12	24.17	264	176923	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.72	112	38163	8.19	ng	0.00
5) Phenol-d6	7.37	99	49798	6.53	ng	0.02
9) Nitrobenzene-d5	9.37	82	27995	3.98	ng	0.00
16) 2,4,6-Tribromophenol	16.35	330	11007	5.82	ng	0.00
17) 2-Fluorobiphenyl	13.49	172	73686	3.98	ng	0.00
34) Terphenyl-d14	20.22	244	121449	4.23	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061516\
Data File : BE091927.D
Acq On : 15 Jun 2016 16:28
Operator : UM/SJ
Sample : PB91035BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB91035BL

Quant Time: Jun 15 17:16:17 2016
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 15 12:00:38 2016
Response via : Initial Calibration

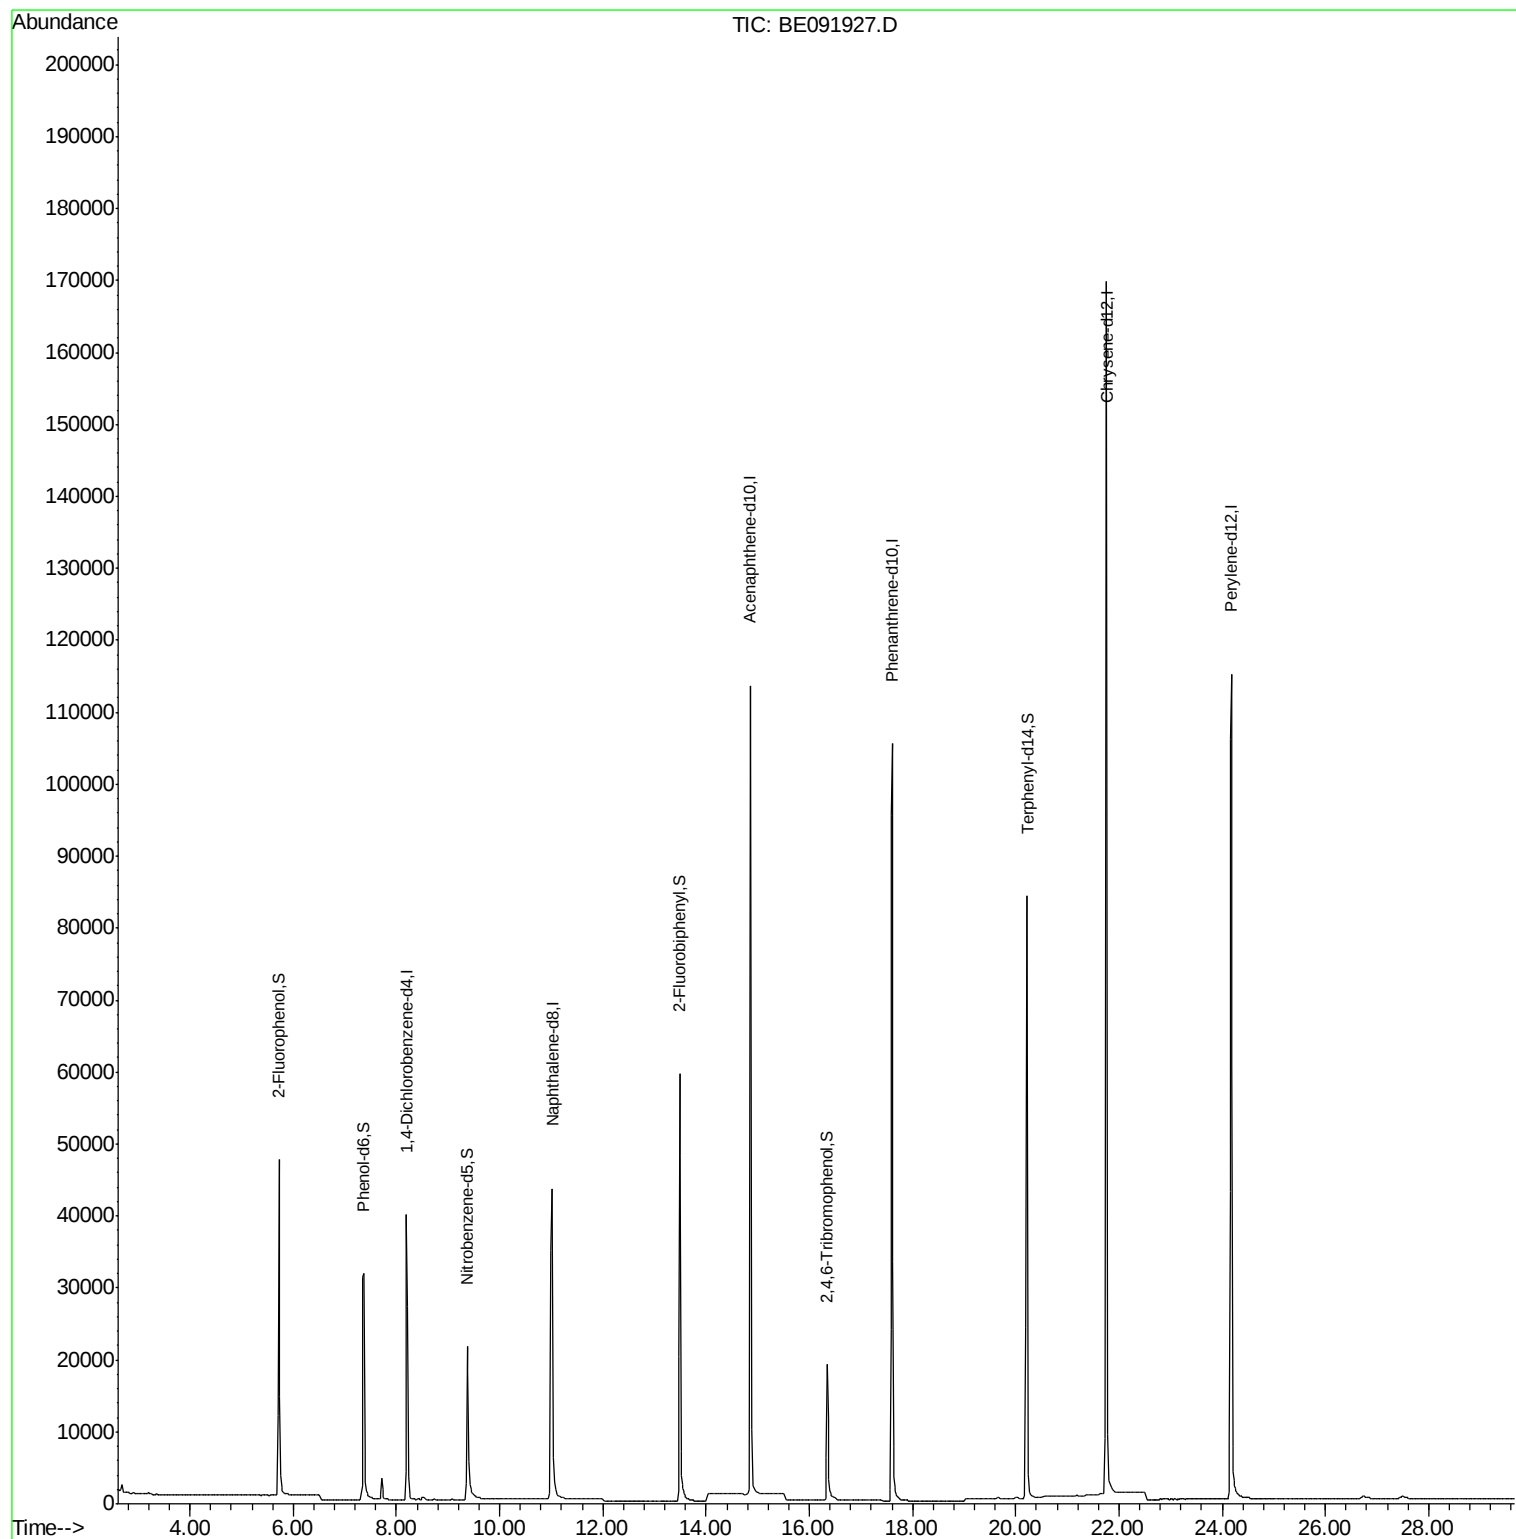

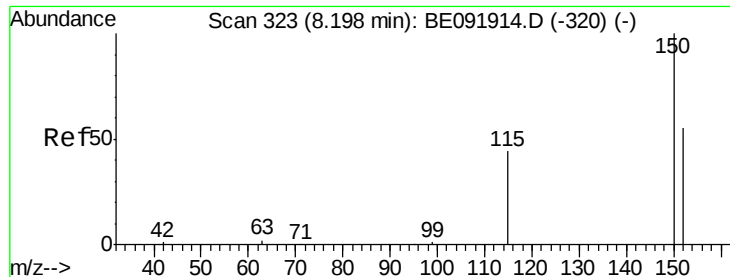

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.20 min Scan# 323

Delta R.T. -0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28

Instrument :

BNA_E

ClientSampleId :

PB91035BL


Tgt Ion:152 Resp: 23847

Ion Ratio Lower Upper

152 100

150 177.0 123.9 185.9




115 78.3 48.3 72.5#

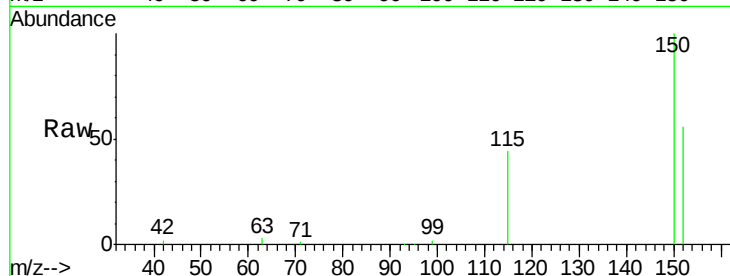

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

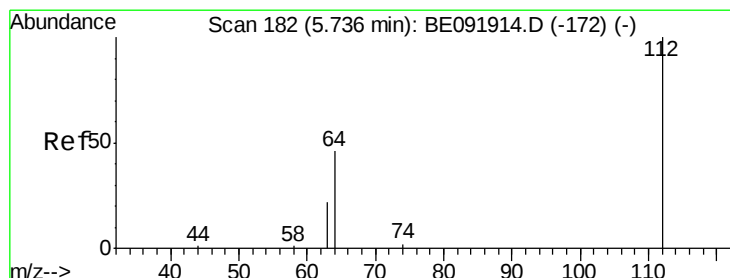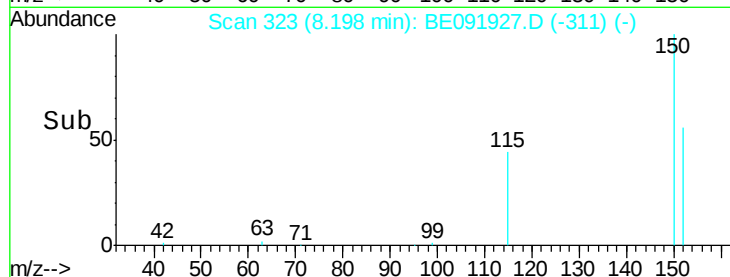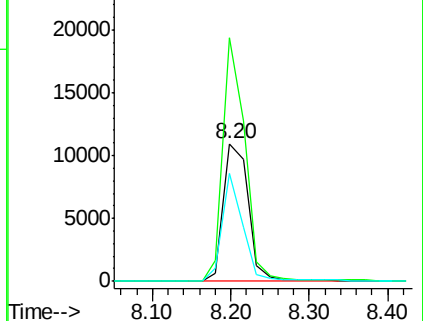

#4

2-Fluorophenol

Concen: 8.19 ng

RT: 5.72 min Scan# 181

Delta R.T. 0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28


Tgt Ion:112 Resp: 38163

Ion Ratio Lower Upper

112 100

64 67.3 53.7 80.5



63 36.0 29.5 44.3

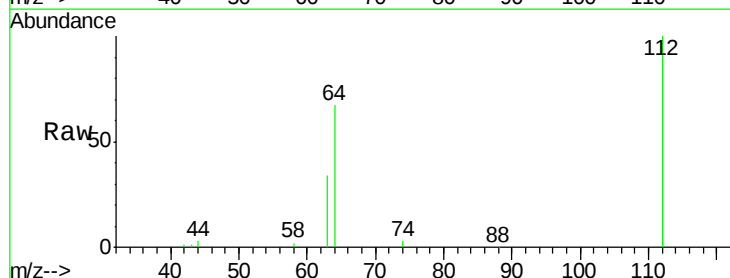


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

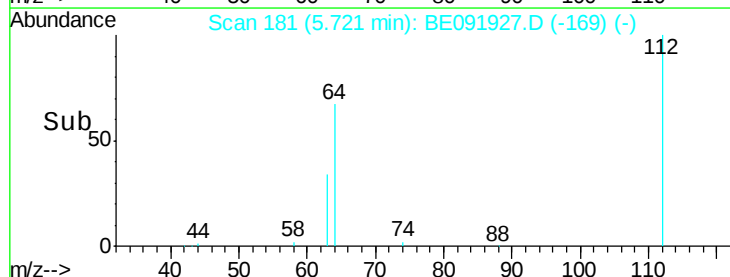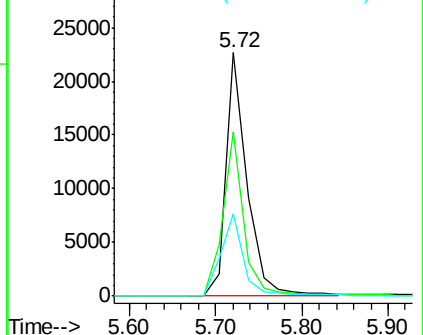

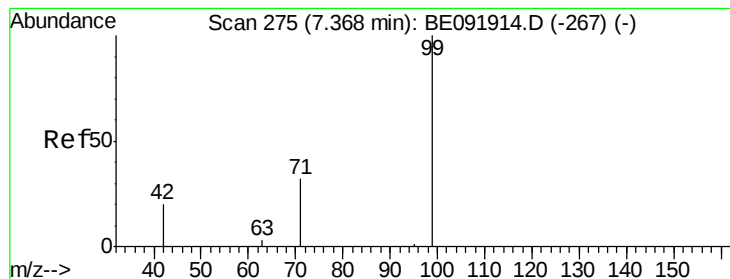

#5

Phenol-d6

Concen: 6.53 ng

RT: 7.37 min Scan# 275

Delta R.T. 0.02 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28

Instrument :

BNA_E

ClientSampleId :

PB91035BL


Tgt Ion: 99 Resp: 49798

Ion Ratio Lower Upper

99 100

42 25.6 19.6 29.4




71 35.7 28.1 42.1

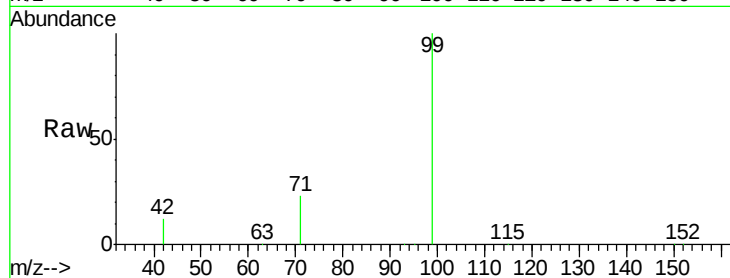

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

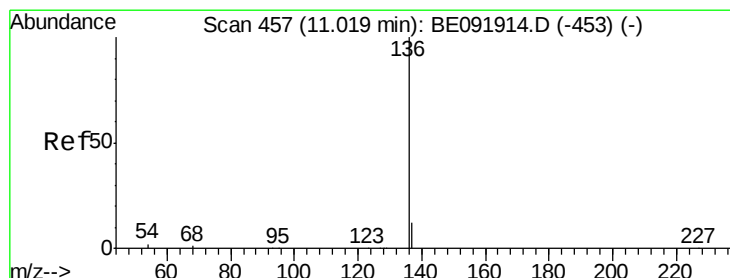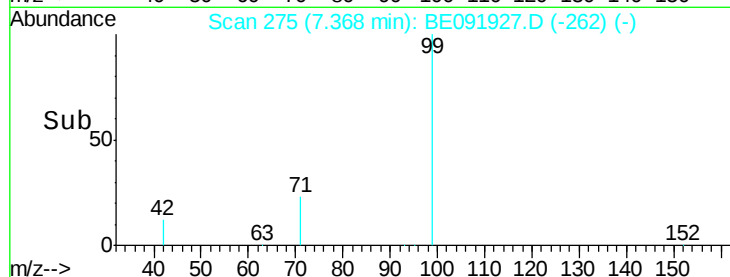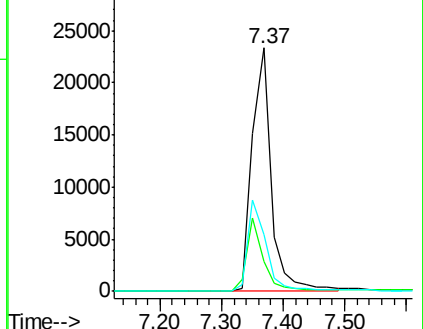

#8

Naphthalene-d8

Concen: 5.00 ng

RT: 11.02 min Scan# 457

Delta R.T. 0.03 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28

Tgt Ion: 136 Resp: 101973


Ion Ratio Lower Upper

136 100

137 12.1 8.3 12.5

54 2.7 8.2 12.4#

68 2.1 5.9 8.9#


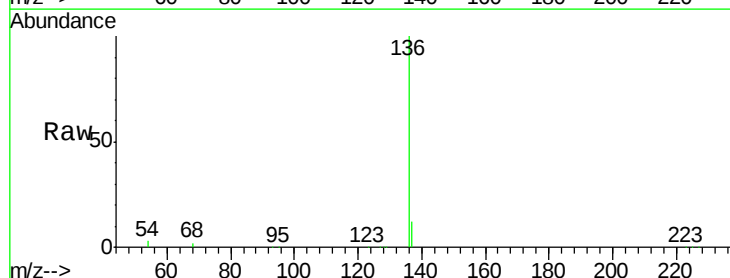



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

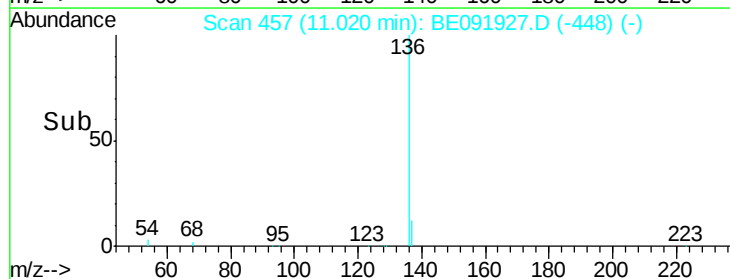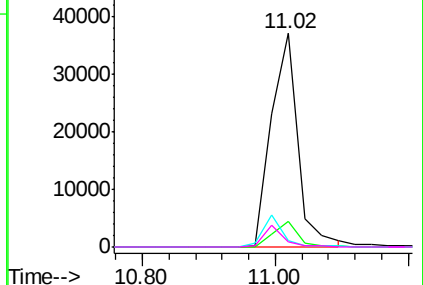

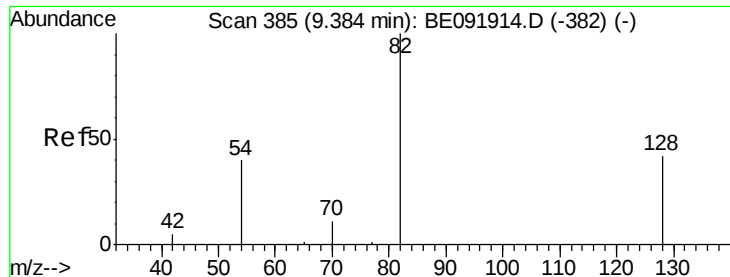

#9

Nitrobenzene-d5

Concen: 3.98 ng

RT: 9.37 min Scan# 384

Delta R.T. -0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28

Instrument :

BNA_E

ClientSampleId :

PB91035BL


Tgt Ion: 82 Resp: 27995

Ion Ratio Lower Upper

82 100

128 21.6 39.5 59.3#




54 79.3 30.3 45.5#

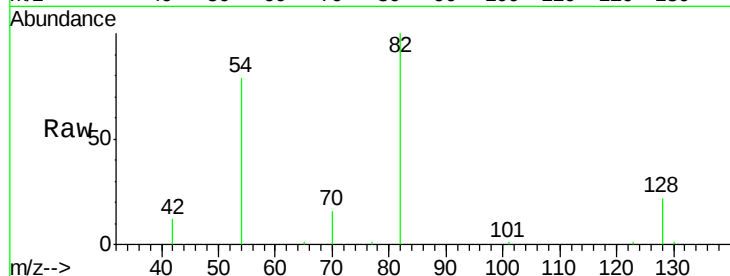

Abundance Ion 82.00 (81.70 to 82.70): BE091914.D (-382) (-)

Ion 128.00 (127.70 to 128.70): BE091914.D (-382) (-)

Ion 54.00 (53.70 to 54.70): BE091914.D (-382) (-)

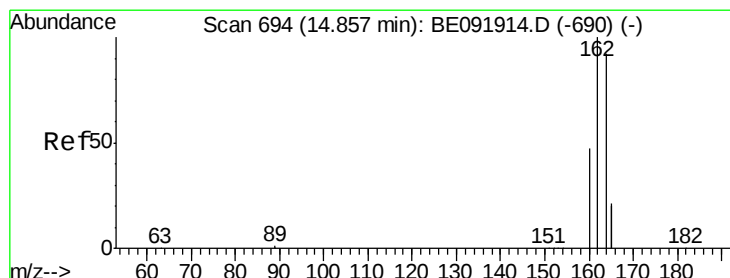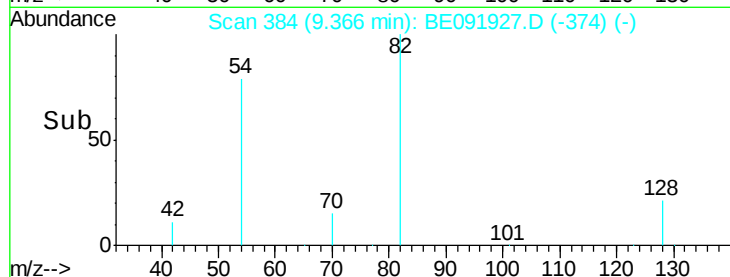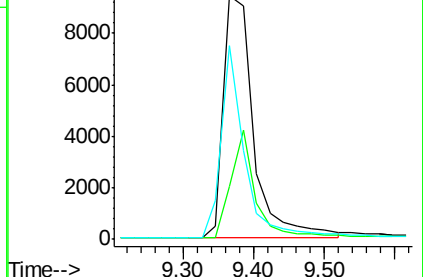

#15

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.86 min Scan# 694

Delta R.T. 0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28


Tgt Ion: 164 Resp: 72982

Ion Ratio Lower Upper

164 100

162 107.4 71.8 107.8



160 50.3 28.0 42.0#

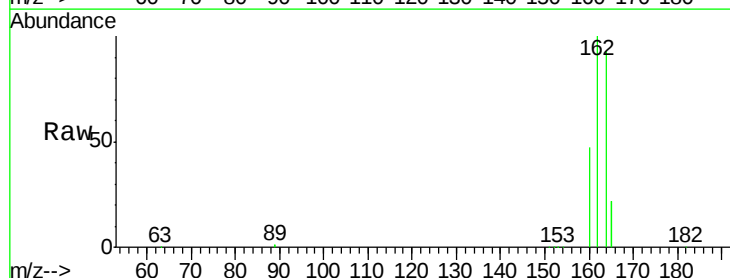


Abundance Ion 164.00 (163.70 to 164.70): BE091914.D (-690) (-)

Ion 162.00 (161.70 to 162.70): BE091914.D (-690) (-)

Ion 160.00 (159.70 to 160.70): BE091914.D (-690) (-)



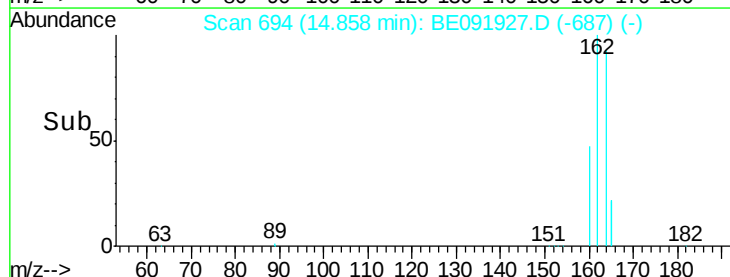
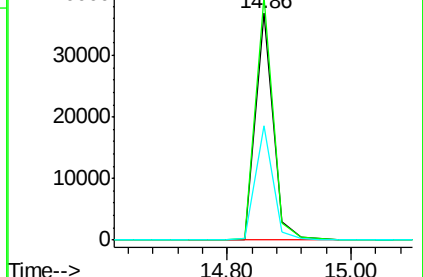


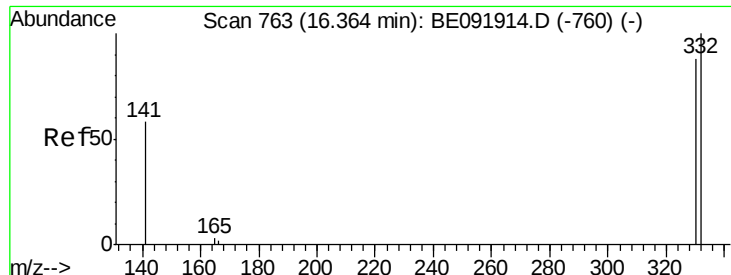

#16
 2,4,6-Tribromophenol
 Concen: 5.82 ng
 RT: 16.35 min Scan# 762
 Delta R.T. 0.00 min
 Lab File: BE091927.D
 Acq: 15 Jun 2016 16:28




Instrument :
 BNA_E
 ClientSampleId :
 PB91035BL


Tgt Ion:330 Resp: 11007
 Ion Ratio Lower Upper
 330 100
 332 97.2 77.0 115.6
 141 181.2 138.4 207.6

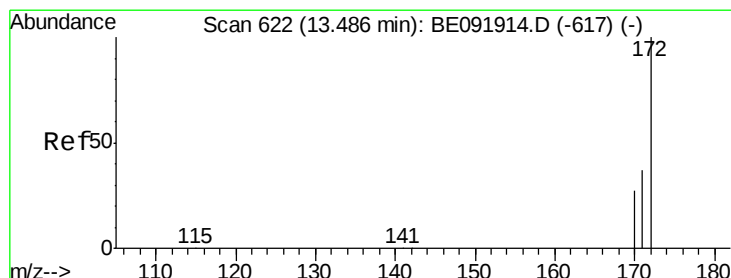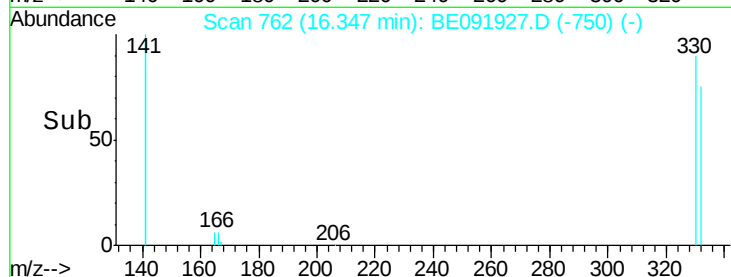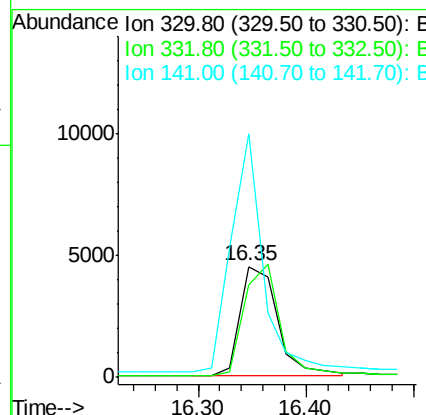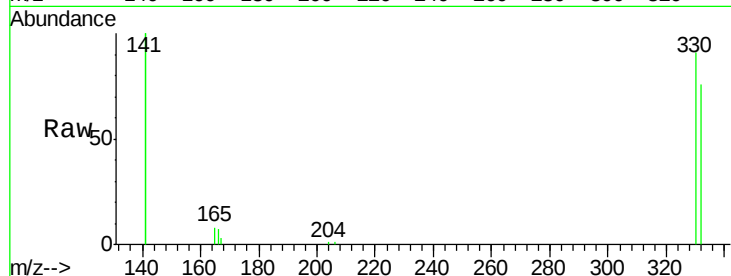

#17
 2-Fluorobiphenyl
 Concen: 3.98 ng
 RT: 13.49 min Scan# 622
 Delta R.T. 0.00 min
 Lab File: BE091927.D
 Acq: 15 Jun 2016 16:28

Tgt Ion:172 Resp: 73686
 Ion Ratio Lower Upper
 172 100
 171 36.7 24.3 36.5#
 170 25.9 14.9 22.3#

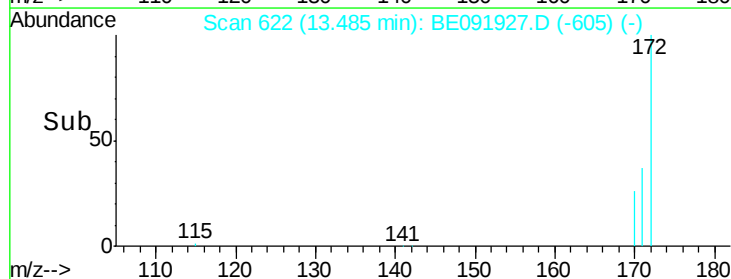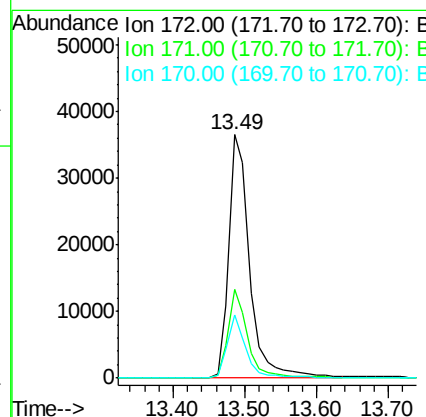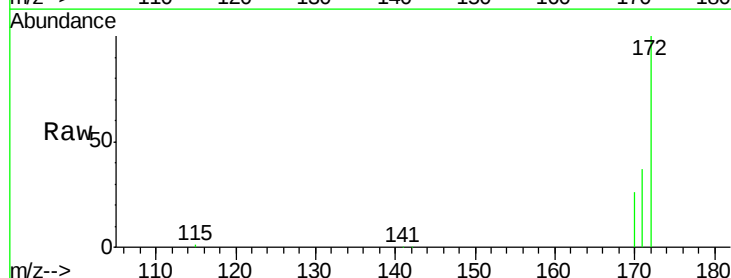


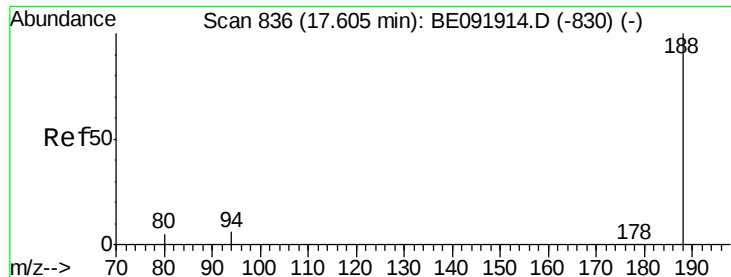




#24
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.61 min Scan# 836
Delta R.T. -0.00 min
Lab File: BE091927.D
Acq: 15 Jun 2016 16:28

Instrument :
BNA_E
ClientSampleId :
PB91035BL

Tgt Ion:188 Resp: 158485
Ion Ratio Lower Upper
188 100
94 5.6 4.1 6.1
80 4.9 3.4 5.2

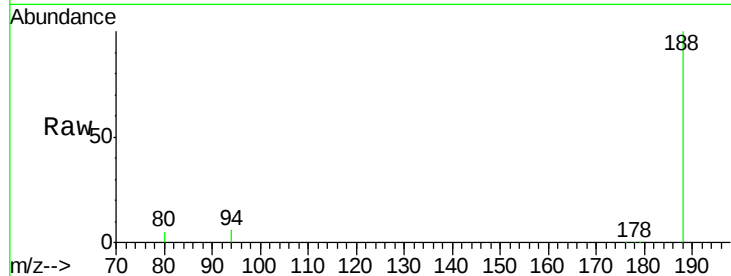


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

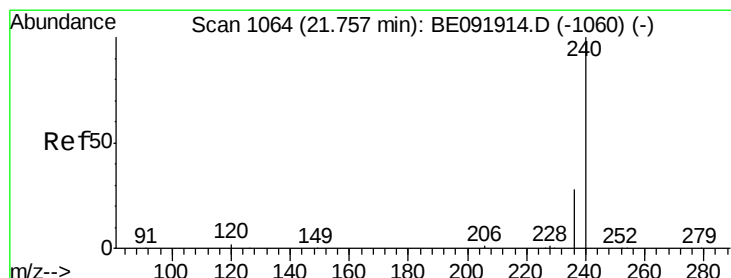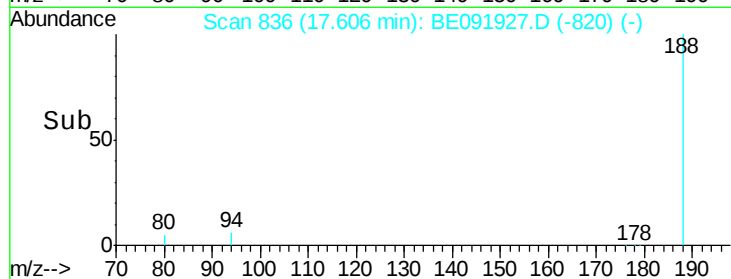
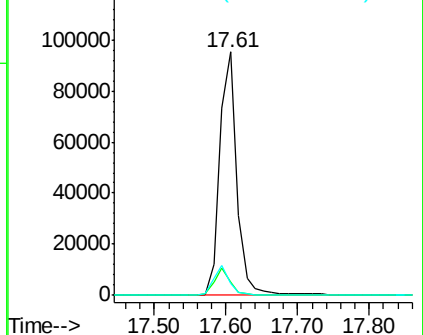



#31
Chrysene-d12
Concen: 5.00 ng
RT: 21.76 min Scan# 1064
Delta R.T. -0.00 min
Lab File: BE091927.D
Acq: 15 Jun 2016 16:28

Tgt Ion:240 Resp: 234345
Ion Ratio Lower Upper
240 100
120 2.3 1.2 1.8#
236 28.5 19.8 29.8

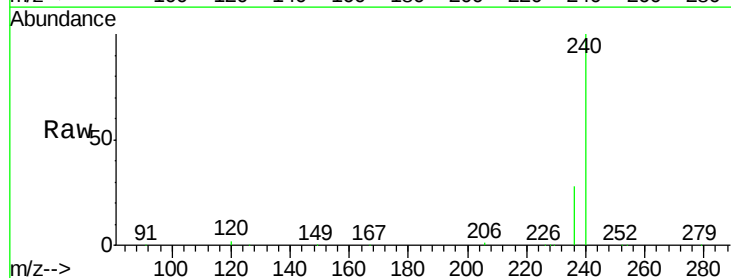

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

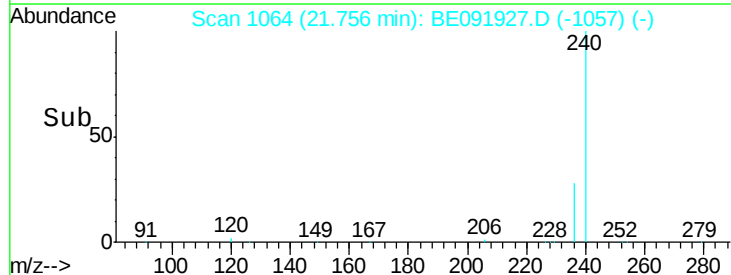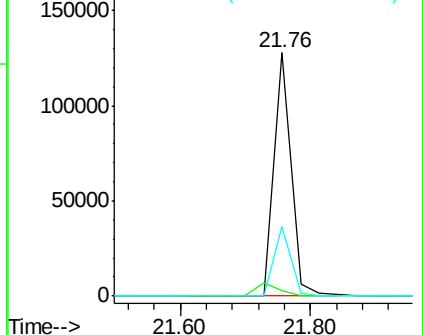

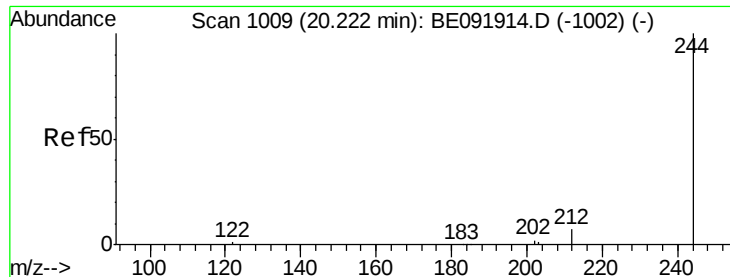

#34

Terphenyl-d14

Concen: 4.23 ng

RT: 20.22 min Scan# 1009

Delta R.T. 0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28

Instrument :

BNA_E

ClientSampleId :

PB91035BL


Tgt Ion:244 Resp: 121449

Ion Ratio Lower Upper

244 100

212 7.0 6.5 9.7




122 0.9 2.9 4.3#

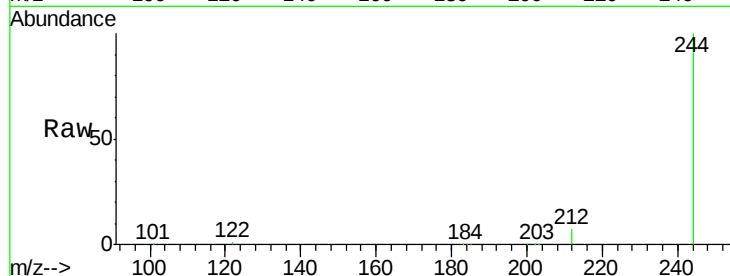

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

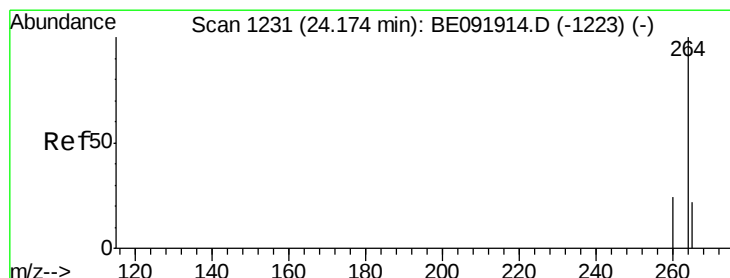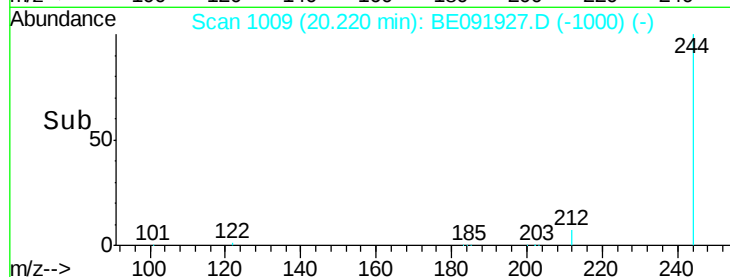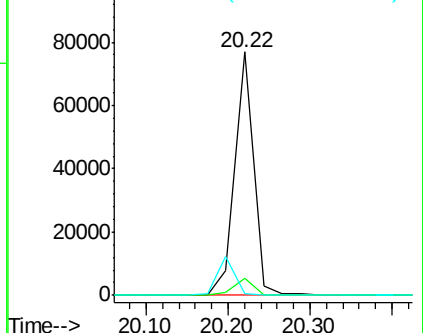

#40

Perylene-d12

Concen: 5.00 ng

RT: 24.17 min Scan# 1232

Delta R.T. -0.00 min

Lab File: BE091927.D

Acq: 15 Jun 2016 16:28


Tgt Ion:264 Resp: 176923

Ion Ratio Lower Upper

264 100

260 23.6 20.3 30.5

265 22.5 17.6 26.4

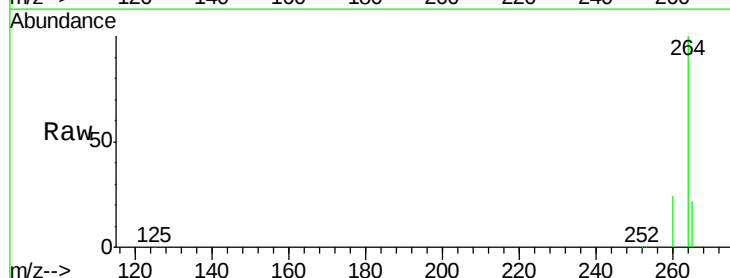

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

