


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061516\
 Data File : BE091918.D
 Acq On : 15 Jun 2016 10:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 15 12:00:38 2016

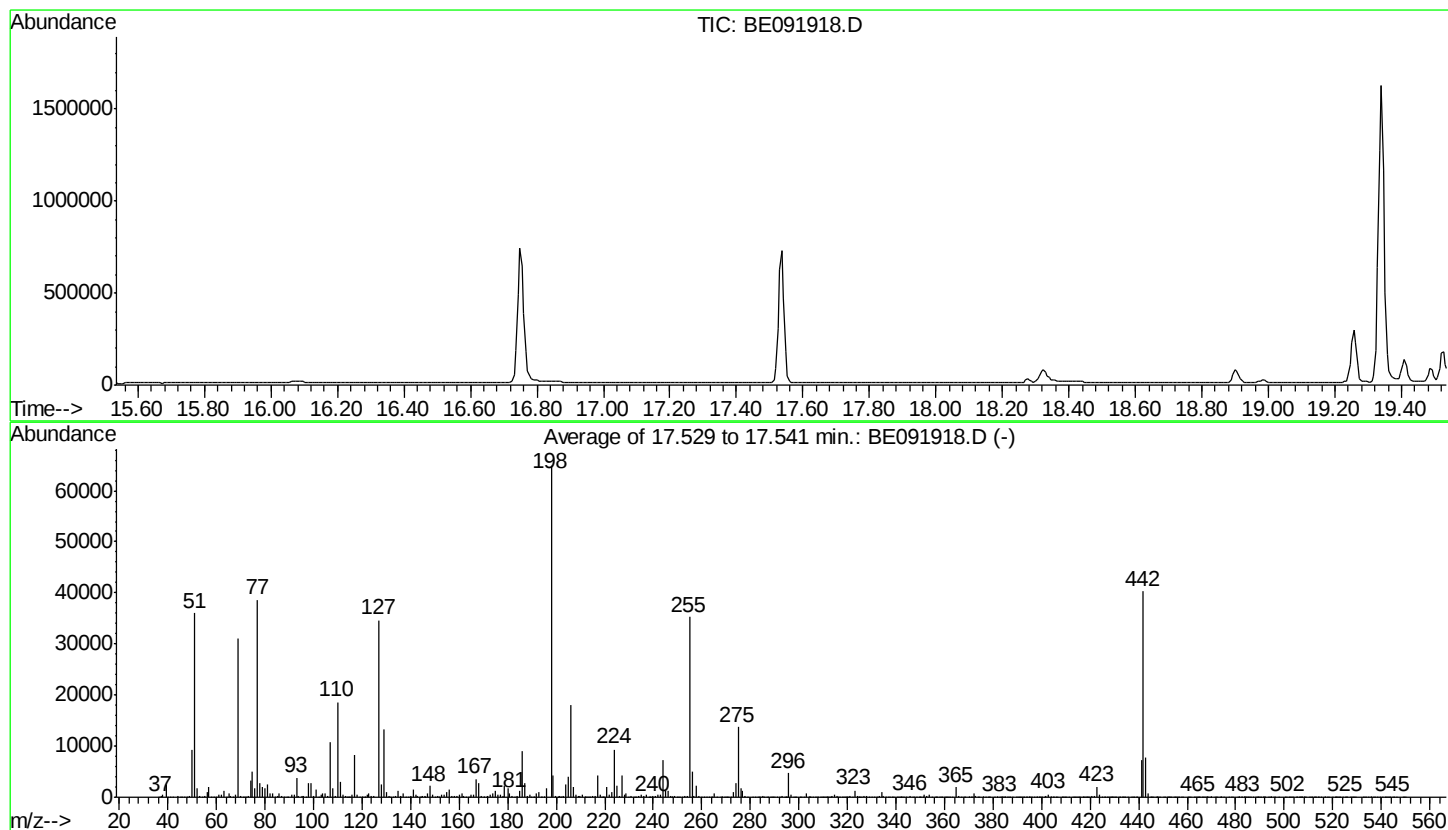

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2532

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	35972	PASS
68	69	0.00	2	1.6	494	PASS
69	198	0.00	100	48.0	31165	PASS
70	69	0.00	2	0.6	202	PASS
127	198	10	80	53.3	34623	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64904	PASS
199	198	5	9	6.7	4378	PASS
275	198	10	60	21.1	13708	PASS
365	198	1	100	2.9	1913	PASS
441	442	0.01	24	17.9	7198	PASS
442	198	50	100	62.0	40236	PASS
443	442	15	24	19.2	7741	PASS