

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061517\
 Data File : BE093213.D
 Acq On : 15 Jun 2017 18:05
 Operator : SJ/MA
 Sample : I3520-19DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 16 04:44:01 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 04:43:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2628	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	14089	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	8721	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	20406	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	21196	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	19341	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1012	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	2661	0.05	ng/ul	0.00
Target Compounds				Ovalue		
3) Naphthalene	10.57	128	3418	0.10	ng/ul#	95
5) 2-Methylnaphthalene	12.18	142	814	0.03	ng/ul	96
7) Acenaphthylene	14.09	152	10518	0.28	ng/ul	96
8) Acenaphthene	14.43	153	606	0.02	ng/ul	95
9) Fluorene	15.42	166	514	0.01	ng/ul#	87
12) Phenanthrene	17.13	178	6290	0.11	ng/ul#	86
13) Anthracene	17.22	178	15311	0.31	ng/ul#	86
15) Fluoranthene	19.16	202	35136	0.51	ng/ul	83
17) Pyrene	19.52	202	53937	0.86	ng/ul#	83
18) Benzo(a)anthracene	21.24	228	36592	0.65	ng/ul#	84
19) Chrysene	21.30	228	47312	0.81	ng/ul	98
21) Benzo(b)fluoranthene	22.94	252	133526	2.27	ng/ul	87
22) Benzo(k)fluoranthene	23.12	252	15852	0.25	ng/ul	93
23) Benzo(a)pyrene	23.56	252	50952	0.92	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	26.18	276	40076	0.62	ng/ul#	86
25) Dibenzo(a,h)anthracene	26.20	278	10381	0.19	ng/ul#	85
26) Benzo(a,h,i)perylene	26.96	276	33889	0.61	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061517\
Data File : BE093213.D
Acq On : 15 Jun 2017 18:05
Operator : SJ/MA
Sample : I3520-19DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 16 04:44:01 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 04:43:11 2017
Response via : Initial Calibration

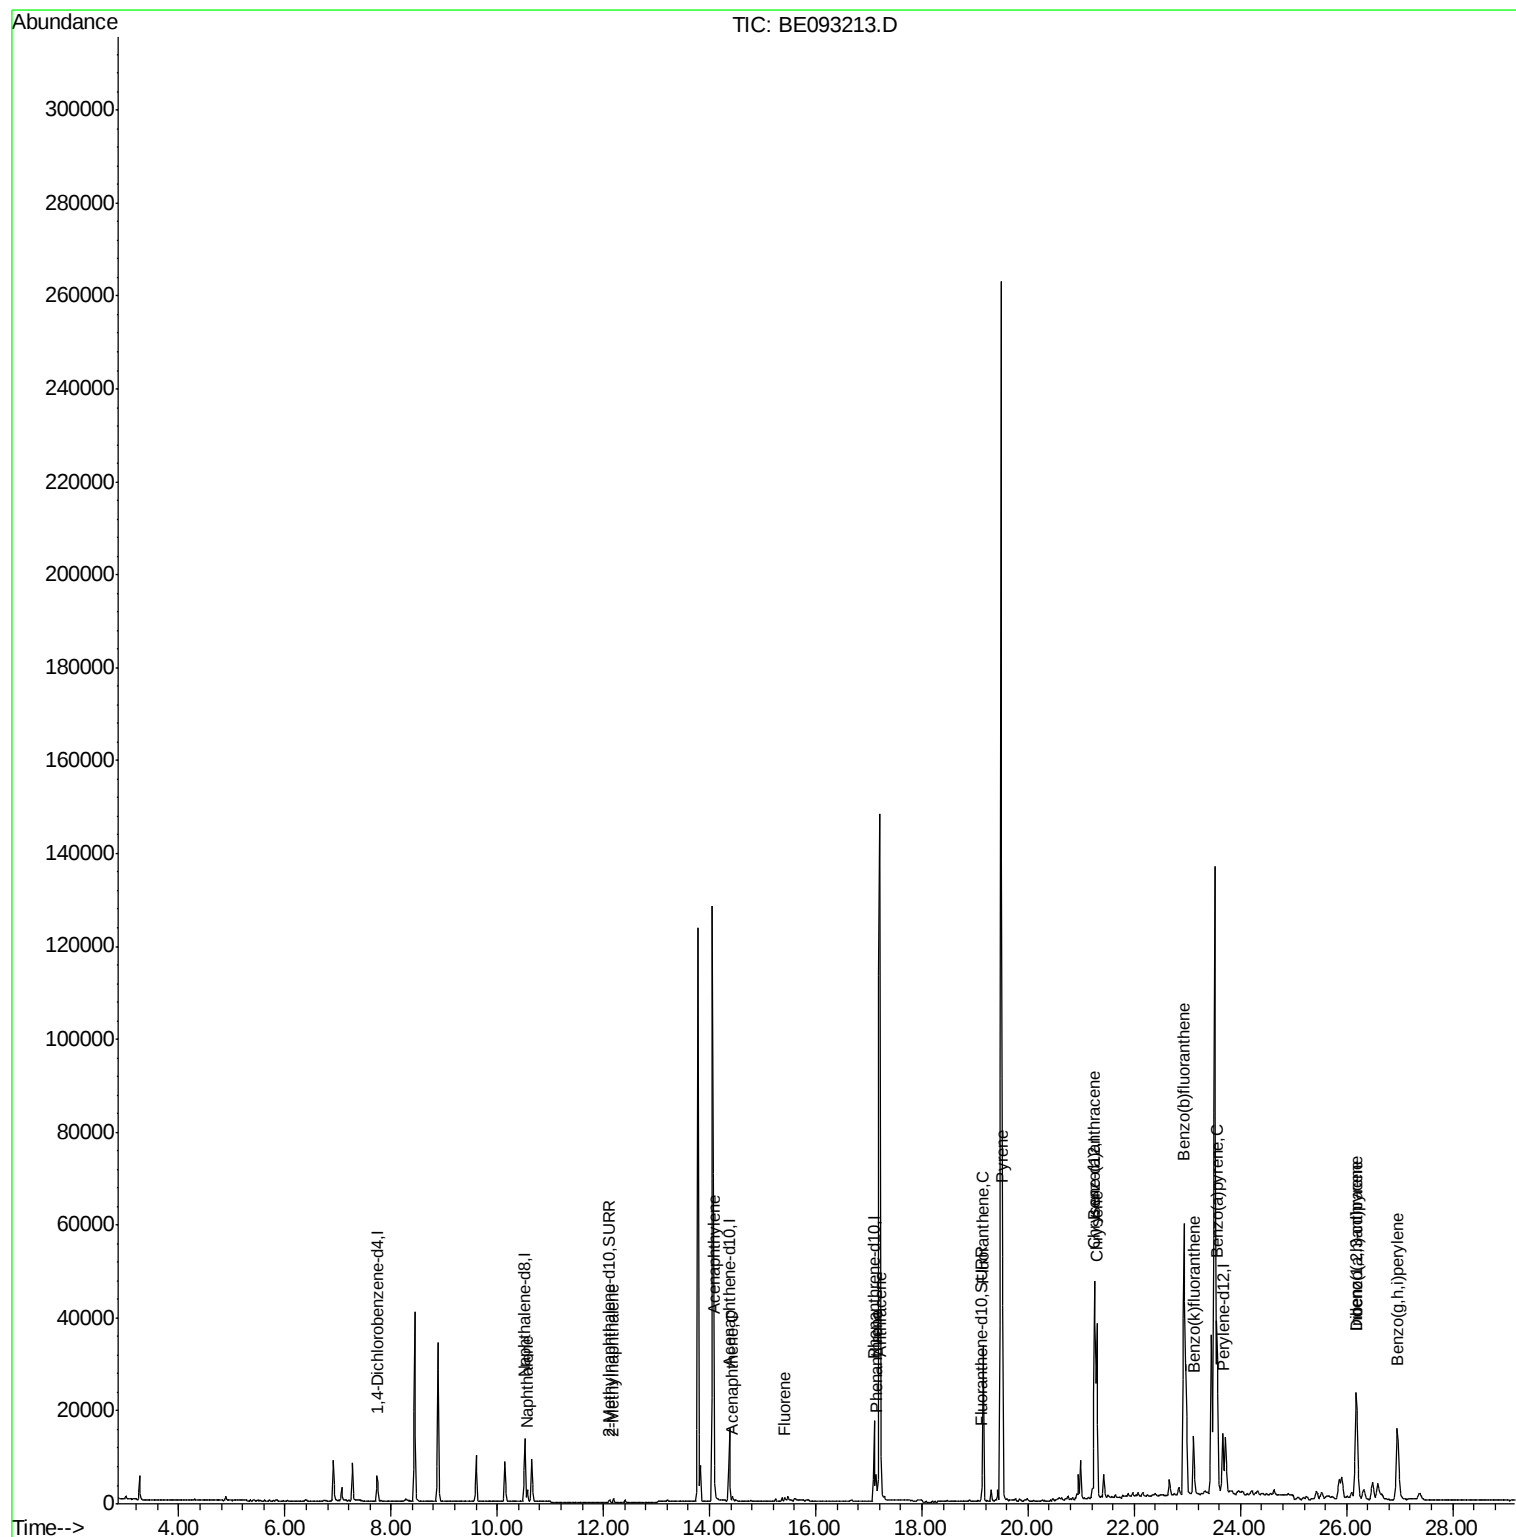

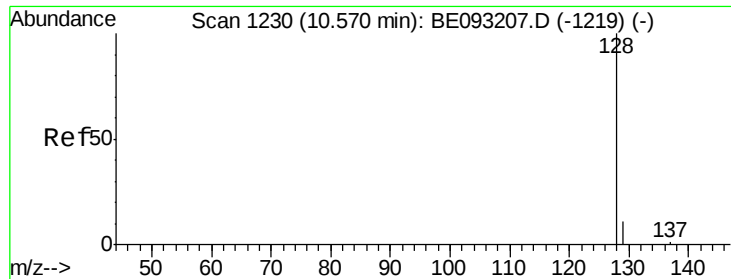

#3

Naphthalene

Concen: 0.10 ng/ul

RT: 10.57 min Scan# 1230

Delta R.T. -0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 3418

Ion Ratio Lower Upper

128 100

129 13.6 11.3 16.9




127 0.0 4.0 6.0#

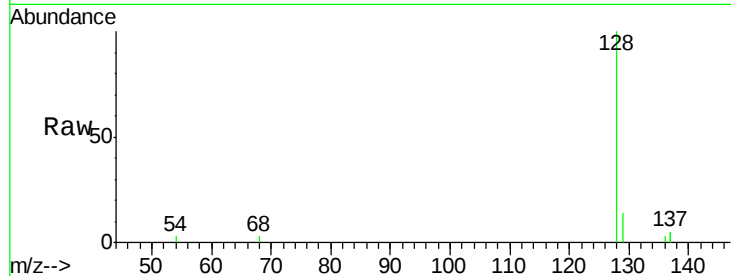

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

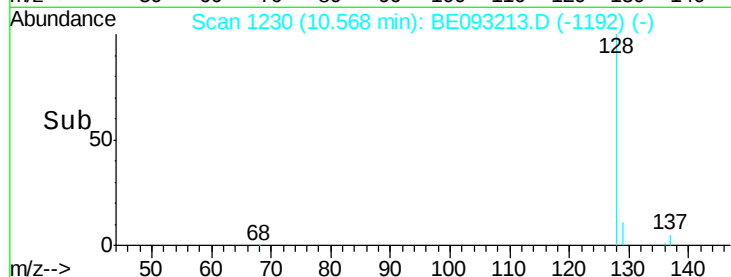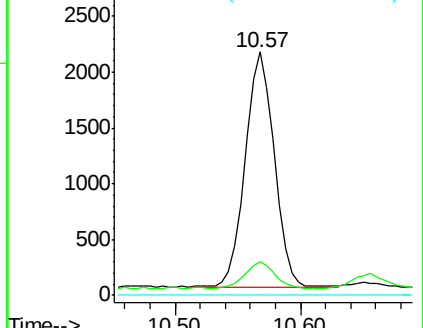

#5

2-Methylnaphthalene

Concen: 0.03 ng/ul

RT: 12.18 min Scan# 1695

Delta R.T. -0.00 min

Lab File: BE093213.D


Acq: 15 Jun 2017 18:05

Tgt Ion:142 Resp: 814

Ion Ratio Lower Upper



142 100


141 86.6 72.6 108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

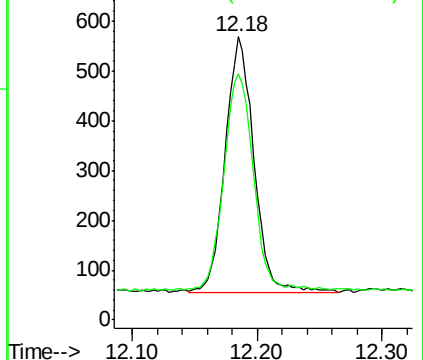

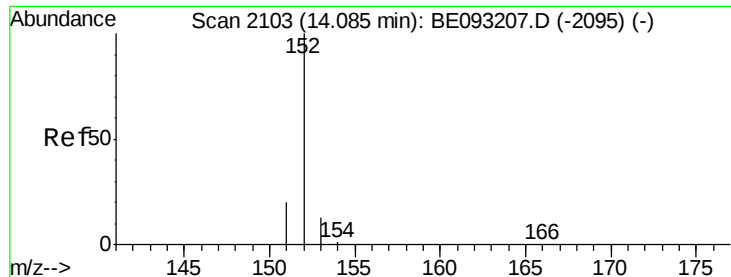

#7

Acenaphthylene

Concen: 0.28 ng/ul

RT: 14.09 min Scan# 2103

Delta R.T. 0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :





Tot Ion:152 Resp: 10518

Ion Ratio Lower Upper

152 100

151 20.0 17.1 25.7

153 13.6 12.8 19.2

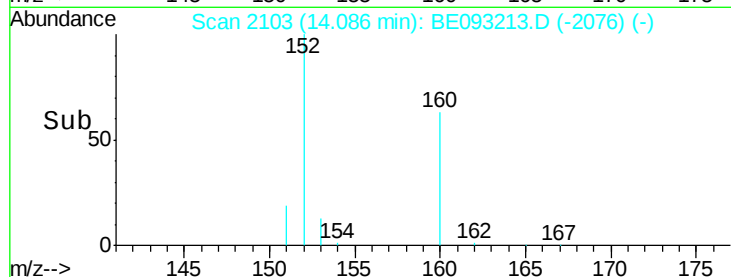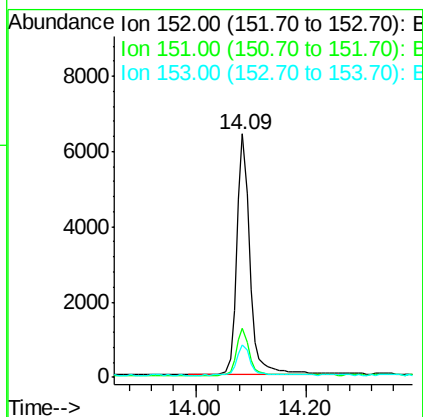

#8

Acenaphthene

Concen: 0.02 ng/ul

RT: 14.43 min Scan# 2149

Delta R.T. 0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05




Tgt Ion:153 Resp: 606


Ion Ratio Lower Upper

153 100

152 59.9 40.3 60.5

154 89.0 71.4 107.2

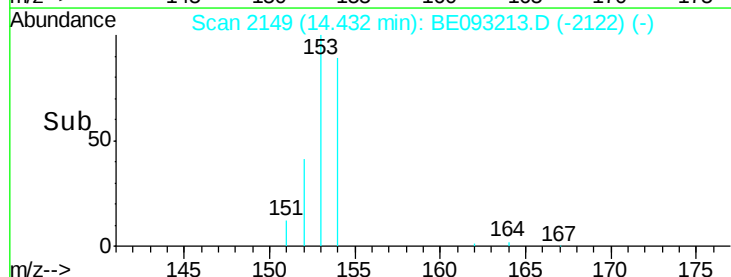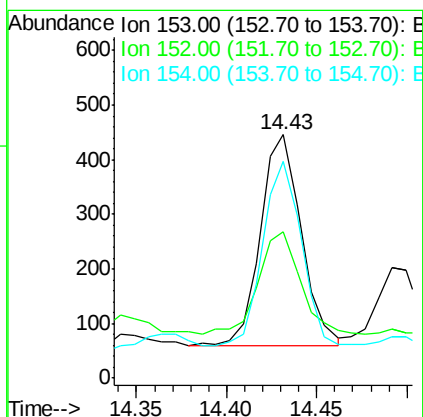

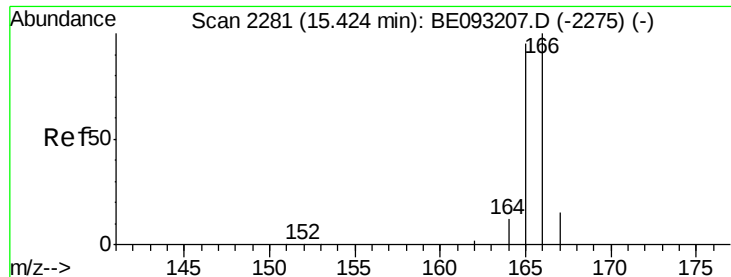

#9

Fluorene

Concen: 0.01 ng/ul

RT: 15.42 min Scan# 2280

Delta R.T. -0.01 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 514

Ion Ratio Lower Upper

166 100

165 101.8 73.4 110.2

167 29.4 14.6 22.0#

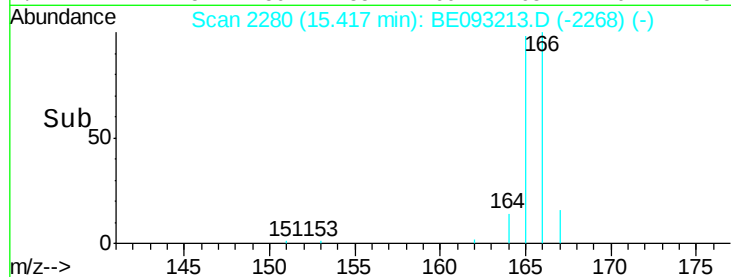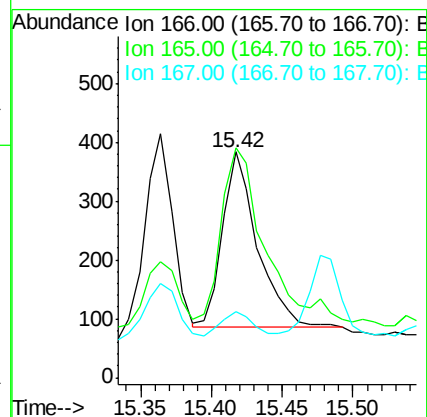

#12

Phenanthrene

Concen: 0.11 ng/ul

RT: 17.13 min Scan# 2422

Delta R.T. -0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05




Tgt Ion:178 Resp: 6290


Ion Ratio Lower Upper

178 100

179 15.5 18.4 27.6#

176 21.7 13.6 20.4#

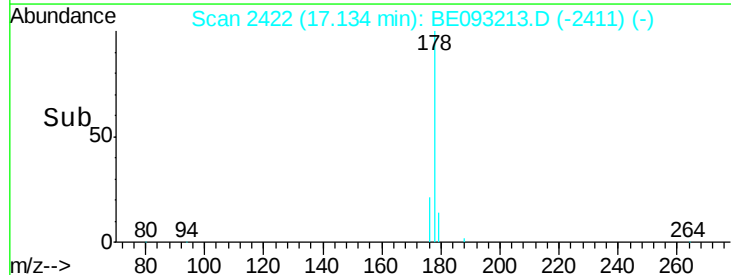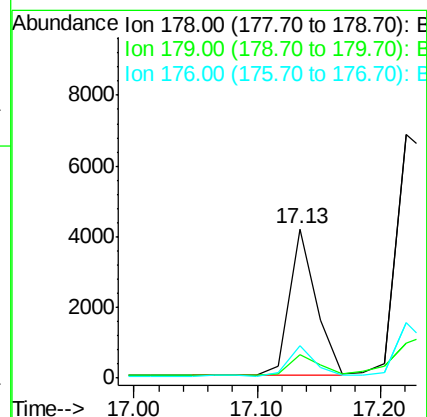



#13

Anthracene

Concen: 0.31 ng/ul

RT: 17.22 min Scan# 2427

Delta R.T. -0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 15311

Ion Ratio Lower Upper

178 100

179 14.3 18.1 27.1#




176 22.7 14.7 22.1#



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

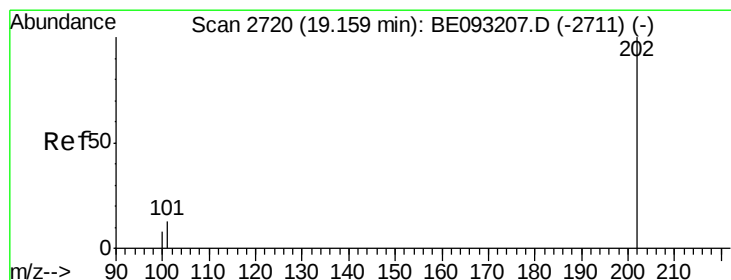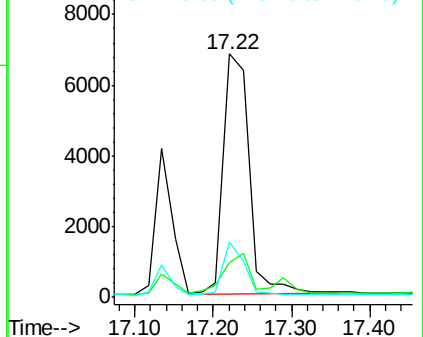

#15

Fluoranthene

Concen: 0.51 ng/ul

RT: 19.16 min Scan# 2720

Delta R.T. -0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05


Tgt Ion:202 Resp: 35136

Ion Ratio Lower Upper

202 100

101 13.5 0.0 30.3



100 10.0 0.0 39.5




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E



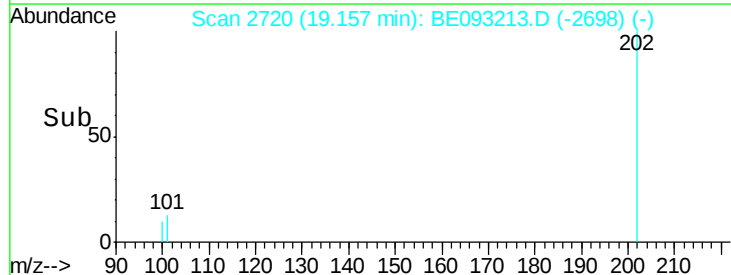
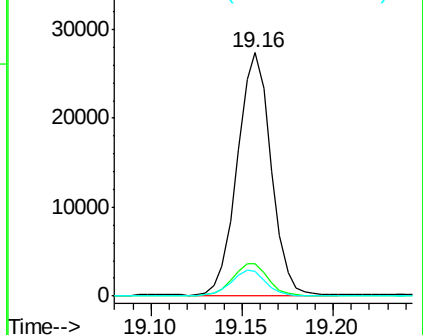


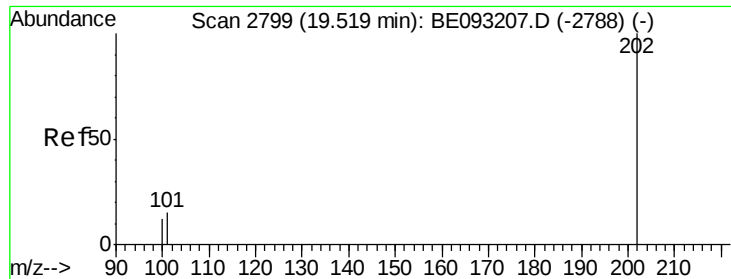

#17
Pvrene
Concen: 0.86 ng/ul
RT: 19.52 min Scan# 2799
Delta R.T. -0.00 min
Lab File: BE093213.D
Acq: 15 Jun 2017 18:05




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 53937
Ion Ratio Lower Upper
202 100
101 14.7 18.2 27.4#
100 11.9 15.6 23.4#

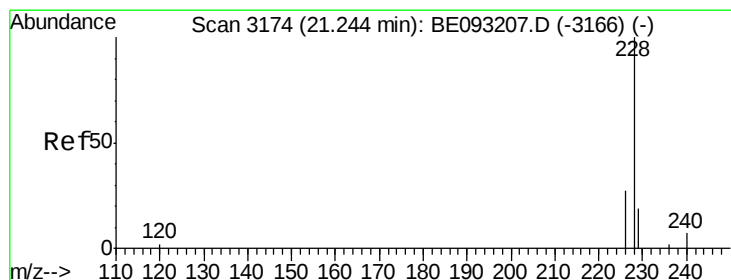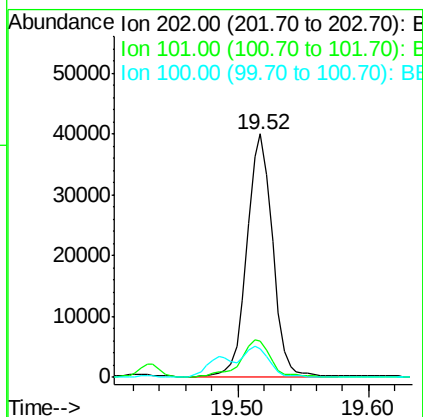

#18
Benzo(a)anthracene
Concen: 0.65 ng/ul
RT: 21.24 min Scan# 3175
Delta R.T. 0.00 min
Lab File: BE093213.D
Acq: 15 Jun 2017 18:05

Tgt Ion:228 Resp: 36592
Ion Ratio Lower Upper
228 100
229 21.2 22.8 34.2#
226 29.7 17.0 25.6#

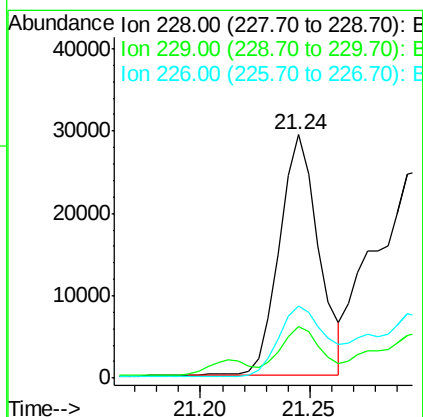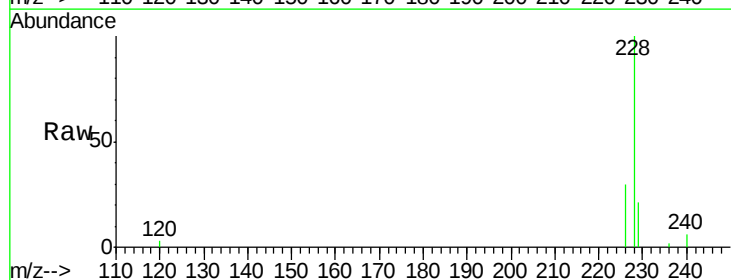

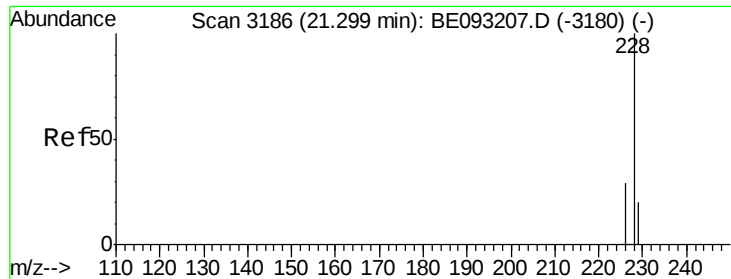

#19

Chrysene

Concen: 0.81 ng/ul

RT: 21.30 min Scan# 3187

Delta R.T. 0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 47312

Ion Ratio Lower Upper

228 100

226 30.3 23.4 35.0




229 21.6 17.7 26.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

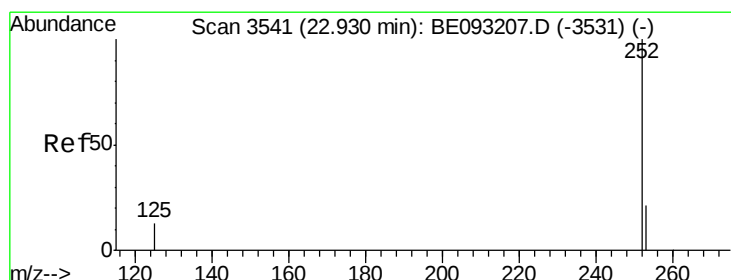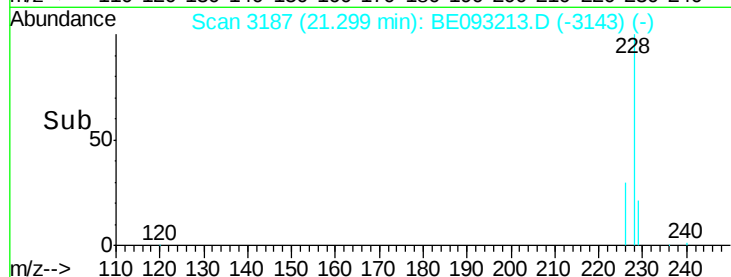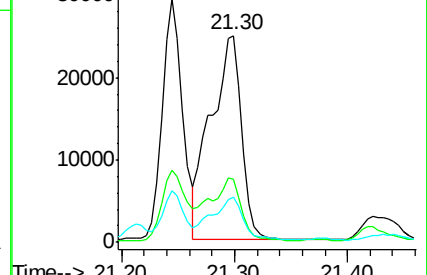

#21

Benzo(b)fluoranthene

Concen: 2.27 ng/ul

RT: 22.94 min Scan# 3543

Delta R.T. 0.01 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05


Tgt Ion:252 Resp: 133526

Ion Ratio Lower Upper

252 100

253 22.6 0.0 64.2



125 14.4 0.0 35.0

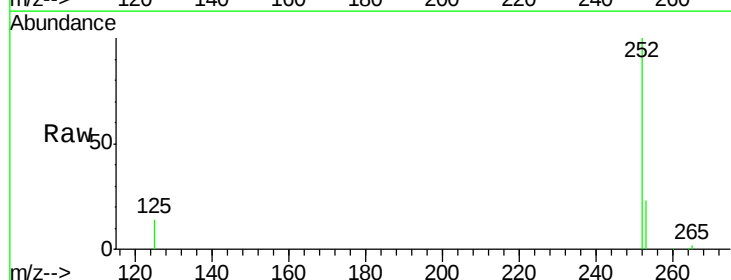


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

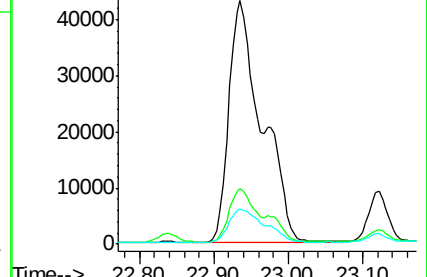

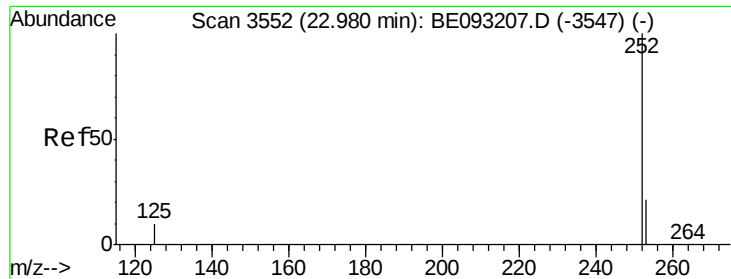

#22

Benzo(k)fluoranthene

Concen: 0.25 ng/ul

RT: 23.12 min Scan# 3584

Delta R.T. 0.14 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 15852

Ion Ratio Lower Upper

252 100

253 26.5 24.5 36.7




125 19.5 13.7 20.5

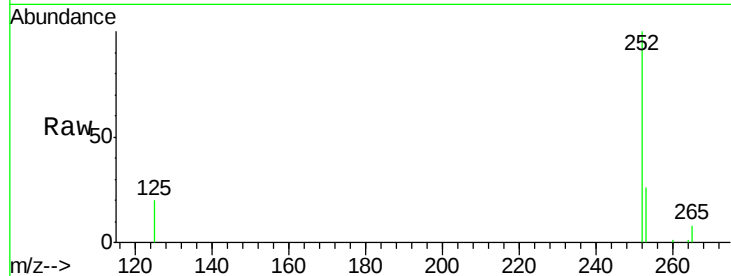

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

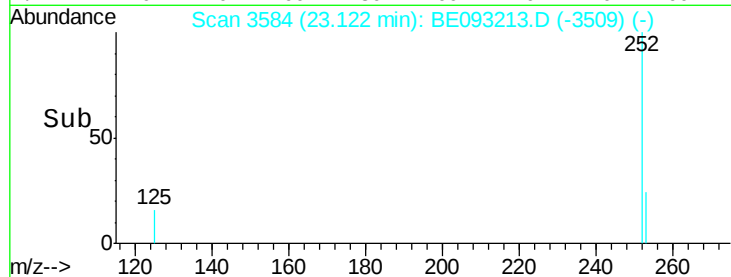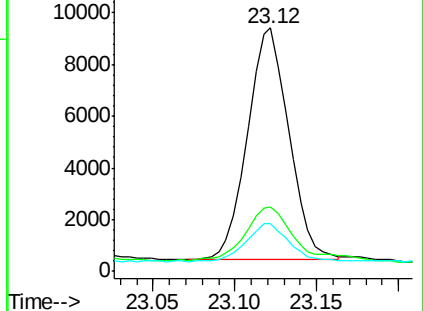

#23

Benzo(a)pyrene

Concen: 0.92 ng/ul

RT: 23.56 min Scan# 3680

Delta R.T. 0.00 min

Lab File: BE093213.D

Acq: 15 Jun 2017 18:05


Tgt Ion:252 Resp: 50952

Ion Ratio Lower Upper

252 100

253 23.5 28.5 42.7#



125 15.5 18.1 27.1#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




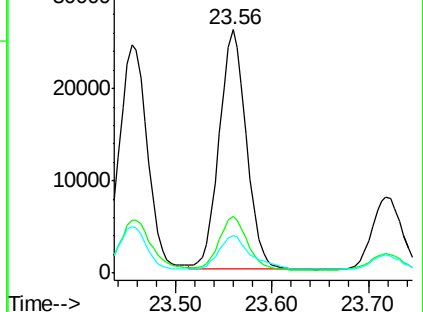




#24
 Indeno(1,2,3-cd)pyrene
 Concen: 0.62 ng/ul
 RT: 26.18 min Scan# 4252
 Delta R.T. -0.01 min
 Lab File: BE093213.D
 Acq: 15 Jun 2017 18:05




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:276 Resp: 40076
 Ion Ratio Lower Upper
 276 100
 138 28.8 28.0 42.0
 227 0.0 8.0 12.0#

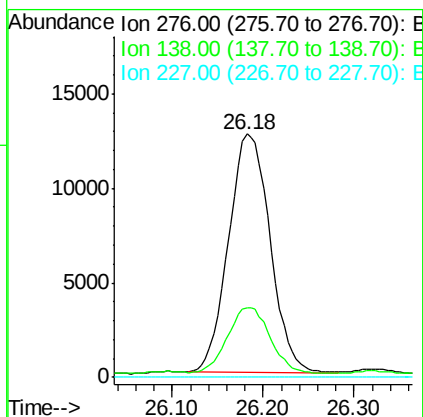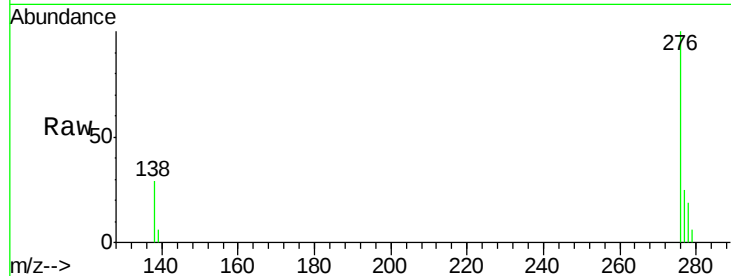

#25
 Dibenzo(a,h)anthracene
 Concen: 0.19 ng/ul
 RT: 26.20 min Scan# 4256
 Delta R.T. -0.01 min
 Lab File: BE093213.D
 Acq: 15 Jun 2017 18:05

Tgt Ion:278 Resp: 10381
 Ion Ratio Lower Upper
 278 100
 139 32.3 17.4 26.0#
 279 26.8 25.9 38.9

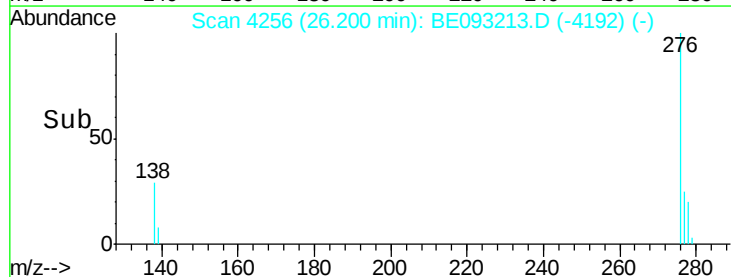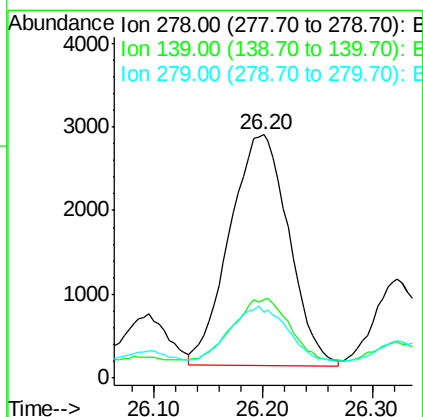


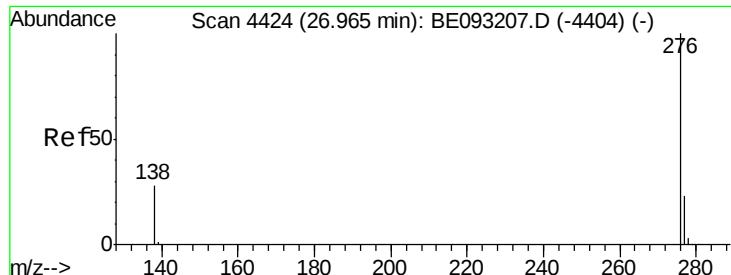

#26
 Benzo(a,h,i)perylene
 Concen: 0.61 ng/ul
 RT: 26.96 min Scan# 4423
 Delta R.T. -0.00 min
 Lab File: BE093213.D
 Acq: 15 Jun 2017 18:05

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	28.5	21.8	32.8
277	24.1	20.5	30.7

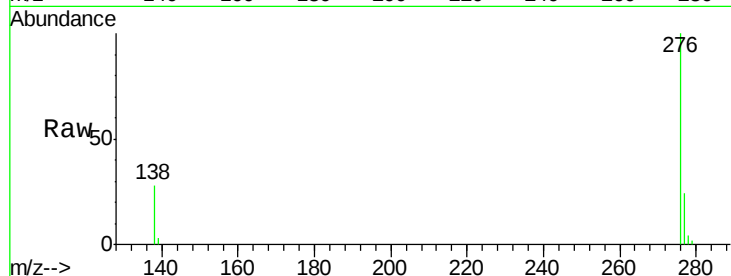

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

