

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061517\
 Data File : BE093225.D
 Acq On : 16 Jun 2017 1:27
 Operator : SJ/MA
 Sample : I3521-02DL 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 16 05:37:23 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 16 05:36:31 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	3021	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	16124	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	9488	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	22437	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	24132	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	19521	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	1251	0.05	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	3346	0.05	ng/ul	0.00
Target Compounds					Ovalue	
3) Naphthalene	10.57	128	6451	0.16	ng/ul#	93
5) 2-Methylnaphthalene	12.18	142	1604	0.06	ng/ul	99
7) Acenaphthylene	14.09	152	40538	1.00	ng/ul	95
8) Acenaphthene	14.43	153	1342	0.04	ng/ul#	94
9) Fluorene	15.42	166	1668	0.04	ng/ul	90
12) Phenanthrene	17.14	178	22117	0.36	ng/ul#	89
13) Anthracene	17.22	178	62063	1.15	ng/ul#	87
15) Fluoranthene	19.16	202	283672	3.75	ng/ul	83
17) Pyrene	19.52	202	431674	6.07	ng/ul#	83
18) Benzo(a)anthracene	21.24	228	262191	4.07	ng/ul#	84
19) Chrysene	21.30	228	290872	4.36	ng/ul	99
21) Benzo(b)fluoranthene	22.93	252	762347	12.87	ng/ul	86
22) Benzo(k)fluoranthene	23.12	252	71722	1.14	ng/ul	95
23) Benzo(a)pyrene	23.56	252	283612	5.06	ng/ul#	81
24) Indeno(1,2,3-cd)pyrene	26.19	276	178853	2.76	ng/ul#	86
25) Dibenzo(a,h)anthracene	26.20	278	46751	0.86	ng/ul	91
26) Benzo(a,h,i)perylene	26.96	276	139704	2.51	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061517\
Data File : BE093225.D
Acq On : 16 Jun 2017 1:27
Operator : SJ/MA
Sample : I3521-02DL 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 16 05:37:23 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 16 05:36:31 2017
Response via : Initial Calibration

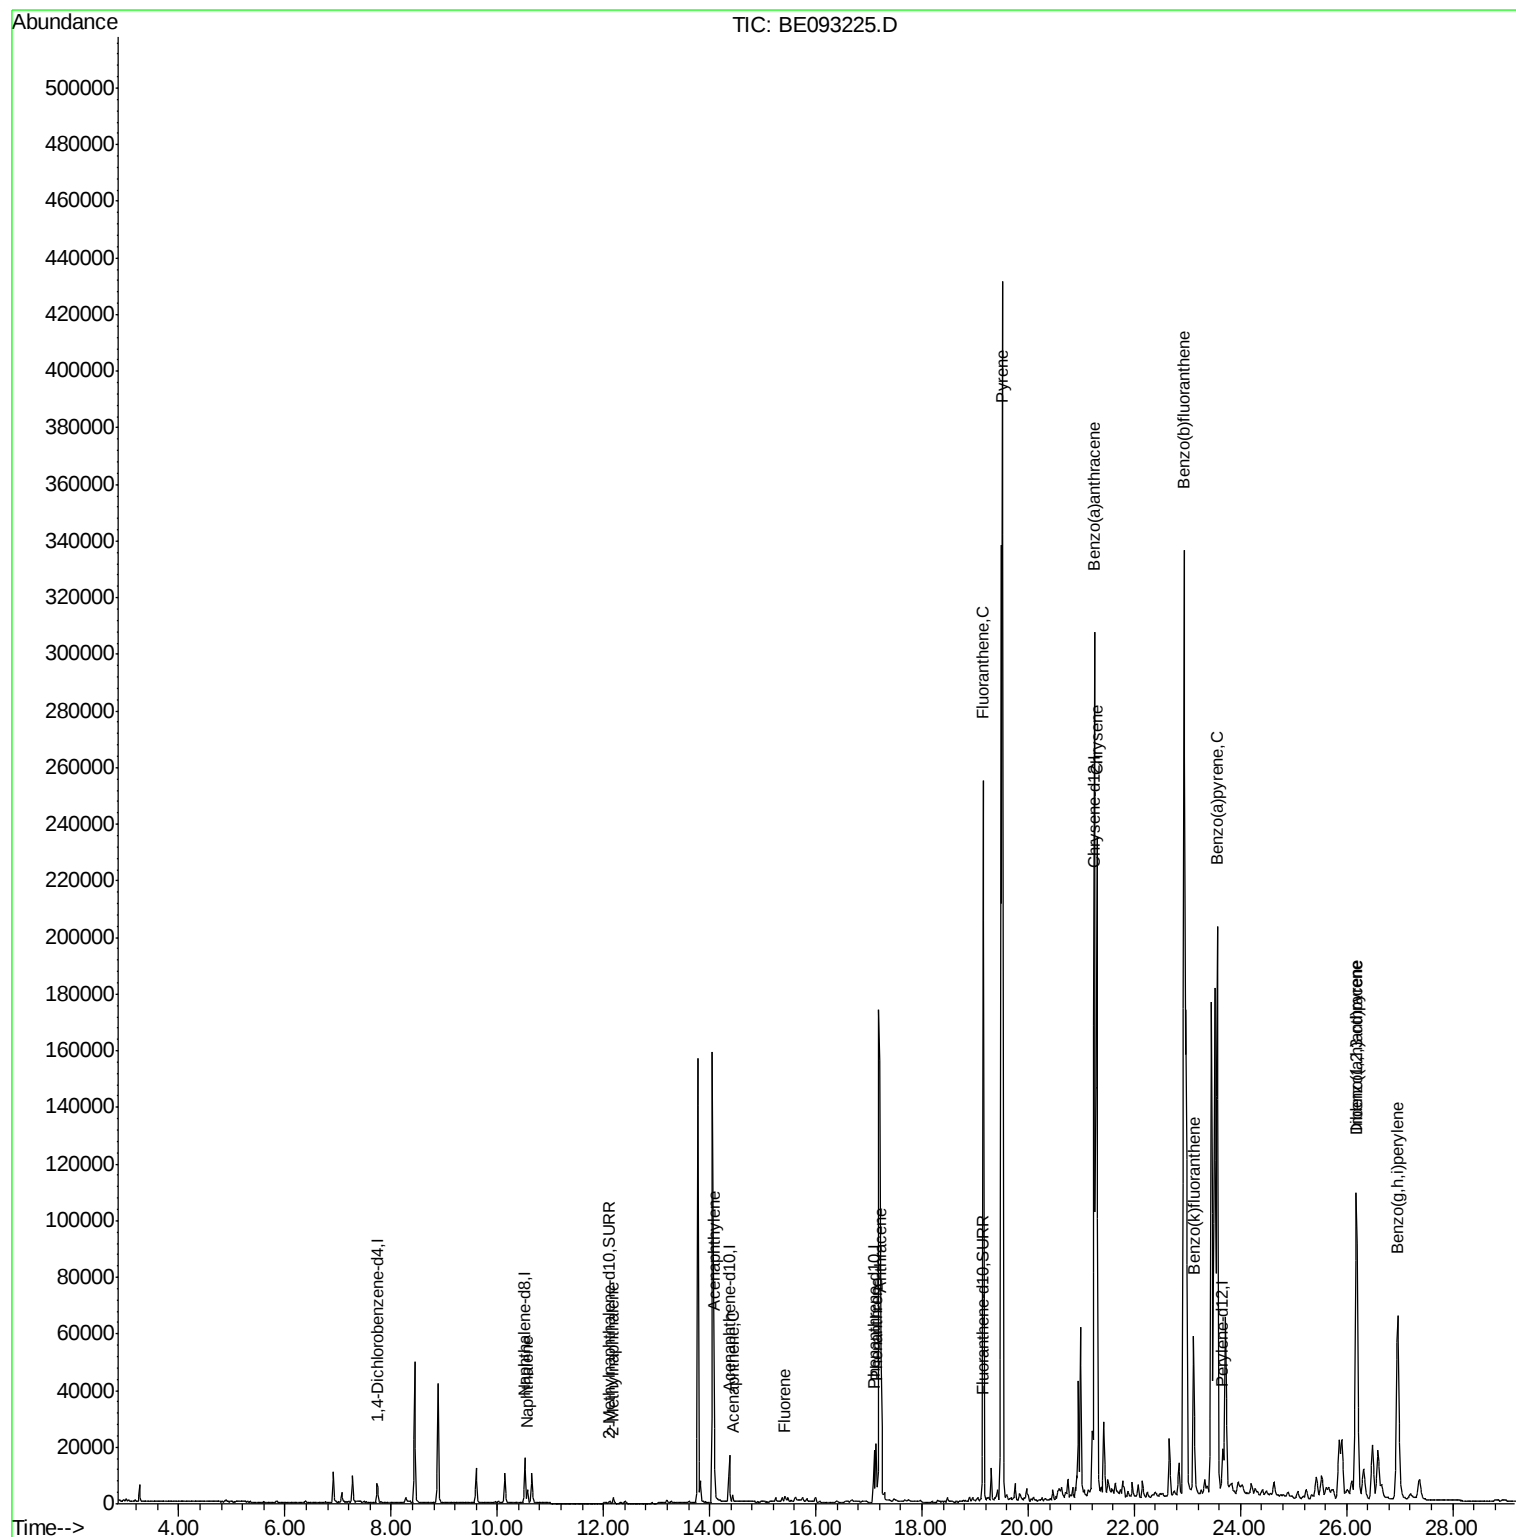



#3

Naphthalene

Concen: 0.16 ng/ul

RT: 10.57 min Scan# 1230

Delta R.T. -0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 6451

Ion Ratio Lower Upper

128 100

129 12.5 11.3 16.9




127 0.0 4.0 6.0#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

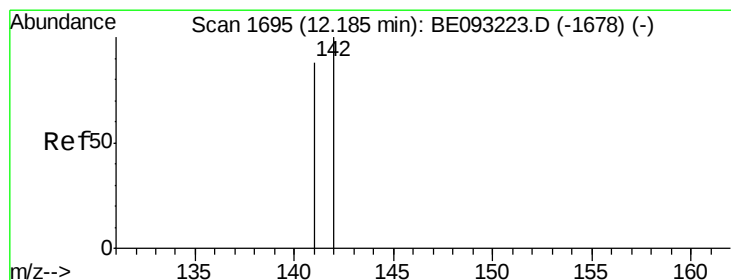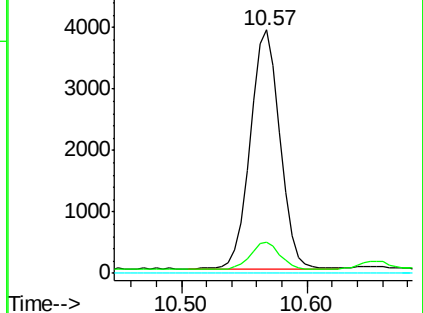

#5

2-Methylnaphthalene

Concen: 0.06 ng/ul

RT: 12.18 min Scan# 1695

Delta R.T. -0.00 min

Lab File: BE093225.D


Acq: 16 Jun 2017 1:27

Tgt Ion:142 Resp: 1604

Ion Ratio Lower Upper



142 100


141 89.5 72.6 108.8

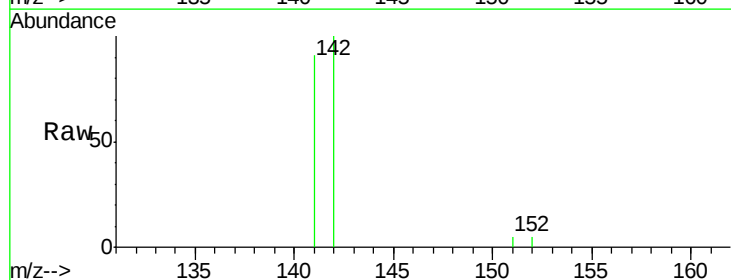

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

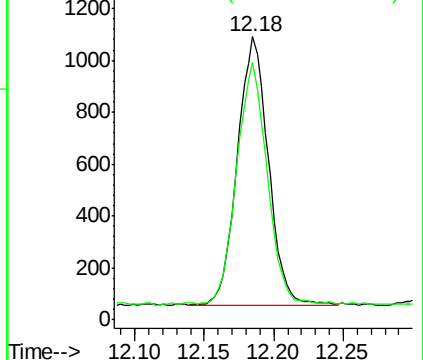

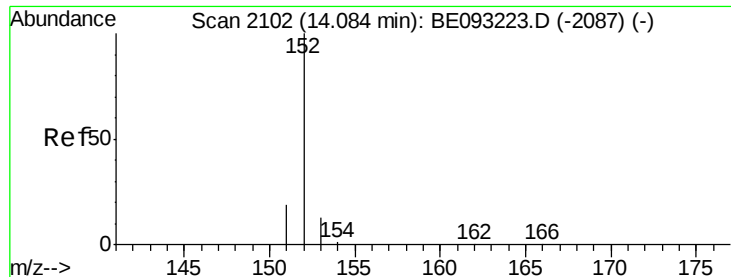

#7

Acenaphthylene

Concen: 1.00 ng/ul

RT: 14.09 min Scan# 2103

Delta R.T. 0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 40538

Ion Ratio Lower Upper

152 100

151 20.1 17.1 25.7




153 13.0 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

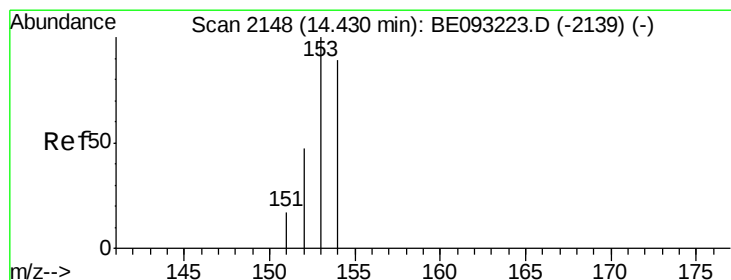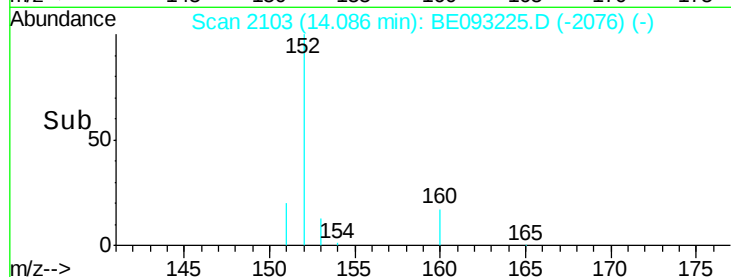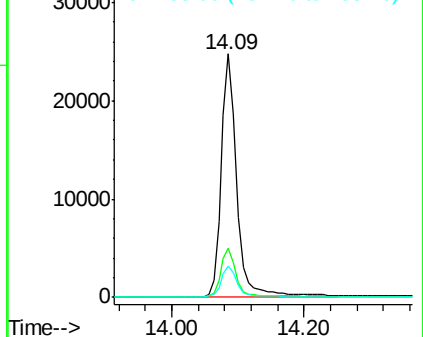

#8

Acenaphthene

Concen: 0.04 ng/ul

RT: 14.43 min Scan# 2149

Delta R.T. 0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27


Tgt Ion:153 Resp: 1342

Ion Ratio Lower Upper

153 100

152 60.9 40.3 60.5#



154 90.0 71.4 107.2




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



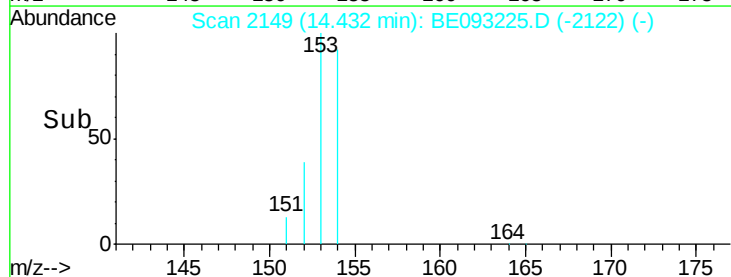
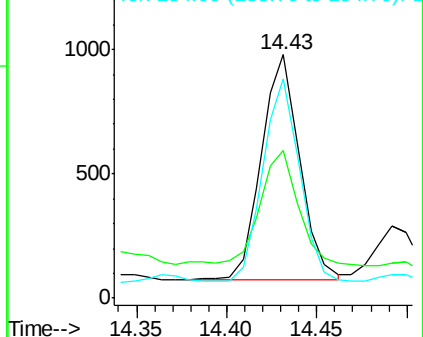


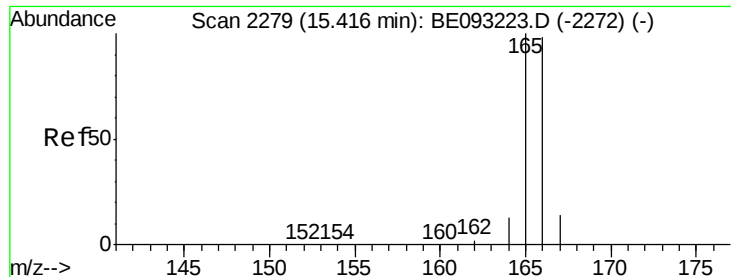

#9
Fluorene
 Concen: 0.04 ng/ul
 RT: 15.42 min Scan# 2280
 Delta R.T. 0.00 min
 Lab File: BE093225.D
 Acq: 16 Jun 2017 1:27




Instrument :
 BNA_E
 ClientSampled :


Tot Ion:166 Resp: 1668
 Ion Ratio Lower Upper
 166 100
 165 101.5 73.4 110.2
 167 21.1 14.6 22.0

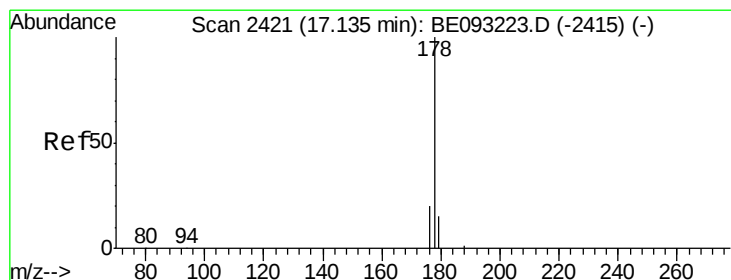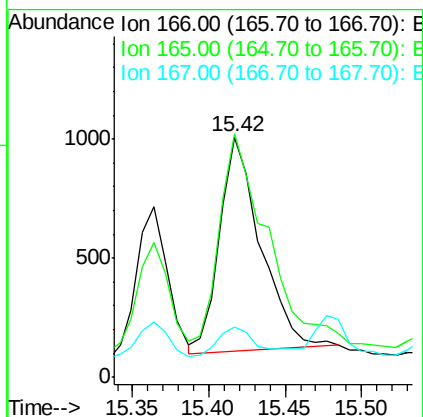

#12
Phenanthrene
 Concen: 0.36 ng/ul
 RT: 17.14 min Scan# 2422
 Delta R.T. 0.00 min
 Lab File: BE093225.D
 Acq: 16 Jun 2017 1:27

Tgt Ion:178 Resp: 22117
 Ion Ratio Lower Upper
 178 100
 179 15.4 18.4 27.6#
 176 19.5 13.6 20.4

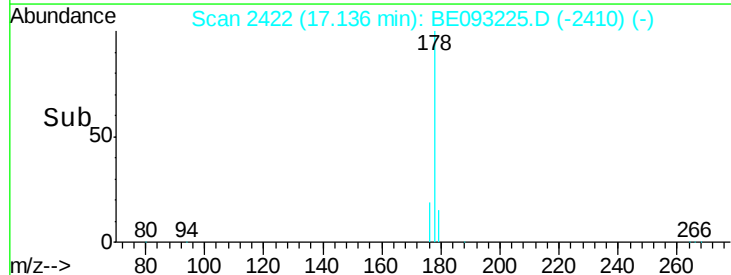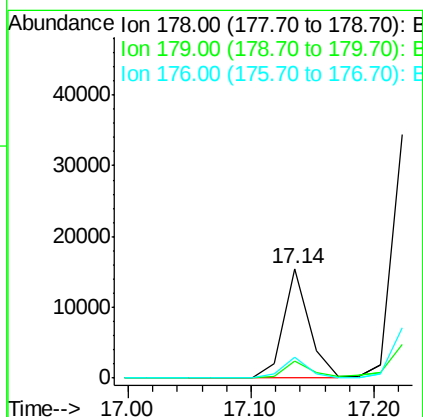

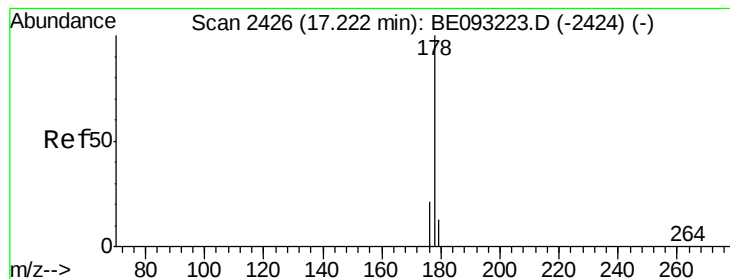

#13

Anthracene

Concen: 1.15 ng/ul

RT: 17.22 min Scan# 2427

Delta R.T. 0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 62063

Ion Ratio Lower Upper

178 100

179 13.8 18.1 27.1#




176 20.8 14.7 22.1

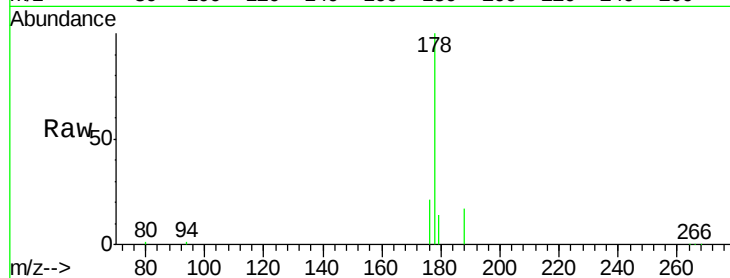

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

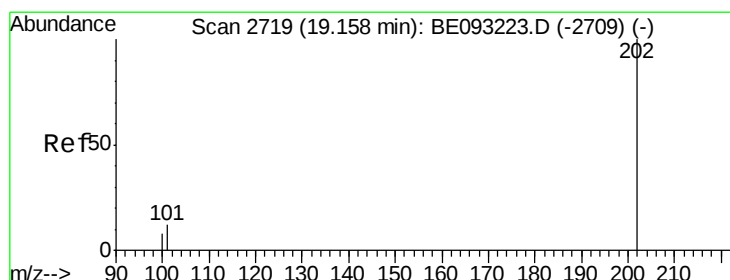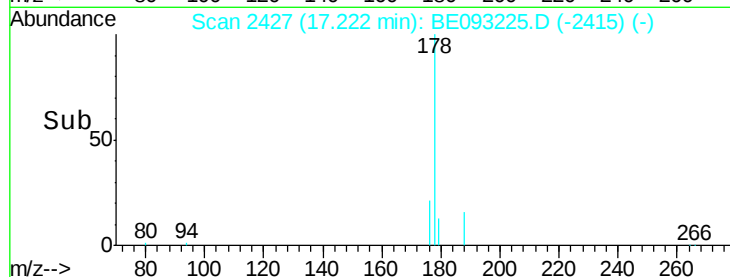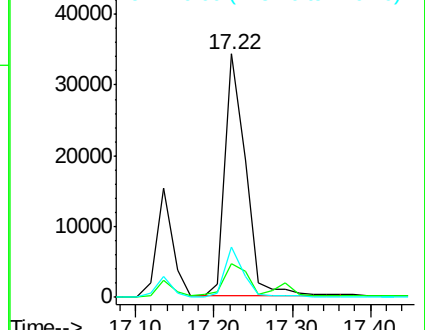

#15

Fluoranthene

Concen: 3.75 ng/ul

RT: 19.16 min Scan# 2719

Delta R.T. -0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27


Tgt Ion:202 Resp: 283672

Ion Ratio Lower Upper

202 100

101 13.0 0.0 30.3



100 9.7 0.0 39.5

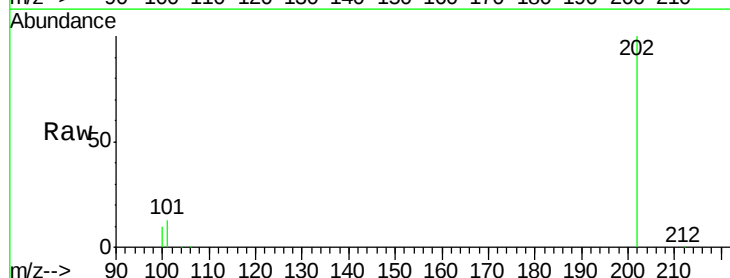


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

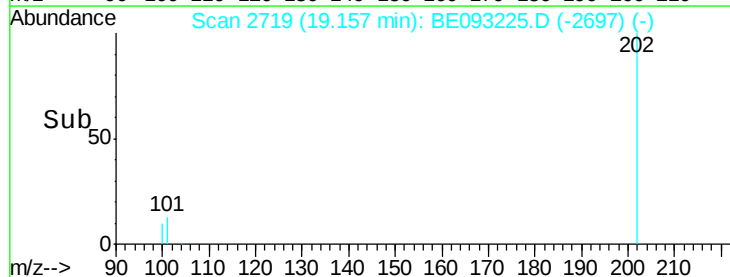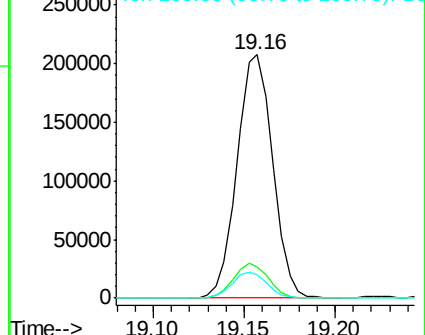

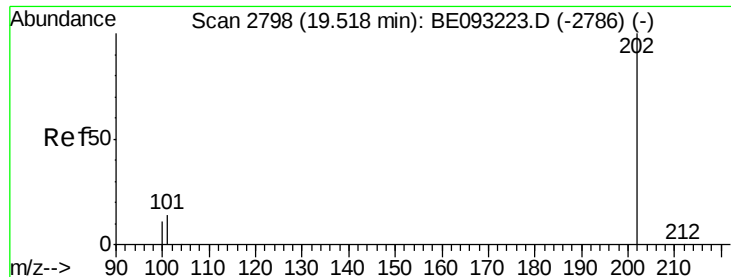

#17

Pvrene

Concen: 6.07 ng/ul

RT: 19.52 min Scan# 2798

Delta R.T. -0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 431674

Ion Ratio Lower Upper

202 100

101 14.9 18.2 27.4#




100 11.9 15.6 23.4#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

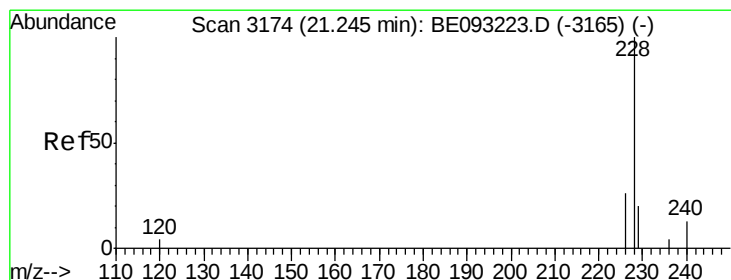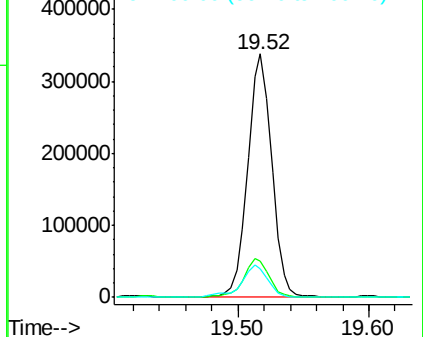

#18

Benzo(a)anthracene

Concen: 4.07 ng/ul

RT: 21.24 min Scan# 3174

Delta R.T. -0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27


Tgt Ion:228 Resp: 262191

Ion Ratio Lower Upper

228 100

229 21.2 22.8 34.2#



226 29.7 17.0 25.6#




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

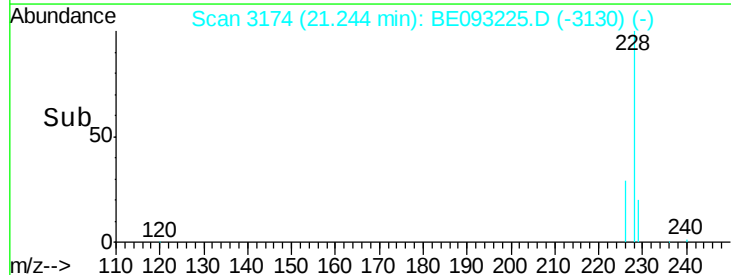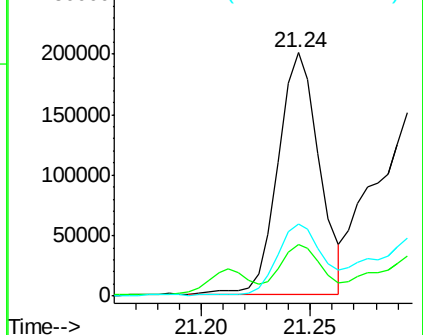



#19

Chrysene

Concen: 4.36 ng/ul

RT: 21.30 min Scan# 3186

Delta R.T. 0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 290872

Ion Ratio Lower Upper

228 100

226 30.1 23.4 35.0




229 22.2 17.7 26.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

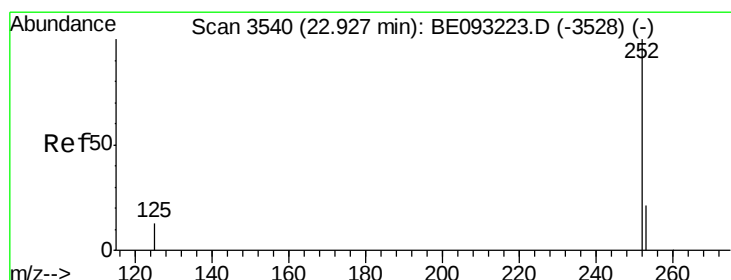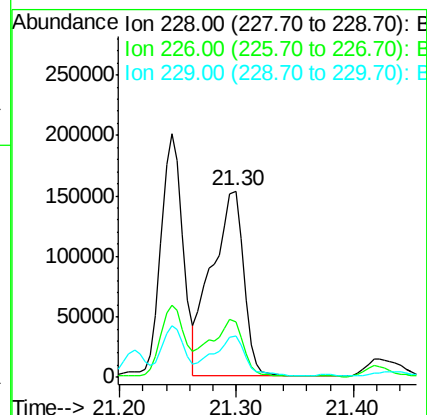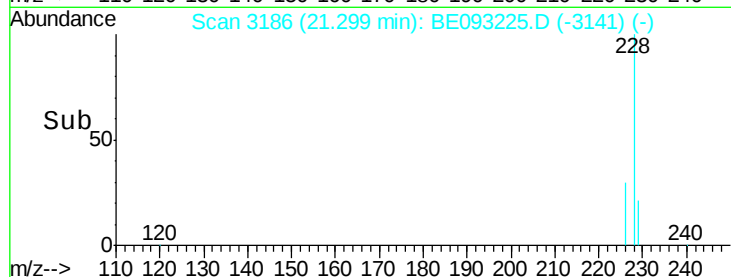

#21

Benzo(b)fluoranthene

Concen: 12.87 ng/ul

RT: 22.93 min Scan# 3542

Delta R.T. 0.01 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27


Tgt Ion:252 Resp: 762347

Ion Ratio Lower Upper

252 100

253 22.7 0.0 64.2



125 14.2 0.0 35.0

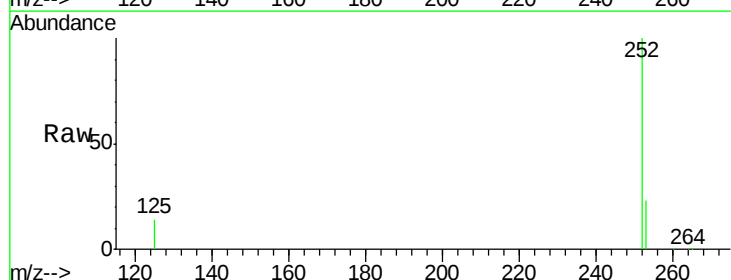


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

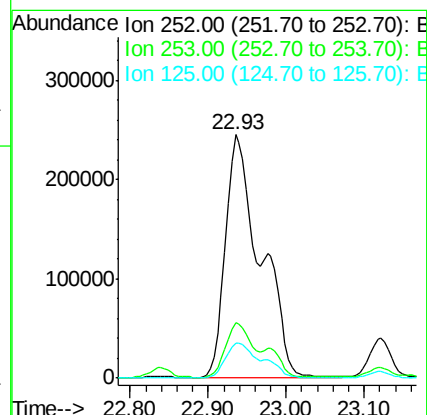



#22

Benzo(k)fluoranthene

Concen: 1.14 ng/ul

RT: 23.12 min Scan# 3583

Delta R.T. 0.14 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 71722

Ion Ratio Lower Upper




252 100

253 26.9 24.5 36.7

125 17.4 13.7 20.5

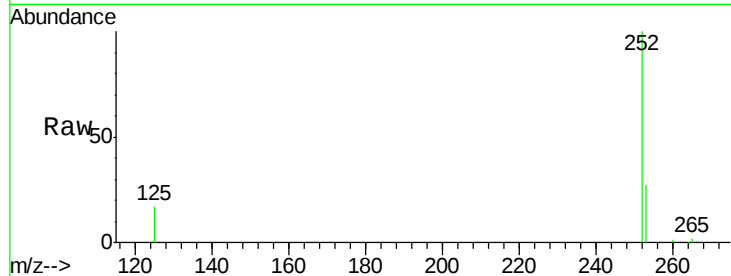

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

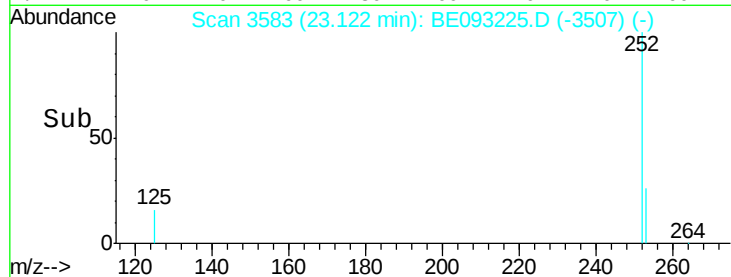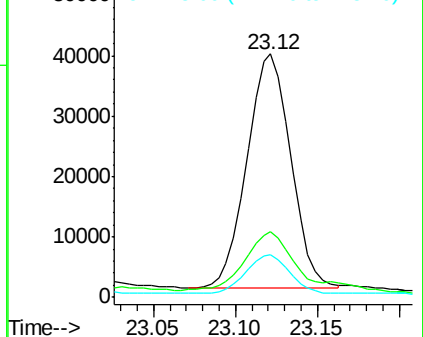

#23

Benzo(a)pyrene

Concen: 5.06 ng/ul

RT: 23.56 min Scan# 3679

Delta R.T. 0.00 min

Lab File: BE093225.D

Acq: 16 Jun 2017 1:27


Tgt Ion:252 Resp: 283612

Ion Ratio Lower Upper



252 100


253 23.2 28.5 42.7#

125 15.2 18.1 27.1#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E




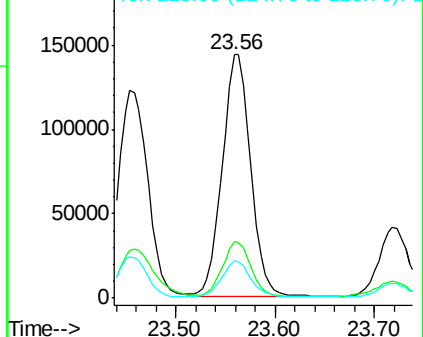




#24
 Indeno(1,2,3-cd)pyrene
 Concen: 2.76 ng/ul
 RT: 26.19 min Scan# 4252
 Delta R.T. 0.01 min
 Lab File: BE093225.D
 Acq: 16 Jun 2017 1:27




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:276 Resp: 178853
 Ion Ratio Lower Upper
 276 100
 138 29.2 28.0 42.0
 227 0.0 8.0 12.0#

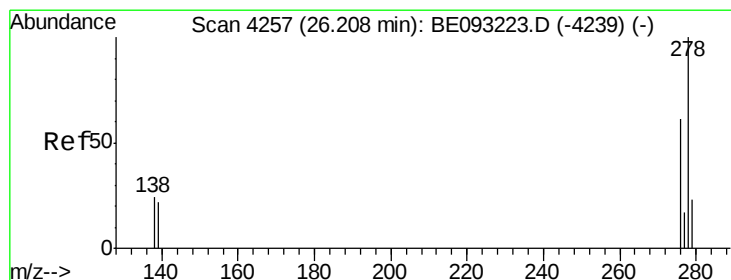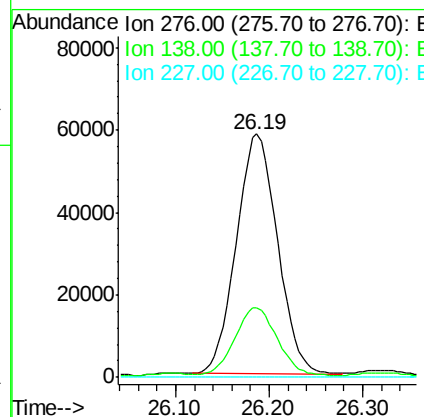

#25
 Dibenzo(a,h)anthracene
 Concen: 0.86 ng/ul
 RT: 26.20 min Scan# 4255
 Delta R.T. -0.01 min
 Lab File: BE093225.D
 Acq: 16 Jun 2017 1:27

Tgt Ion:278 Resp: 46751
 Ion Ratio Lower Upper
 278 100
 139 24.8 17.4 26.0
 279 26.8 25.9 38.9

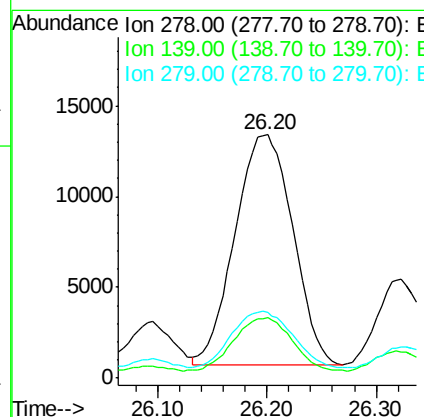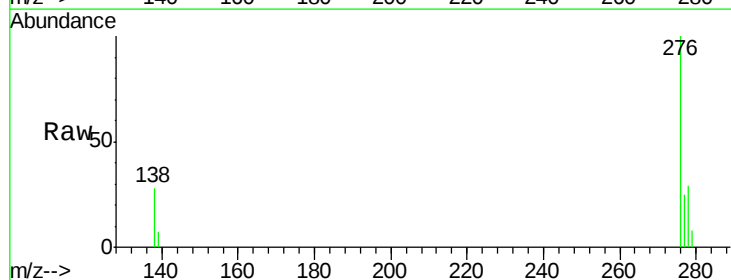


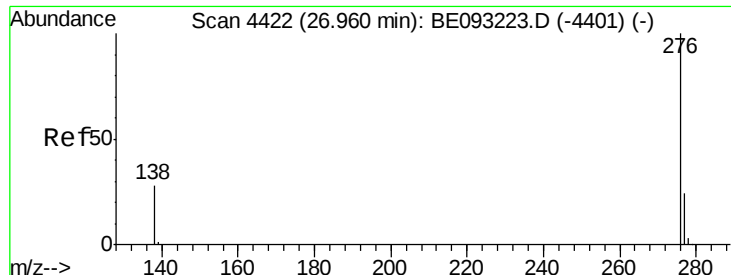

#26
 Benzo(a,h,i)perylene
 Concen: 2.51 ng/ul
 RT: 26.96 min Scan# 4422
 Delta R.T. 0.00 min
 Lab File: BE093225.D
 Acq: 16 Jun 2017 1:27

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
276	100		
138	28.8	21.8	32.8
277	24.2	20.5	30.7

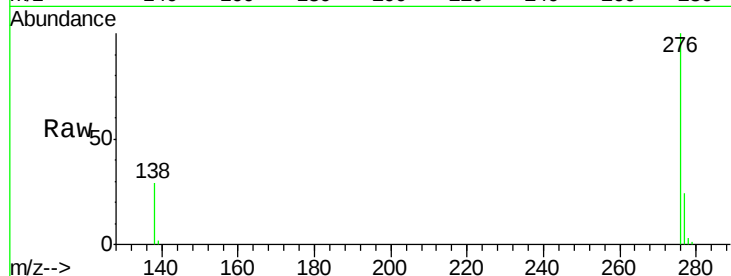

Abundance Ion 276.00 (275.70 to 276.70): E
 Ion 138.00 (137.70 to 138.70): E
 Ion 277.00 (276.70 to 277.70): E

