
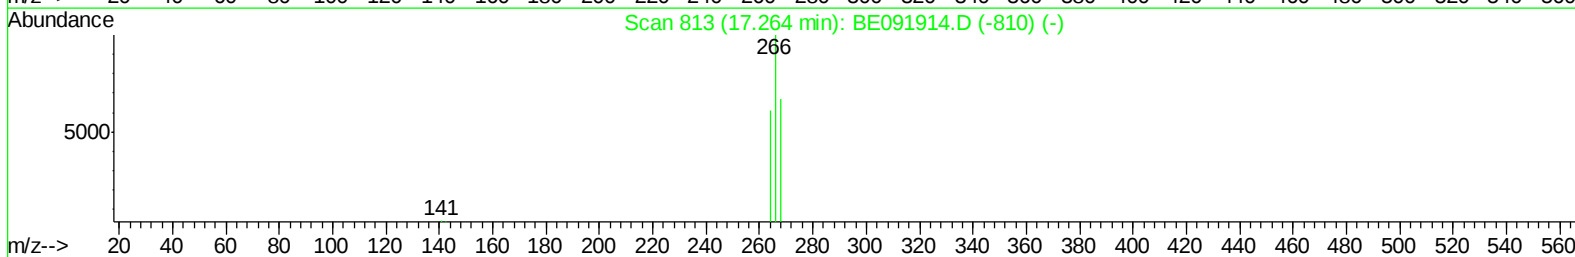
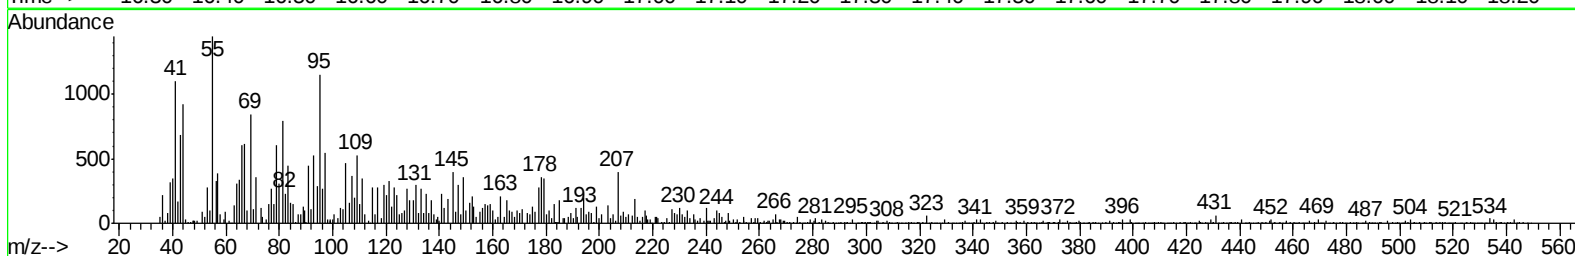


Data Path : Z:\HPCHEM1\BNA E\Data\BE061616\
 Data File : BE091934.D
 Acq On : 16 Jun 2016 10:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 18:59:23 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE061416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 15 12:00:38 2016
 Response via : Initial Calibration

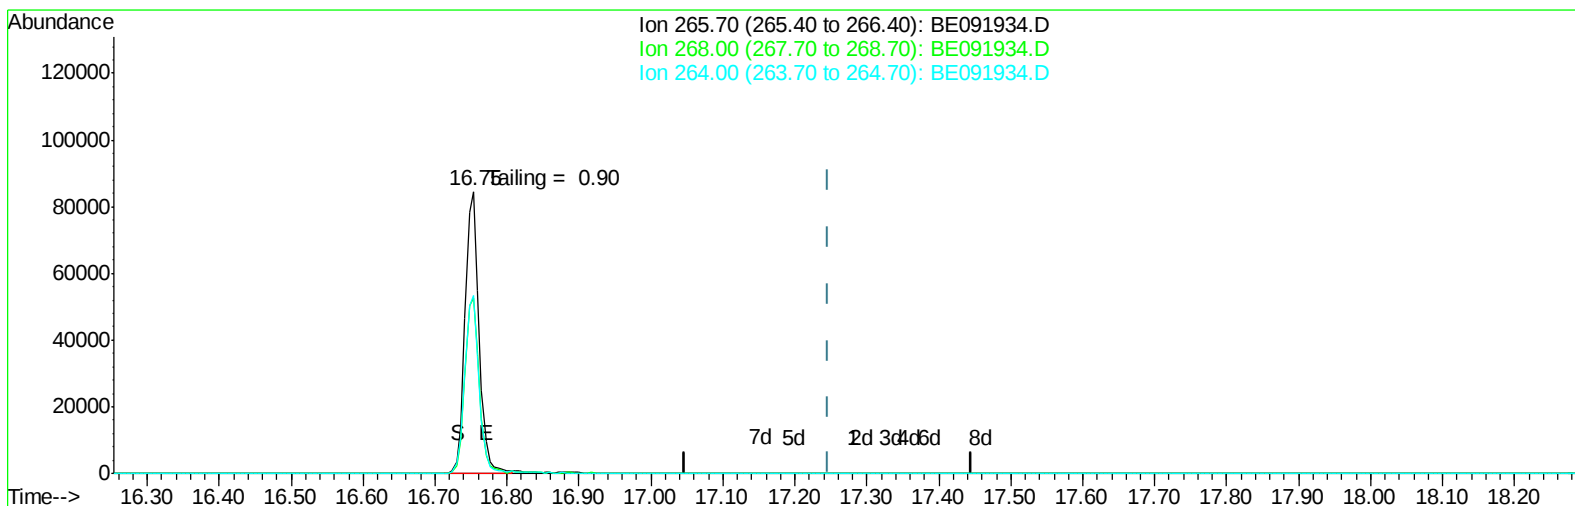

TIC: BE091934.D

(27) Pentachlorophenol




17.282min (+0.035) 24.78ng

response 62

Ion	Exp%	Act%
265.70	100	100
268.00	75.60	36.71#
264.00	63.70	31.65#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE061616\
Data File : BE091934.D
Acq On : 16 Jun 2016 10:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 16 18:59:23 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE061416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 15 12:00:38 2016
Response via : Initial Calibration

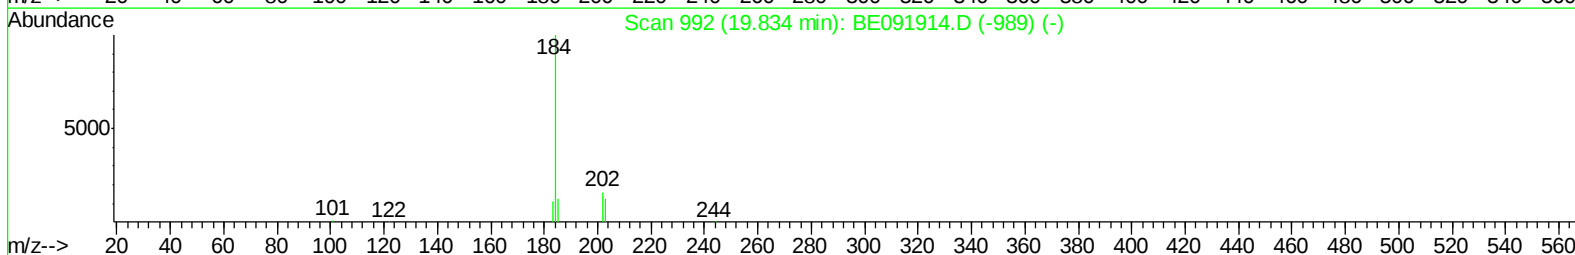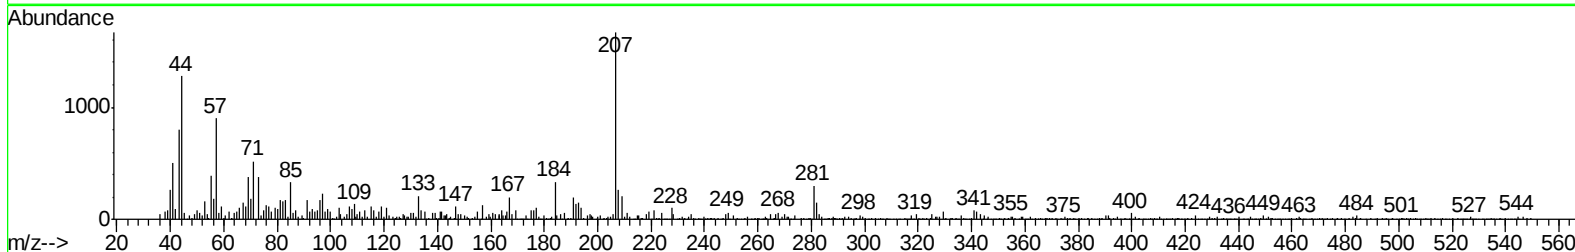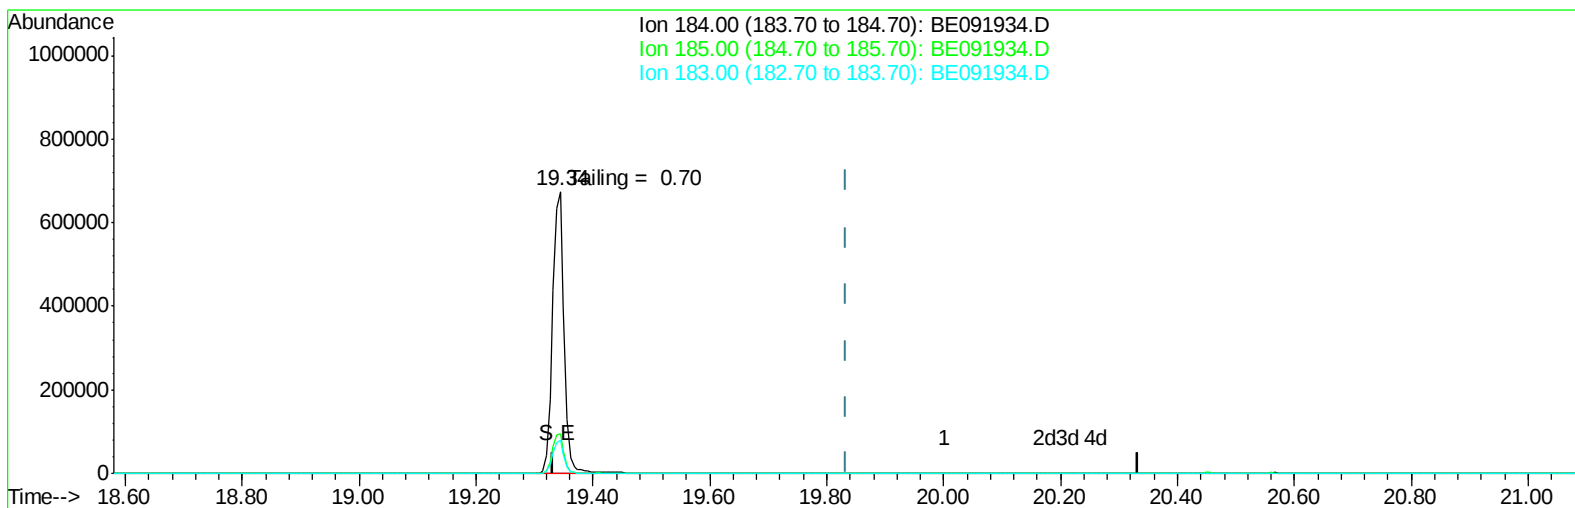

TIC: BE091934.D

(32) Benzidine

20.002min (+0.169) 45.52ng

response 252

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	9.04#
183.00	14.70	6.02#
0.00	0.00	0.00