

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093246.D
 Acq On : 19 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3599-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5A74

Quant Time: Jun 20 04:19:12 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2428	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12158	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7740	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	18232	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	1280449	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6495	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	18121	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.57	128	364	0.012	ng/ul#	57
17) Pyrene	19.49	202	3149	0.059	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093246.D
Acq On : 19 Jun 2017 12:23
Operator : SJ/MA
Sample : I3599-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A74

Quant Time: Jun 20 04:19:12 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

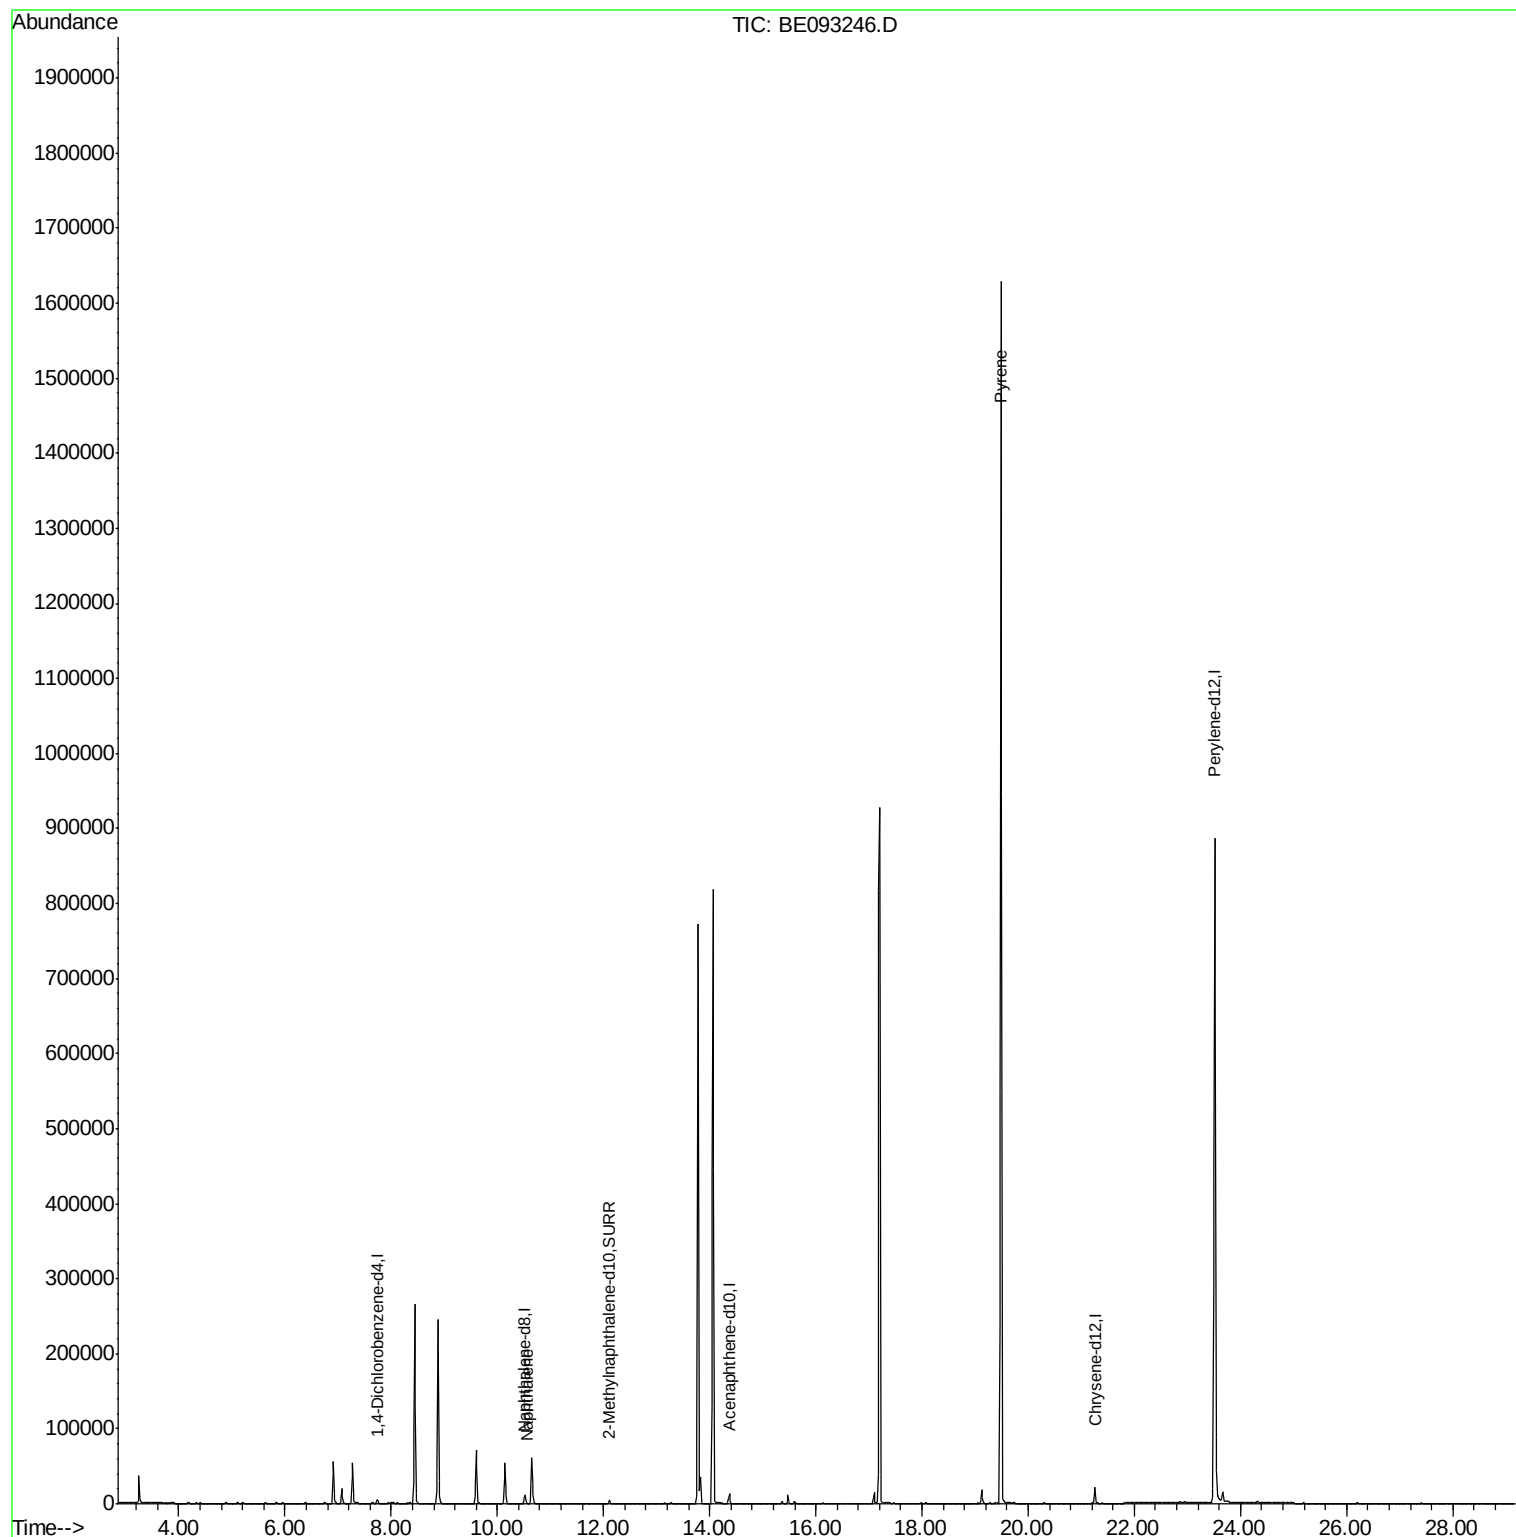

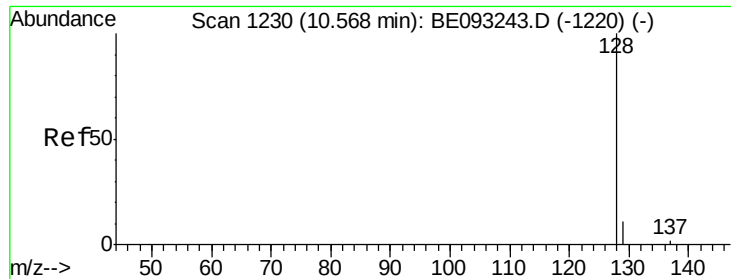

#3

Naphthalene

Concen: 0.012 ng/ul

RT: 10.57 min Scan# 1230

Delta R.T. -0.00 min

Lab File: BE093246.D

Acq: 19 Jun 2017 12:23

Instrument :

BNA_E

ClientSampleId :

F5A74


Tgt Ion:128 Resp: 364

Ion Ratio Lower Upper

128 100

129 35.5 11.3 16.9#




127 0.0 4.0 6.0#

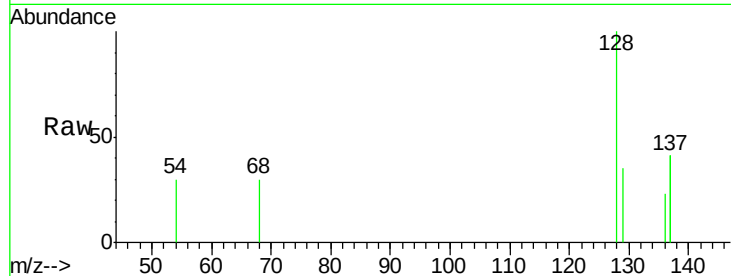

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

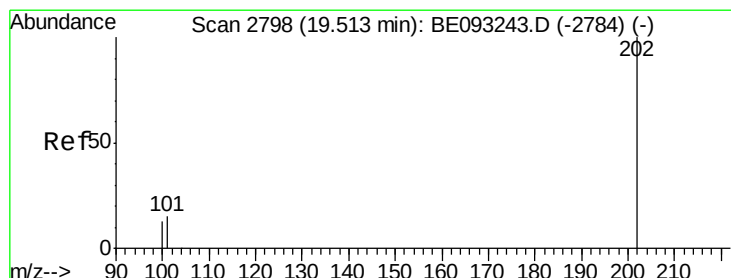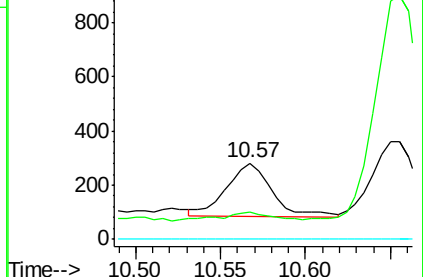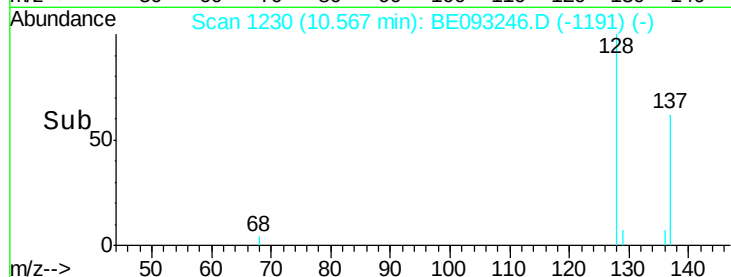

#17

Pyrene

Concen: 0.059 ng/ul

RT: 19.49 min Scan# 2792

Delta R.T. -0.02 min

Lab File: BE093246.D

Acq: 19 Jun 2017 12:23


Tgt Ion:202 Resp: 3149

Ion Ratio Lower Upper

202 100

101 194.8 18.2 27.4#

100 1122.8 15.6 23.4#

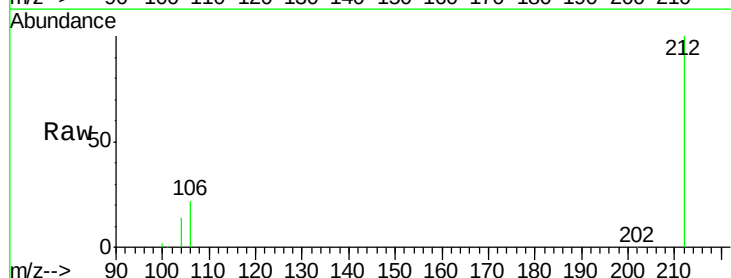

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

