

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093247.D
 Acq On : 19 Jun 2017 12:59
 Operator : SJ/MA
 Sample : I3599-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E13

Quant Time: Jun 20 04:19:17 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2412	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	11959	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7483	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	18733	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	1074826	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	4554	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	14520	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.57	128	417	0.014	ng/ul#	62
17) Pyrene	19.52	202	1566	0.028	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093247.D
Acq On : 19 Jun 2017 12:59
Operator : SJ/MA
Sample : I3599-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5E13

Quant Time: Jun 20 04:19:17 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

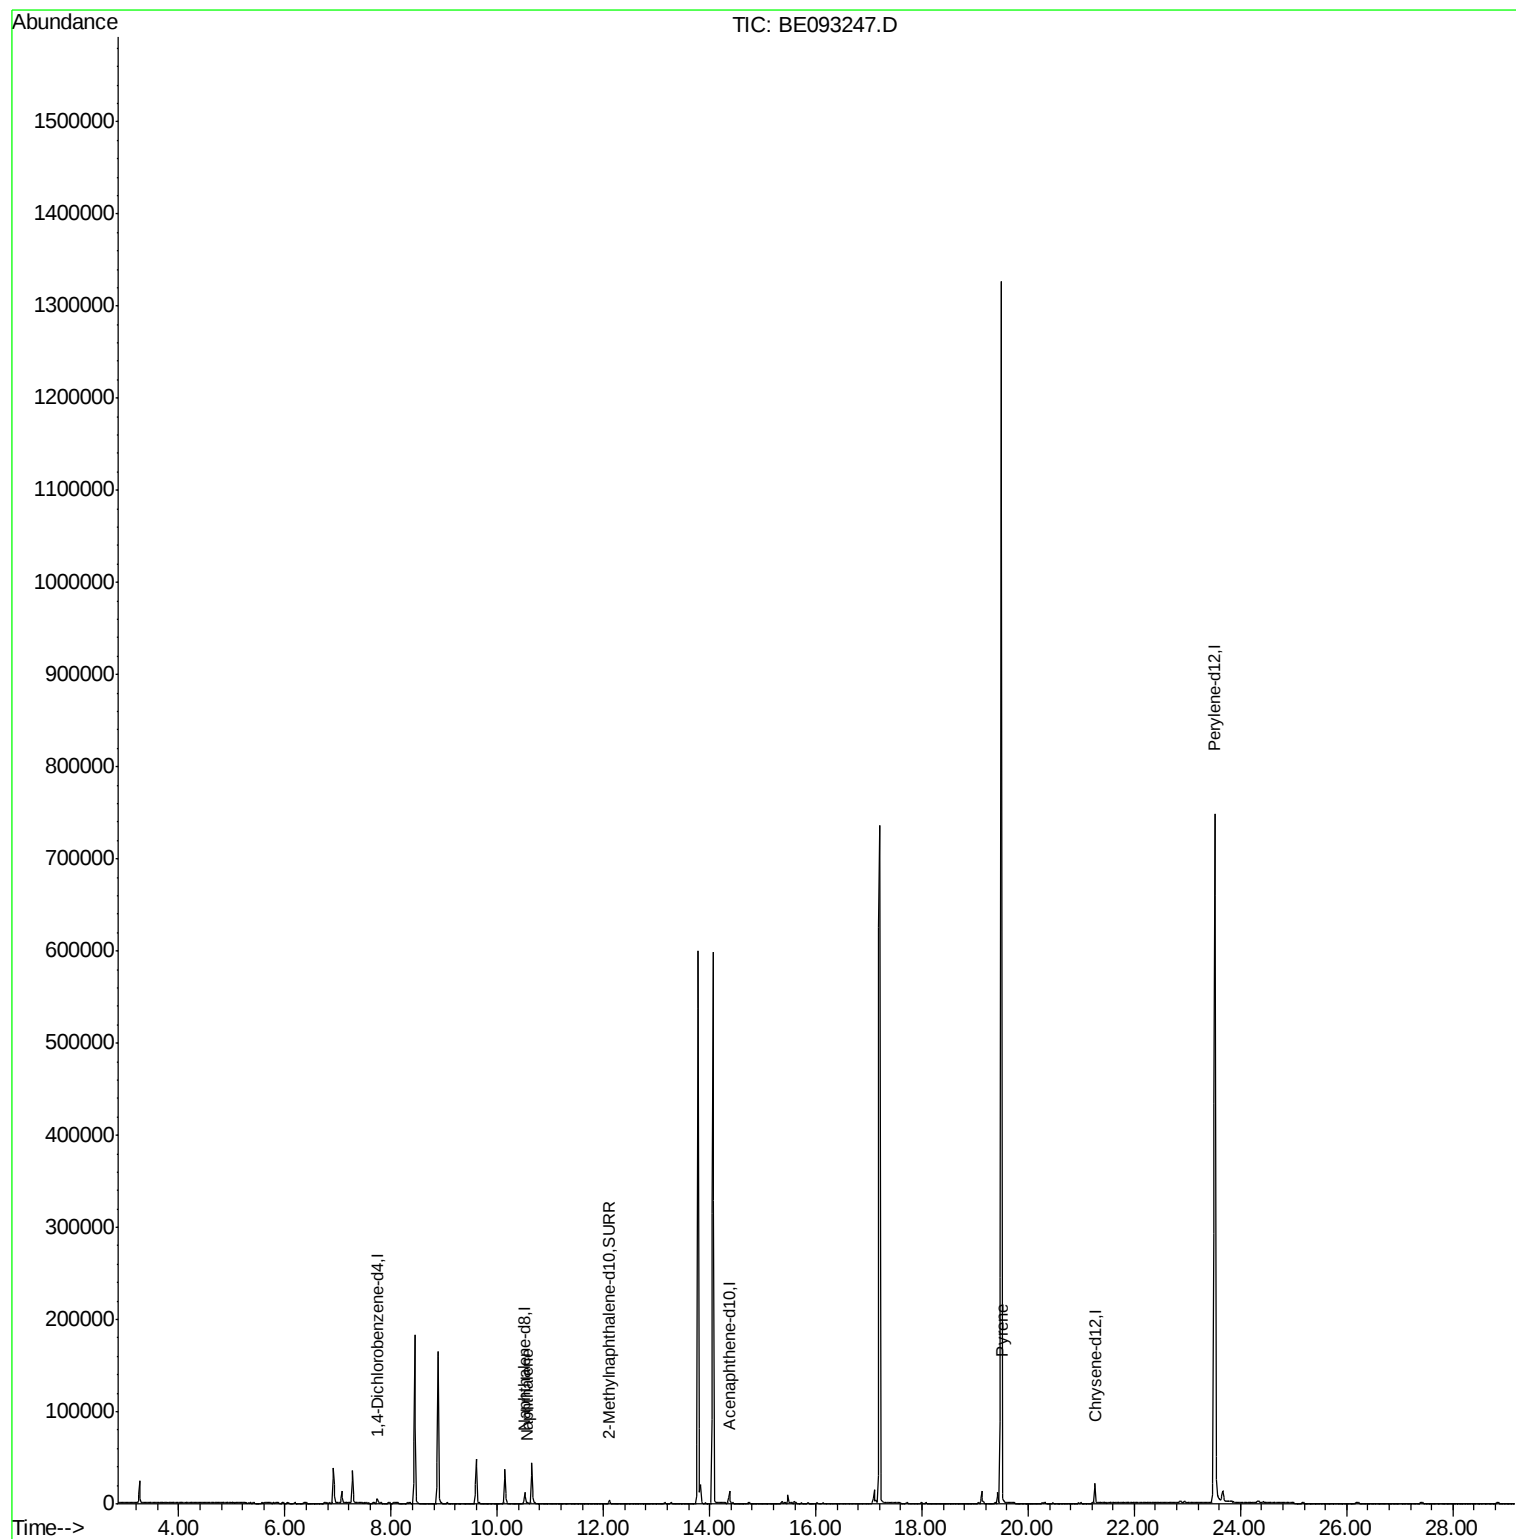

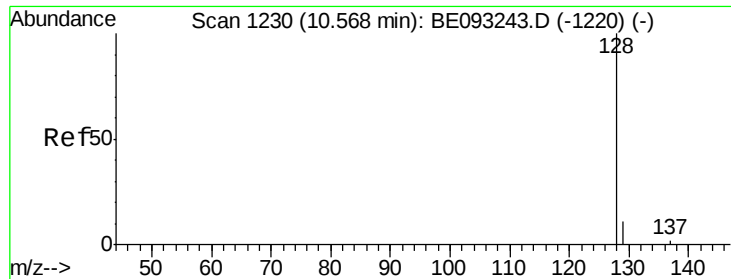

#3

Naphthalene

Concen: 0.014 ng/ul

RT: 10.57 min Scan# 1230

Delta R.T. 0.00 min

Lab File: BE093247.D

Acq: 19 Jun 2017 12:59

Instrument :

BNA_E

ClientSampleId :

F5E13





Tgt Ion:128 Resp: 417

Ion Ratio Lower Upper

128 100

129 32.9 11.3 16.9#

127 0.0 4.0 6.0#

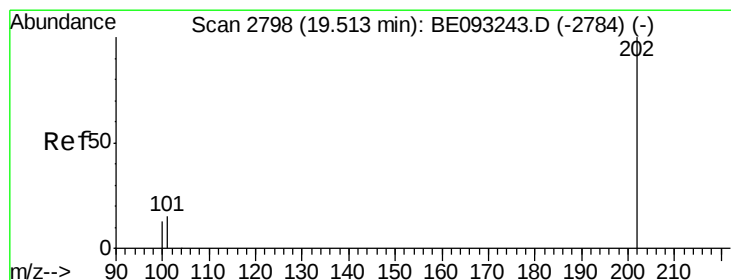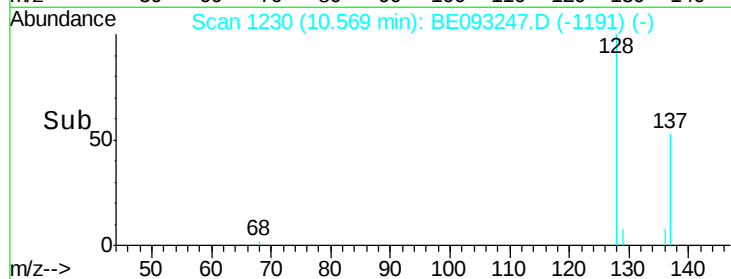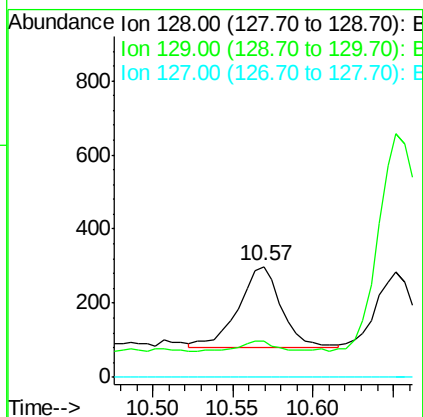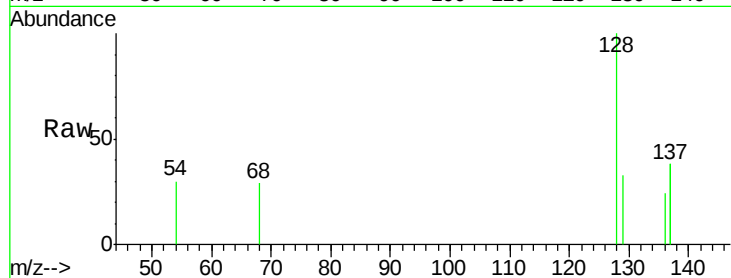

#17

Pyrene

Concen: 0.028 ng/ul

RT: 19.52 min Scan# 2799

Delta R.T. 0.00 min

Lab File: BE093247.D

Acq: 19 Jun 2017 12:59

Tgt Ion:202 Resp: 1566

Ion Ratio Lower Upper

202 100

101 20.4 18.2 27.4

100 21.8 15.6 23.4

