

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093257.D
 Acq On : 19 Jun 2017 19:09
 Operator : SJ/MA
 Sample : I3600-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5A13

Quant Time: Jun 20 04:20:42 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2738	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	13936	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	8312	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	19568	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	19555	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	854747	0.40	ng/ul	-0.15
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	3673	0.18	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	12014	0.23	ng/ul	0.00
Target Compounds						
13) Anthracene	17.22	178	1602	0.034	ng/ul#	69
17) Pyrene	19.49	202	1868	0.032	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093257.D
Acq On : 19 Jun 2017 19:09
Operator : SJ/MA
Sample : I3600-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A13

Quant Time: Jun 20 04:20:42 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

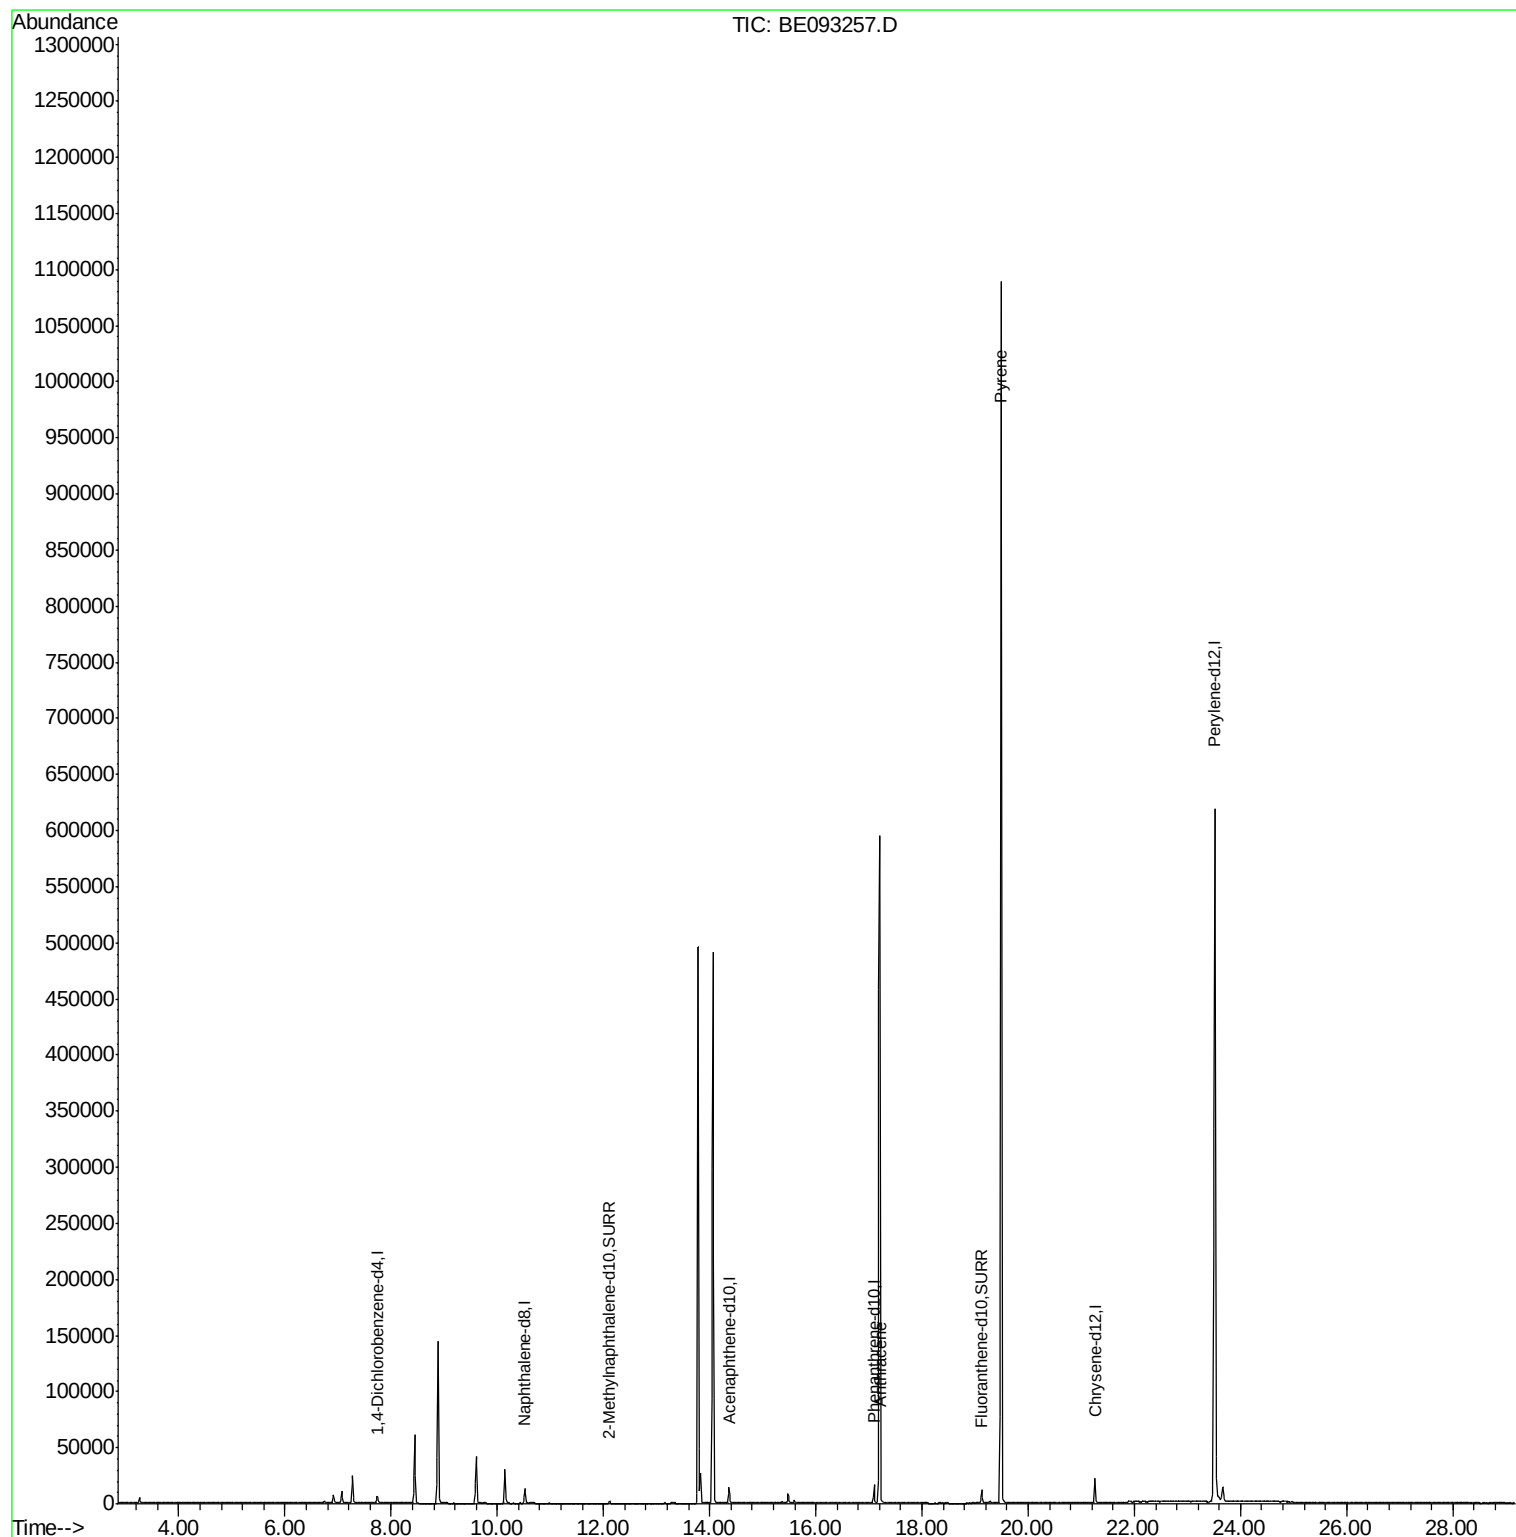

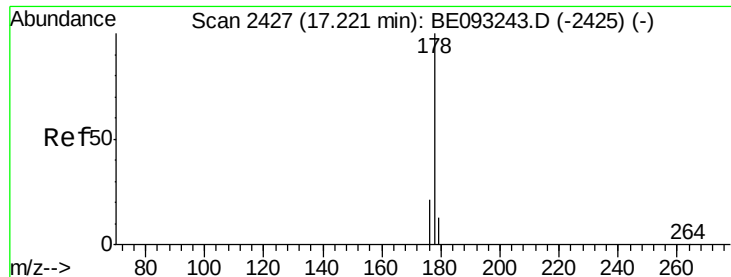

#13

Anthracene

Concen: 0.034 ng/ul

RT: 17.22 min Scan# 2427

Delta R.T. 0.00 min

Lab File: BE093257.D

Acq: 19 Jun 2017 19:09

Instrument :

BNA_E

ClientSampleId :

F5A13


Tgt Ion:178 Resp: 1602

Ion Ratio Lower Upper

178 100

179 38.1 18.1 27.1#




176 31.7 14.7 22.1#

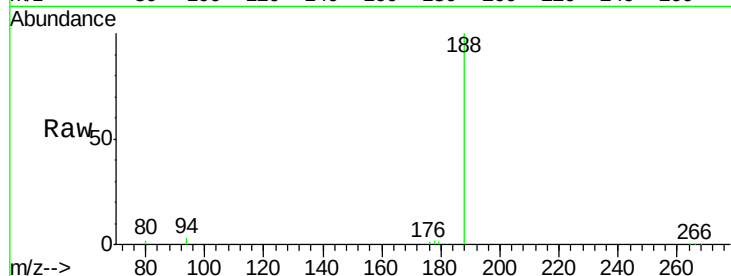

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

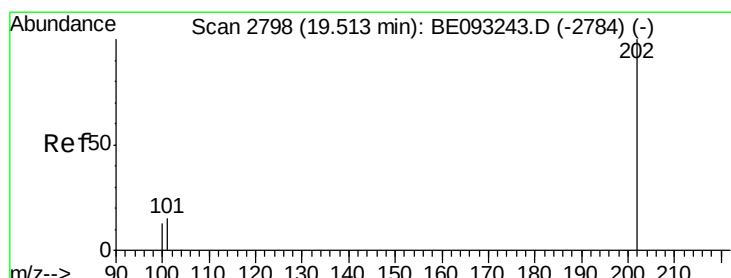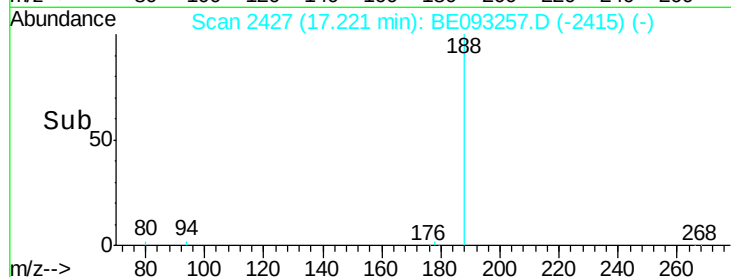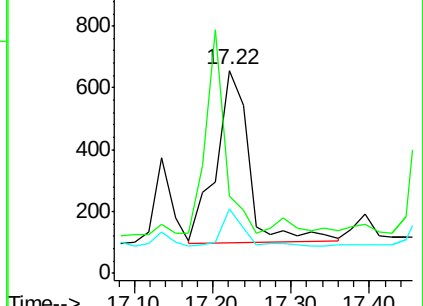

#17

Pyrene

Concen: 0.032 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.02 min

Lab File: BE093257.D

Acq: 19 Jun 2017 19:09


Tgt Ion:202 Resp: 1868

Ion Ratio Lower Upper

202 100

101 184.9 18.2 27.4#

100 993.8 15.6 23.4#

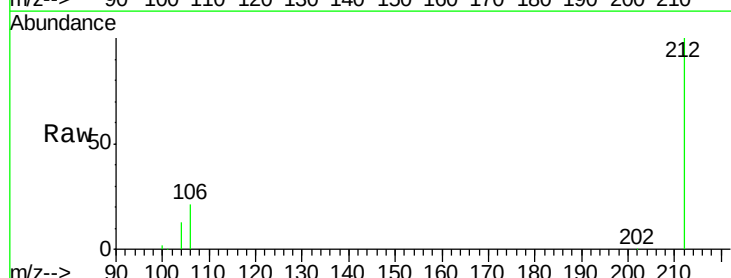

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

