

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093260.D
 Acq On : 19 Jun 2017 20:59
 Operator : SJ/MA
 Sample : I3600-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E12

Quant Time: Jun 20 08:58:39 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2646	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	13136	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	8172	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	18564m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18577	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	15104m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6638	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	18377	0.36	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	937	0.029	ng/ul#	Qvalue 86




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093260.D
Acq On : 19 Jun 2017 20:59
Operator : SJ/MA
Sample : I3600-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5E12

Quant Time: Jun 20 08:58:39 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

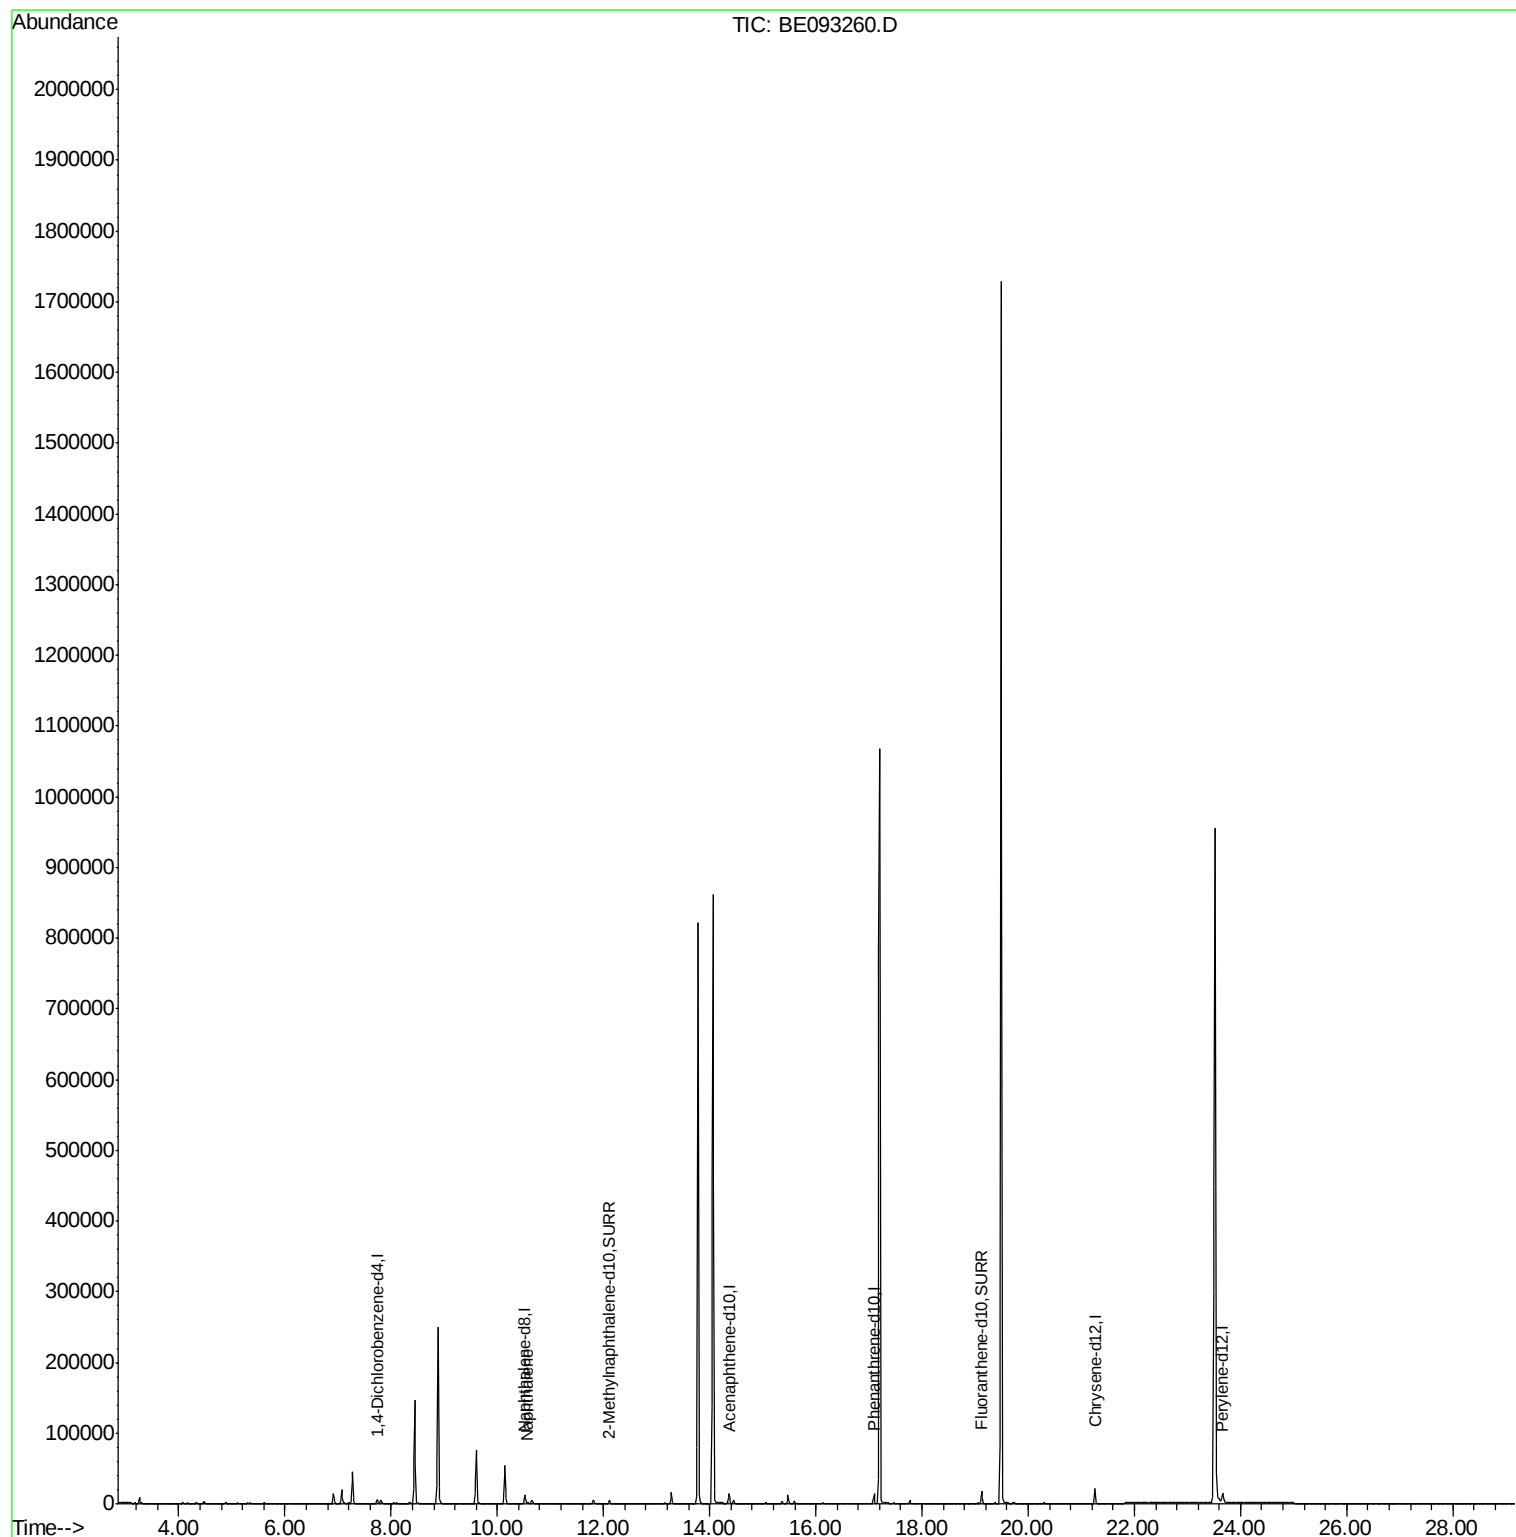

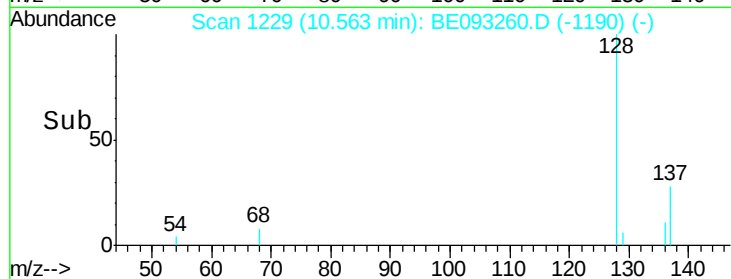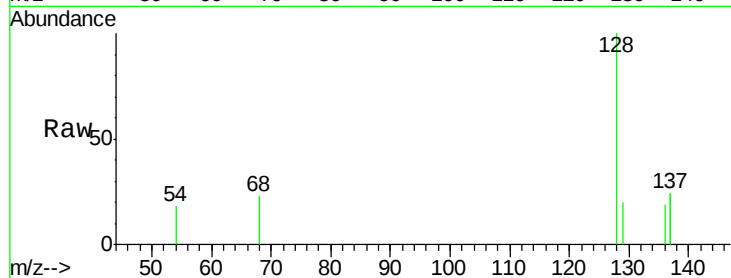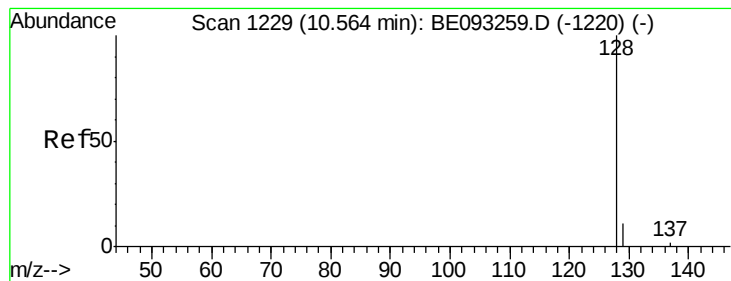

#3

Naphthalene

Concen: 0.029 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093260.D

Acq: 19 Jun 2017 20:59

Instrument :

BNA_E

ClientSampleId :

F5E12

Tgt Ion:128 Resp: 937

Ion Ratio Lower Upper

128 100

129 19.9 11.3 16.9#

127 0.0 4.0 6.0#

