

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
 Data File : BE093265.D
 Acq On : 20 Jun 2017 00:04
 Operator : SJ/MA
 Sample : I3600-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 20 08:50:24 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2648	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	13778	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	9164	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	20688	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	1361025	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	7570	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20611	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	784	0.02	ng/ul#	78
8) Acenaphthene	14.45	153	6187	0.20	ng/ul#	22
17) Pyrene	19.49	202	3671	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
Data File : BE093265.D
Acq On : 20 Jun 2017 00:04
Operator : SJ/MA
Sample : I3600-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 20 08:50:24 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

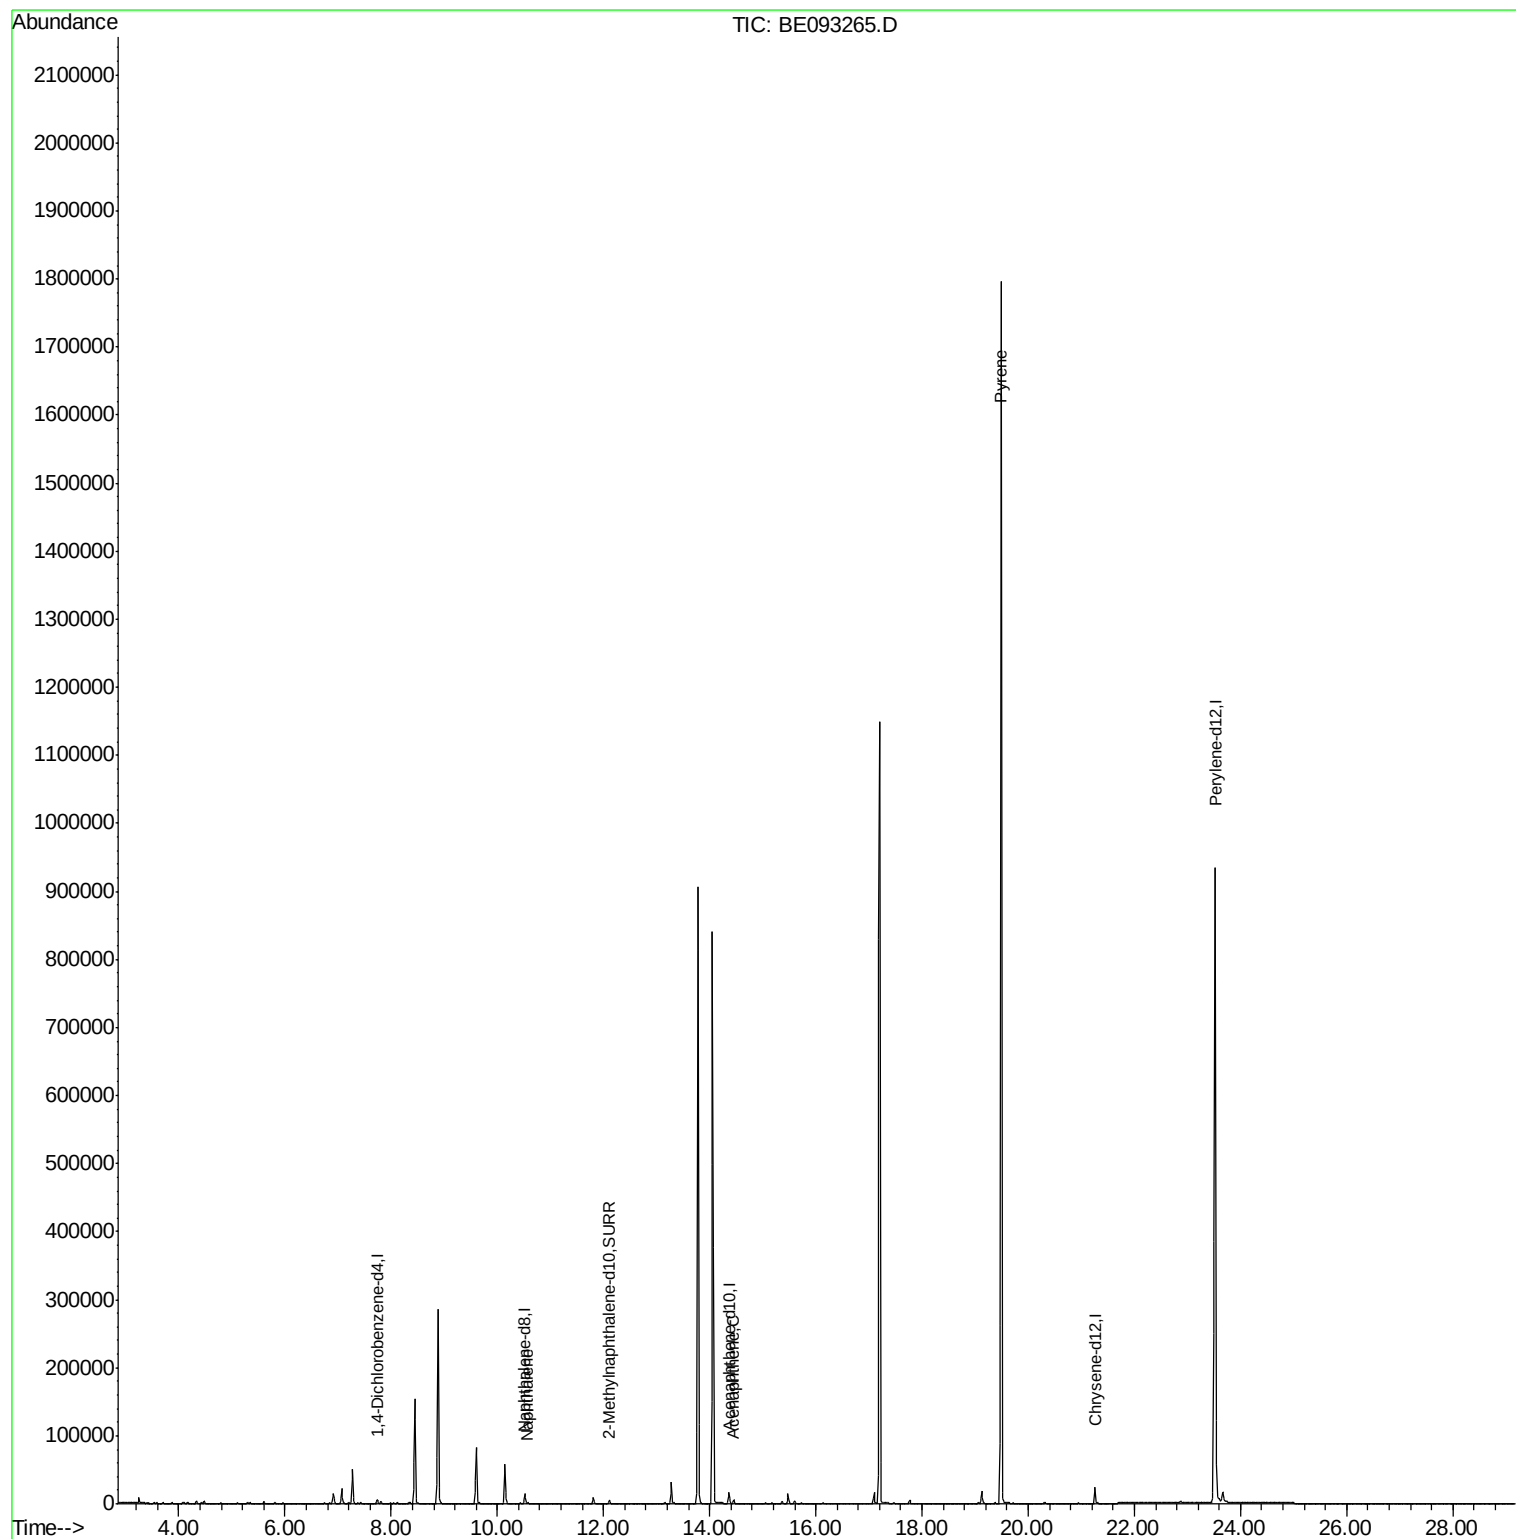

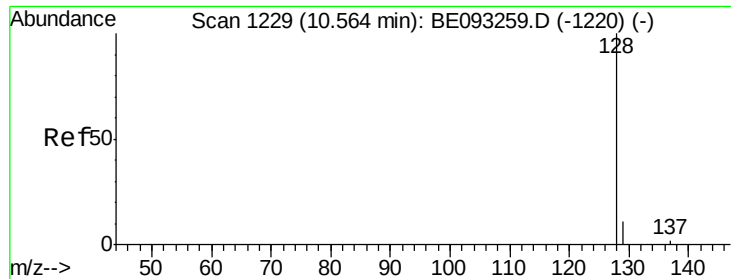

#3

Naphthalene

Concen: 0.02 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 784

Ion Ratio Lower Upper

128 100

129 24.3 11.3 16.9#




127 0.0 4.0 6.0#

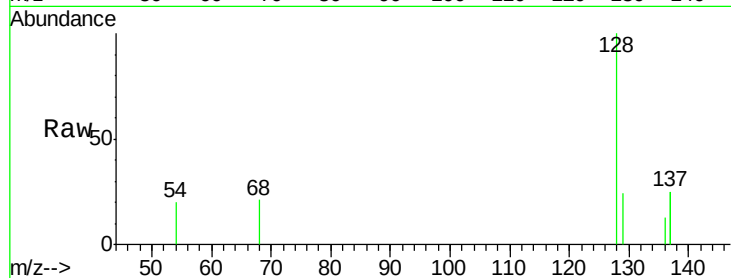

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

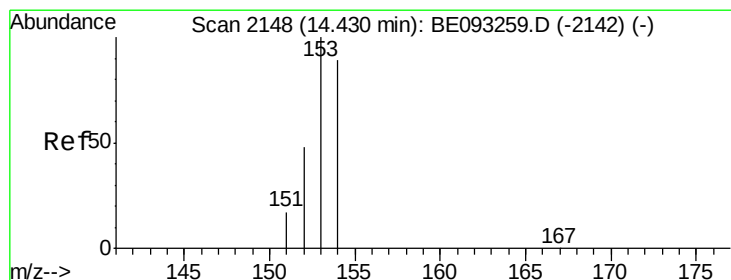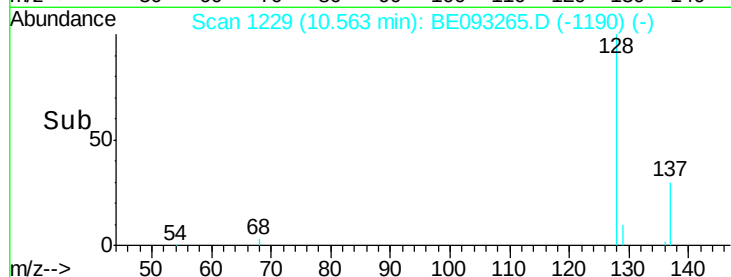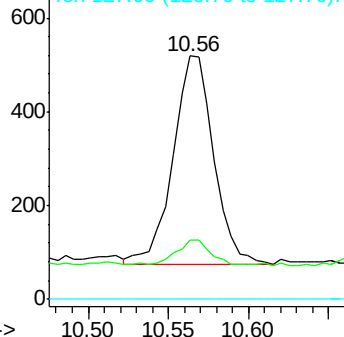

#8

Acenaphthene

Concen: 0.20 ng/ul

RT: 14.45 min Scan# 2152

Delta R.T. 0.02 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04


Tgt Ion:153 Resp: 6187

Ion Ratio Lower Upper

153 100

152 2.9 40.3 60.5#



154 10.5 71.4 107.2#



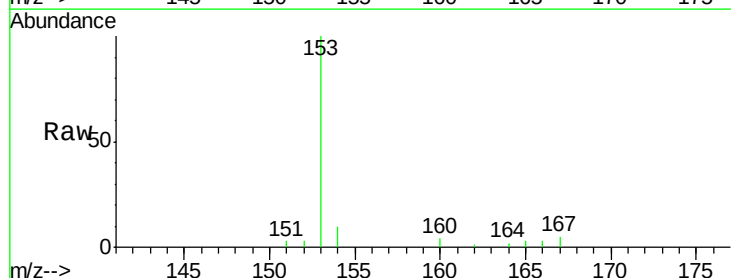


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

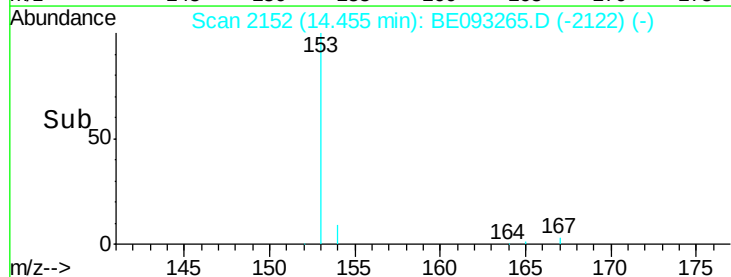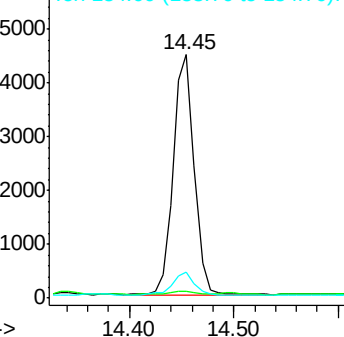

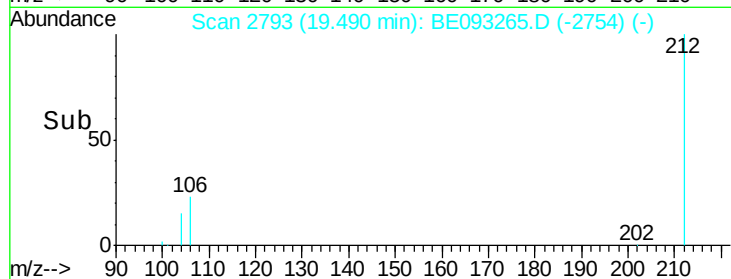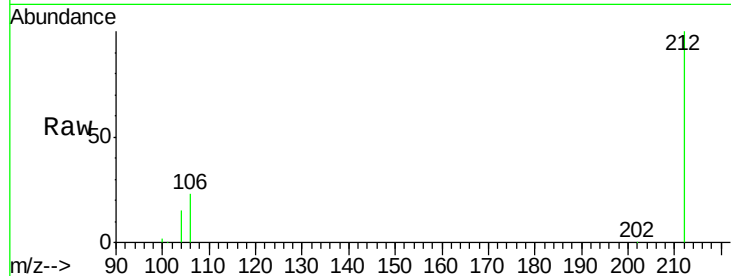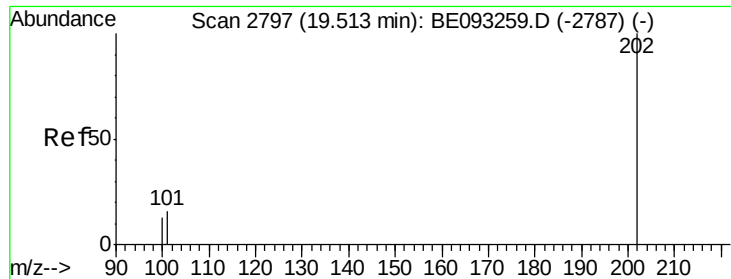

#17
 Pvrene
 Concen: 0.06 ng/ul
 RT: 19.49 min Scan# 2793
 Delta R.T. -0.02 min
 Lab File: BE093265.D
 Acq: 20 Jun 2017 00:04

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:202 Resp: 3671
 Ion Ratio Lower Upper
 202 100
 101 203.2 18.2 27.4#
 100 1156.9 15.6 23.4#

