

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093265.D
 Acq On : 20 Jun 2017 00:04
 Operator : SJ/MA
 Sample : I3600-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E16

Quant Time: Jun 20 09:17:38 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2648	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	13778	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	9164	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	20960m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	20688	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	16964m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	7570	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20611	0.36	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	784	0.023	ng/ul#	78
15) Fluoranthene	19.15	202	1109	0.016	ng/ul	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093265.D
Acq On : 20 Jun 2017 00:04
Operator : SJ/MA
Sample : I3600-10
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5E16

Quant Time: Jun 20 09:17:38 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

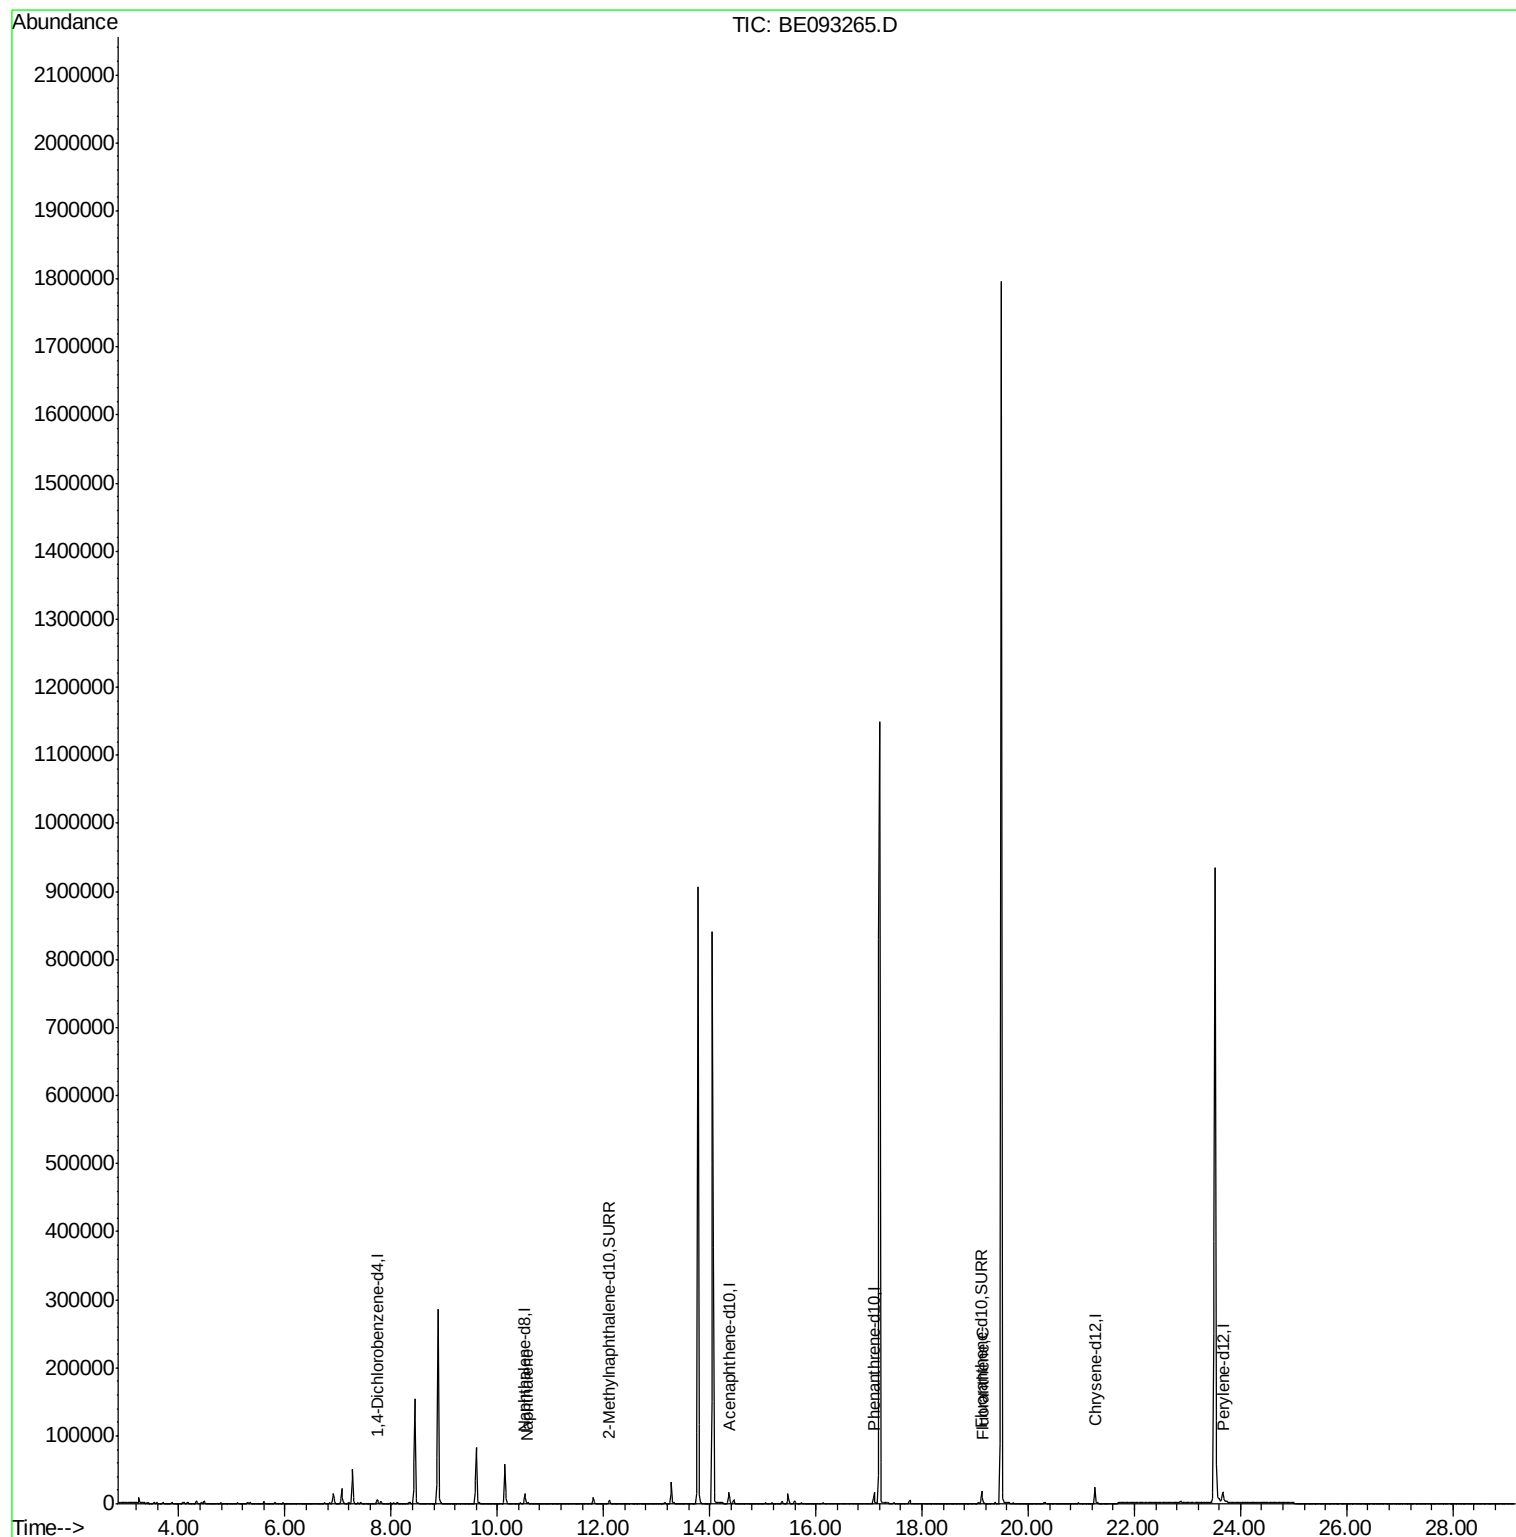

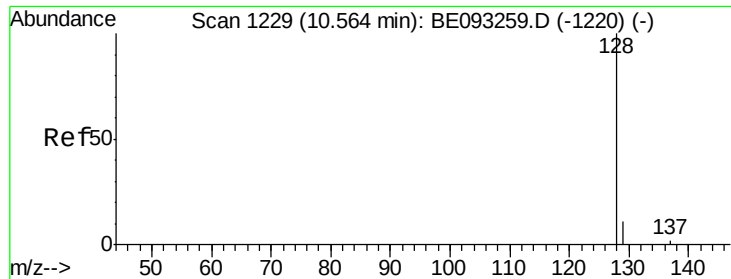

#3

Naphthalene

Concen: 0.023 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04

Instrument :

BNA_E

ClientSampleId :

F5E16


Tgt Ion:128 Resp: 784

Ion Ratio Lower Upper

128 100

129 24.3 11.3 16.9#




127 0.0 4.0 6.0#

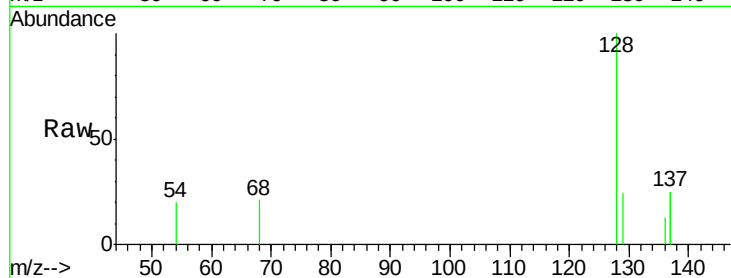

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

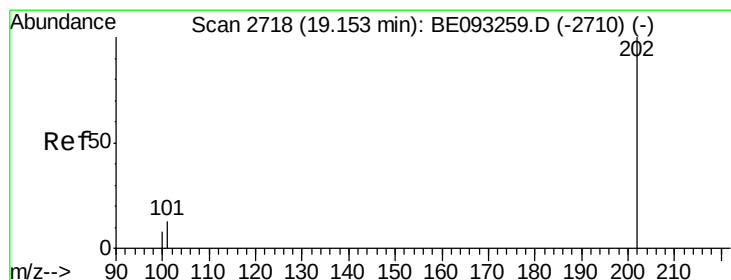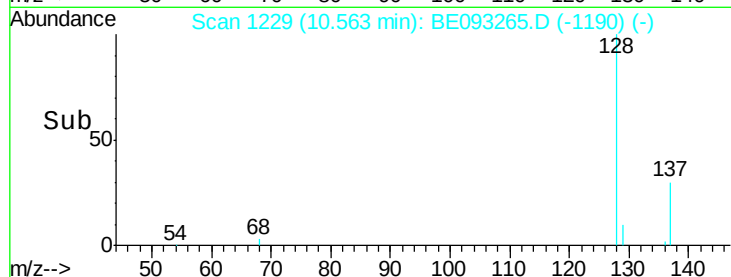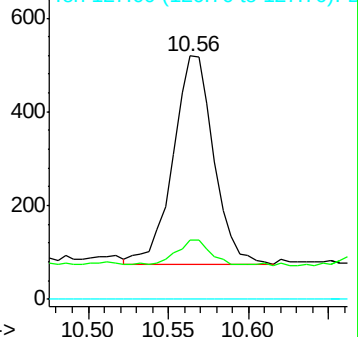

#15

Fluoranthene

Concen: 0.016 ng/ul

RT: 19.15 min Scan# 2719

Delta R.T. -0.00 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04


Tgt Ion:202 Resp: 1109

Ion Ratio Lower Upper

202 100

101 21.6 0.0 30.3

100 15.5 0.0 39.5

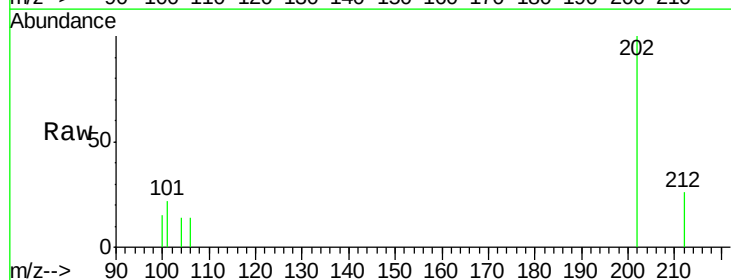

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

