

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
 Data File : BE093267.D
 Acq On : 20 Jun 2017 1:19
 Operator : SJ/MA
 Sample : I3600-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 20 08:50:41 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2369	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12829	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	8487	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	19020	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	1307673	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6963	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20141	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.57	128	419	0.01	ng/ul#	55
7) Acenaphthylene	14.09	152	879	0.02	ng/ul#	80
17) Pyrene	19.49	202	3035	0.05	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
Data File : BE093267.D
Acq On : 20 Jun 2017 1:19
Operator : SJ/MA
Sample : I3600-12
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 20 08:50:41 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration




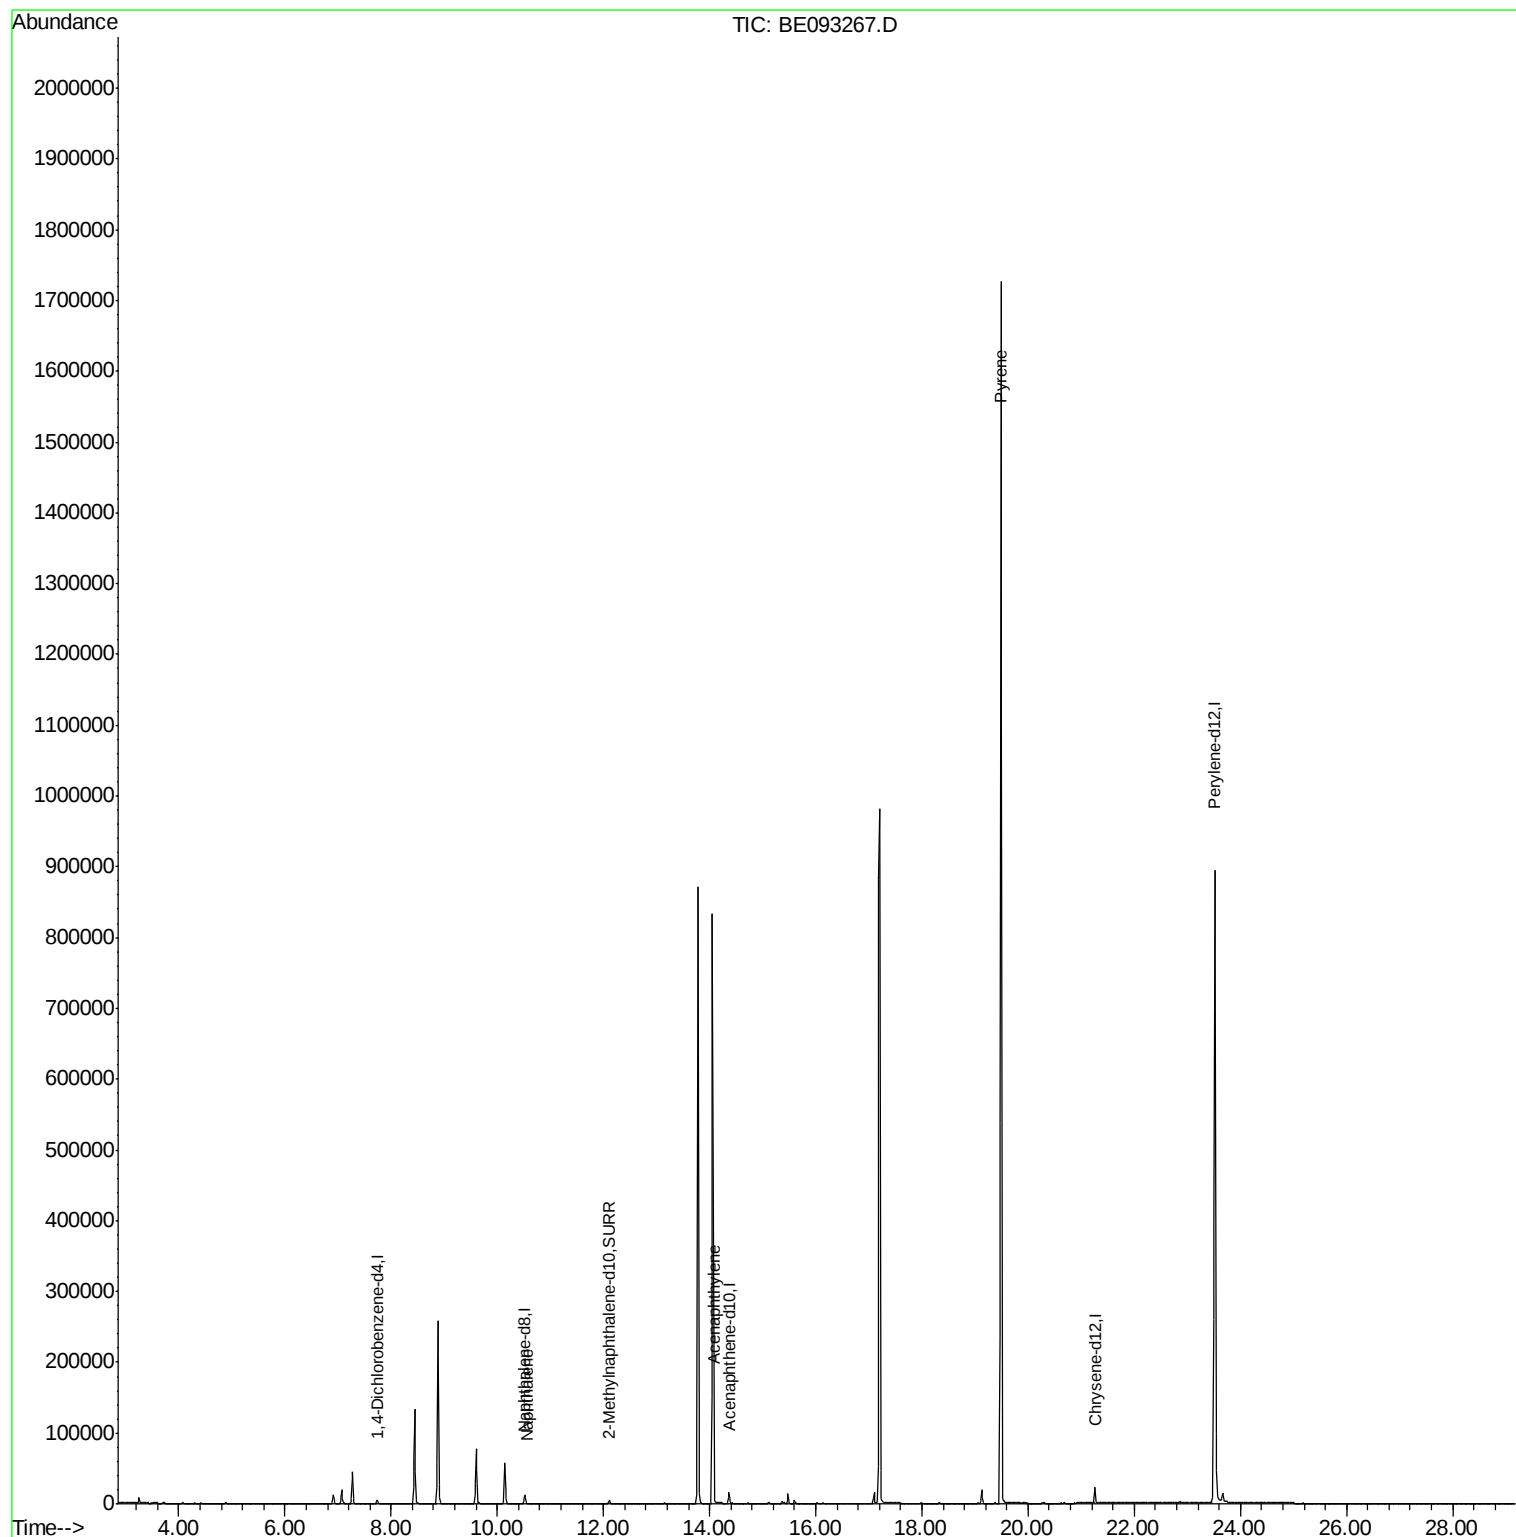


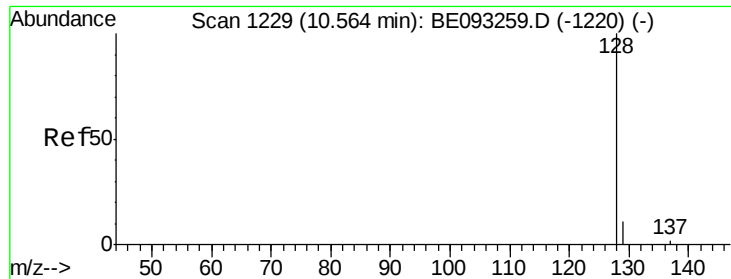

#3
Naphthalene
Concen: 0.01 ng/ul
RT: 10.57 min Scan# 1230
Delta R.T. 0.00 min
Lab File: BE093267.D
Acq: 20 Jun 2017 1:19




Instrument :
BNA_E
ClientSampleId :




Tot Ion:128 Resp: 419
Ion Ratio Lower Upper
128 100
129 36.6 11.3 16.9#
127 0.0 4.0 6.0#

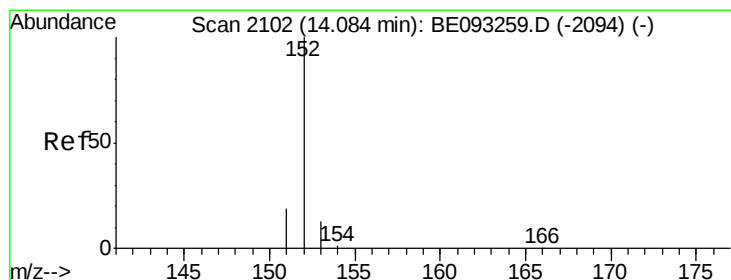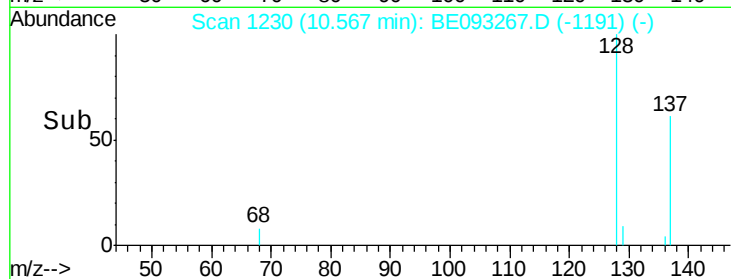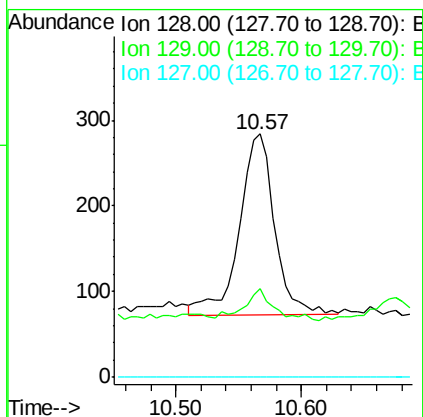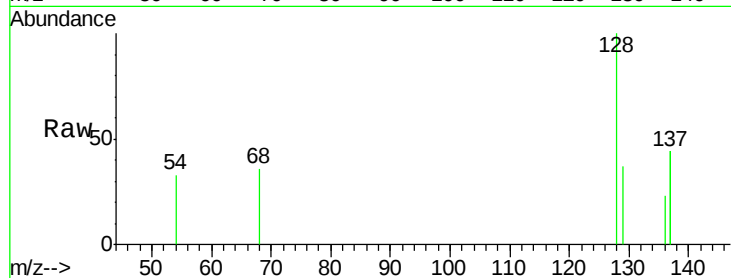

#7
Acenaphthylene
Concen: 0.02 ng/ul
RT: 14.09 min Scan# 2104
Delta R.T. 0.00 min
Lab File: BE093267.D
Acq: 20 Jun 2017 1:19

Tgt Ion:152 Resp: 879
Ion Ratio Lower Upper
152 100
151 29.9 17.1 25.7#
153 25.2 12.8 19.2#

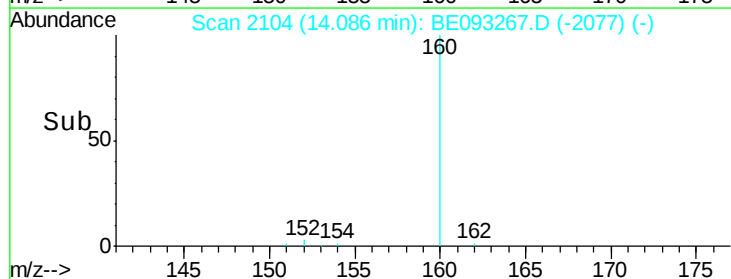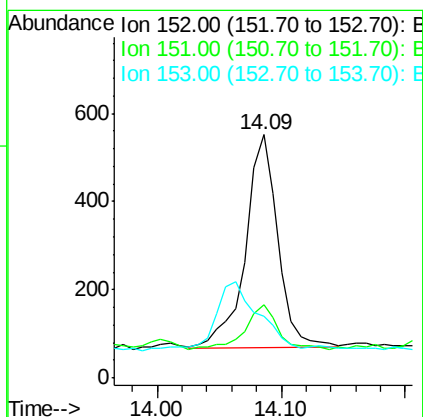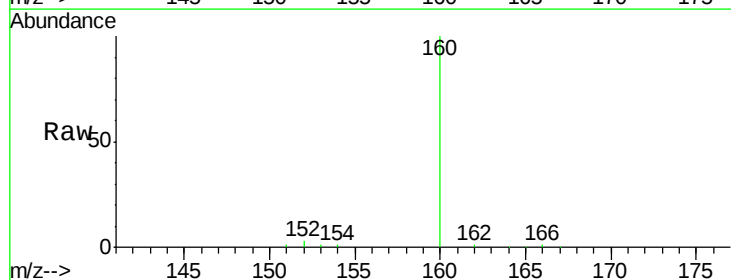

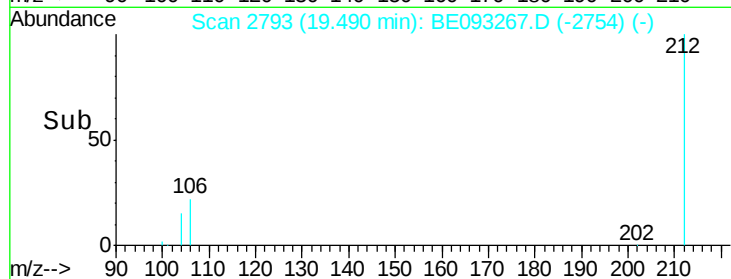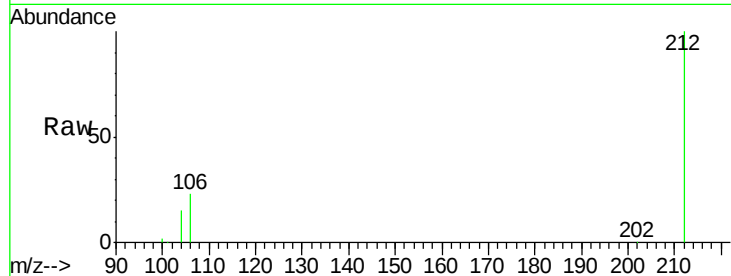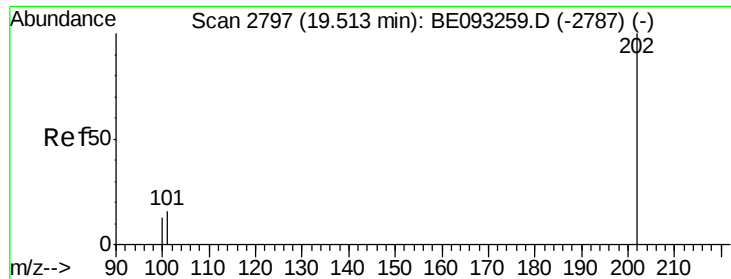

#17
 Pvrene
 Concen: 0.05 ng/ul
 RT: 19.49 min Scan# 2793
 Delta R.T. -0.02 min
 Lab File: BE093267.D
 Acq: 20 Jun 2017 1:19

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	198.0	18.2	27.4#
100	1158.1	15.6	23.4#

