

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
 Data File : BE093269.D
 Acq On : 20 Jun 2017 2:34
 Operator : SJ/MA
 Sample : I3599-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 20 08:51:00 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2507	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12971	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	8050	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	19647	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	21547	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	21694	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	3208	0.17	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	9023	0.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.56	128	5206	0.16	ng/ul#	93
5) 2-Methylnaphthalene	12.18	142	1227	0.06	ng/ul	98
7) Acenaphthylene	14.08	152	28309	0.82	ng/ul	96
8) Acenaphthene	14.42	153	1228	0.04	ng/ul	92
9) Fluorene	15.42	166	1210	0.04	ng/ul#	92
12) Phenanthrene	17.13	178	27094	0.50	ng/ul#	89
13) Anthracene	17.22	178	33031	0.70	ng/ul#	88
15) Fluoranthene	19.15	202	192798	2.91	ng/ul	84
17) Pyrene	19.51	202	229397	3.61	ng/ul#	87
18) Benzo(a)anthracene	21.24	228	147529	2.57	ng/ul#	84
19) Chrysene	21.29	228	162018	2.72	ng/ul	98
21) Benzo(b)fluoranthene	22.93	252	403848	6.13	ng/ul	86
22) Benzo(k)fluoranthene	23.12	252	36903	0.53	ng/ul	94
23) Benzo(a)pyrene	23.56	252	145699	2.34	ng/ul#	81
24) Indeno(1,2,3-cd)pyrene	26.18	276	103290	1.43	ng/ul#	87
25) Dibenzo(a,h)anthracene	26.09	278	4012	0.07	ng/ul	90
26) Benzo(a,h,i)perylene	26.96	276	79774	1.29	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
Data File : BE093269.D
Acq On : 20 Jun 2017 2:34
Operator : SJ/MA
Sample : I3599-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 20 08:51:00 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

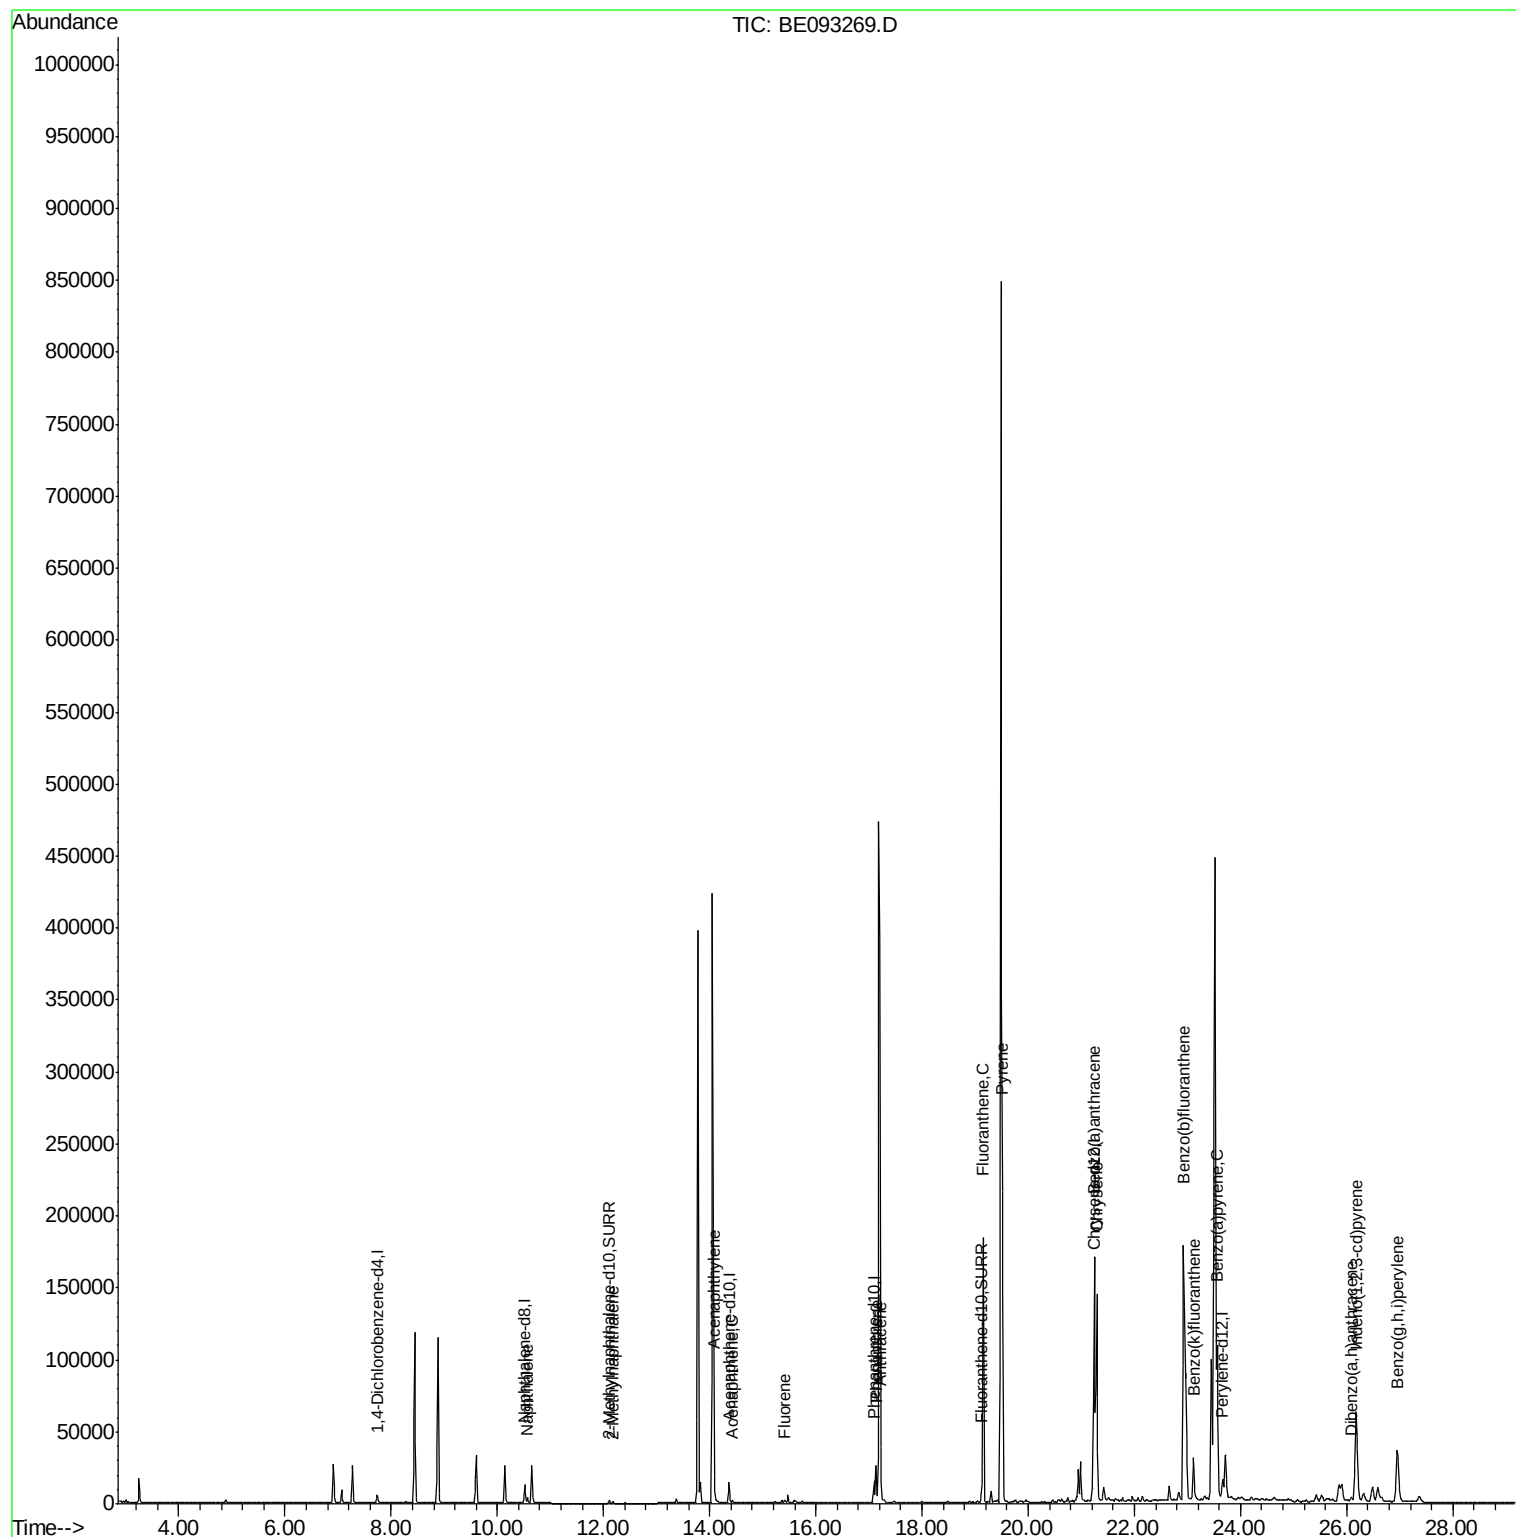

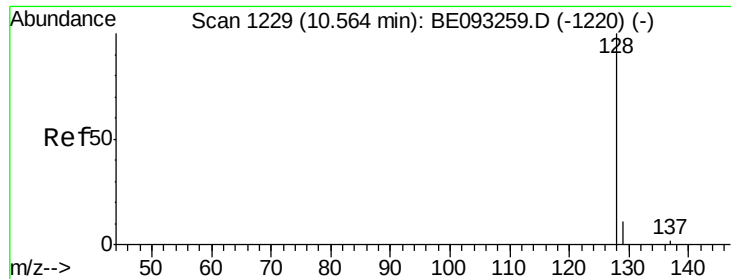

#3

Naphthalene

Concen: 0.16 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 5206

Ion Ratio Lower Upper

128 100

129 12.5 11.3 16.9




127 0.0 4.0 6.0#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

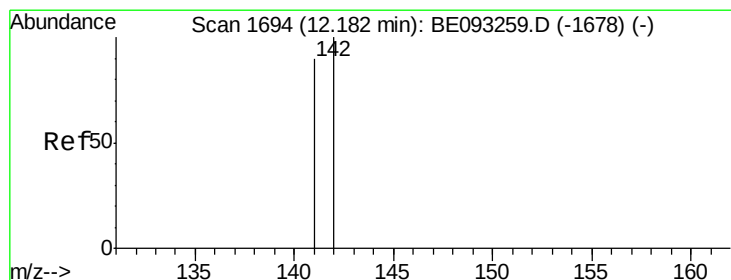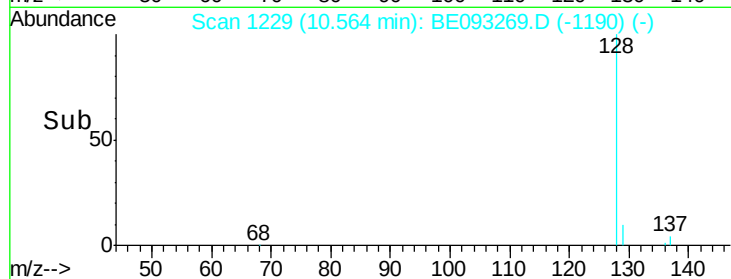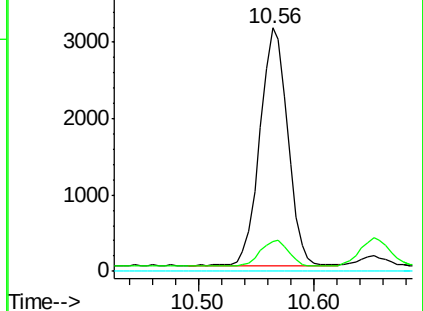

#5

2-Methylnaphthalene

Concen: 0.06 ng/ul

RT: 12.18 min Scan# 1693

Delta R.T. -0.00 min

Lab File: BE093269.D


Acq: 20 Jun 2017 2:34

Tgt Ion:142 Resp: 1227

Ion Ratio Lower Upper



142 100


141 89.1 72.6 108.8

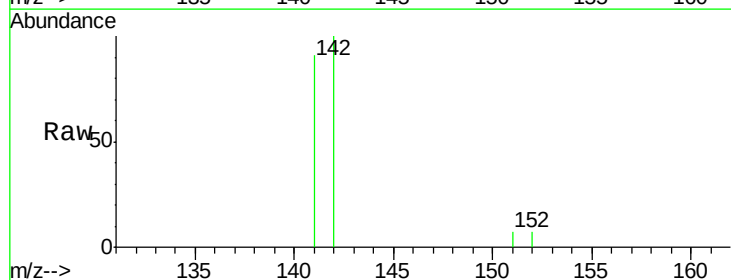

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

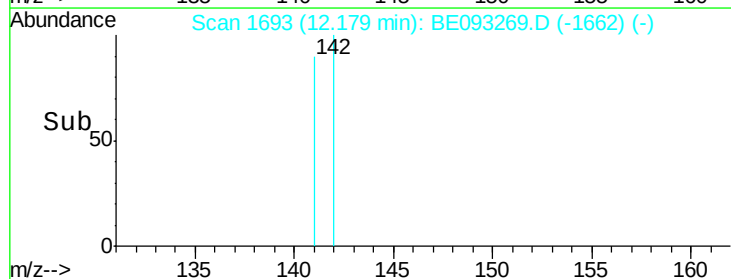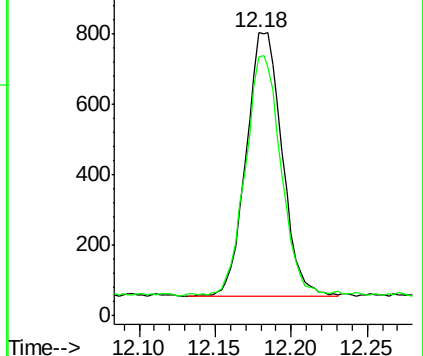



#7

Acenaphthylene

Concen: 0.82 ng/ul

RT: 14.08 min Scan# 2103

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 28309

Ion Ratio Lower Upper




152 100

151 19.9 17.1 25.7

153 13.4 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

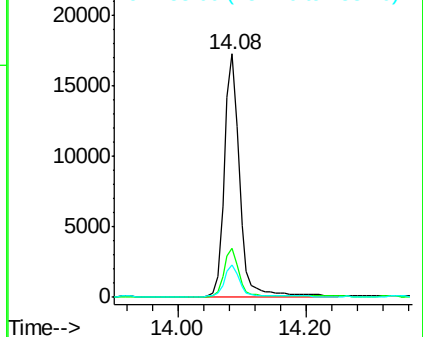

#8

Acenaphthene

Concen: 0.04 ng/ul

RT: 14.42 min Scan# 2148

Delta R.T. -0.01 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34


Tgt Ion:153 Resp: 1228

Ion Ratio Lower Upper



153 100


152 59.2 40.3 60.5

154 84.0 71.4 107.2



Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

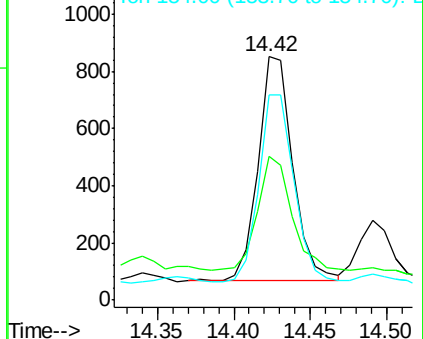



#9

Fluorene

Concen: 0.04 ng/ul

RT: 15.42 min Scan# 2280

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampled :


Tot Ion:166 Resp: 1210

Ion Ratio Lower Upper

166 100

165 98.6 73.4 110.2




167 22.8 14.6 22.0#



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

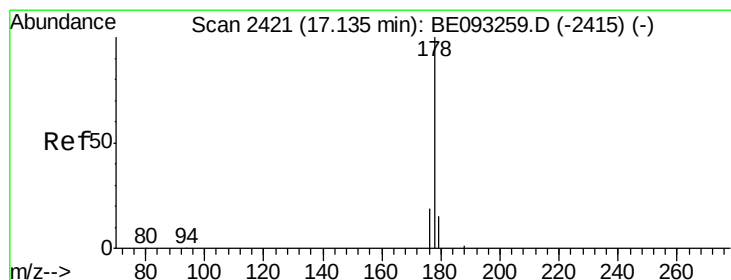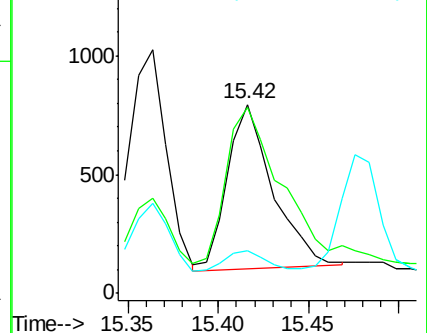

#12

Phenanthrene

Concen: 0.50 ng/ul

RT: 17.13 min Scan# 2422

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34


Tgt Ion:178 Resp: 27094

Ion Ratio Lower Upper

178 100

179 15.3 18.4 27.6#



176 18.7 13.6 20.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

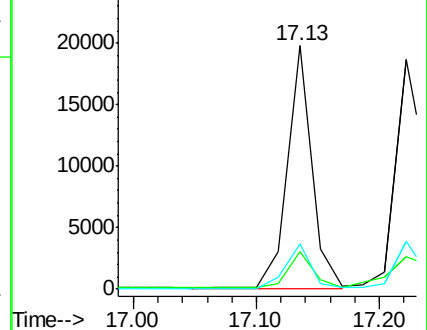

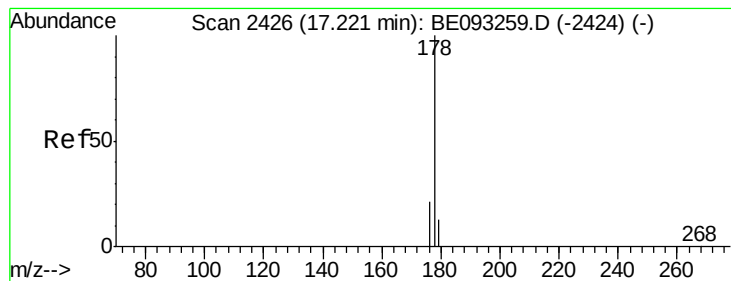

#13

Anthracene

Concen: 0.70 ng/ul

RT: 17.22 min Scan# 2427

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :





Tot Ion:178 Resp: 33031

Ion Ratio Lower Upper

178 100

179 14.4 18.1 27.1#

176 20.8 14.7 22.1

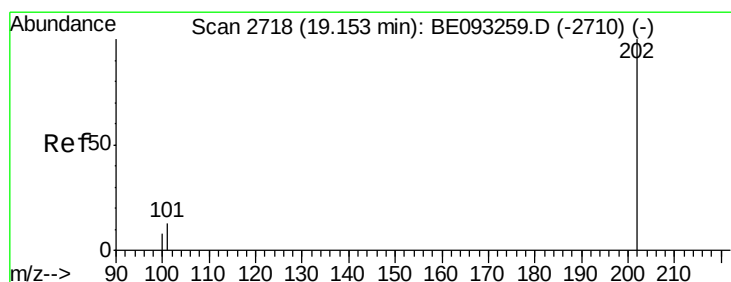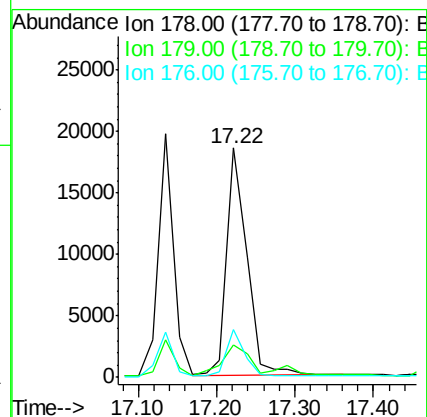

#15

Fluoranthene

Concen: 2.91 ng/ul

RT: 19.15 min Scan# 2719

Delta R.T. -0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34




Tgt Ion:202 Resp: 192798


Ion Ratio Lower Upper

202 100

101 13.9 0.0 30.3

100 10.4 0.0 39.5



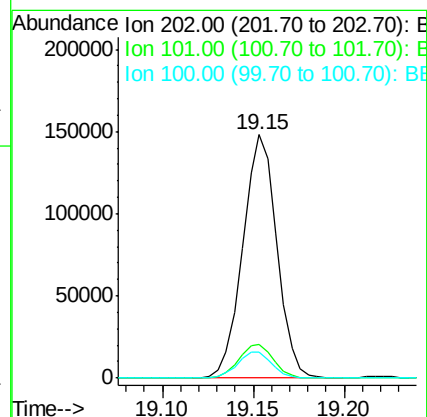
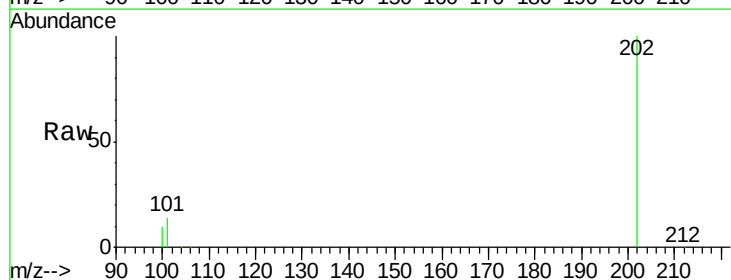




#17
Pvrene
Concen: 3.61 ng/ul
RT: 19.51 min Scan# 2798
Delta R.T. -0.00 min
Lab File: BE093269.D
Acq: 20 Jun 2017 2:34




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 229397
Ion Ratio Lower Upper
202 100
101 16.5 18.2 27.4#
100 13.7 15.6 23.4#

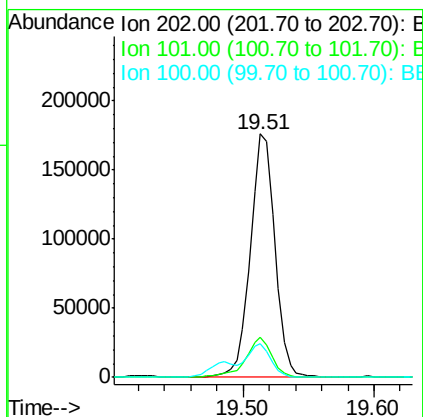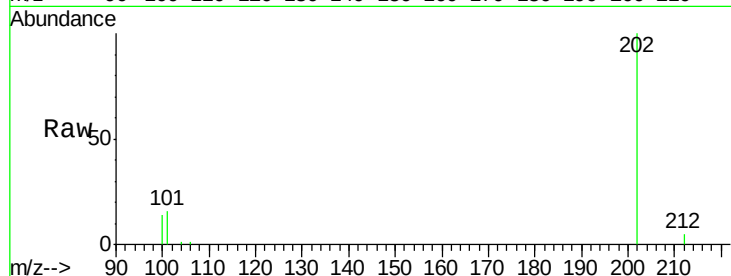

#18
Benzo(a)anthracene
Concen: 2.57 ng/ul
RT: 21.24 min Scan# 3174
Delta R.T. -0.00 min
Lab File: BE093269.D
Acq: 20 Jun 2017 2:34

Tgt Ion:228 Resp: 147529
Ion Ratio Lower Upper
228 100
229 20.4 22.8 34.2#
226 29.4 17.0 25.6#

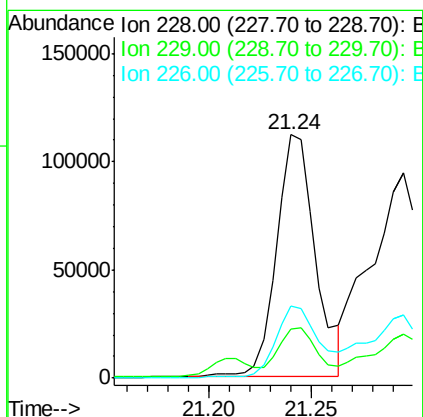

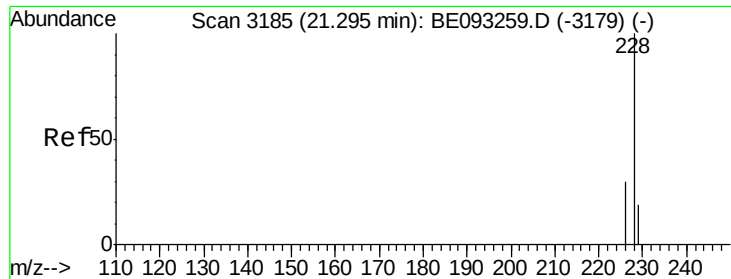

#19

Chrysene

Concen: 2.72 ng/ul

RT: 21.29 min Scan# 3186

Delta R.T. -0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 162018

Ion Ratio Lower Upper

228 100

226 30.6 23.4 35.0




229 21.7 17.7 26.5



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

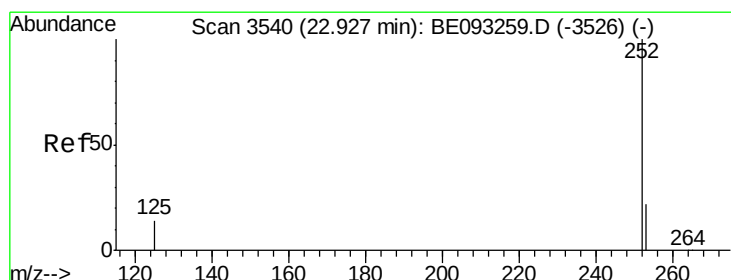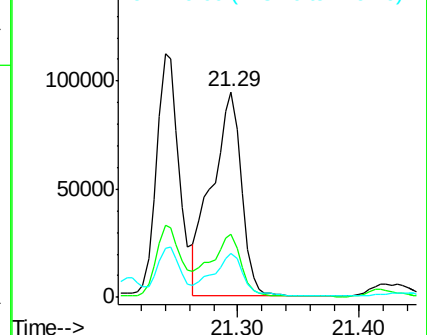

#21

Benzo(b)fluoranthene

Concen: 6.13 ng/ul

RT: 22.93 min Scan# 3542

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34


Tgt Ion:252 Resp: 403848

Ion Ratio Lower Upper

252 100

253 22.5 0.0 64.2



125 14.3 0.0 35.0

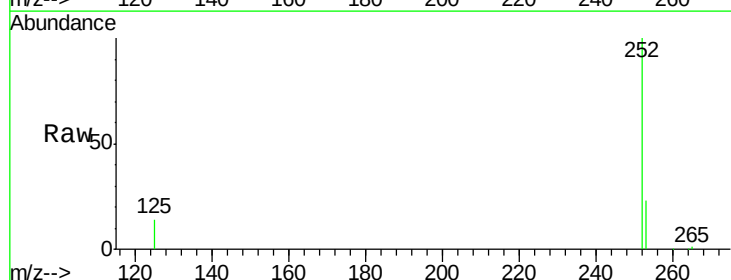


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

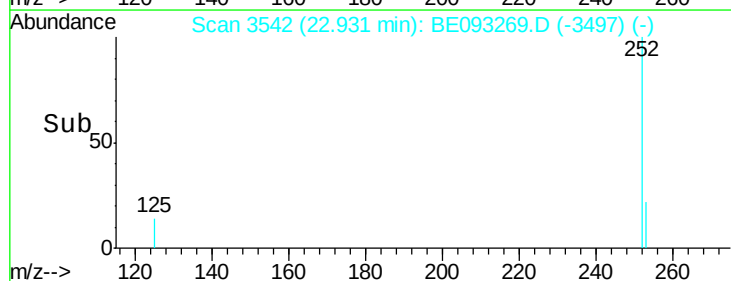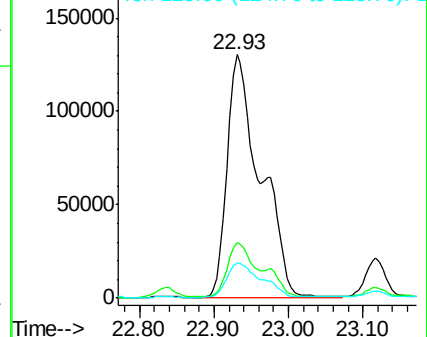

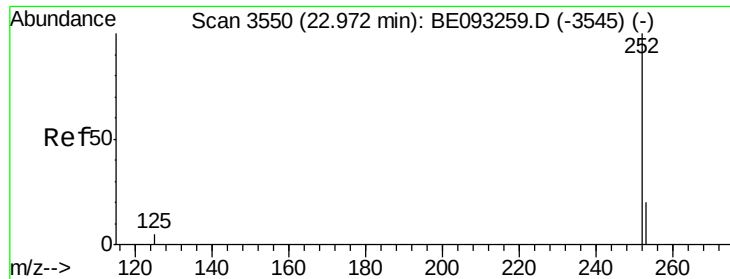

#22

Benzo(k)fluoranthene

Concen: 0.53 ng/ul

RT: 23.12 min Scan# 3583

Delta R.T. 0.15 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 36903

Ion Ratio Lower Upper




252 100

253 26.6 24.5 36.7

125 18.3 13.7 20.5

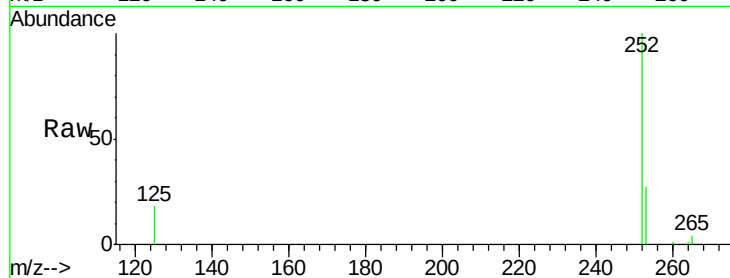

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

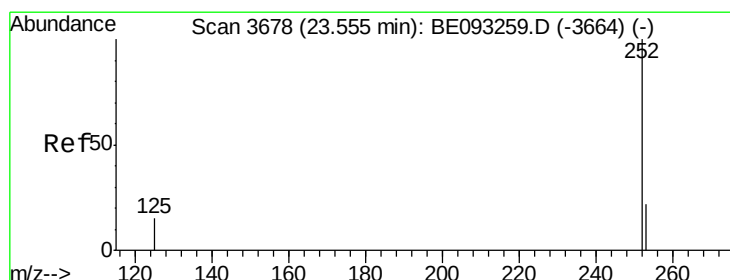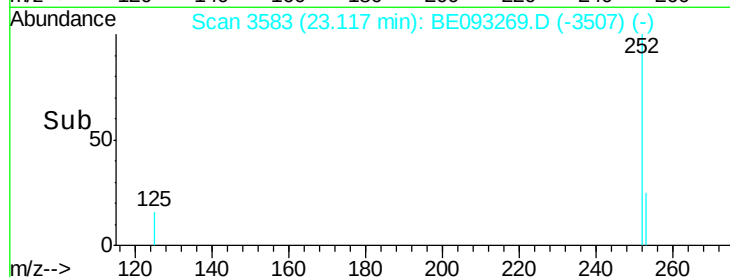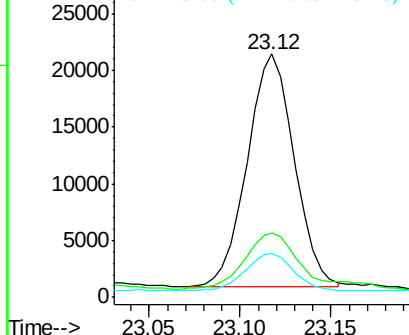

#23

Benzo(a)pyrene

Concen: 2.34 ng/ul

RT: 23.56 min Scan# 3680

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34


Tgt Ion:252 Resp: 145699

Ion Ratio Lower Upper



252 100


253 23.1 28.5 42.7#

125 15.4 18.1 27.1#

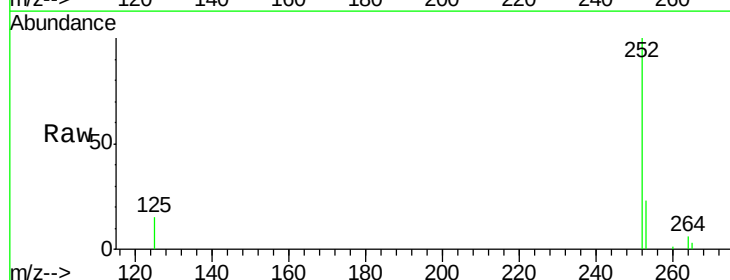

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

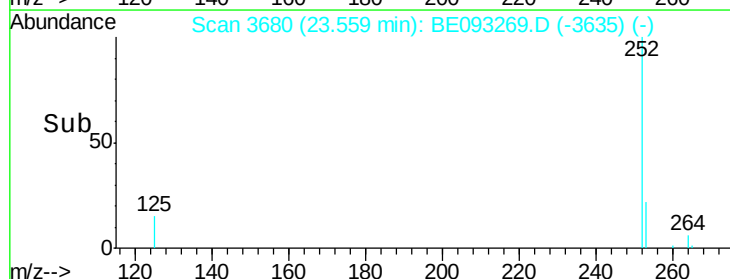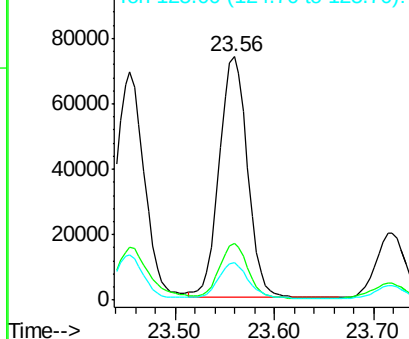



#24

Indeno(1,2,3-cd)pyrene

Concen: 1.43 ng/ul

RT: 26.18 min Scan# 4252

Delta R.T. 0.00 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34

Instrument :

BNA_E

ClientSampleId :


Tot Ion:276 Resp: 103290

Ion Ratio Lower Upper

276 100

138 29.5 28.0 42.0




227 0.0 8.0 12.0#

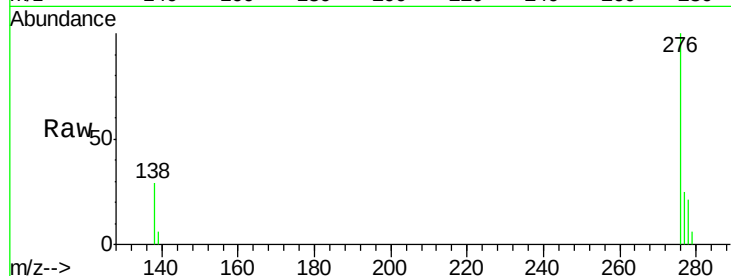

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

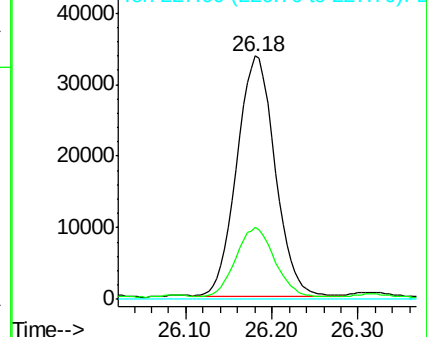

#25

Dibenzo(a,h)anthracene

Concen: 0.07 ng/ul

RT: 26.09 min Scan# 4231

Delta R.T. -0.12 min

Lab File: BE093269.D

Acq: 20 Jun 2017 2:34


Tgt Ion:278 Resp: 4012

Ion Ratio Lower Upper

278 100

139 25.8 17.4 26.0



279 38.6 25.9 38.9






Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

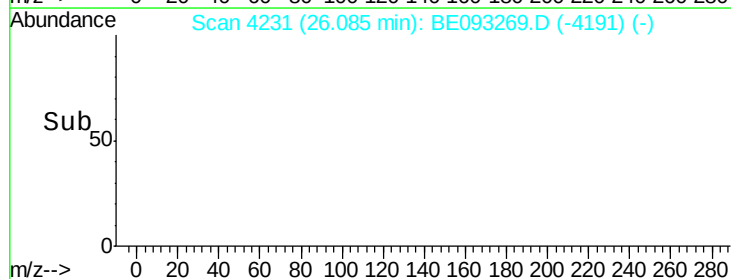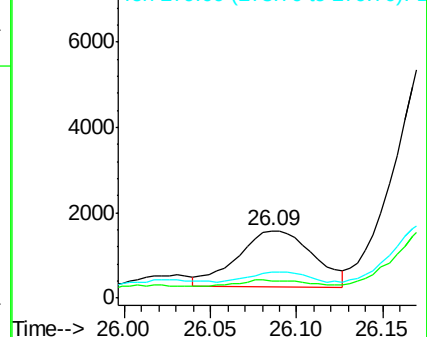

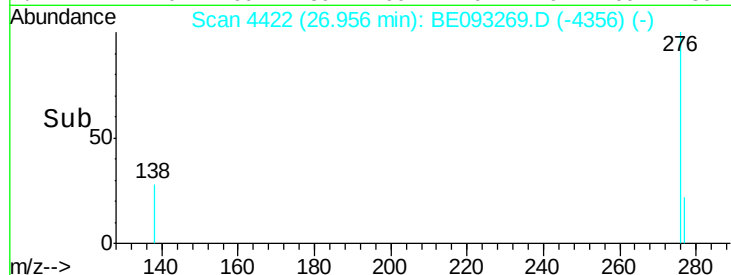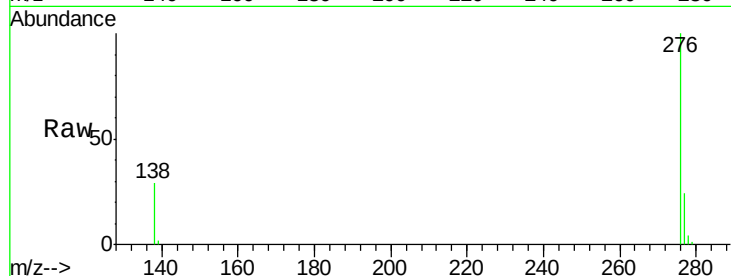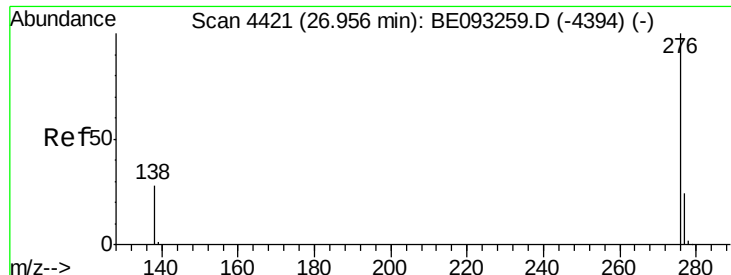

#26
Benzo(a,h,i)perylene
Concen: 1.29 ng/ul
RT: 26.96 min Scan# 4422
Delta R.T. 0.00 min
Lab File: BE093269.D
Acq: 20 Jun 2017 2:34

Instrument :
BNA_E
ClientSampleId :

Tot Ion:	276	Resp:	79774
Ion Ratio	Lower	Upper	
276	100		
138	29.2	21.8	32.8
277	24.3	20.5	30.7

