

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
 Data File : BE093272.D
 Acq On : 20 Jun 2017 4:24
 Operator : SJ/MA
 Sample : I3599-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jun 20 08:51:34 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2319	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	11748	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	7109	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	16657	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	17728	0.40	ng/ul	0.00
20) Perylene-d12	23.68	264	18980	0.40	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	2790	0.16	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	7509	0.17	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.56	128	77626	2.66	ng/ul#	91
5) 2-Methylnaphthalene	12.18	142	14505	0.73	ng/ul	99
7) Acenaphthylene	14.09	152	164104	5.38	ng/ul	95
8) Acenaphthene	14.42	153	14584	0.59	ng/ul	97
9) Fluorene	15.42	166	18231	0.63	ng/ul	93
11) Pentachlorophenol	16.77	266	47	0.02	ng/ul#	31
12) Phenanthrene	17.14	178	212386	4.63	ng/ul#	88
13) Anthracene	17.22	178	314915	7.89	ng/ul#	87
15) Fluoranthene	19.16	202	1823420	32.44	ng/ul	83
17) Pyrene	19.52	202	2275431	43.52	ng/ul#	90
18) Benzo(a)anthracene	21.25	228	1175149	24.85	ng/ul#	84
19) Chrysene	21.30	228	1498925	30.56	ng/ul	97
21) Benzo(b)fluoranthene	22.96	252	3499239	60.75	ng/ul	88
22) Benzo(k)fluoranthene	23.13	252	325338	5.32	ng/ul	95
23) Benzo(a)pyrene	23.58	252	1210954	22.23	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	26.21	276	826069	13.10	ng/ul#	87
25) Dibenzo(a,h)anthracene	26.21	278	246477	4.64	ng/ul	93
26) Benzo(g,h,i)perylene	26.99	276	510577	9.44	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE061917\
Data File : BE093272.D
Acq On : 20 Jun 2017 4:24
Operator : SJ/MA
Sample : I3599-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jun 20 08:51:34 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

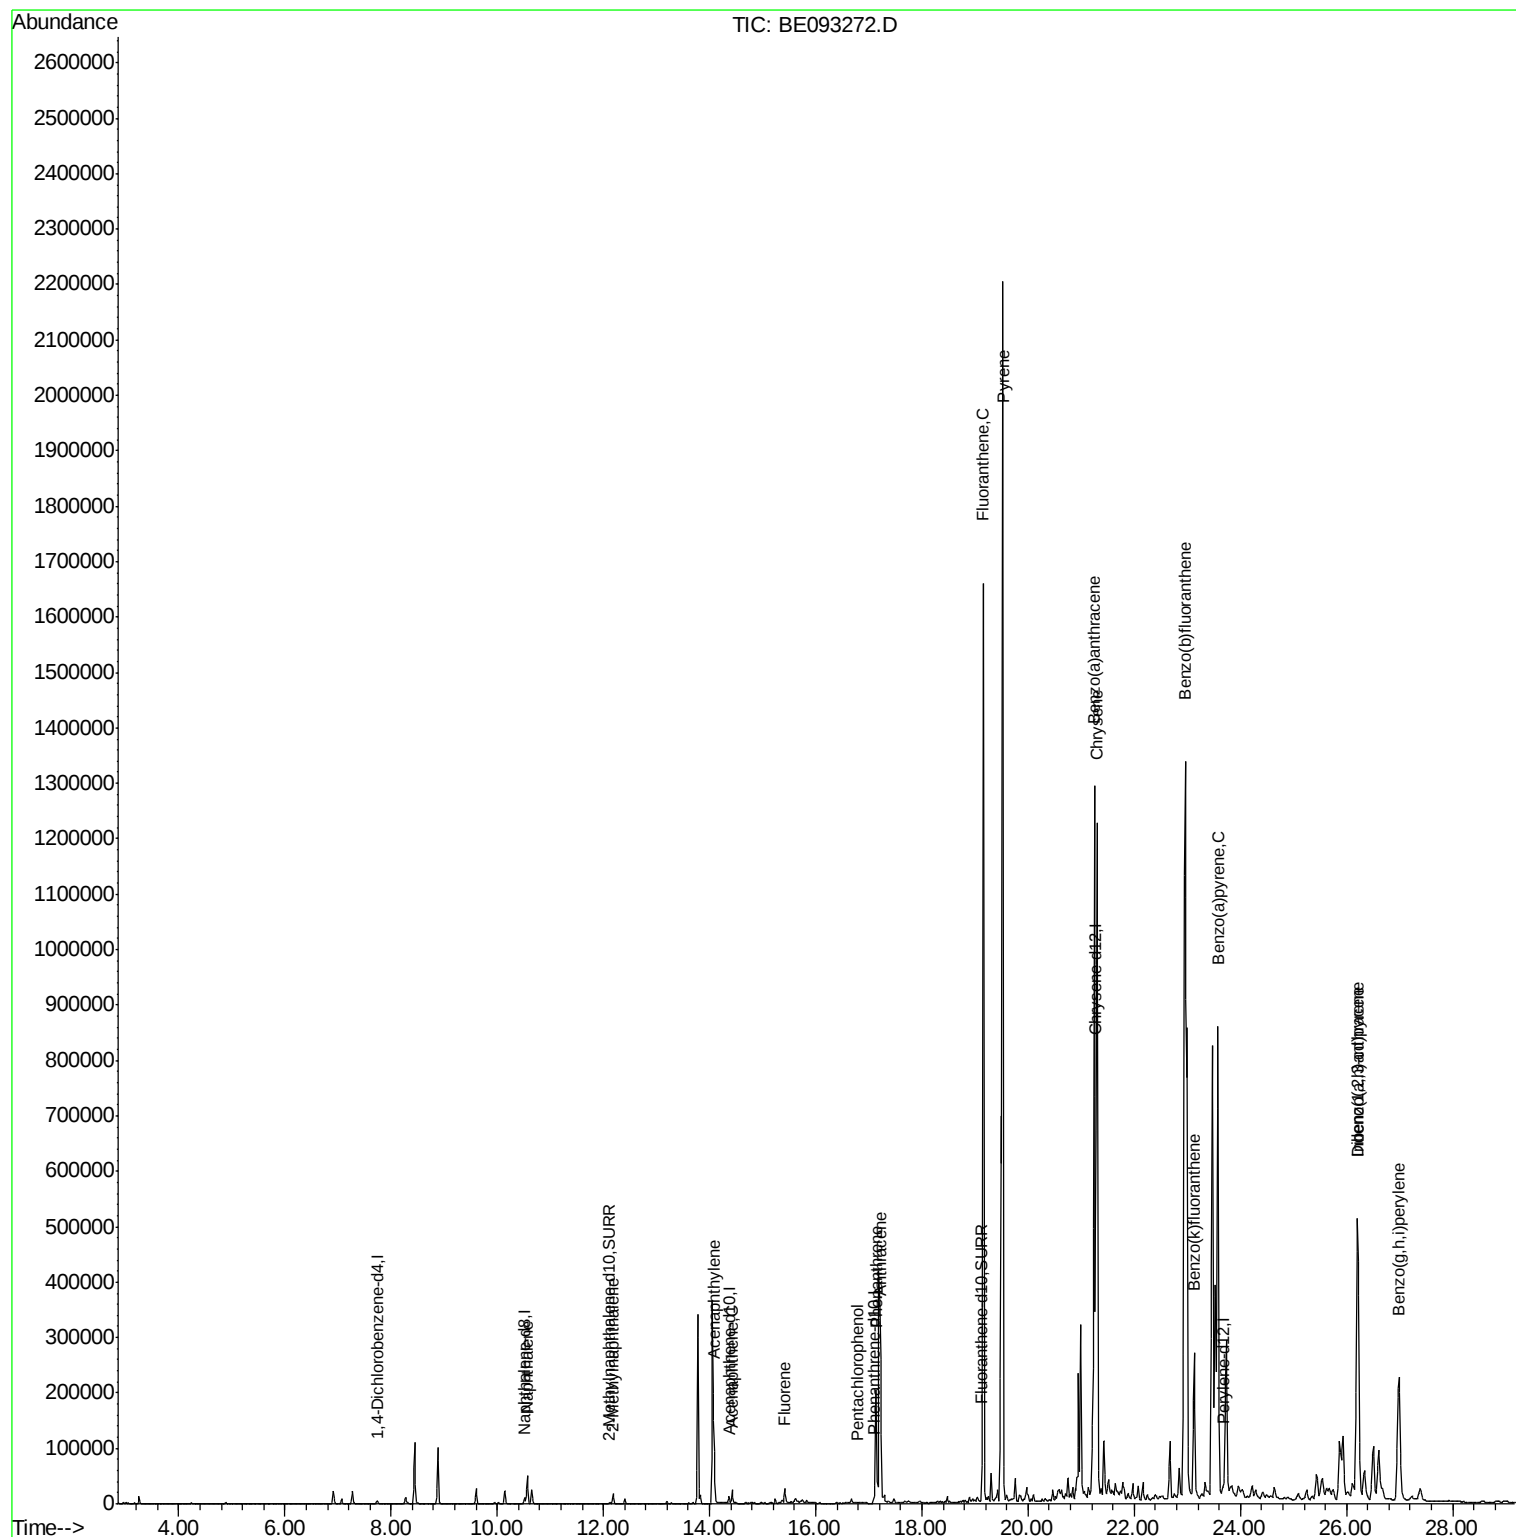

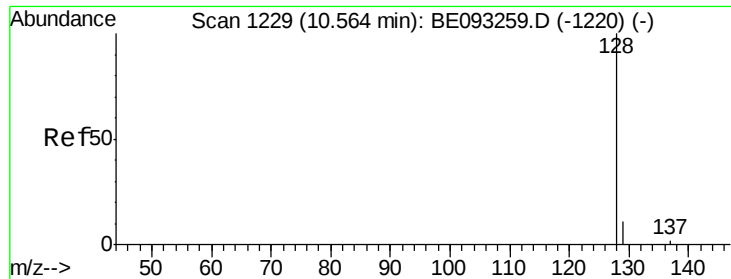

#3

Naphthalene

Concen: 2.66 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :





Tot Ion:128 Resp: 77626

Ion Ratio Lower Upper

128 100

129 11.1 11.3 16.9#

127 0.0 4.0 6.0#

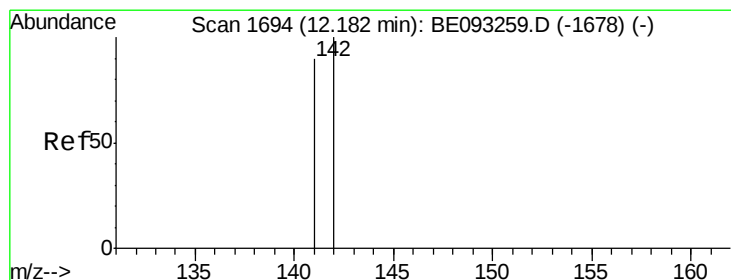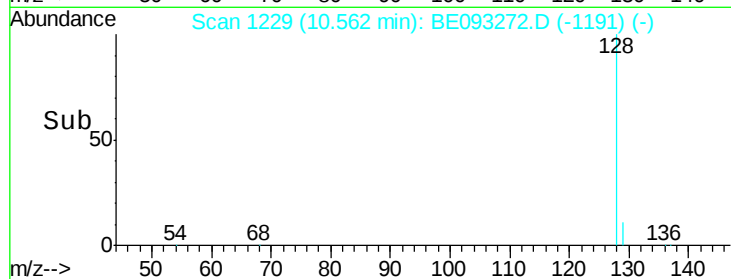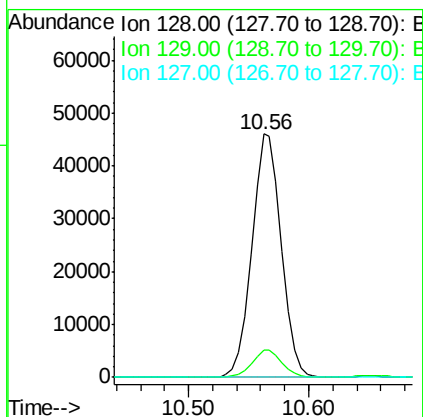

#5

2-Methylnaphthalene

Concen: 0.73 ng/ul

RT: 12.18 min Scan# 1694

Delta R.T. -0.00 min

Lab File: BE093272.D




Acq: 20 Jun 2017 4:24


Tgt Ion:142 Resp: 14505

Ion Ratio Lower Upper

142 100

141 89.5 72.6 108.8

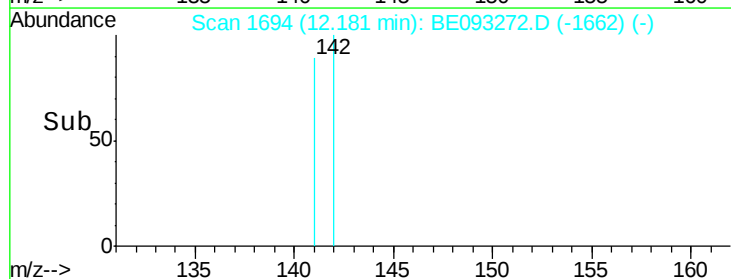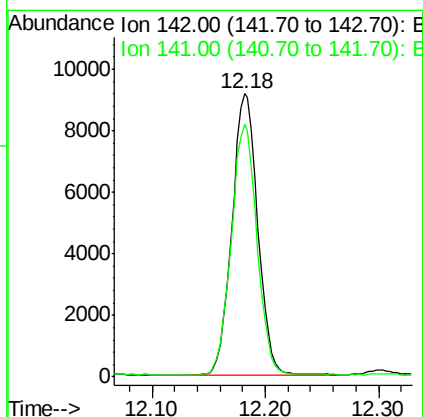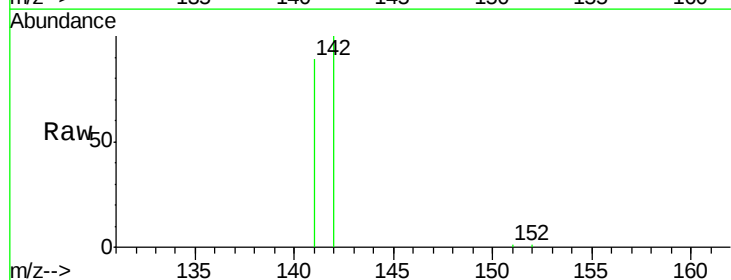



#7

Acenaphthylene

Concen: 5.38 ng/ul

RT: 14.09 min Scan# 2103

Delta R.T. 0.00 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 164104

Ion Ratio Lower Upper

152 100

151 19.6 17.1 25.7




153 13.4 12.8 19.2



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

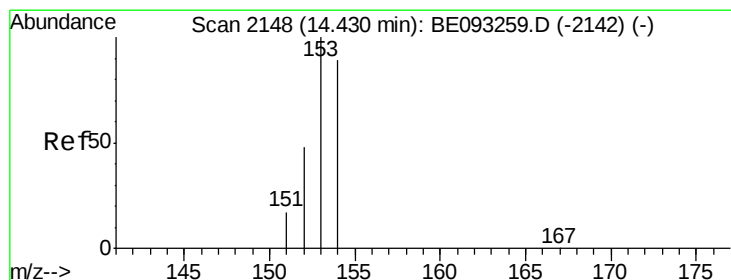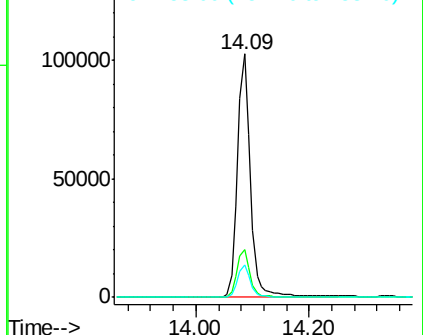

#8

Acenaphthene

Concen: 0.59 ng/ul

RT: 14.42 min Scan# 2148

Delta R.T. -0.01 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24


Tgt Ion:153 Resp: 14584

Ion Ratio Lower Upper

153 100

152 51.3 40.3 60.5



154 84.9 71.4 107.2




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

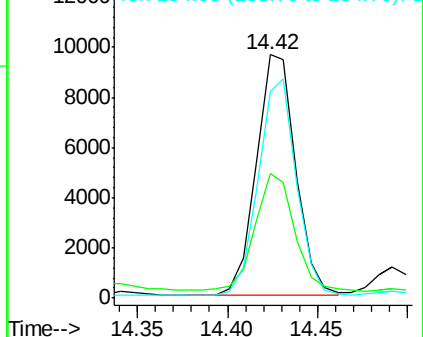



#9

Fluorene

Concen: 0.63 ng/ul

RT: 15.42 min Scan# 2280

Delta R.T. 0.00 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 18231

Ion Ratio Lower Upper

166 100

165 98.9 73.4 110.2

167 15.0 14.6 22.0

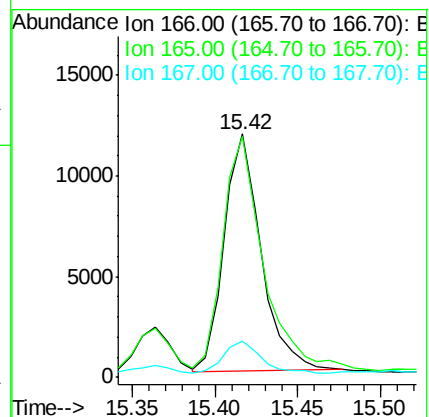

#11

Pentachlorophenol

Concen: 0.02 ng/ul

RT: 16.77 min Scan# 2401

Delta R.T. 0.02 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24




Tgt Ion:266 Resp: 47


Ion Ratio Lower Upper

266 100

264 17.0 47.9 71.9#

268 0.0 49.8 74.8#

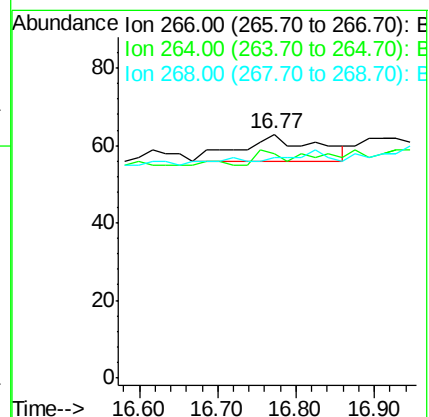

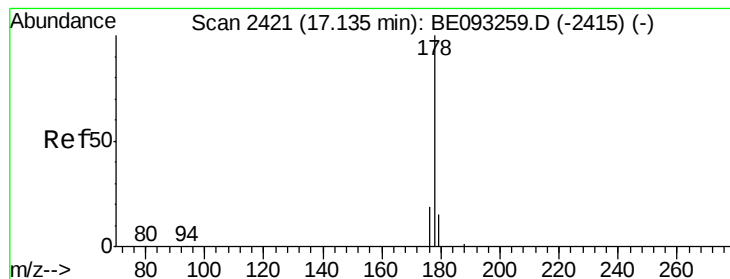

#12

Phenanthrene

Concen: 4.63 ng/ul

RT: 17.14 min Scan# 2422

Delta R.T. 0.00 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 212386

Ion Ratio Lower Upper

178 100

179 15.1 18.4 27.6#




176 19.4 13.6 20.4

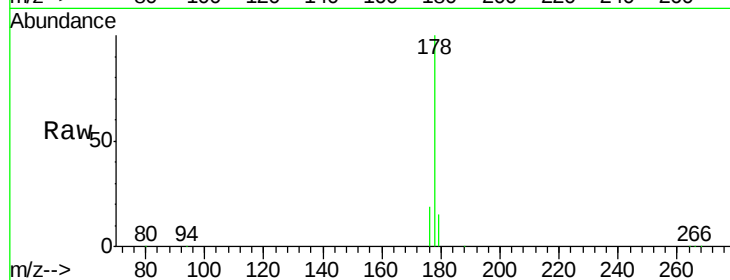

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

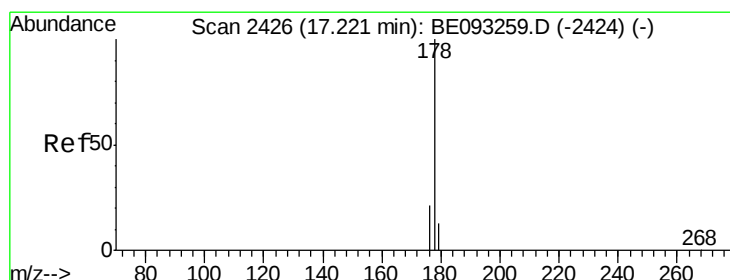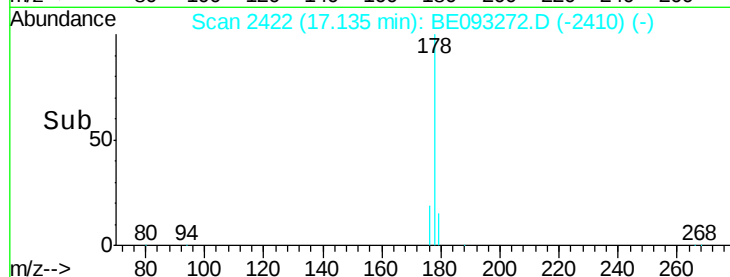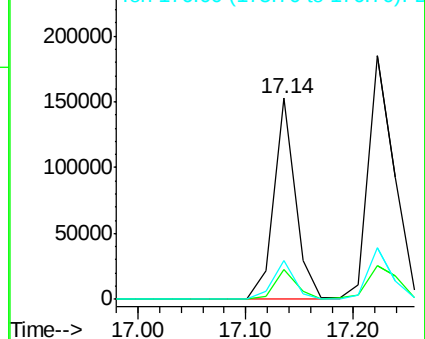

#13

Anthracene

Concen: 7.89 ng/ul

RT: 17.22 min Scan# 2427

Delta R.T. 0.00 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24


Tgt Ion:178 Resp: 314915

Ion Ratio Lower Upper

178 100

179 13.6 18.1 27.1#



176 21.3 14.7 22.1

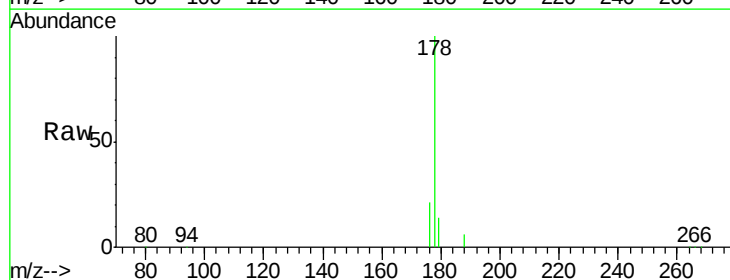


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



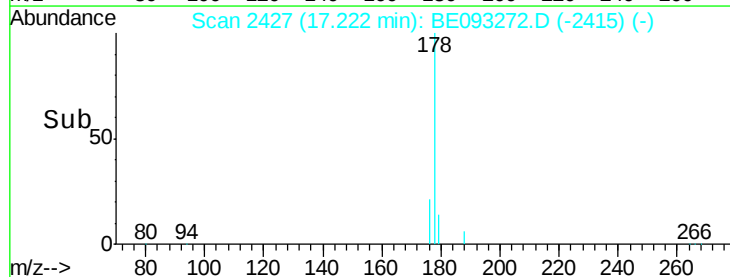
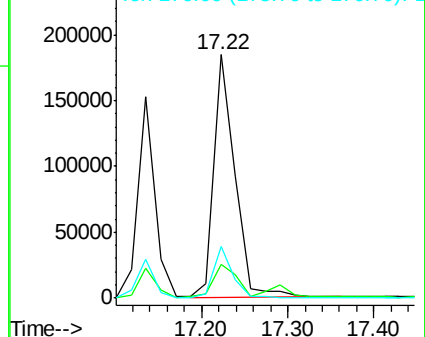


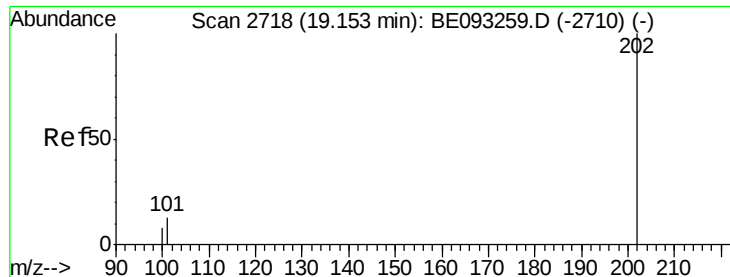

#15
Fluoranthene
Concen: 32.44 ng/ul
RT: 19.16 min Scan# 2720
Delta R.T. 0.01 min
Lab File: BE093272.D
Acq: 20 Jun 2017 4:24




Instrument :
BNA_E
ClientSampleId :


Tot Ion:202 Resp: 1823420
Ion Ratio Lower Upper
202 100
101 13.8 0.0 30.3
100 10.1 0.0 39.5

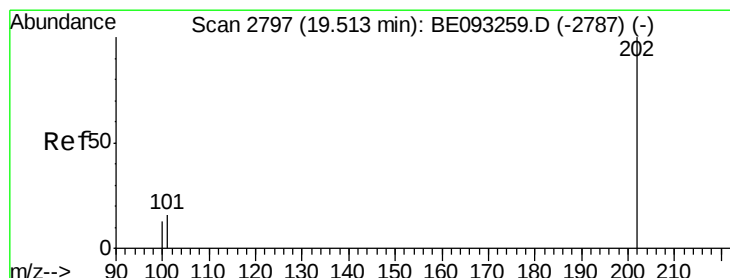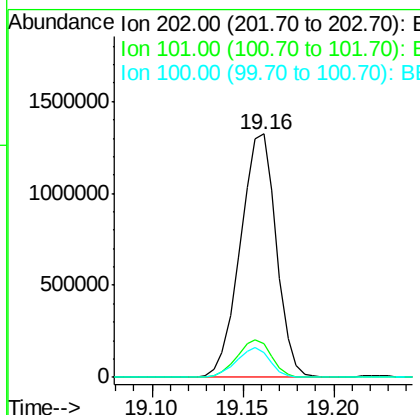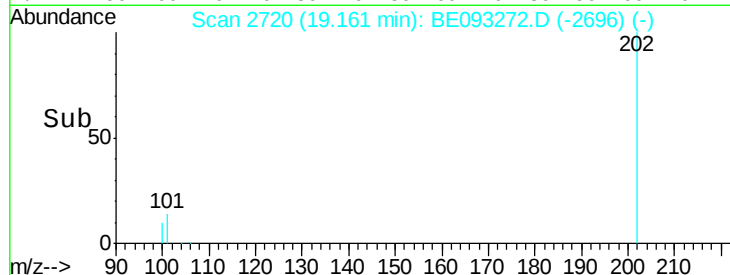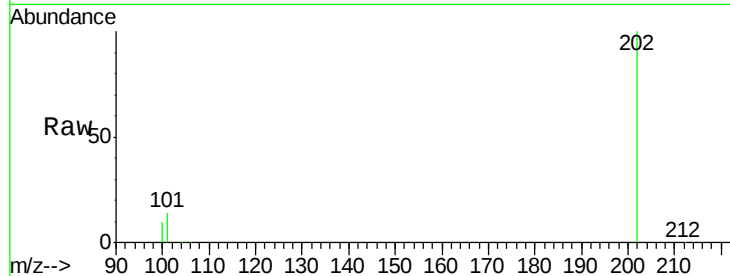

#17
Pyrene
Concen: 43.52 ng/ul
RT: 19.52 min Scan# 2799
Delta R.T. 0.01 min
Lab File: BE093272.D
Acq: 20 Jun 2017 4:24

Tgt Ion:202 Resp: 2275431
Ion Ratio Lower Upper
202 100
101 18.0 18.2 27.4#
100 14.9 15.6 23.4#

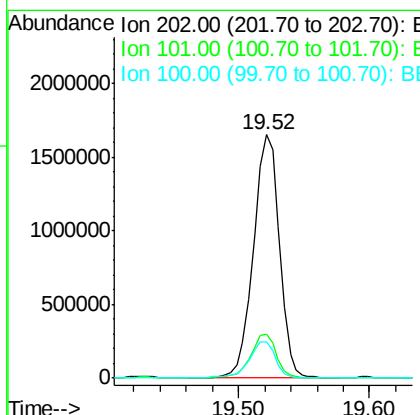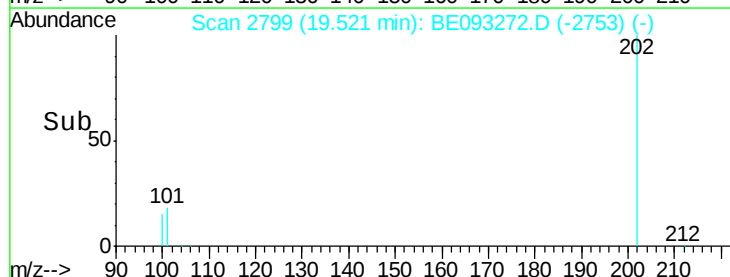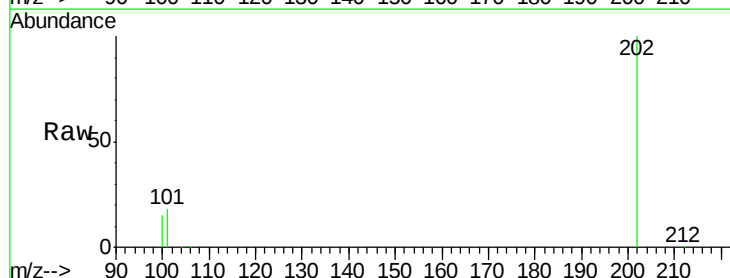



#18

Benzo(a)anthracene

Concen: 24.85 ng/ul

RT: 21.25 min Scan# 3175

Delta R.T. 0.01 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 1175149

Ion Ratio Lower Upper




228 100

229 21.8 22.8 34.2#

226 30.9 17.0 25.6#

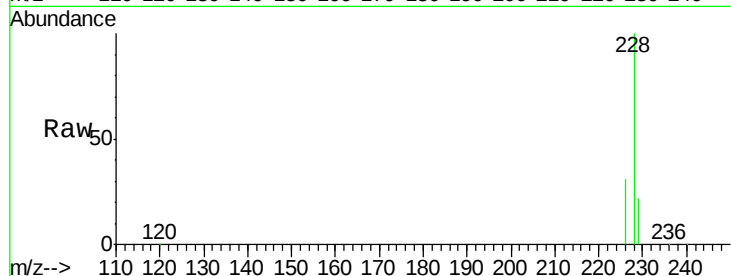

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

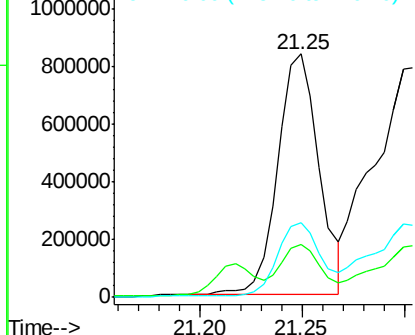

#19

Chrysene

Concen: 30.56 ng/ul

RT: 21.30 min Scan# 3187

Delta R.T. 0.01 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24


Tgt Ion:228 Resp: 1498925

Ion Ratio Lower Upper



228 100


226 31.6 23.4 35.0

229 22.5 17.7 26.5



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

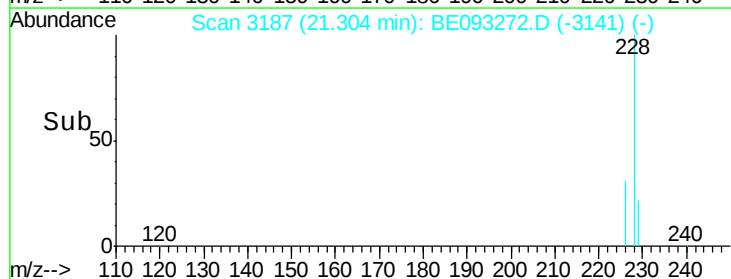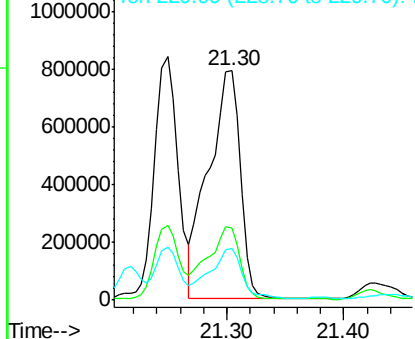

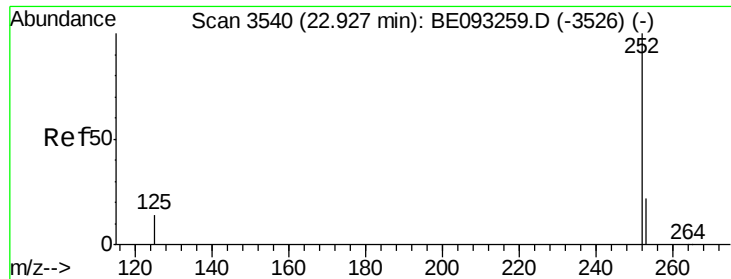

#21

Benzo(b)fluoranthene

Concen: 60.75 ng/ul

RT: 22.96 min Scan# 3547

Delta R.T. 0.03 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 3499239

Ion Ratio Lower Upper




252 100

253 23.1 0.0 64.2

125 15.8 0.0 35.0



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

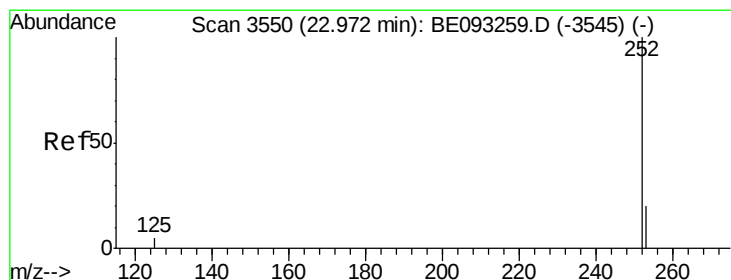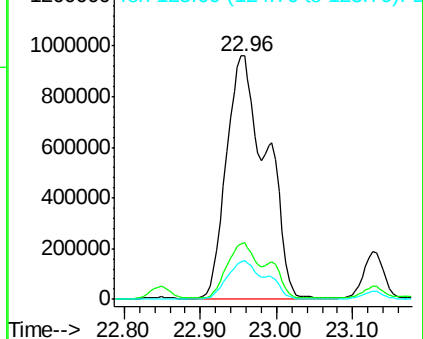

#22

Benzo(k)fluoranthene

Concen: 5.32 ng/ul

RT: 23.13 min Scan# 3584

Delta R.T. 0.15 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24


Tgt Ion:252 Resp: 325338

Ion Ratio Lower Upper



252 100


253 26.7 24.5 36.7

125 17.7 13.7 20.5



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

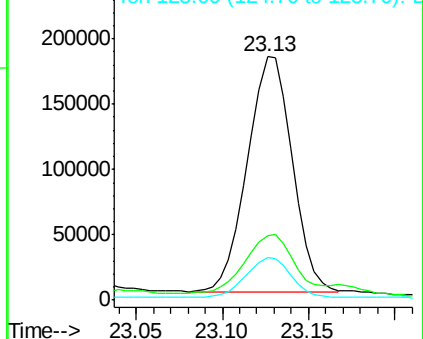

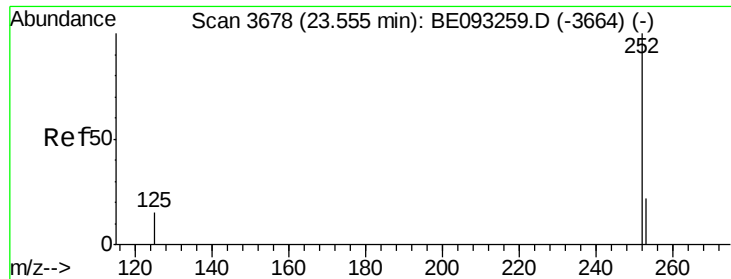

#23

Benzo(a)pyrene

Concen: 22.23 ng/ul

RT: 23.58 min Scan# 3683

Delta R.T. 0.02 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 1210954

Ion Ratio Lower Upper




252 100

253 23.5 28.5 42.7#

125 15.8 18.1 27.1#

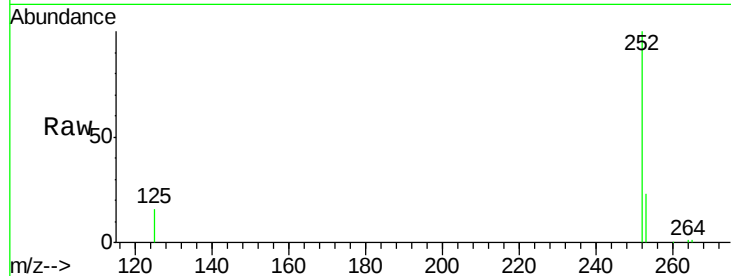

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

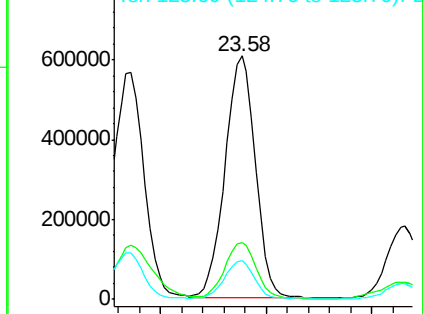

#24

Indeno(1,2,3-cd)pyrene

Concen: 13.10 ng/ul

RT: 26.21 min Scan# 4257

Delta R.T. 0.03 min

Lab File: BE093272.D

Acq: 20 Jun 2017 4:24


Tgt Ion:276 Resp: 826069

Ion Ratio Lower Upper



276 100


138 30.0 28.0 42.0

227 0.0 8.0 12.0#



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 227.00 (226.70 to 227.70): E

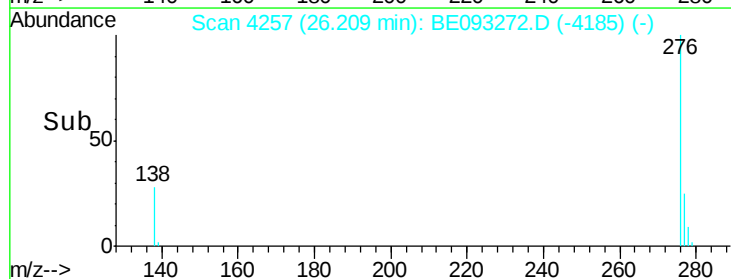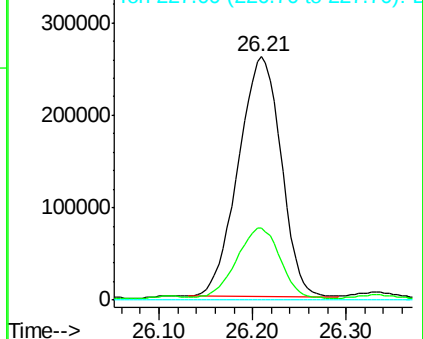




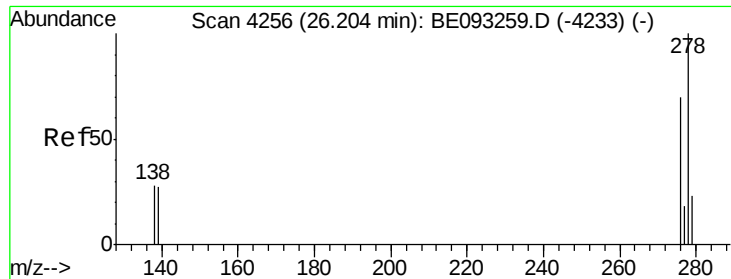


#25
Dibenzo(a,h)anthracene
Concen: 4.64 ng/ul
RT: 26.21 min Scan# 4258
Delta R.T. 0.01 min
Lab File: BE093272.D
Acq: 20 Jun 2017 4:24

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 246477

Ion	Ratio	Lower	Upper
278	100		
139	22.8	17.4	26.0
279	26.9	25.9	38.9

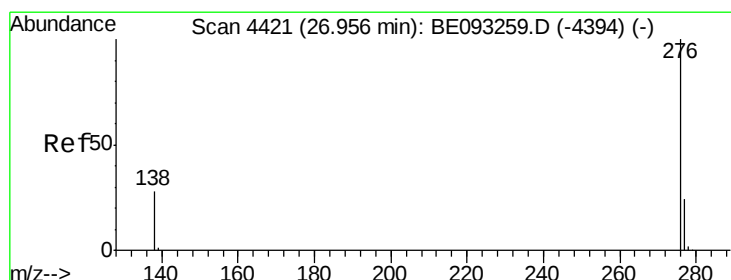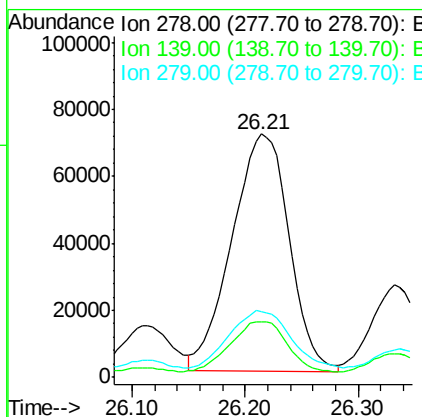

#26
Benzo(g,h,i)perylene
Concen: 9.44 ng/ul
RT: 26.99 min Scan# 4428
Delta R.T. 0.03 min
Lab File: BE093272.D
Acq: 20 Jun 2017 4:24

Tgt Ion:276 Resp: 510577

Ion	Ratio	Lower	Upper
276	100		
138	29.2	21.8	32.8
277	24.3	20.5	30.7

