

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093244.D
 Acq On : 19 Jun 2017 11:09
 Operator : SJ/MA
 Sample : PB99688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP71

Quant Time: Jun 20 04:18:58 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:12 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2335	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12212	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7734	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	18751	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	1325749	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6419	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	17573	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.36	166	2123	0.068	ng/ul#	20
17) Pyrene	19.49	202	2522	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093244.D
Acq On : 19 Jun 2017 11:09
Operator : SJ/MA
Sample : PB99688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP71

Quant Time: Jun 20 04:18:58 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:12 2017
Response via : Initial Calibration

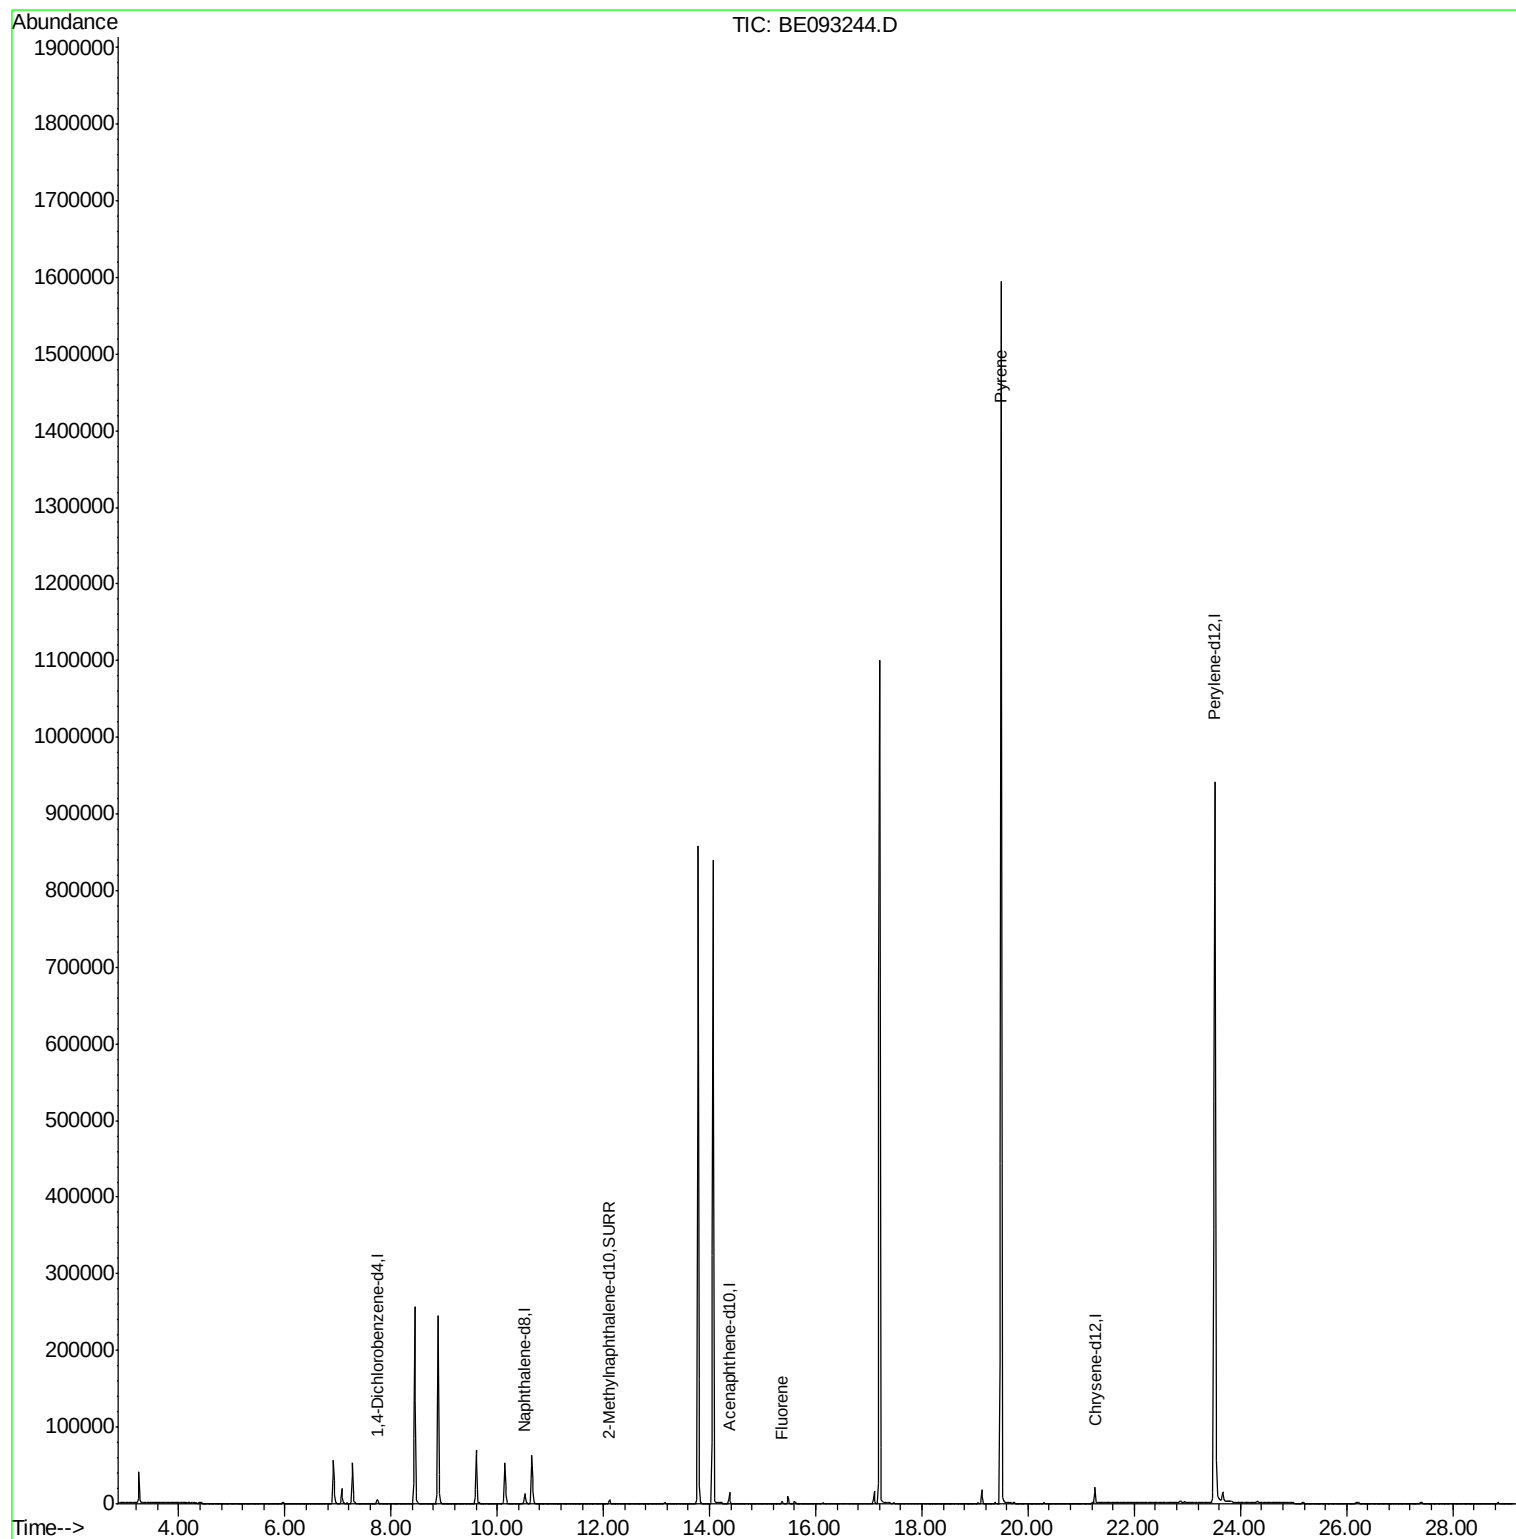

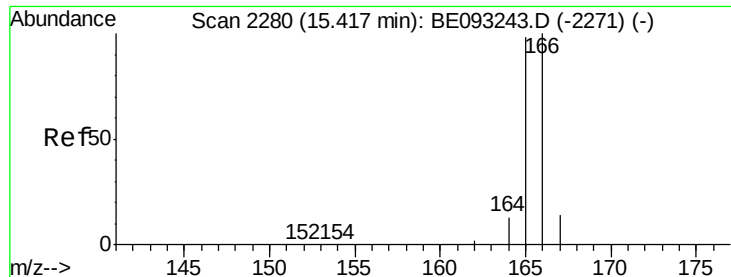

#9

Fluorene

Concen: 0.068 ng/ul

RT: 15.36 min Scan# 2273

Delta R.T. -0.05 min

Lab File: BE093244.D

Acq: 19 Jun 2017 11:09

Instrument :

BNA_E

ClientSampleId :

DFTPP71


Tgt Ion:166 Resp: 2123

Ion Ratio Lower Upper

166 100

165 8.2 73.4 110.2#




167 35.8 14.6 22.0#

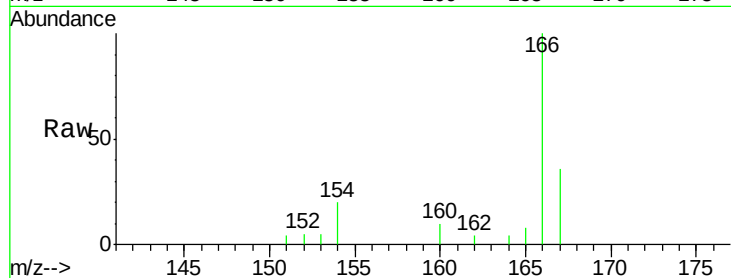

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

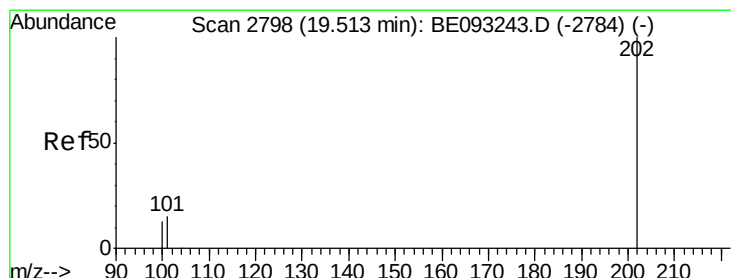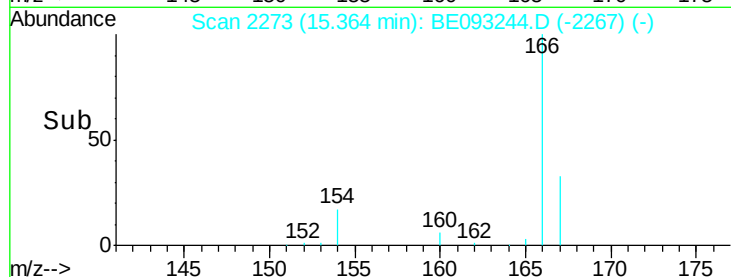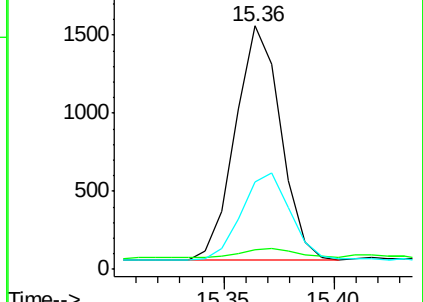

#17

Pyrene

Concen: 0.046 ng/ul

RT: 19.49 min Scan# 2793

Delta R.T. -0.02 min

Lab File: BE093244.D

Acq: 19 Jun 2017 11:09


Tgt Ion:202 Resp: 2522

Ion Ratio Lower Upper

202 100

101 183.2 18.2 27.4#

100 975.1 15.6 23.4#

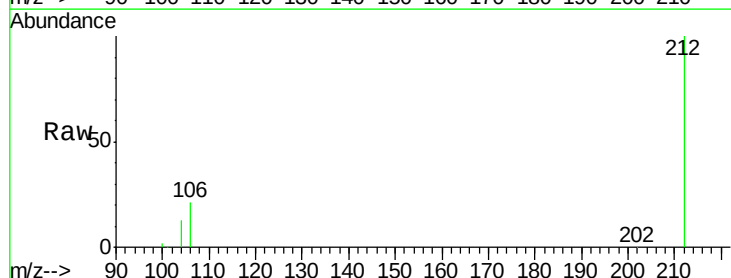

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

