




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093244.D
Acq On : 19 Jun 2017 11:09
Operator : SJ/MA
Sample : PB99688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 04:18:58 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:12 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampled :
SBLK89

Manual Integrations
APPROVED

mohammad
6/20/2017 3:11:58 PM

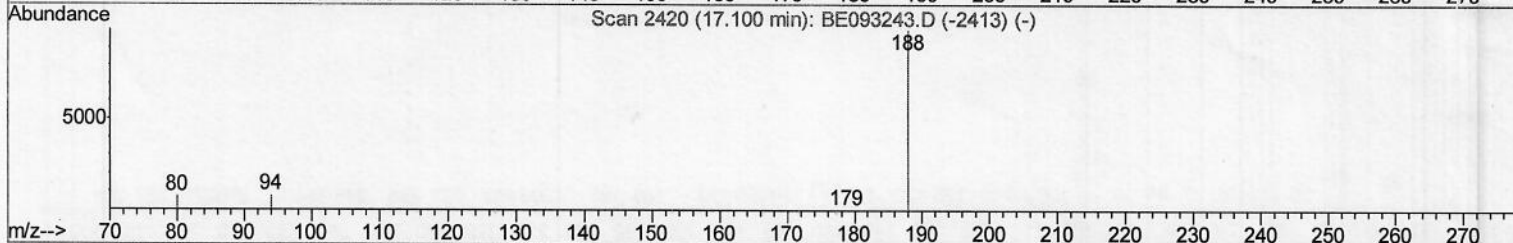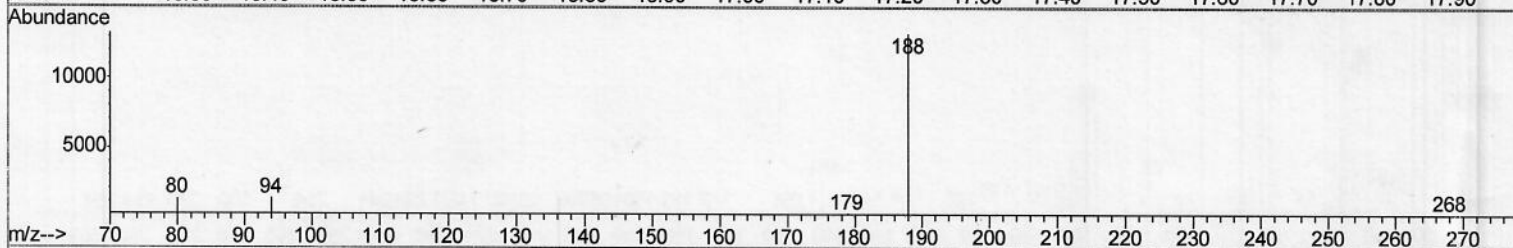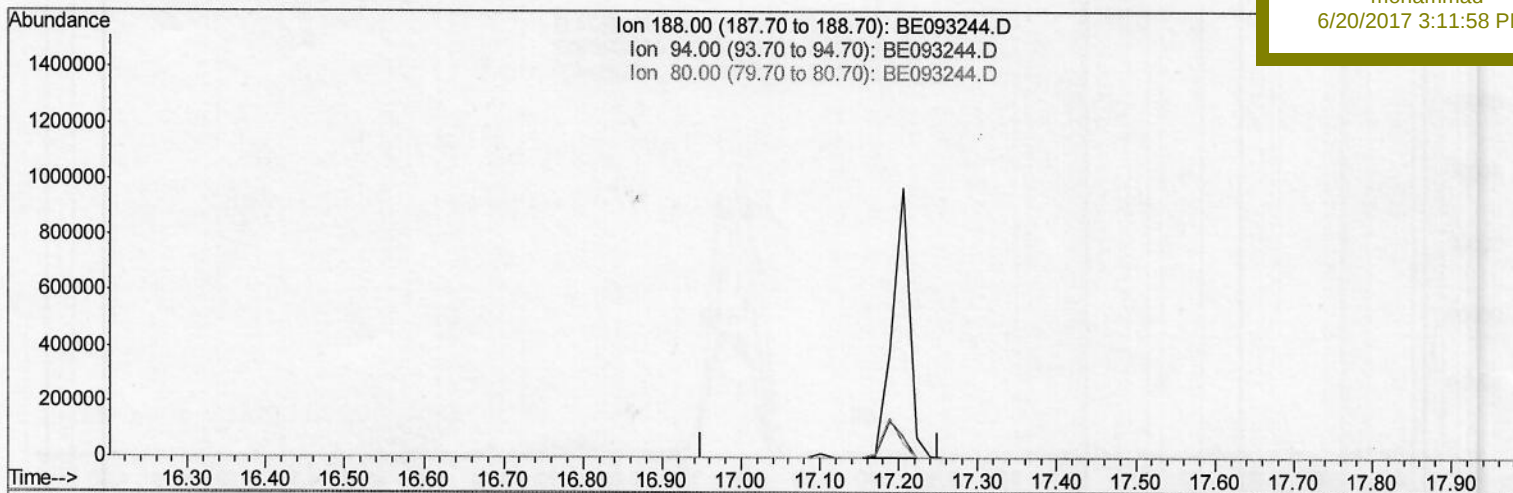

TIC: BE093244.D

(10) Phenanthrene-d10 (I)

17.100min (-17.100) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093244.D
 Acq On : 19 Jun 2017 11:09
 Operator : SJ/MA
 Sample : PB99688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 04:18:58 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:12 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK89

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:11:58 PM

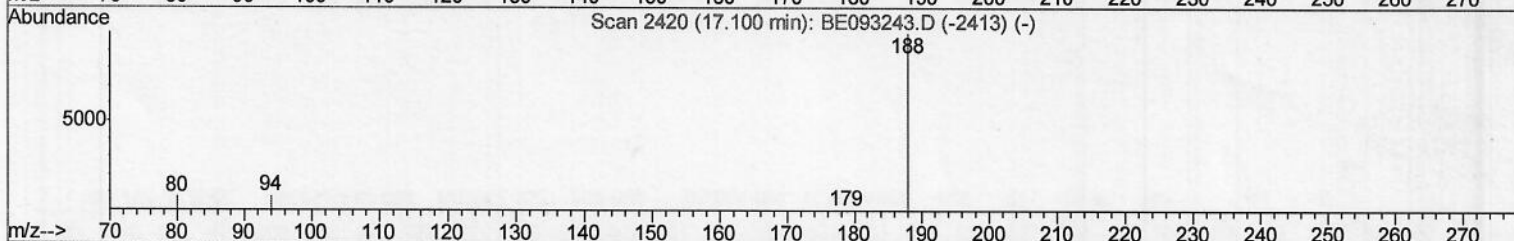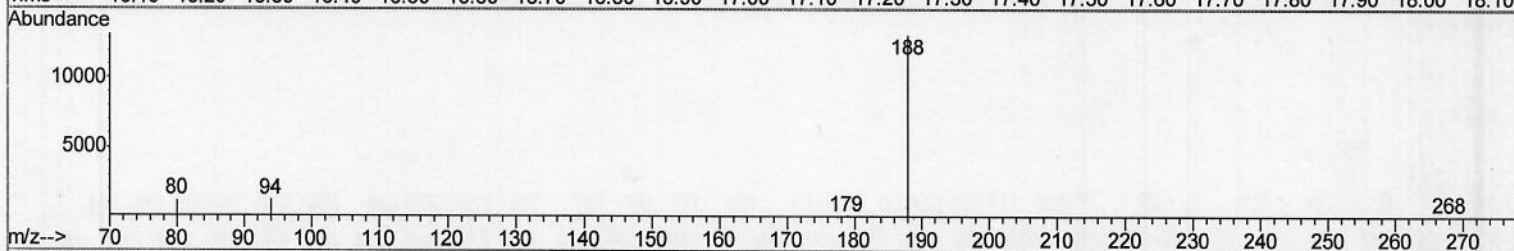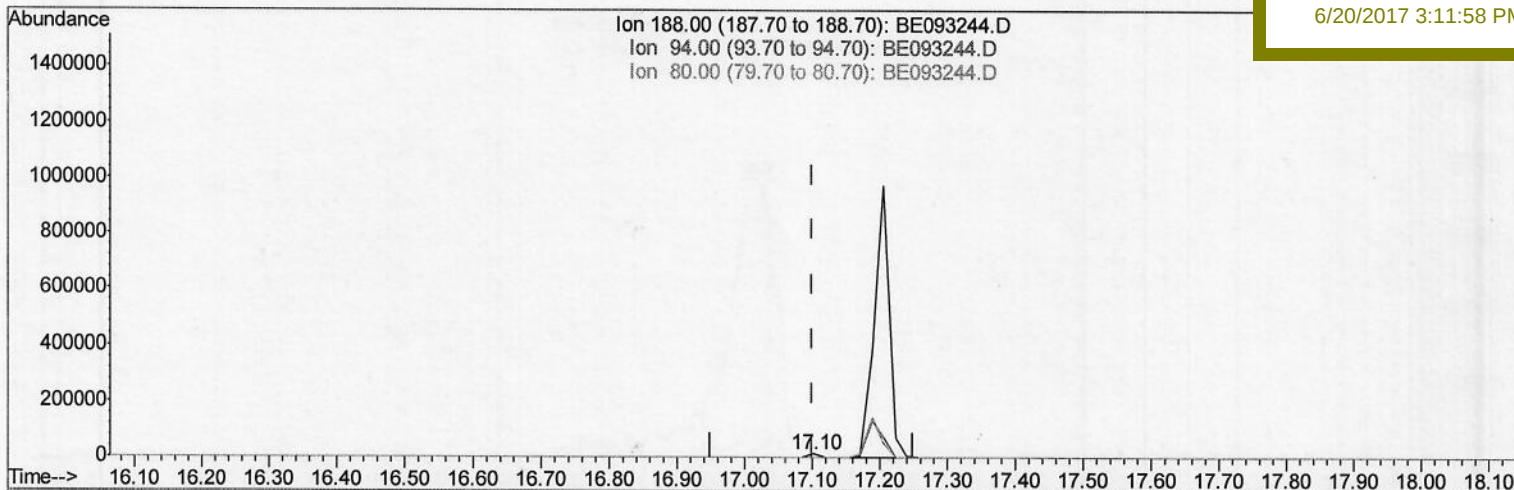

TIC: BE093244.D

(10) Phenanthrene-d10 (I)

17.102min (+0.002) 0.40ng/ul m

response 18495

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.14
80.00	11.80	8.75#
0.00	0.00	0.00

S.J
 06/20/2017

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093244.D
 Acq On : 19 Jun 2017 11:09
 Operator : SJ/MA
 Sample : PB99688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 06:55:30 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:12 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
ClientSampleId :
 SBLK89

Manual Integrations
APPROVED

mohammad
 6/20/2017 3:11:58 PM

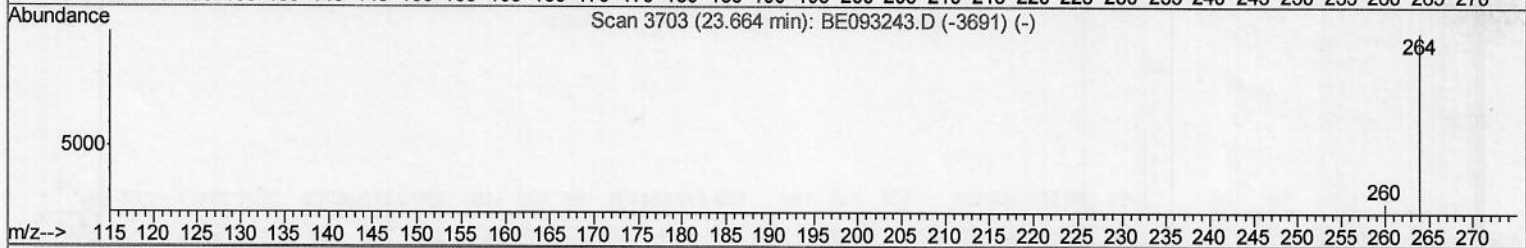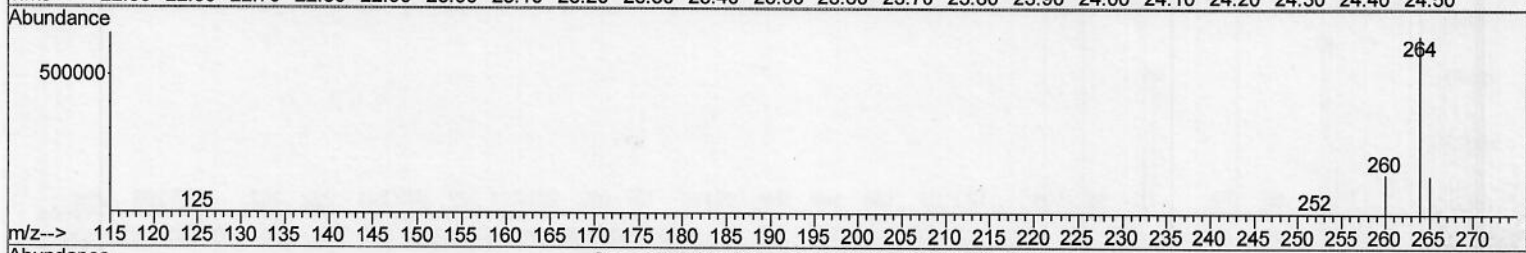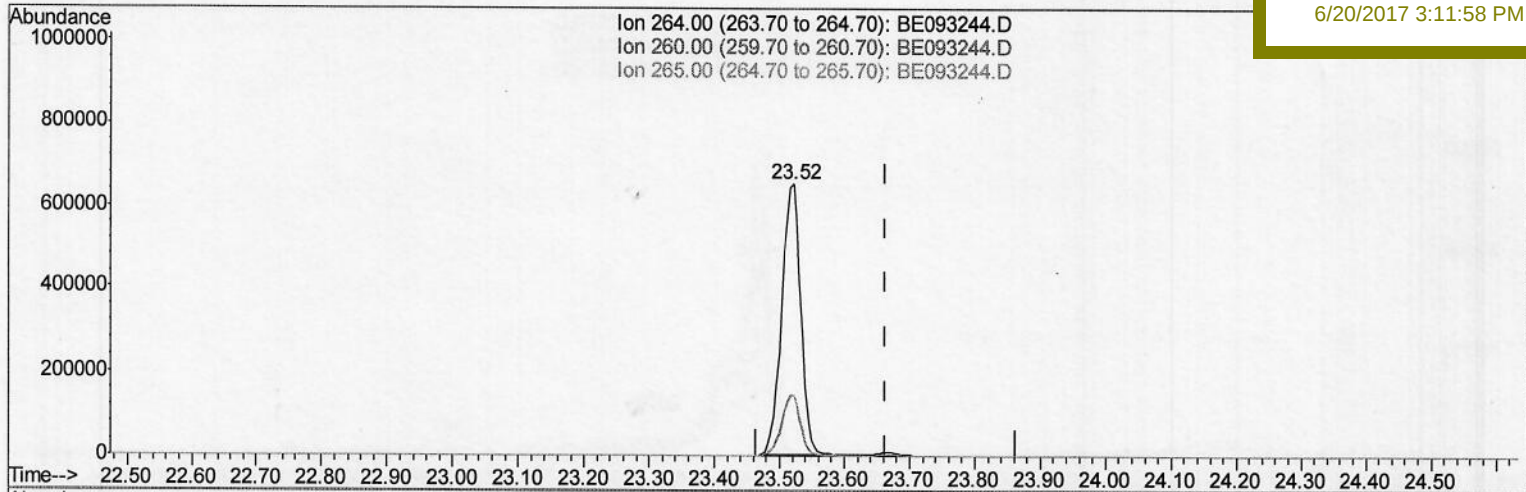

TIC: BE093244.D

(20) Perylene-d12 (I)
 23.522min (-0.142) 0.40ng/ul
 response 1325749

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.77#
265.00	103.50	21.66#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093244.D
 Acq On : 19 Jun 2017 11:09
 Operator : SJ/MA
 Sample : PB99688BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 06:55:30 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:12 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK89

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:11:58 PM

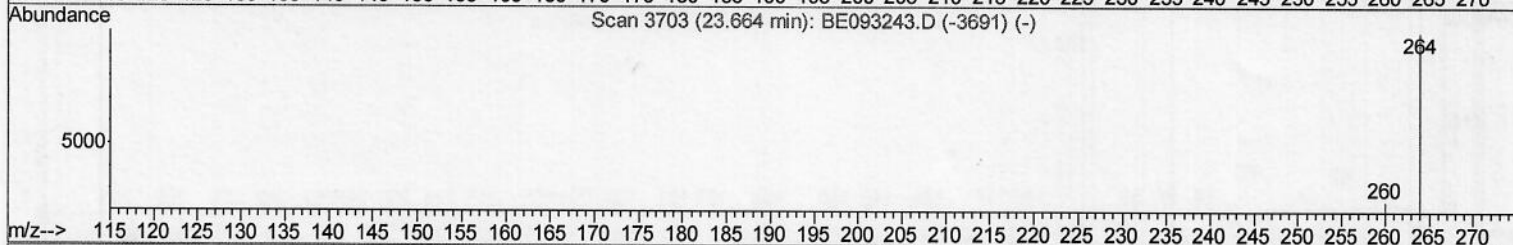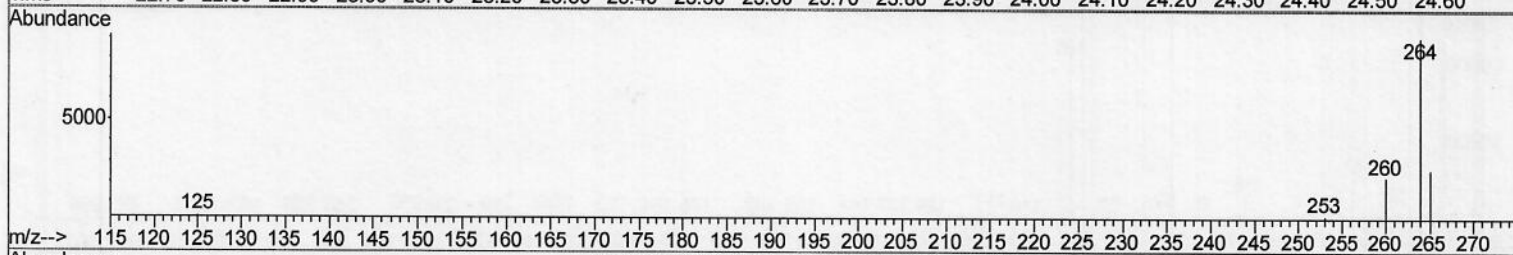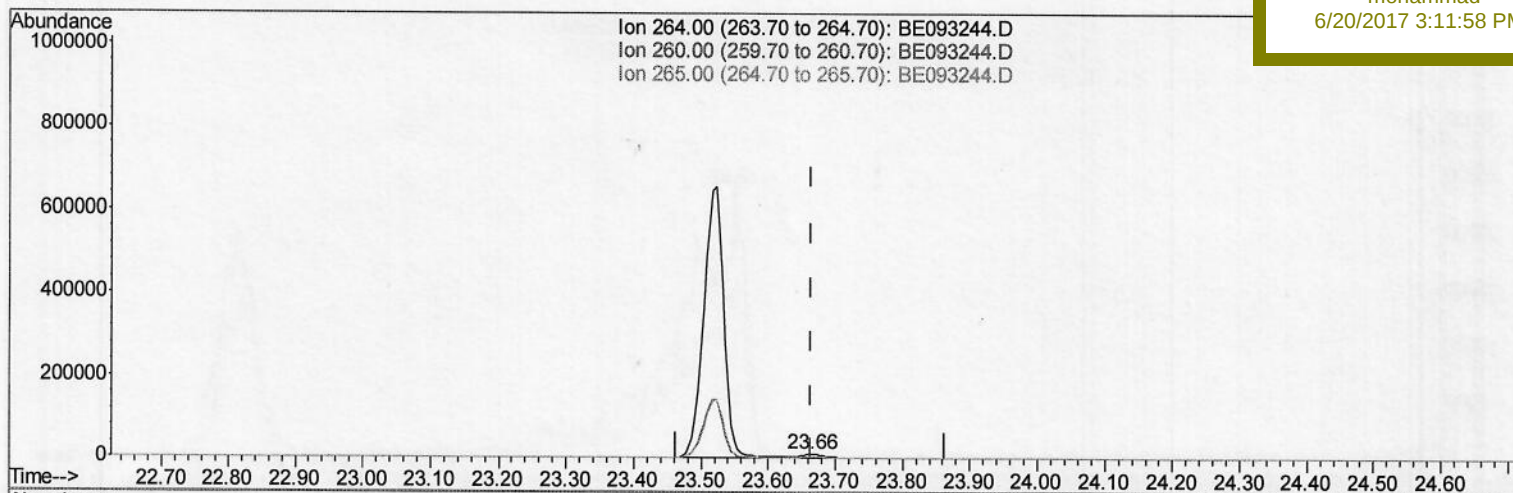

TIC: BE093244.D

(20) Perylene-d12 (I)

23.663min (-0.001) 0.40ng/ul m

response 14987

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.19
265.00	103.50	29.46#
0.00	0.00	0.00

SJ
06/20/2017

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093244.D
Acq On : 19 Jun 2017 11:09
Operator : SJ/MA
Sample : PB99688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 06:56:54 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:12 2017
Response via : Initial Calibration

Instrument :
BNA_E
Client Sample ID :
SBLK89

Manual Integrations
APPROVED

mohammad
6/20/2017 3:11:58 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2335	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12212	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7734	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	18495m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18751	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	14987m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6419	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	17573	0.35	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

39.5
06/20/2017

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093244.D
Acq On : 19 Jun 2017 11:09
Operator : SJ/MA
Sample : PB99688BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 20 06:56:54 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:12 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK89

Manual Integrations
APPROVED

mohammad
6/20/2017 3:11:58 PM

