

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093246.D
 Acq On : 19 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3599-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampleId :
 F5A74

Quant Time: Jun 20 04:19:12 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 6/20/2017 3:12:04 PM

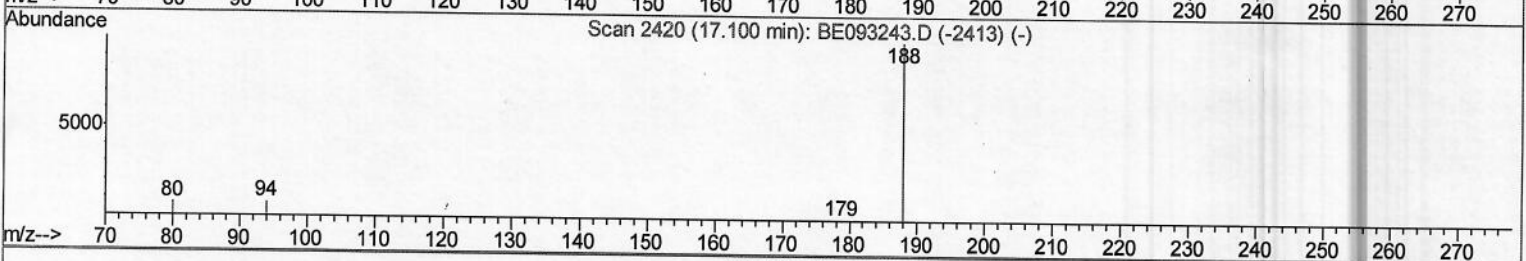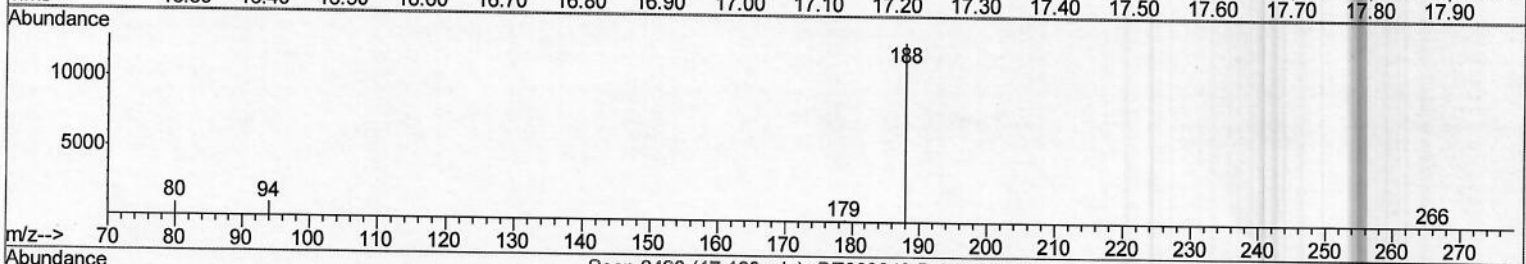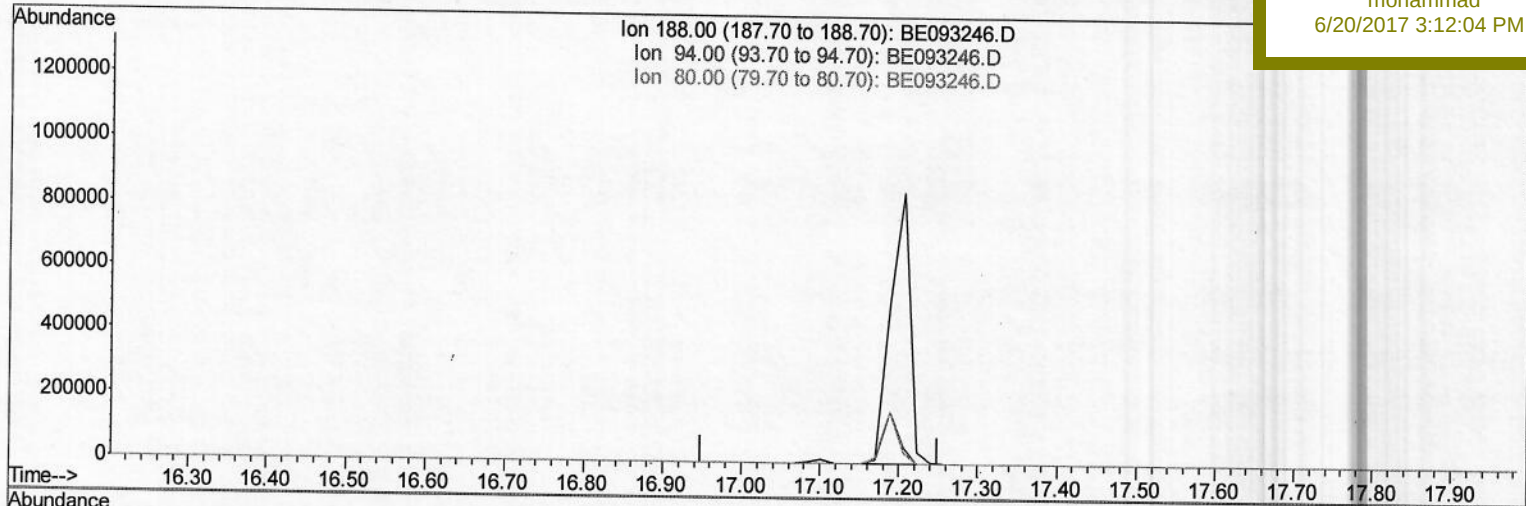

TIC: BE093246.D

(10) Phenanthrene-d10 (I)
 17.100min (-17.100) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093246.D
 Acq On : 19 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3599-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 20 04:19:12 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5A74

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:04 PM

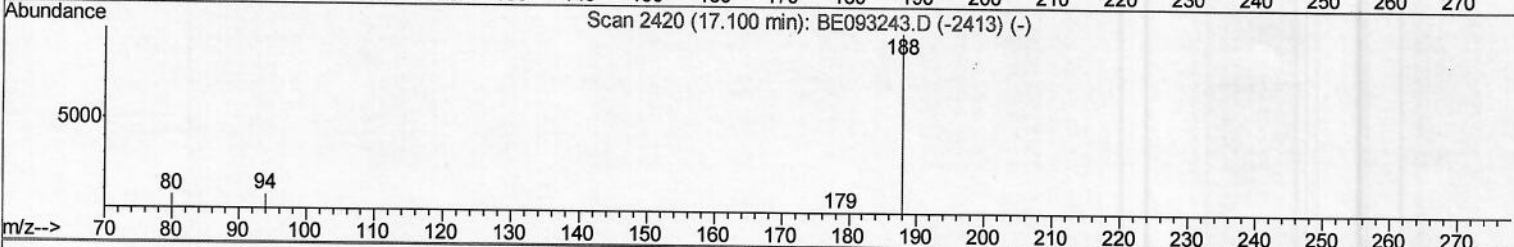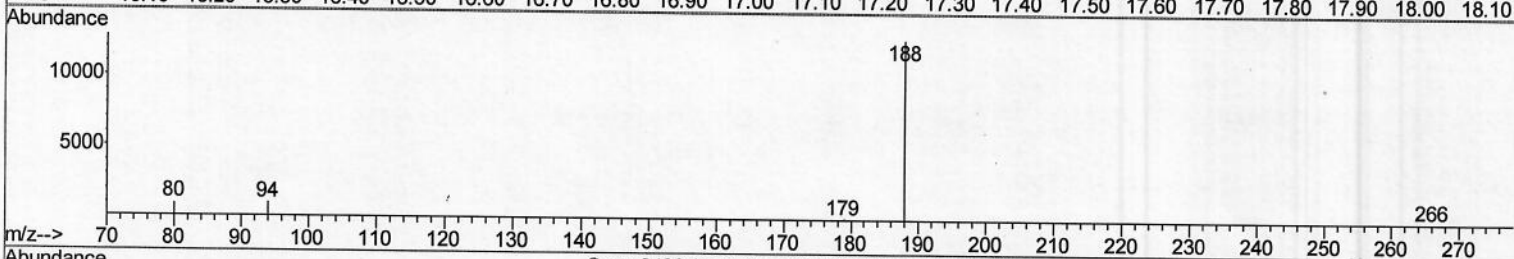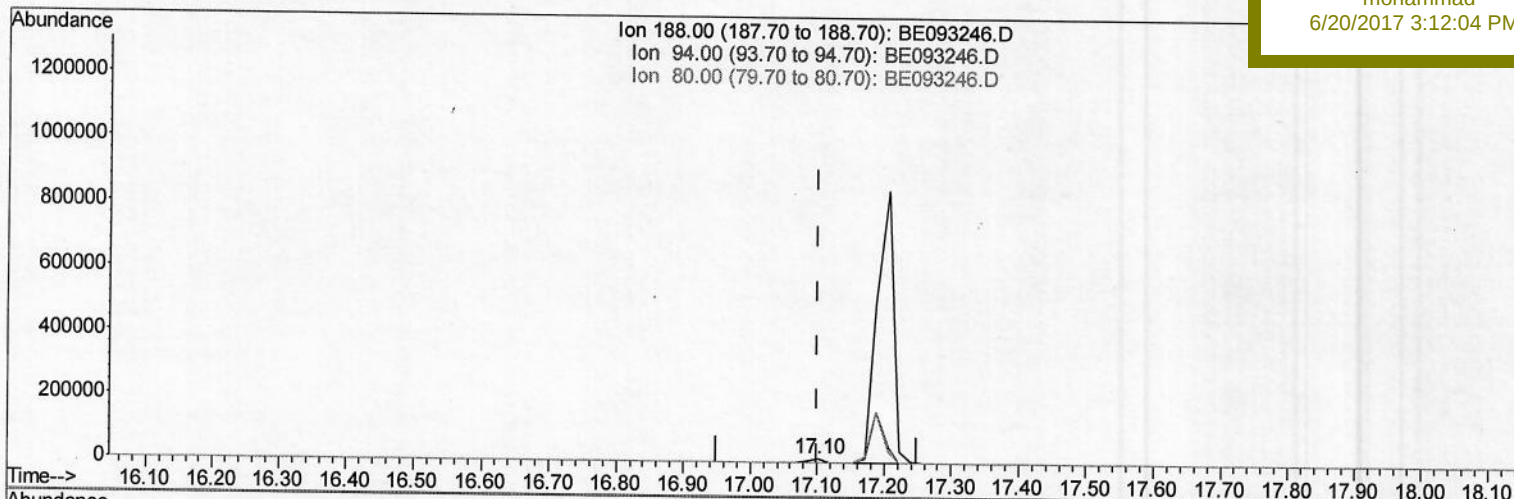

TIC: BE093246.D

(10) Phenanthrene-d10 (I)

17.101min (+0.001) 0.40ng/ul m

response 18309

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.79#
80.00	11.80	7.30#
0.00	0.00	0.00

SJ
06/20/2017

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093246.D
 Acq On : 19 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3599-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 20 04:19:12 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5A74

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:04 PM

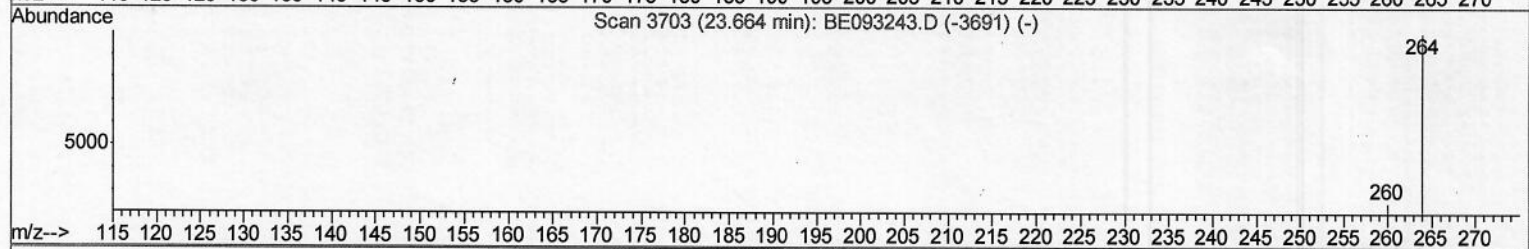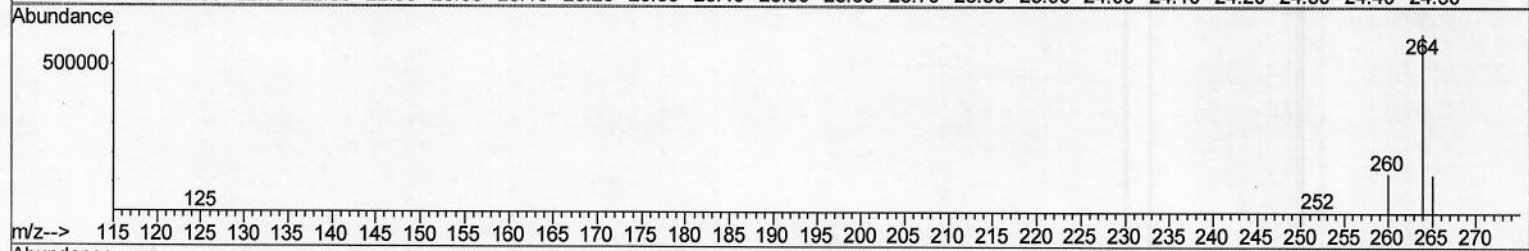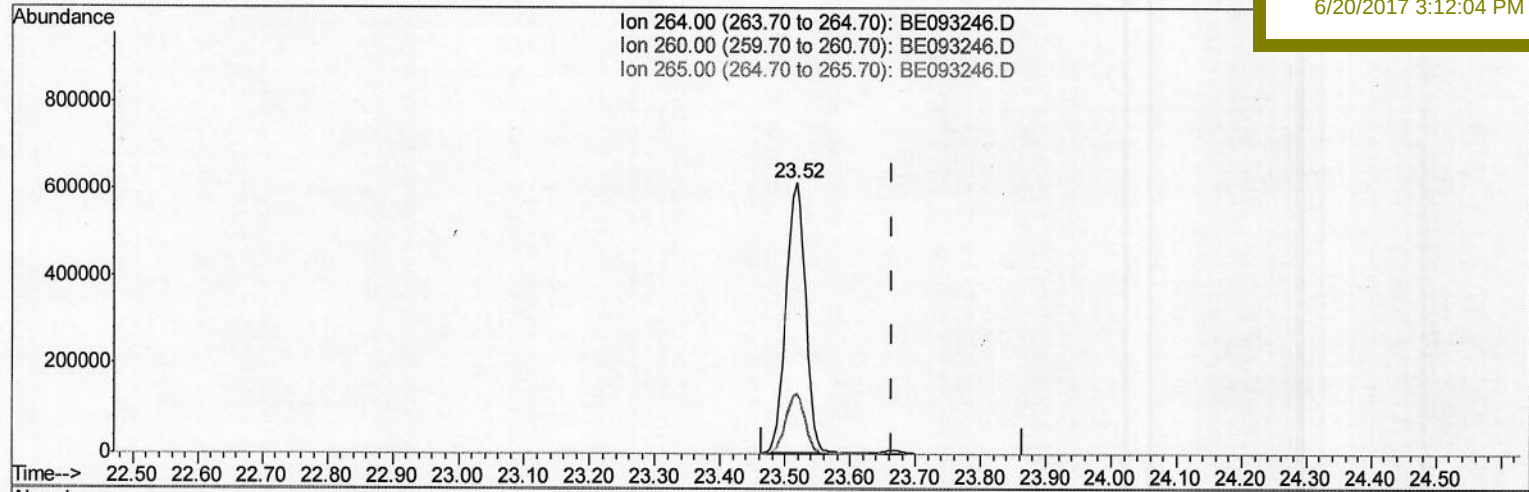

TIC: BE093246.D

(20) Perylene-d12 (I)
 23.518min (-0.146) 0.40ng/ul
 response 1280449

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.05#
265.00	103.50	21.46#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093246.D
 Acq On : 19 Jun 2017 12:23
 Operator : SJ/MA
 Sample : I3599-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 20 04:19:12 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5A74

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:04 PM

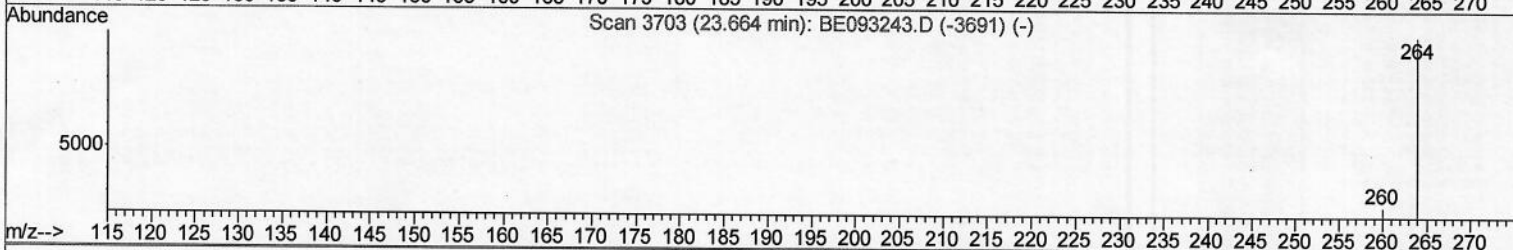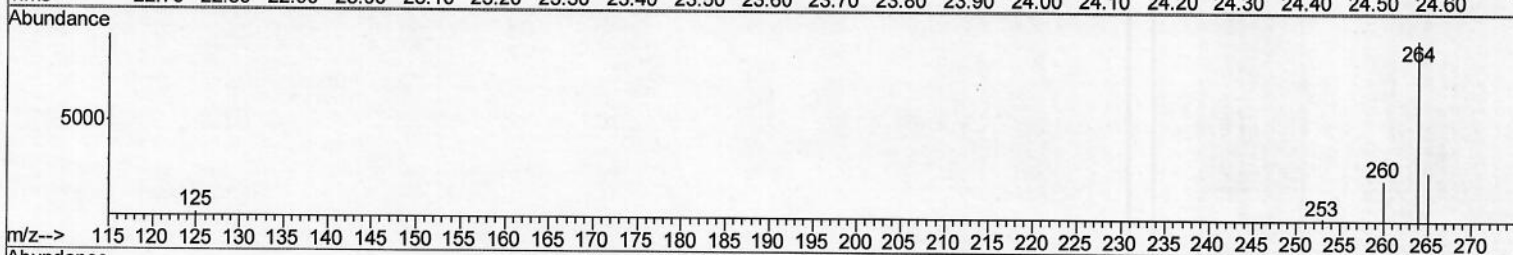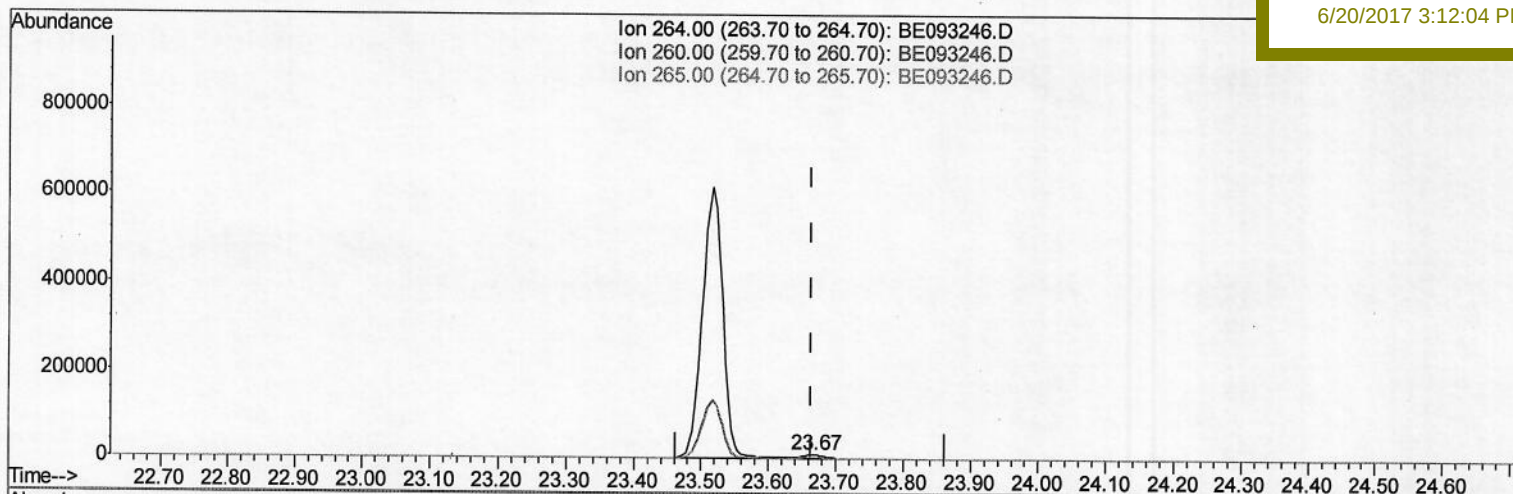

TIC: BE093246.D

(20) Perylene-d12 (I)
 23.668min (+0.004) 0.40ng/ul m
 response 14588

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.52
265.00	103.50	29.36#
0.00	0.00	0.00

SJ
 06/20/2017

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093246.D
Acq On : 19 Jun 2017 12:23
Operator : SJ/MA
Sample : I3599-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 20 14:50:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F5A74

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:04 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2428	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12158	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7740	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	18309m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18232	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	14588m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6495	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	18121	0.36	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ
06/20/2017

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093246.D
Acq On : 19 Jun 2017 12:23
Operator : SJ/MA
Sample : I3599-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Jun 20 14:50:37 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F5A74

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:04 PM

