

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093251.D
 Acq On : 19 Jun 2017 15:28
 Operator : SJ/MA
 Sample : I3599-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jun 20 04:19:53 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5D38

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:20 PM

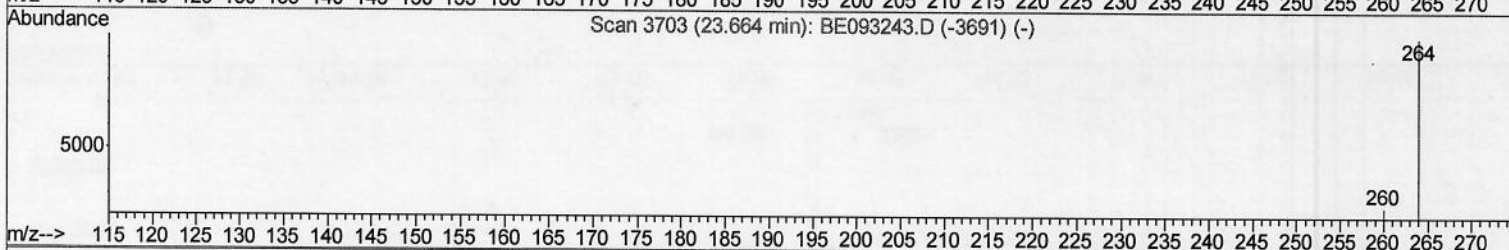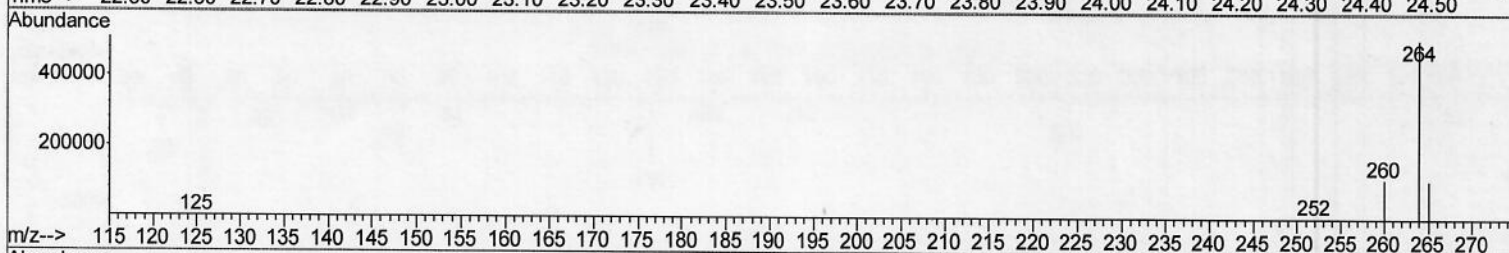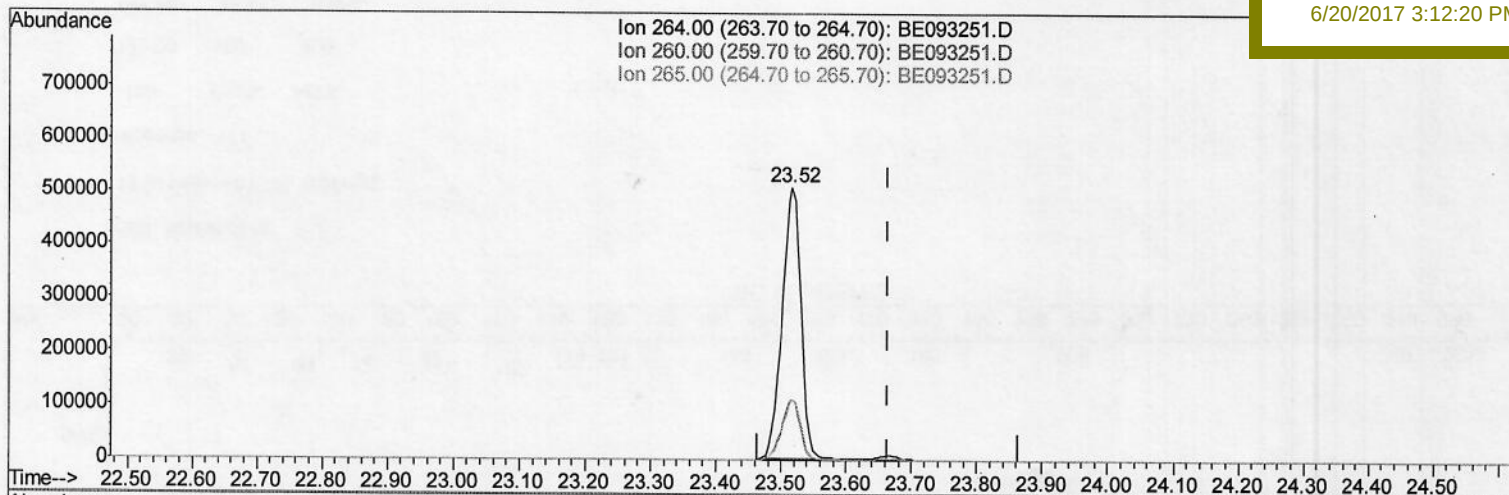

TIC: BE093251.D

(20) Perylene-d12 (I)
 23.517min (-0.147) 0.40ng/ul
 response 1018508

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.80#
265.00	103.50	21.63#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093251.D
 Acq On : 19 Jun 2017 15:28
 Operator : SJ/MA
 Sample : I3599-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jun 20 04:19:53 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5D38

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:20 PM

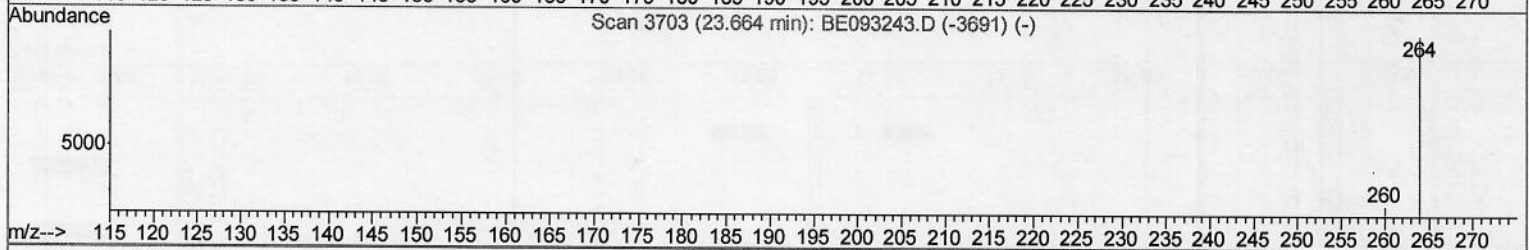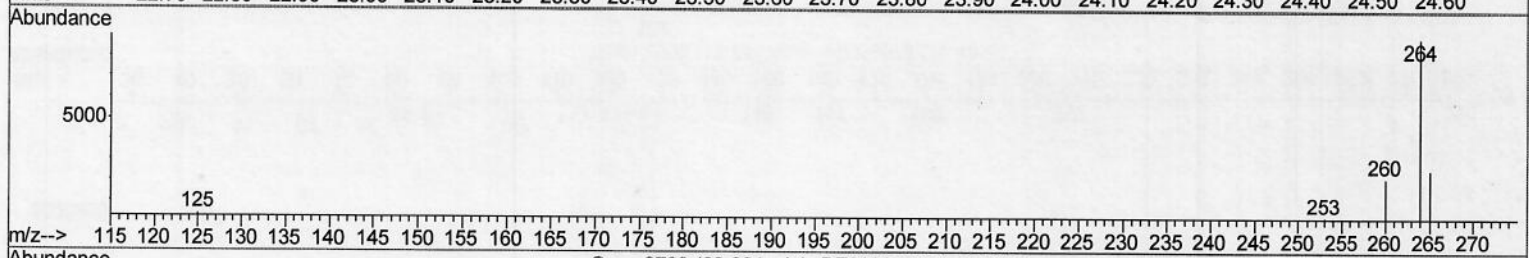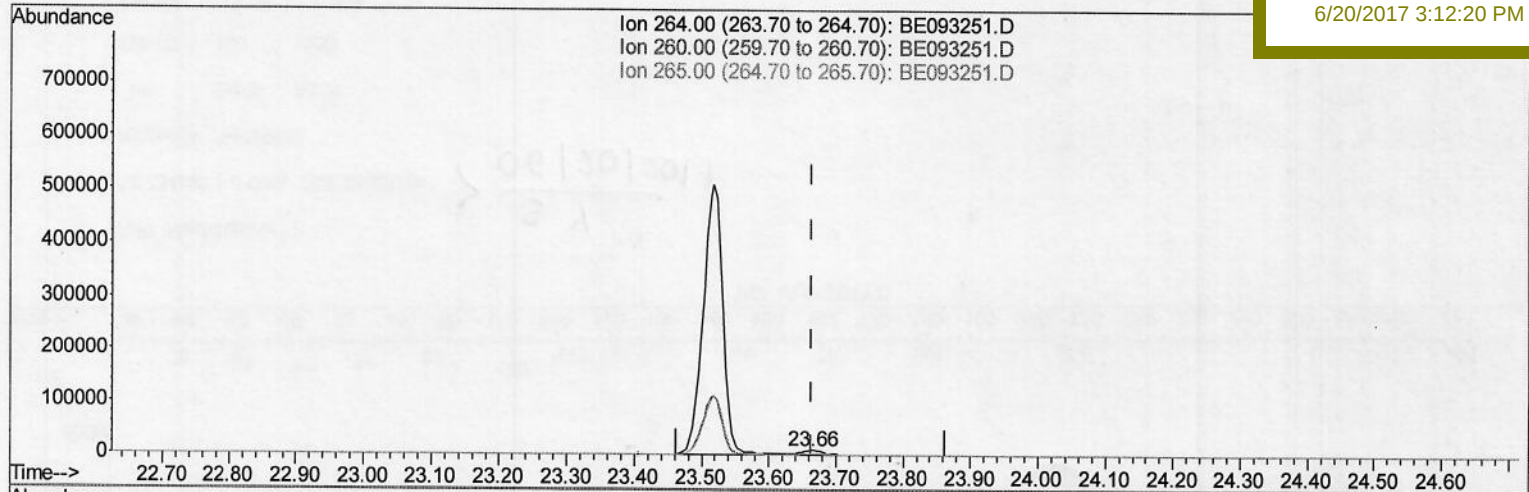

TIC: BE093251.D

(20) Perylene-d12 (I)

23.663min (-0.001) 0.40ng/ul m

response 15479

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.78
265.00	103.50	28.91#
0.00	0.00	0.00

S.J
06/20/17

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093251.D
Acq On : 19 Jun 2017 15:28
Operator : SJ/MA
Sample : I3599-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jun 20 08:09:34 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F5D38

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:20 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2395	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12361	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7744	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	18629	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	19009	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	15479m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	4512	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	13858	0.27	ng/ul	0.00

Target Compounds					Qvalue
3) Naphthalene	10.57	128	1101	0.036 ng/ul#	87
5) 2-Methylnaphthalene	12.18	142	368	0.018 ng/ul	99
8) Acenaphthene	14.43	153	629	0.023 ng/ul	98
9) Fluorene	15.42	166	857	0.027 ng/ul	91
12) Phenanthrene	17.14	178	3724	0.073 ng/ul#	90
15) Fluoranthene	19.15	202	2825	0.045 ng/ul	84
17) Pyrene	19.51	202	2353	0.042 ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JS-J
06/20/17

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093251.D
Acq On : 19 Jun 2017 15:28
Operator : SJ/MA
Sample : I3599-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Jun 20 08:09:34 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F5D38

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:20 PM

