

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093254.D
Acq On : 19 Jun 2017 17:19
Operator : SJ/MA
Sample : PB99746BL
Misc :
ALS Vial : 13 Sample Multiplier: 1




Quant Time: Jun 20 04:20:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

SBLK46

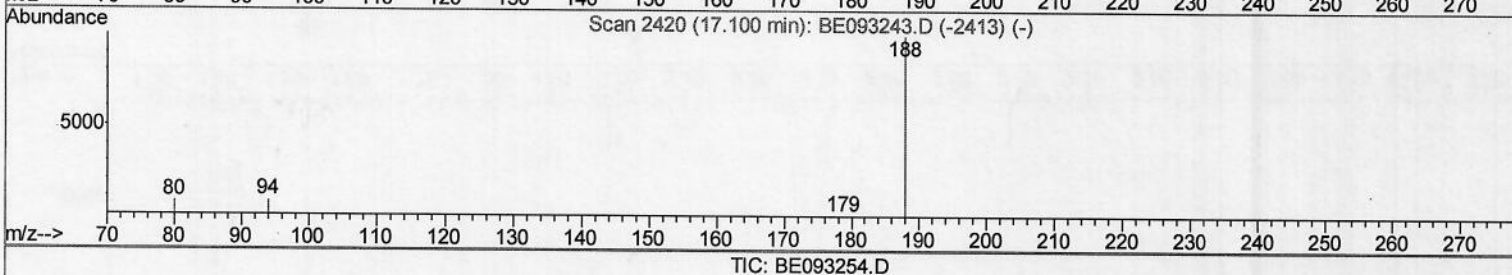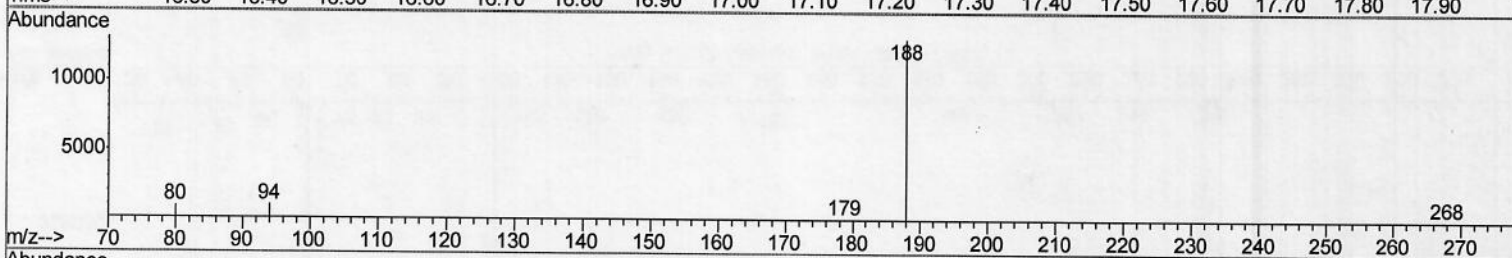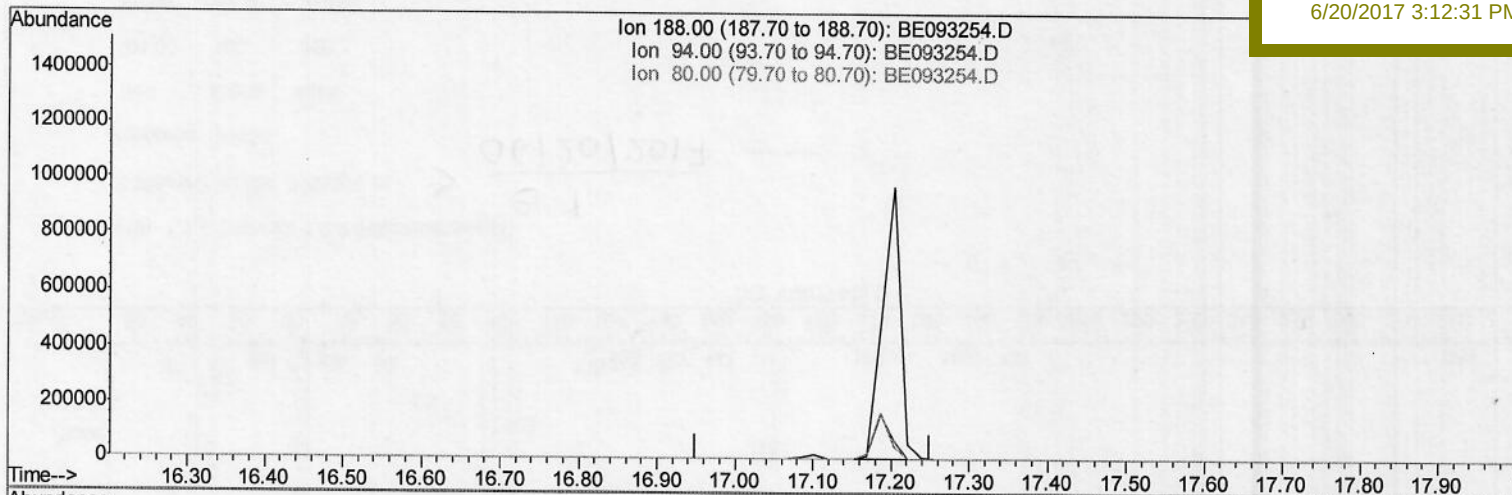Manual Integrations
APPROVEDmohammad
6/20/2017 3:12:31 PM

(10) Phenanthrene-d10 (I)

17.100min (-17.100) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093254.D
 Acq On : 19 Jun 2017 17:19
 Operator : SJ/MA
 Sample : PB99746BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
ClientSampleId :
 SBLK46

Quant Time: Jun 20 04:20:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 6/20/2017 3:12:31 PM

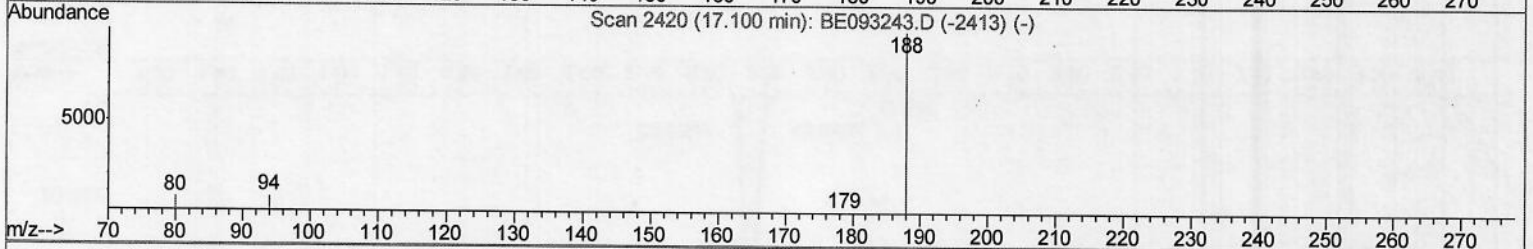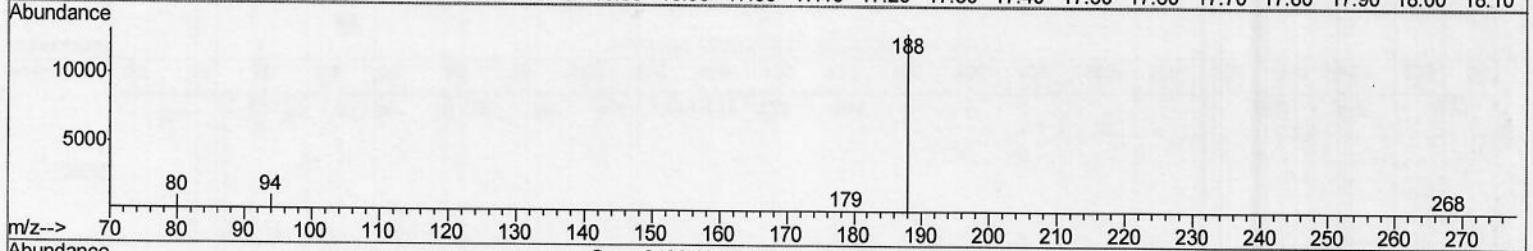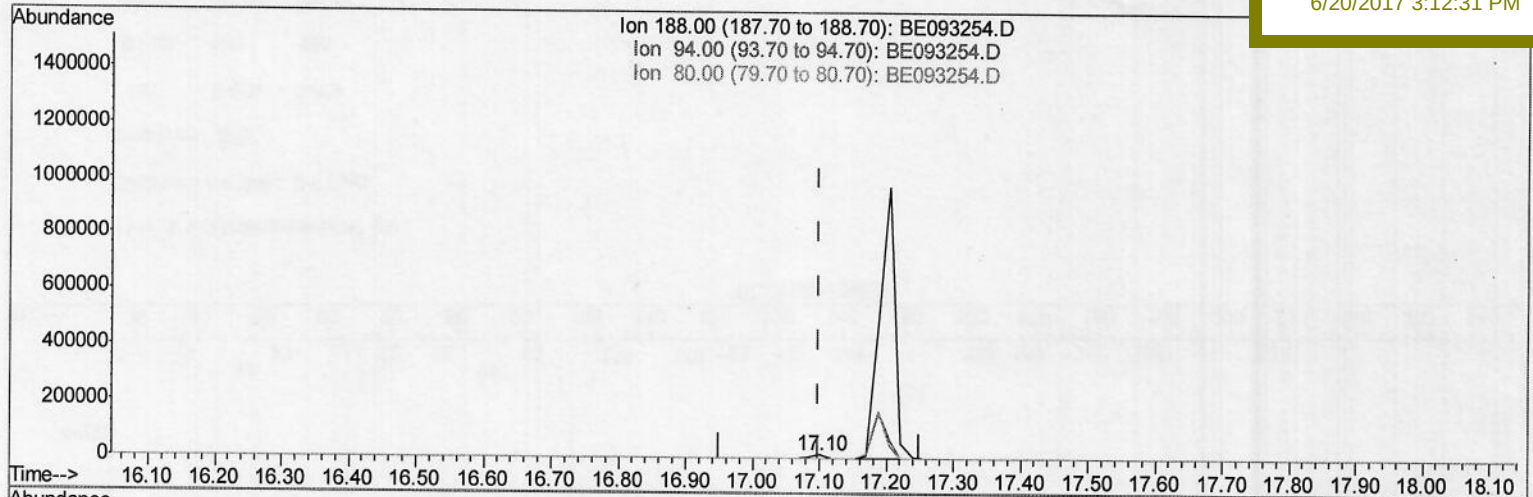

TIC: BE093254.D

(10) Phenanthrene-d10 (I)

17.101min (+0.001) 0.40ng/ul m

response 18519

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	7.77#
80.00	11.80	7.14#
0.00	0.00	0.00

S.S
06/20/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093254.D
 Acq On : 19 Jun 2017 17:19
 Operator : SJ/MA
 Sample : PB99746BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jun 20 04:20:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
ClientSampleId :
 SBLK46

Manual Integrations
APPROVED

mohammad
 6/20/2017 3:12:31 PM

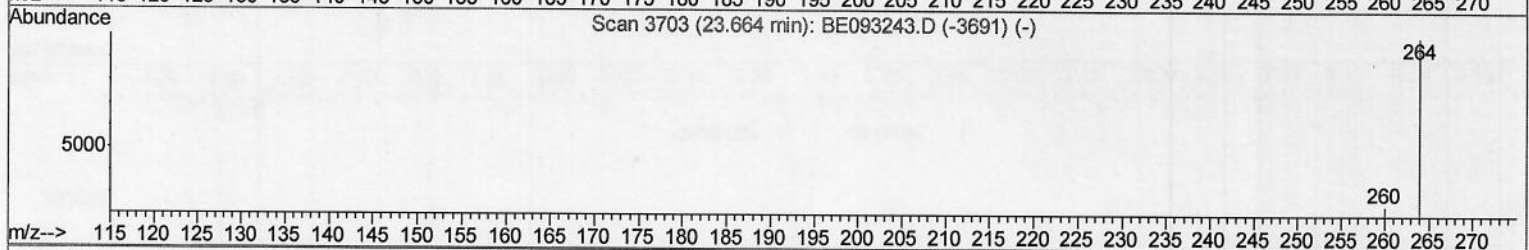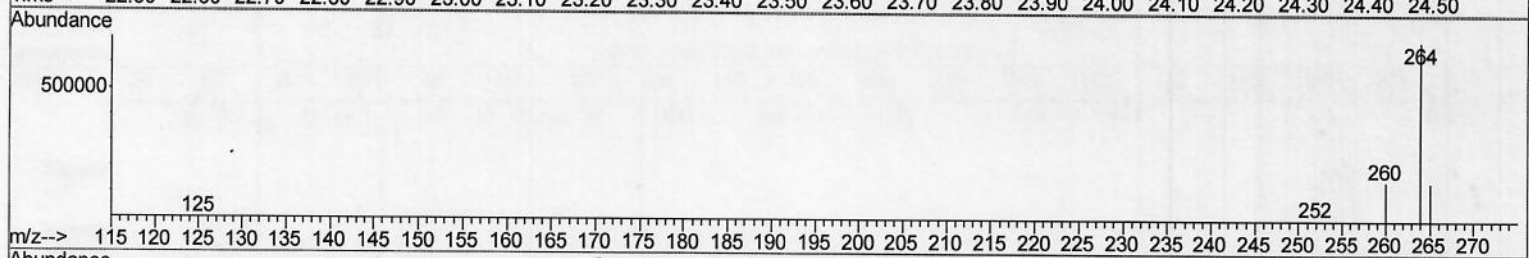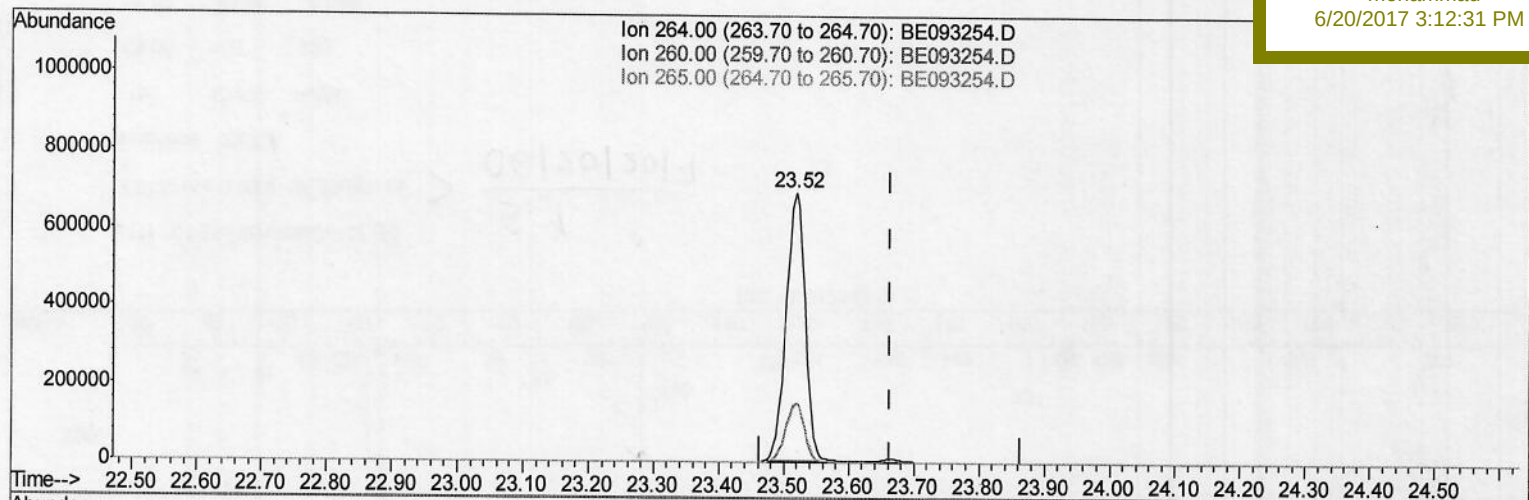

TIC: BE093254.D

(20) Perylene-d12 (I)
 23.519min (-0.145) 0.40ng/ul
 response 1422823

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.03#
265.00	103.50	21.59#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093254.D
 Acq On : 19 Jun 2017 17:19
 Operator : SJ/MA
 Sample : PB99746BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jun 20 04:20:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 SBLK46

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:12:31 PM

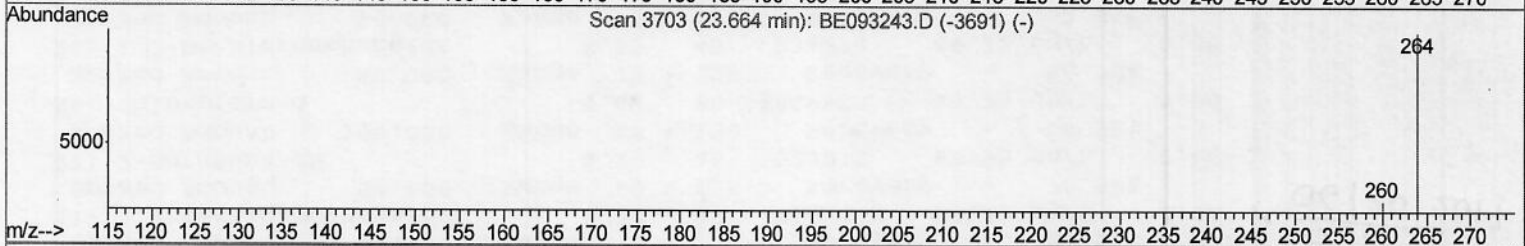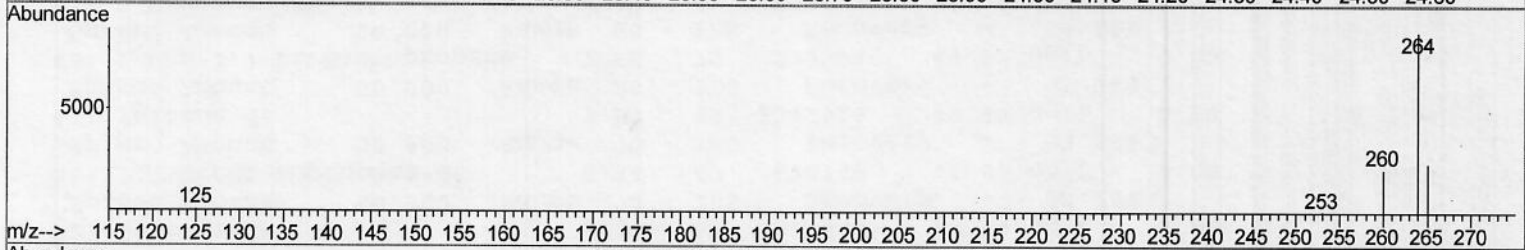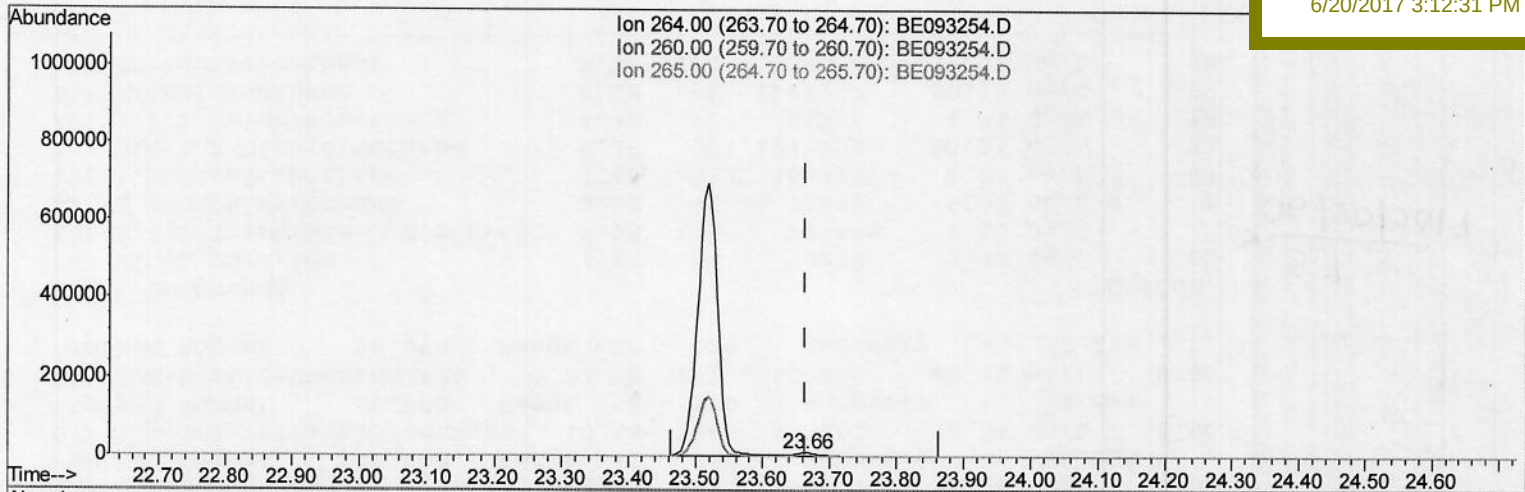

TIC: BE093254.D

(20) Perylene-d12 (I)

23.664min (+0.000) 0.40ng/ul m

response 14196

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.95
265.00	103.50	28.49#
0.00	0.00	0.00

S.J
06/20/17

Data Path : Z:\HPCHEM1\BNA E\Data\BE061917\
Data File : BE093254.D
Acq On : 19 Jun 2017 17:19
Operator : SJ/MA
Sample : PB99746BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jun 20 08:32:43 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:31 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2455	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12219	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7699	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	18519m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18273	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	14196m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6946	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	18571	0.37	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

→ } S-J
→ } 06/20/17

Data Path : Z:\HPCHEM1\BNA E\Data\BE061917\
Data File : BE093254.D
Acq On : 19 Jun 2017 17:19
Operator : SJ/MA
Sample : PB99746BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jun 20 08:32:43 2017
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 04:17:17 2017
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
SBLK46

Manual Integrations
APPROVED

mohammad
6/20/2017 3:12:31 PM

