

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE061917\
 Data File : BE093258.D
 Acq On : 19 Jun 2017 19:45
 Operator : SJ/MA
 Sample : I3600-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 20 04:20:48 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5E11

Manual Integrations
 APPROVED

mohammad
 6/20/2017 4:31:37 PM

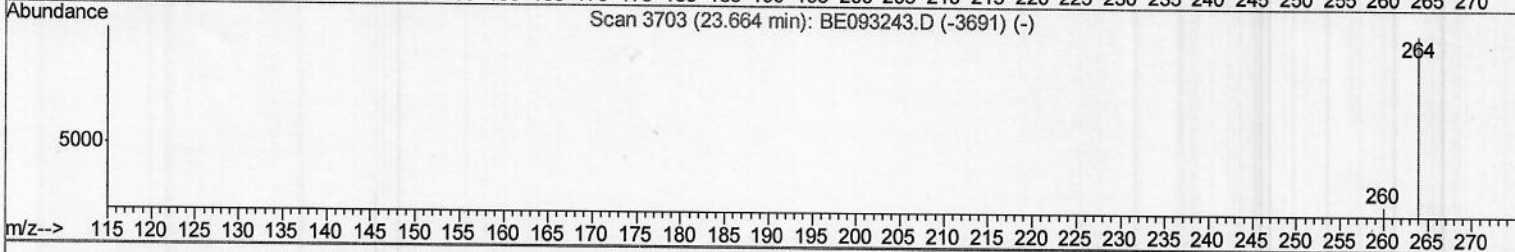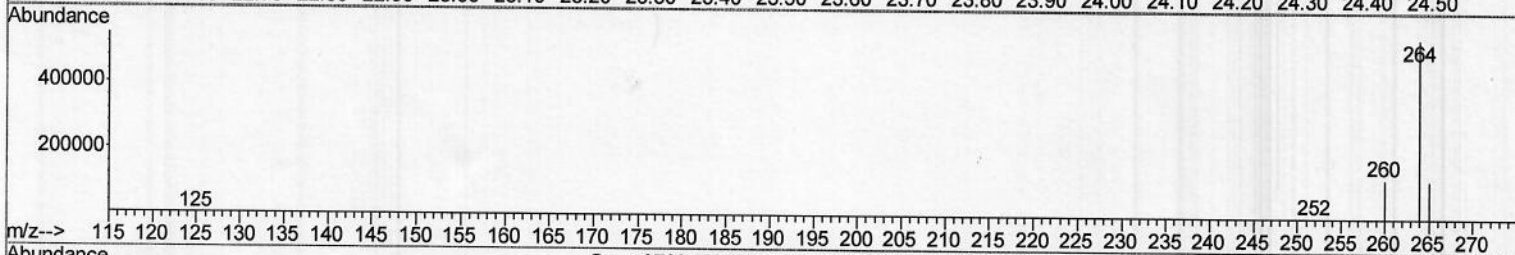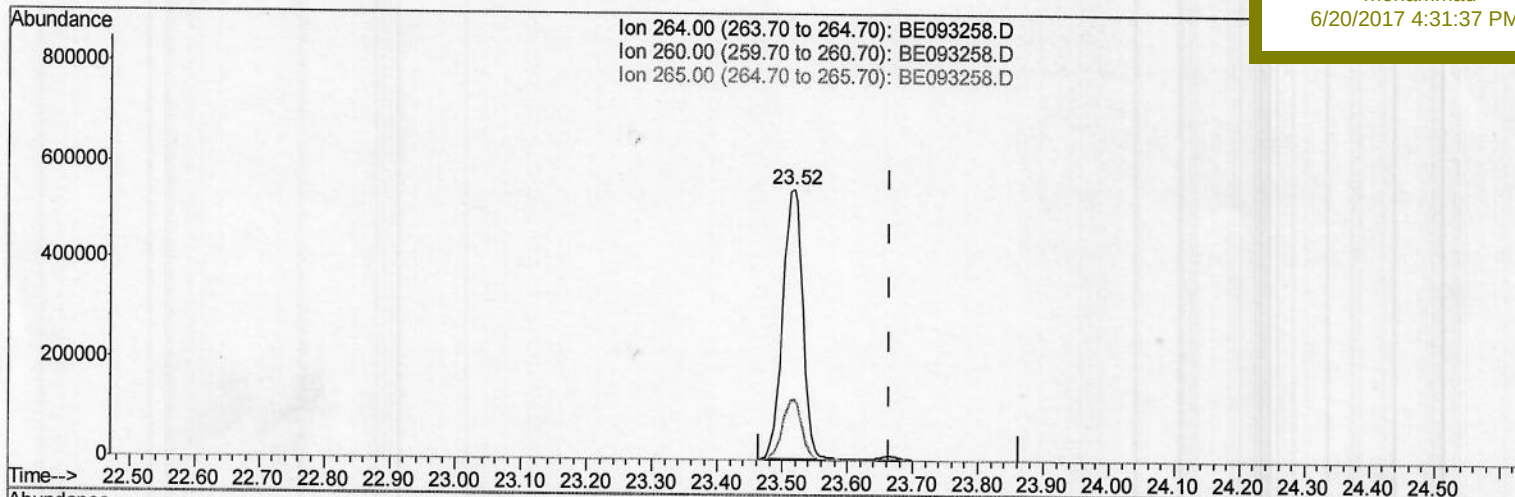

(20) Perylene-d12 (I)
 23.518min (-0.146) 0.40ng/ul
 response 1164146

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.07#
265.00	103.50	21.55#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\Data\BE061917\
 Data File : BE093258.D
 Acq On : 19 Jun 2017 19:45
 Operator : SJ/MA
 Sample : I3600-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 20 04:20:48 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Instrument :
 BNA_E
 ClientSampleId :
 F5E11

Manual Integrations
 APPROVED

mohammad
 6/20/2017 4:31:37 PM

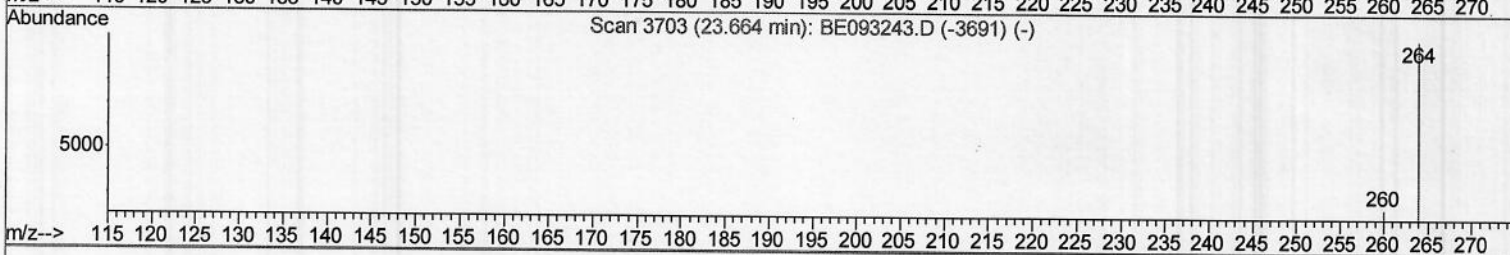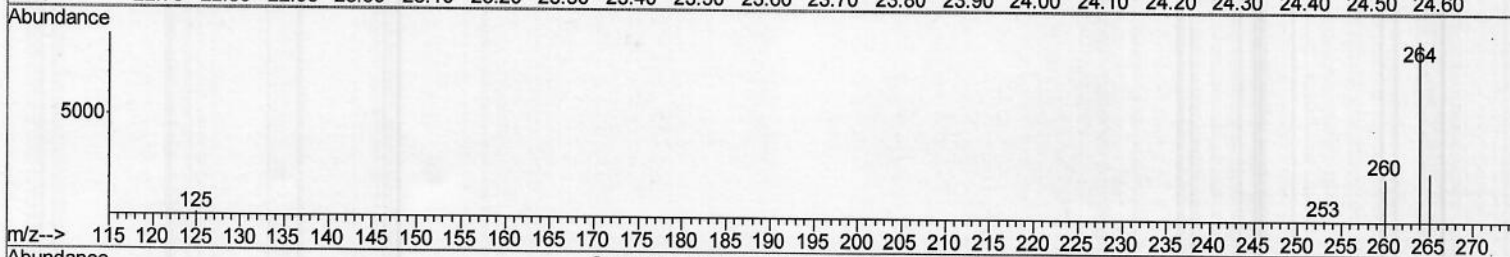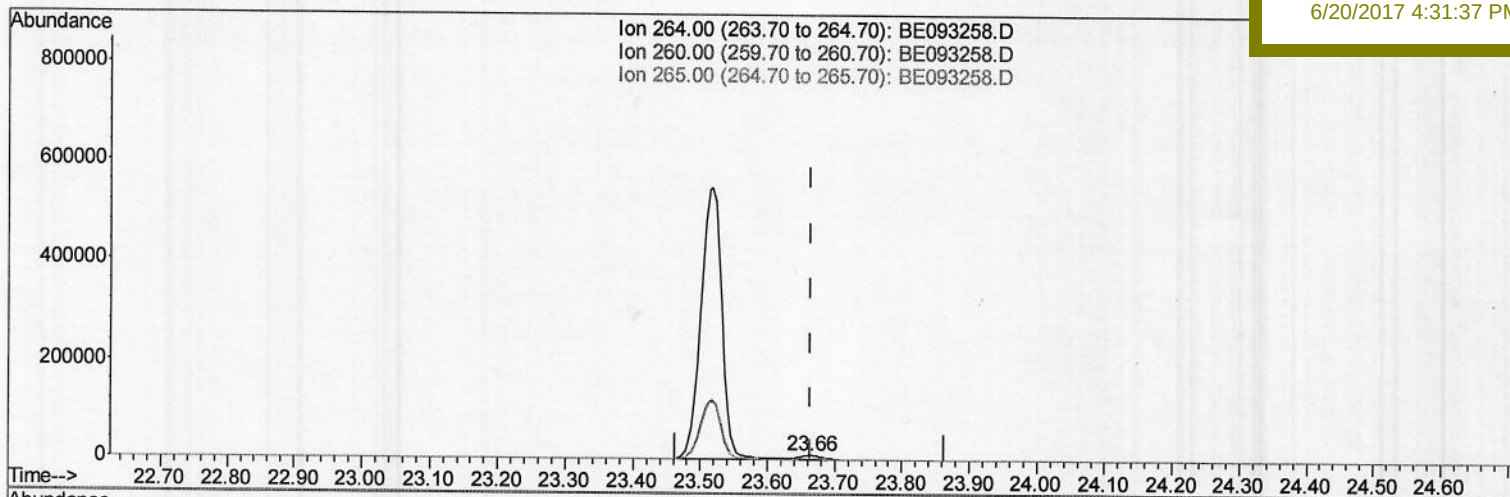

TIC: BE093258.D

(20) Perylene-d12 (I)

23.663min (-0.001) 0.40ng/ul m

response 15390

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.91
265.00	103.50	28.90#
0.00	0.00	0.00

S.J
 06/20/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE061917\
 Data File : BE093258.D
 Acq On : 19 Jun 2017 19:45
 Operator : SJ/MA
 Sample : I3600-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E11

Manual Integrations
 APPROVED

mohammad
 6/20/2017 4:31:37 PM

Quant Time: Jun 20 15:19:42 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

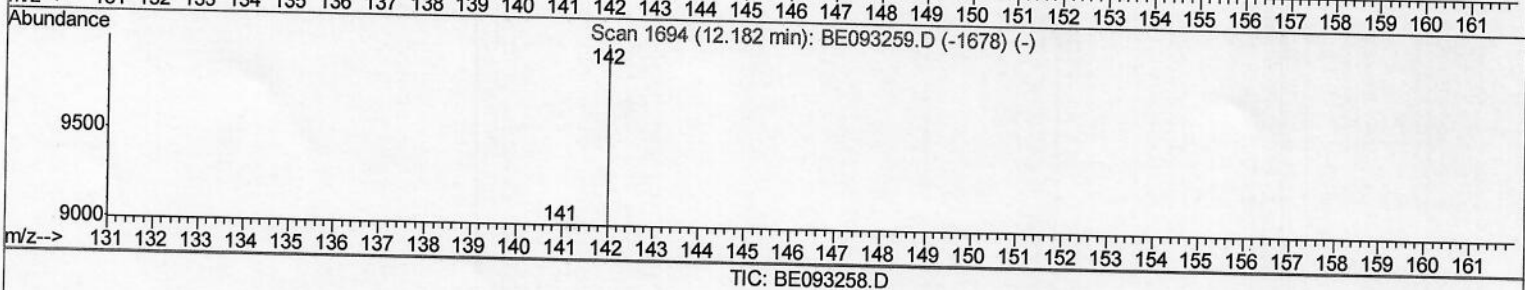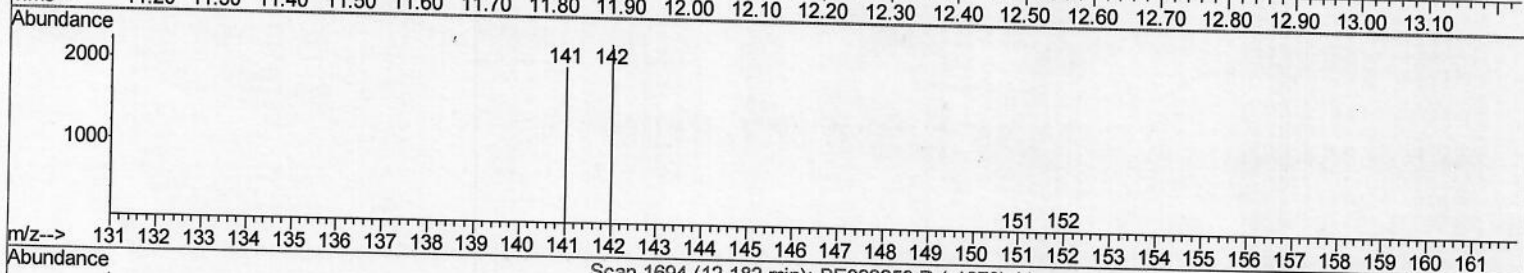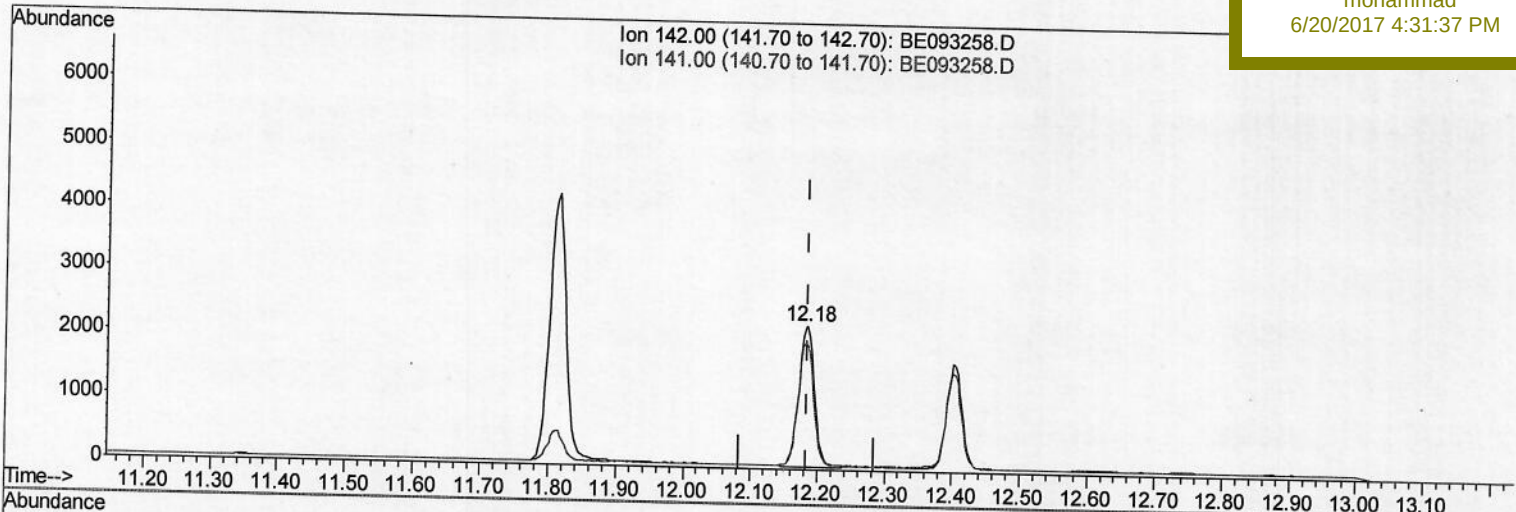

(5) 2-Methylnaphthalene

12.184min (-0.001) 0.17ng/ul m

response 3575

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

S.J
 06/20/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_E\Data\BE061917\
 Data File : BE093258.D
 Acq On : 19 Jun 2017 19:45
 Operator : SJ/MA
 Sample : I3600-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E11

Manual Integrations
 APPROVED

mohammad
 6/20/2017 4:31:37 PM

Quant Time: Jun 30 08:55:29 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 26 01:58:03 2017
 Response via : Initial Calibration

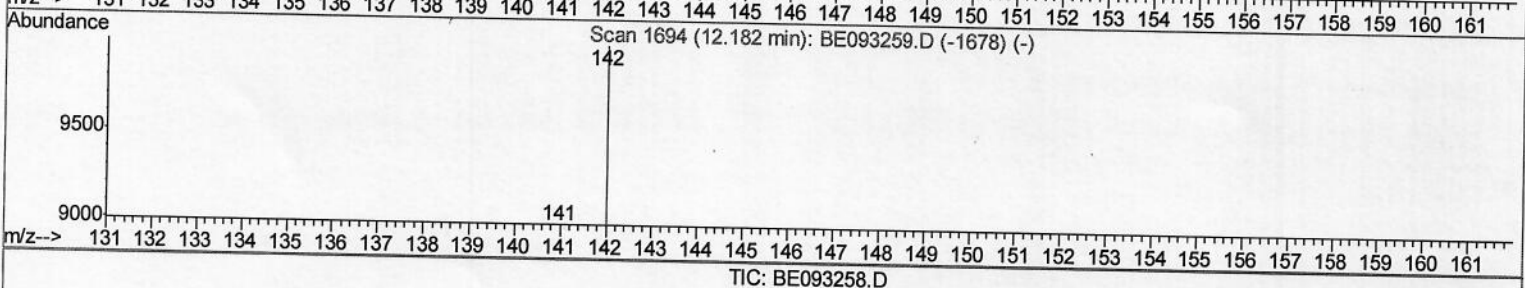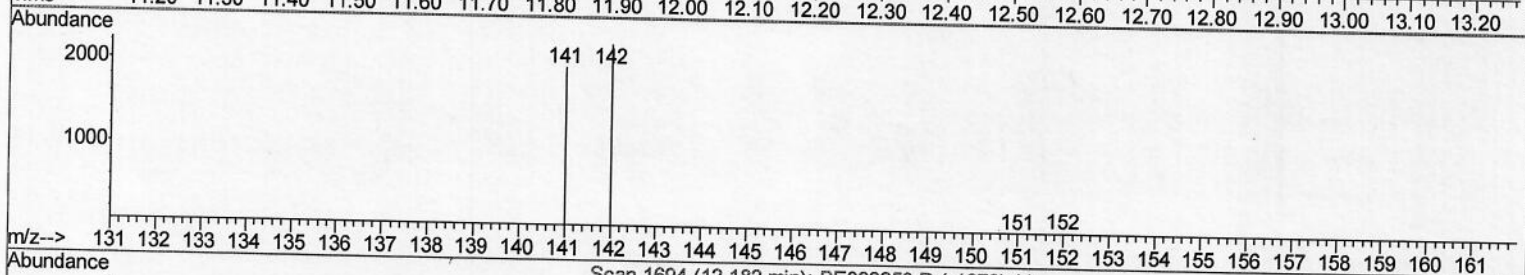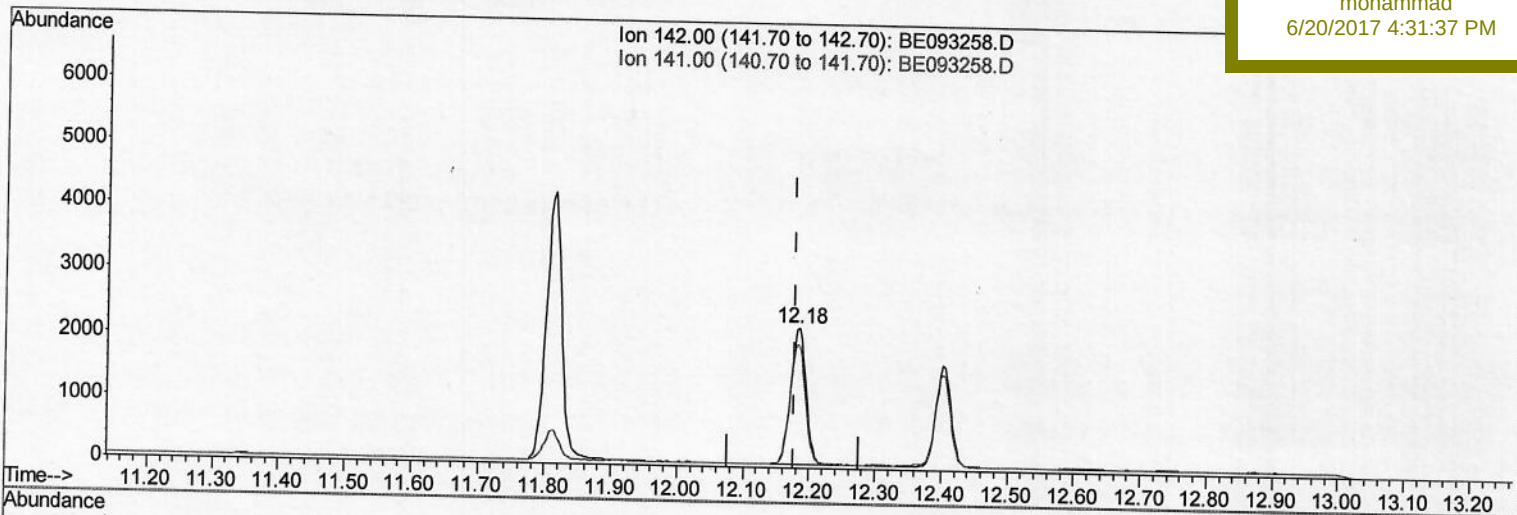

(5) 2-Methylnaphthalene

12.184min (+0.007) 0.16ng/ul

response 3495

Ion	Exp%	Act%
142.00	100	100
141.00	90.70	88.78
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE061917\
 Data File : BE093258.D
 Acq On : 19 Jun 2017 19:45
 Operator : SJ/MA
 Sample : I3600-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E11

Quant Time: Jun 20 15:19:42 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 04:17:17 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/20/2017 4:31:37 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2534	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12544	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	7762	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	17905	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	18676	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	15390m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	4389	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	14862	0.31	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.57	128	20394	0.655	ng/ul#	91
5) 2-Methylnaphthalene	12.18	142	3575m	0.168	ng/ul	
8) Acenaphthene	14.43	153	9915	0.369	ng/ul	94
9) Fluorene	15.42	166	7911	0.251	ng/ul	94
12) Phenanthrene	17.14	178	33500	0.680	ng/ul#	89
15) Fluoranthene	19.15	202	19114	0.316	ng/ul	84
17) Pyrene	19.52	202	16225	0.295	ng/ul#	85
18) Benzo(a)anthracene	21.24	228	3150	0.063	ng/ul#	88
19) Chrysene	21.29	228	3055	0.059	ng/ul	94

S. J
 06/20/17

S. J
 06/20/17

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE061917\
Data File : BE093258.D
Acq On : 19 Jun 2017 19:45
Operator : SJ/MA
Sample : I3600-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Jun 20 15:19:42 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 '04:17:17 2017
Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F5E11

Manual Integrations

APPROVED

mohammad

6/20/2017 4:31:37 PM

