

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093265.D
 Acq On : 20 Jun 2017 00:04
 Operator : SJ/MA
 Sample : I3600-10
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5E16

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:13:06 PM

Quant Time: Jun 20 09:17:38 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2648	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	13778	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	9164	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	20960m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	20688	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	16964m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	7570	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20611	0.36	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.56	128	784	0.023	ng/ul#	78
15) Fluoranthene	19.15	202	1109	0.016	ng/ul	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093265.D
Acq On : 20 Jun 2017 00:04
Operator : SJ/MA
Sample : I3600-10
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F5E16

Manual Integrations
APPROVED

mohammad
6/20/2017 3:13:06 PM

Quant Time: Jun 20 09:17:38 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

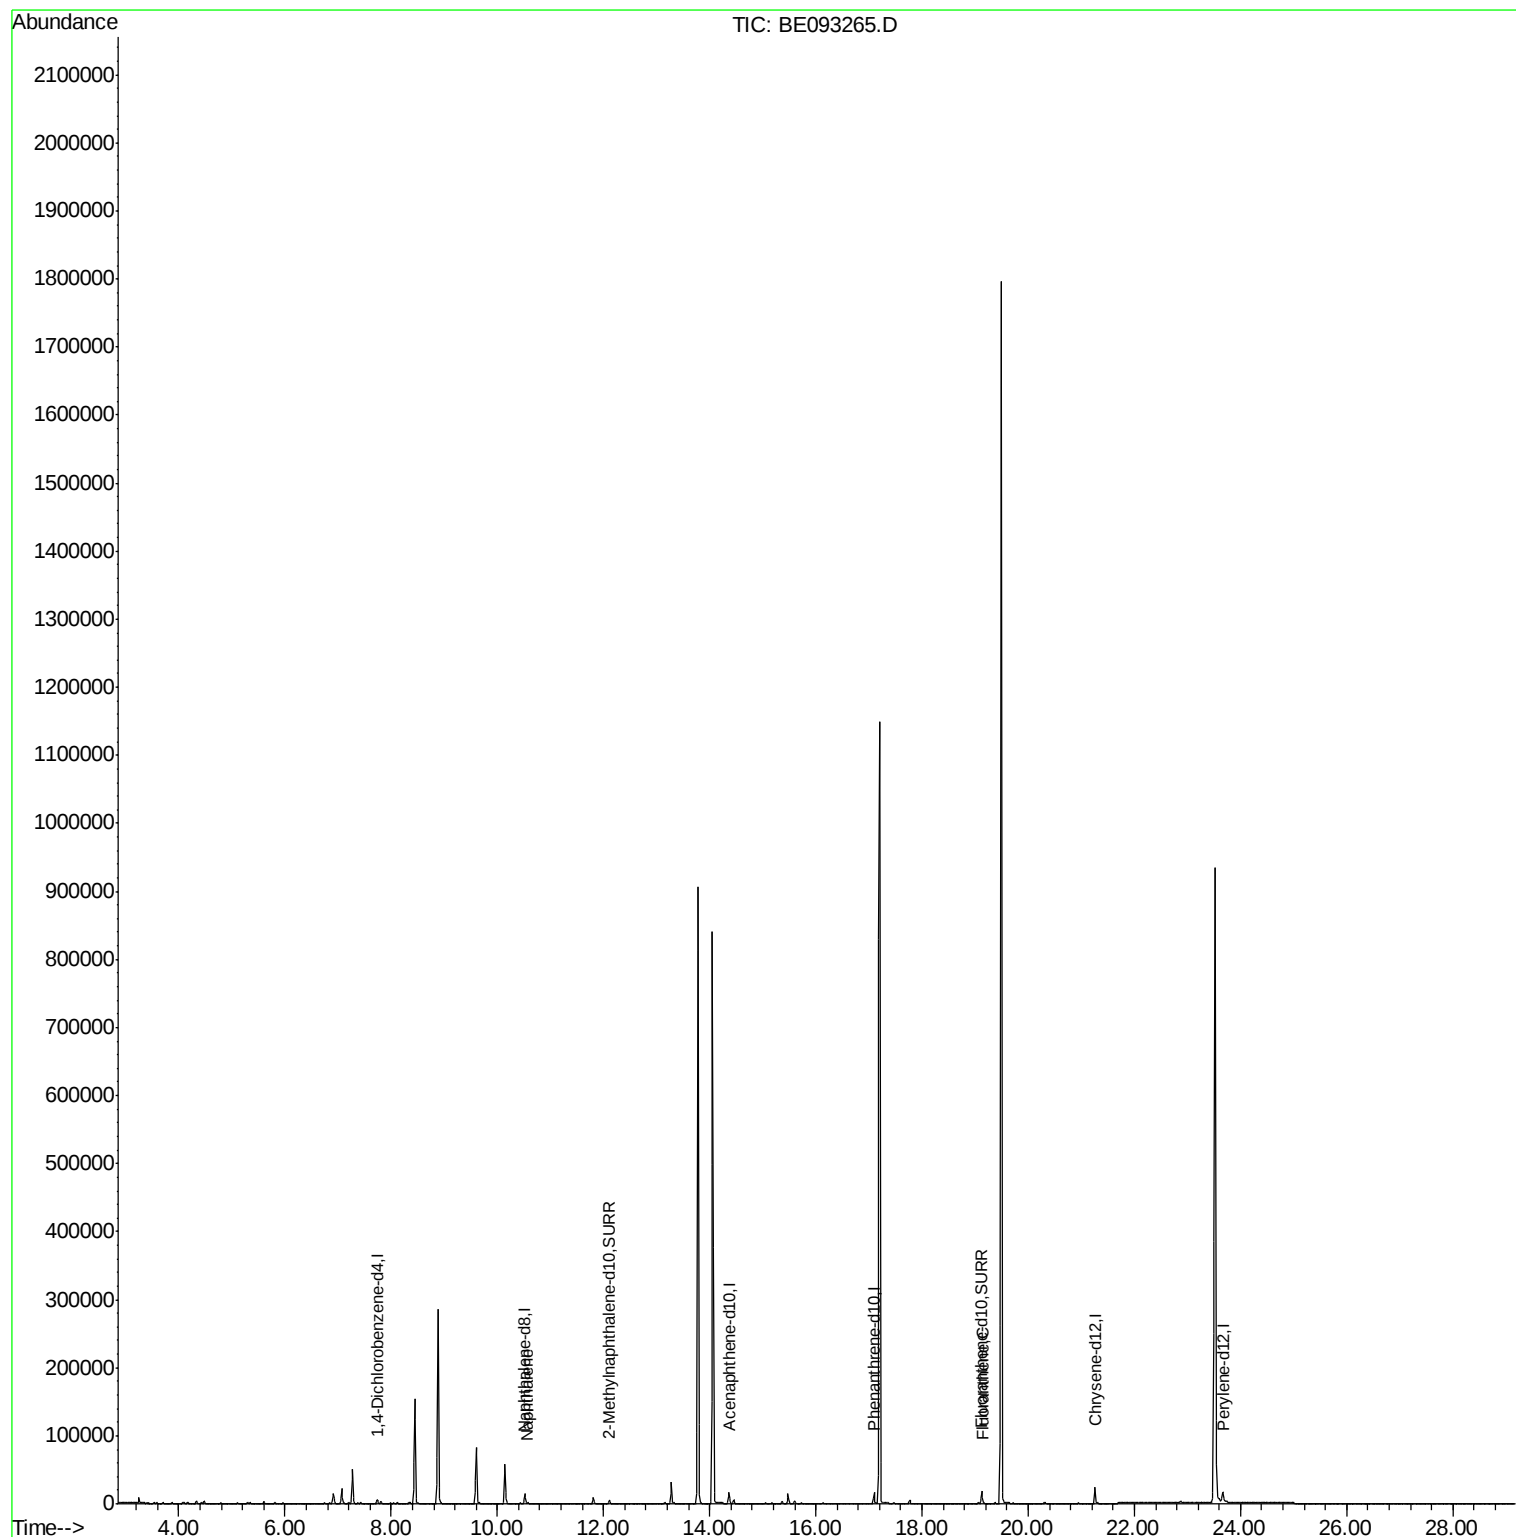

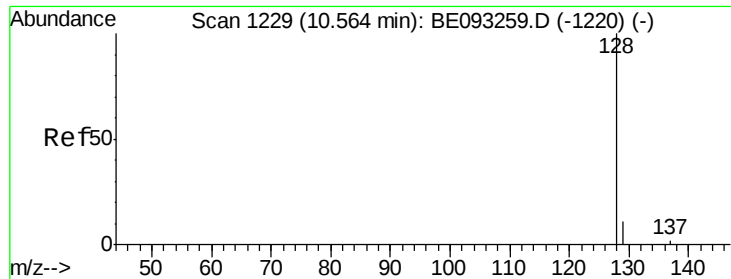

#3

Naphthalene

Concen: 0.023 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04

Instrument :

BNA_E





ClientSampleId :

F5E16

Tgt Ion:	128	Resp:	784
Ion Ratio	Lower	Upper	
128	100		
129	24.3	11.3	16.9#
127	0.0	4.0	6.0#

Manual Integrations
APPROVED

mohammad
6/20/2017 3:13:06 PM

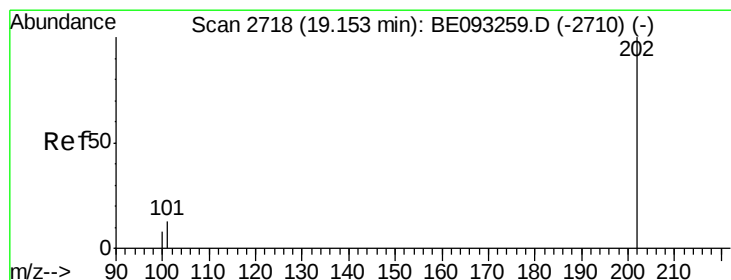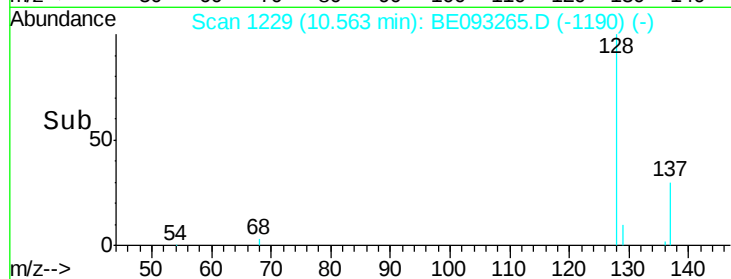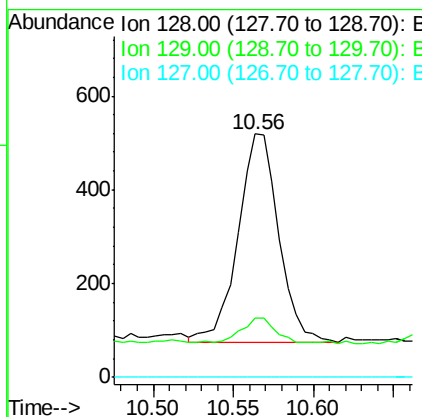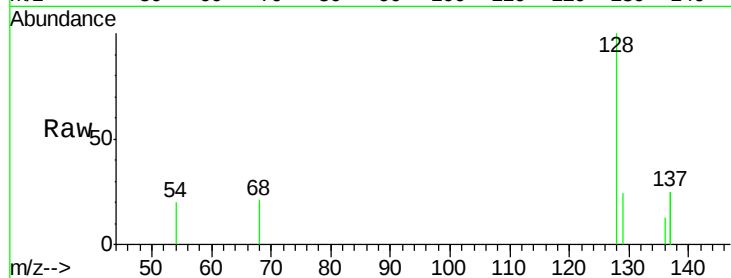

#15

Fluoranthene

Concen: 0.016 ng/ul

RT: 19.15 min Scan# 2719

Delta R.T. -0.00 min

Lab File: BE093265.D

Acq: 20 Jun 2017 00:04

Tgt Ion:	202	Resp:	1109
Ion Ratio	Lower	Upper	
202	100		
101	21.6	0.0	30.3
100	15.5	0.0	39.5

