

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
 Data File : BE093267.D
 Acq On : 20 Jun 2017 1:19
 Operator : SJ/MA
 Sample : I3600-12
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F5A14

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:13:11 PM

Quant Time: Jun 20 09:25:19 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 20 08:49:11 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	2369	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	12829	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	8487	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	20039m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	19020	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	15491m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	6963	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	20141	0.37	ng/ul	0.00
Target Compounds						
13) Anthracene	17.22	178	9283	0.193	ng/ul#	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE061917\
Data File : BE093267.D
Acq On : 20 Jun 2017 1:19
Operator : SJ/MA
Sample : I3600-12
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F5A14

Manual Integrations
APPROVED

mohammad
6/20/2017 3:13:11 PM

Quant Time: Jun 20 09:25:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 20 08:49:11 2017
Response via : Initial Calibration

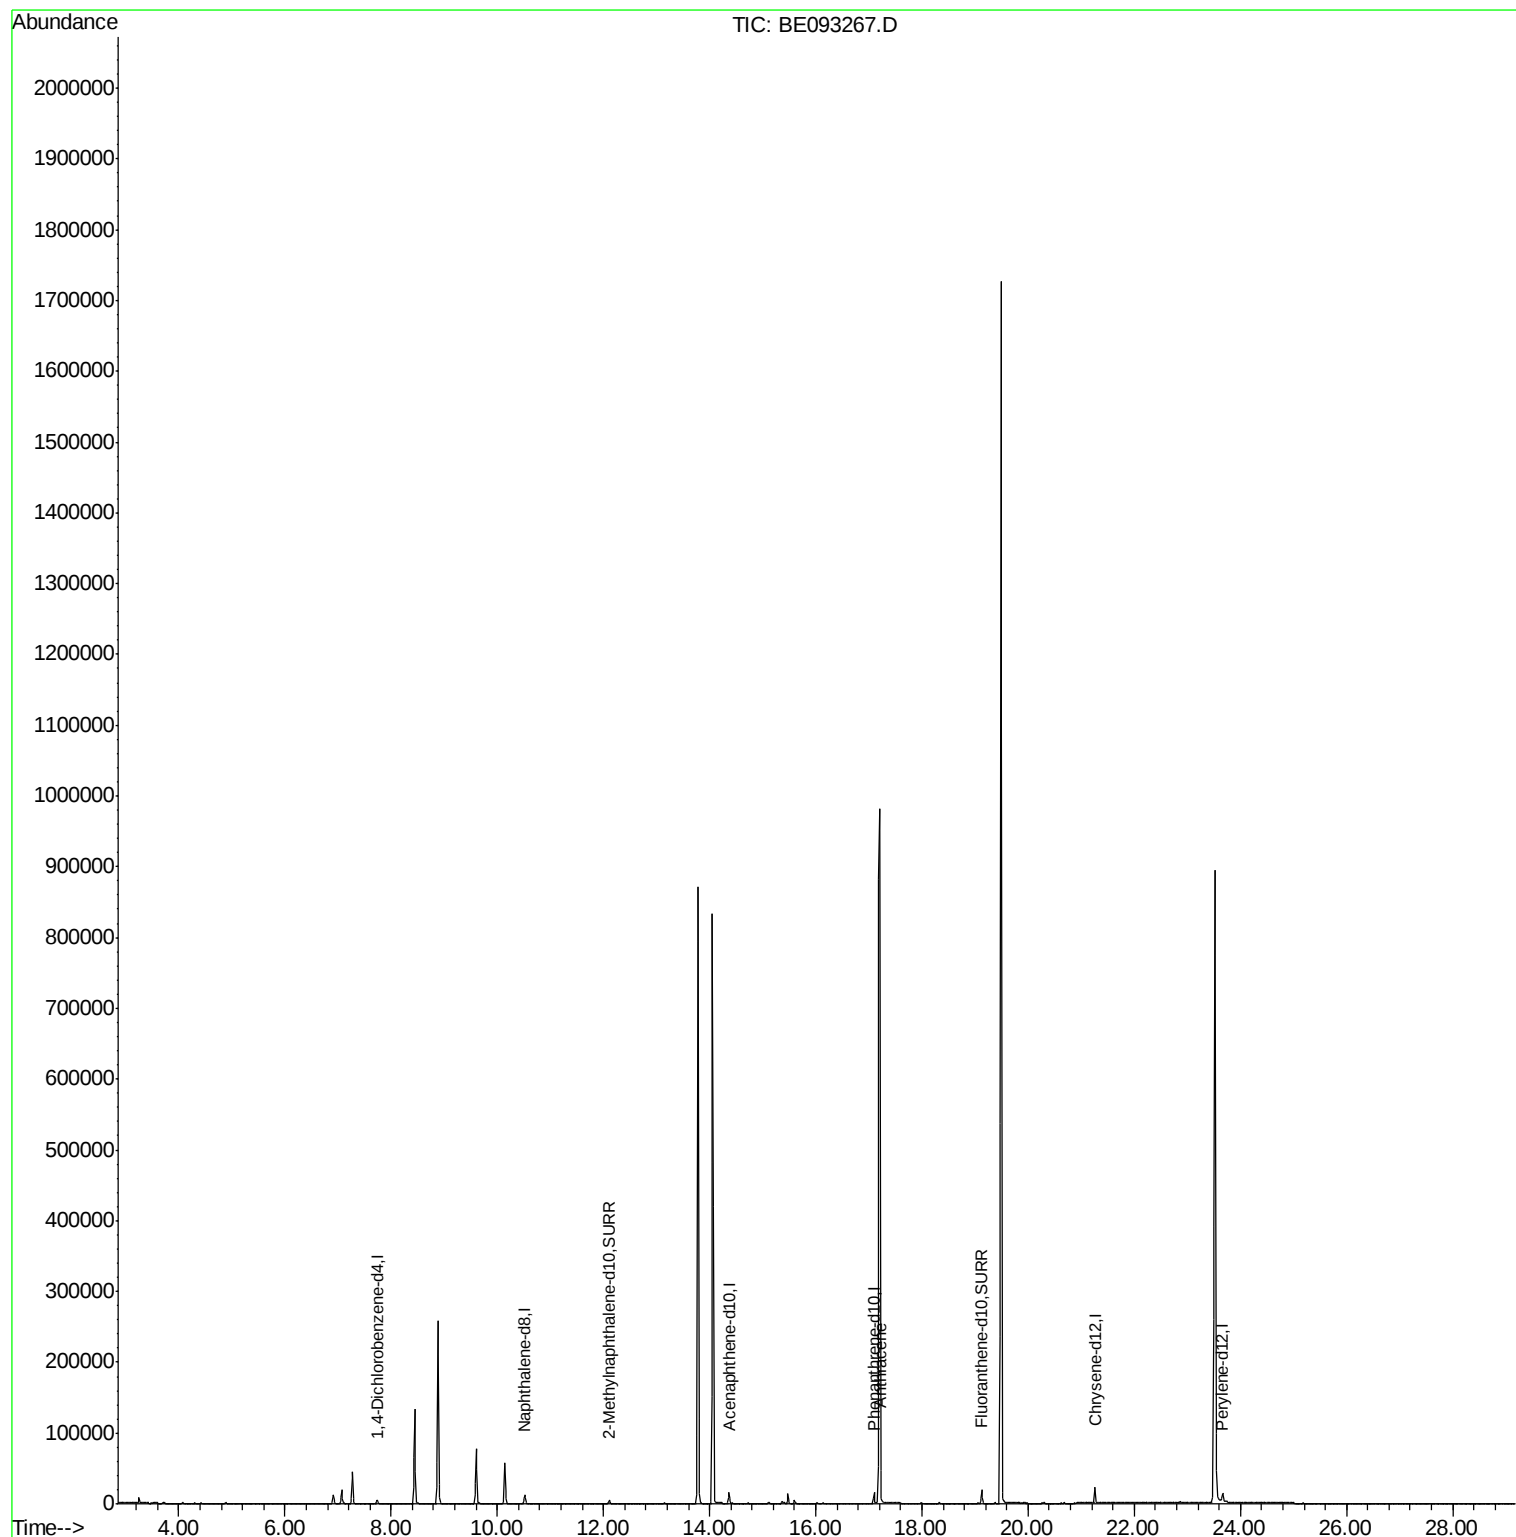

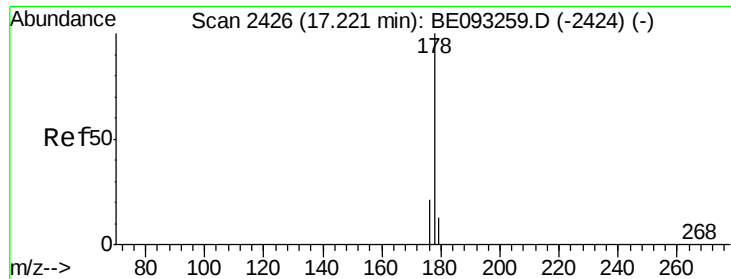

#13
 Anthracene
 Concen: 0.193 ng/ul
 RT: 17.22 min Scan# 2428
 Delta R.T. 0.00 min
 Lab File: BE093267.D
 Acq: 20 Jun 2017 1:19

Instrument :
 BNA_E
 ClientSampleId :
 F5A14

Tgt Ion	Ratio	Lower	Upper
178	100		
179	17.4	18.1	27.1#
176	22.8	14.7	22.1#

Manual Integrations
 APPROVED

mohammad
 6/20/2017 3:13:11 PM

