

Data File : BE093277.D
Acq On : 20 Jun 2017 12:18
Operator : SJ/JU
Sample : PB99755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK55

Quant Time: Jun 21 01:50:05 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	1878	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	9794	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	6103	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	14177	0.40	ng/ul	0.00
20) Perylene-d12	23.52	264	947620	0.40	ng/ul	-0.14
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.11	152	4942	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	12949	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.49	202	2475	0.06	ng/ul#	Qvalue 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093277.D

Acq On : 20 Jun 2017 12:18

Operator : SJ/JU

Sample : PB99755BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

SBLK55


Quant Time: Jun 21 01:50:05 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

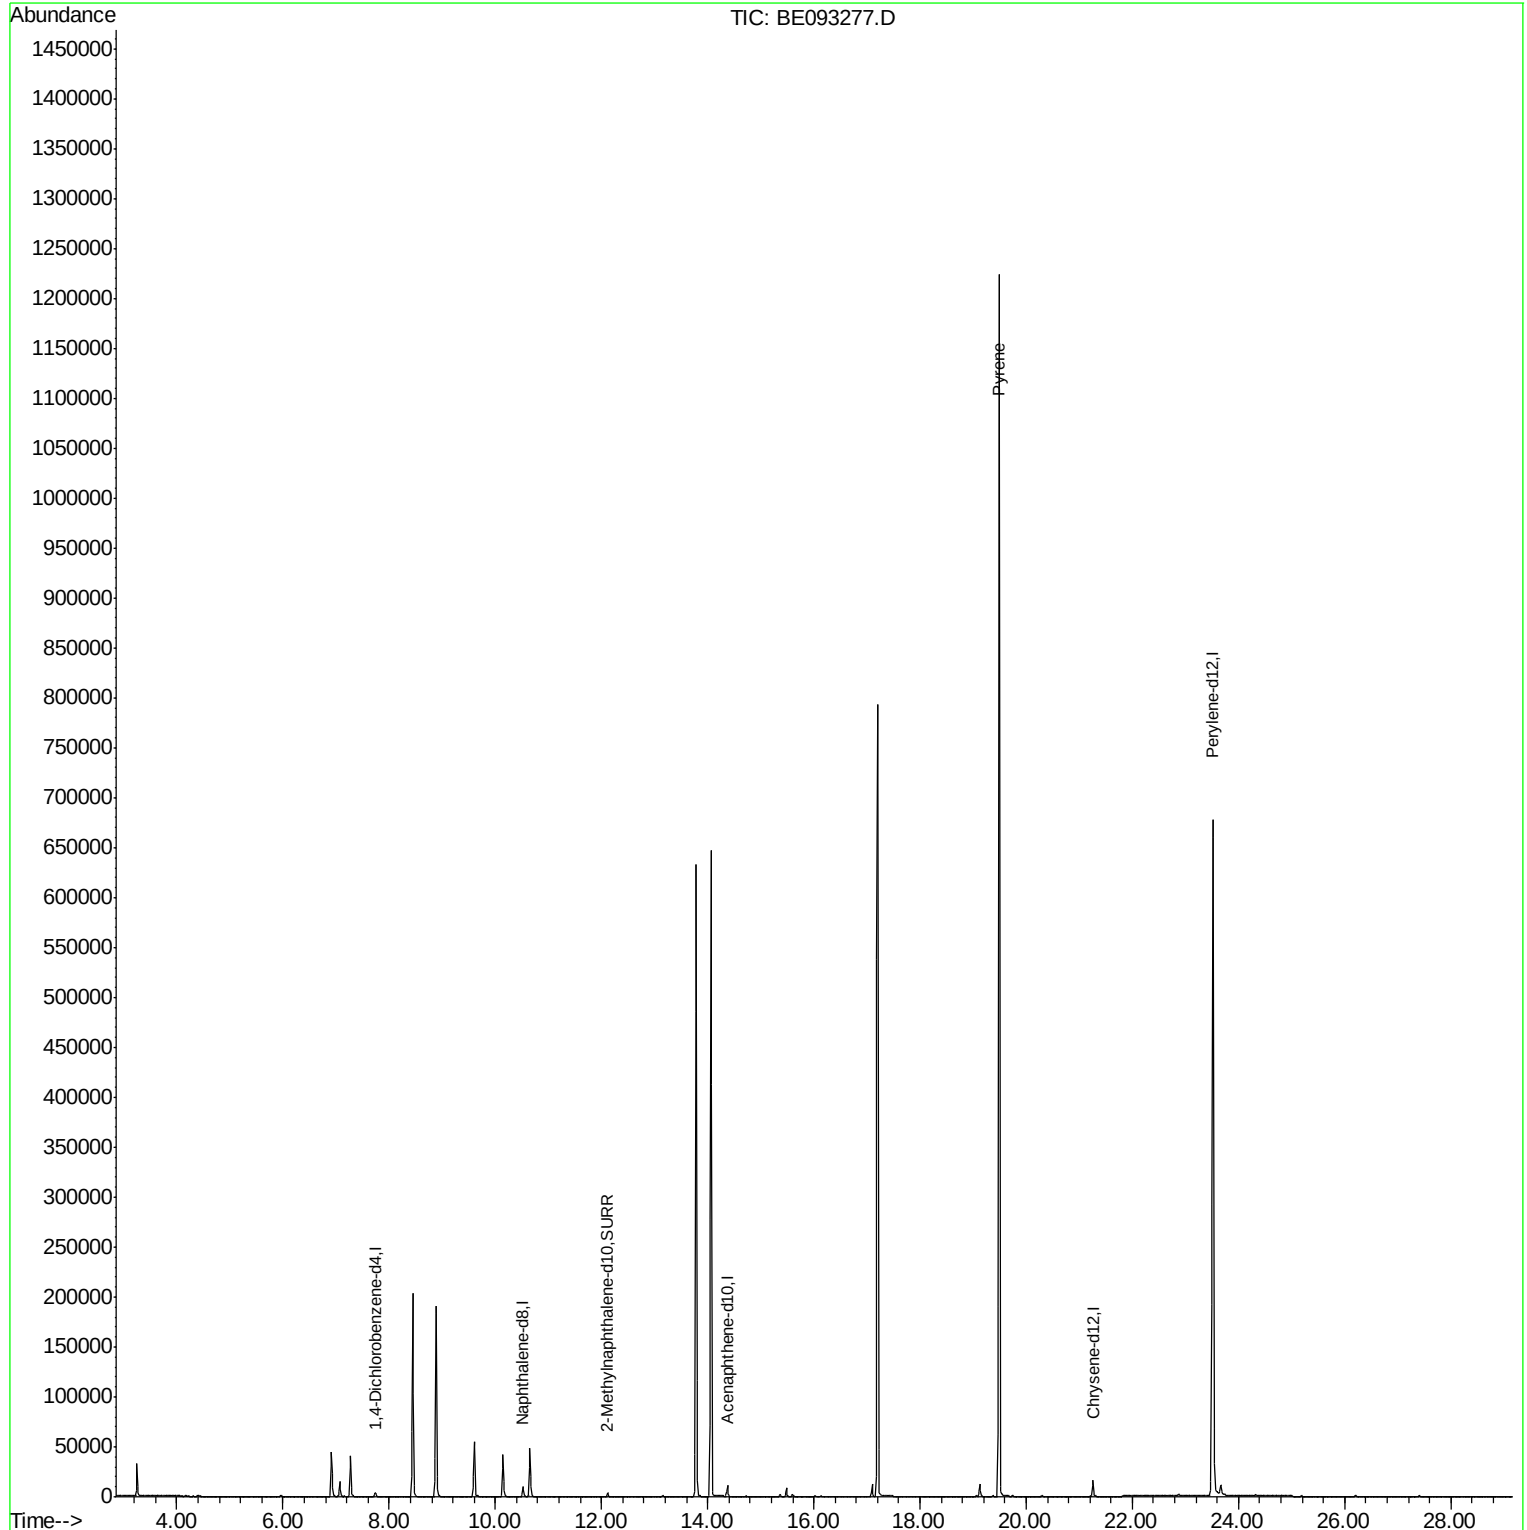

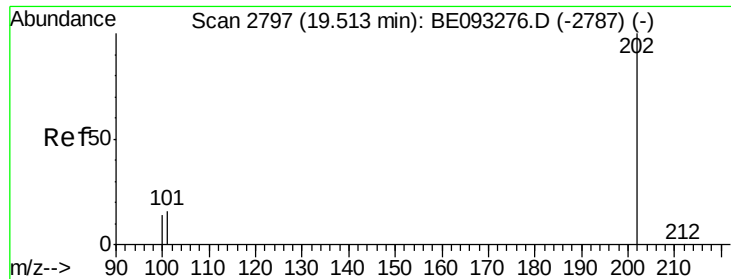

#17
 Pyrene
 Concen: 0.06 ng/ul
 RT: 19.49 min Scan# 2793
 Delta R.T. -0.02 min
 Lab File: BE093277.D
 Acq: 20 Jun 2017 12:18

Instrument :
 BNA_E
 ClientSampleId :
 SBLK55

Tgt Ion: 202 Resp: 2475
 Ion Ratio Lower Upper
 202 100
 101 189.4 18.2 27.4#
 100 1074.8 15.6 23.4#

