

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\
Quantitation Report (QT Reviewed)


Data File : BE093277.D
Acq On : 20 Jun 2017 12:18
Operator : SJ/JU
Sample : PB99755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:01 PM

Quant Time: Jun 21 01:56:51 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

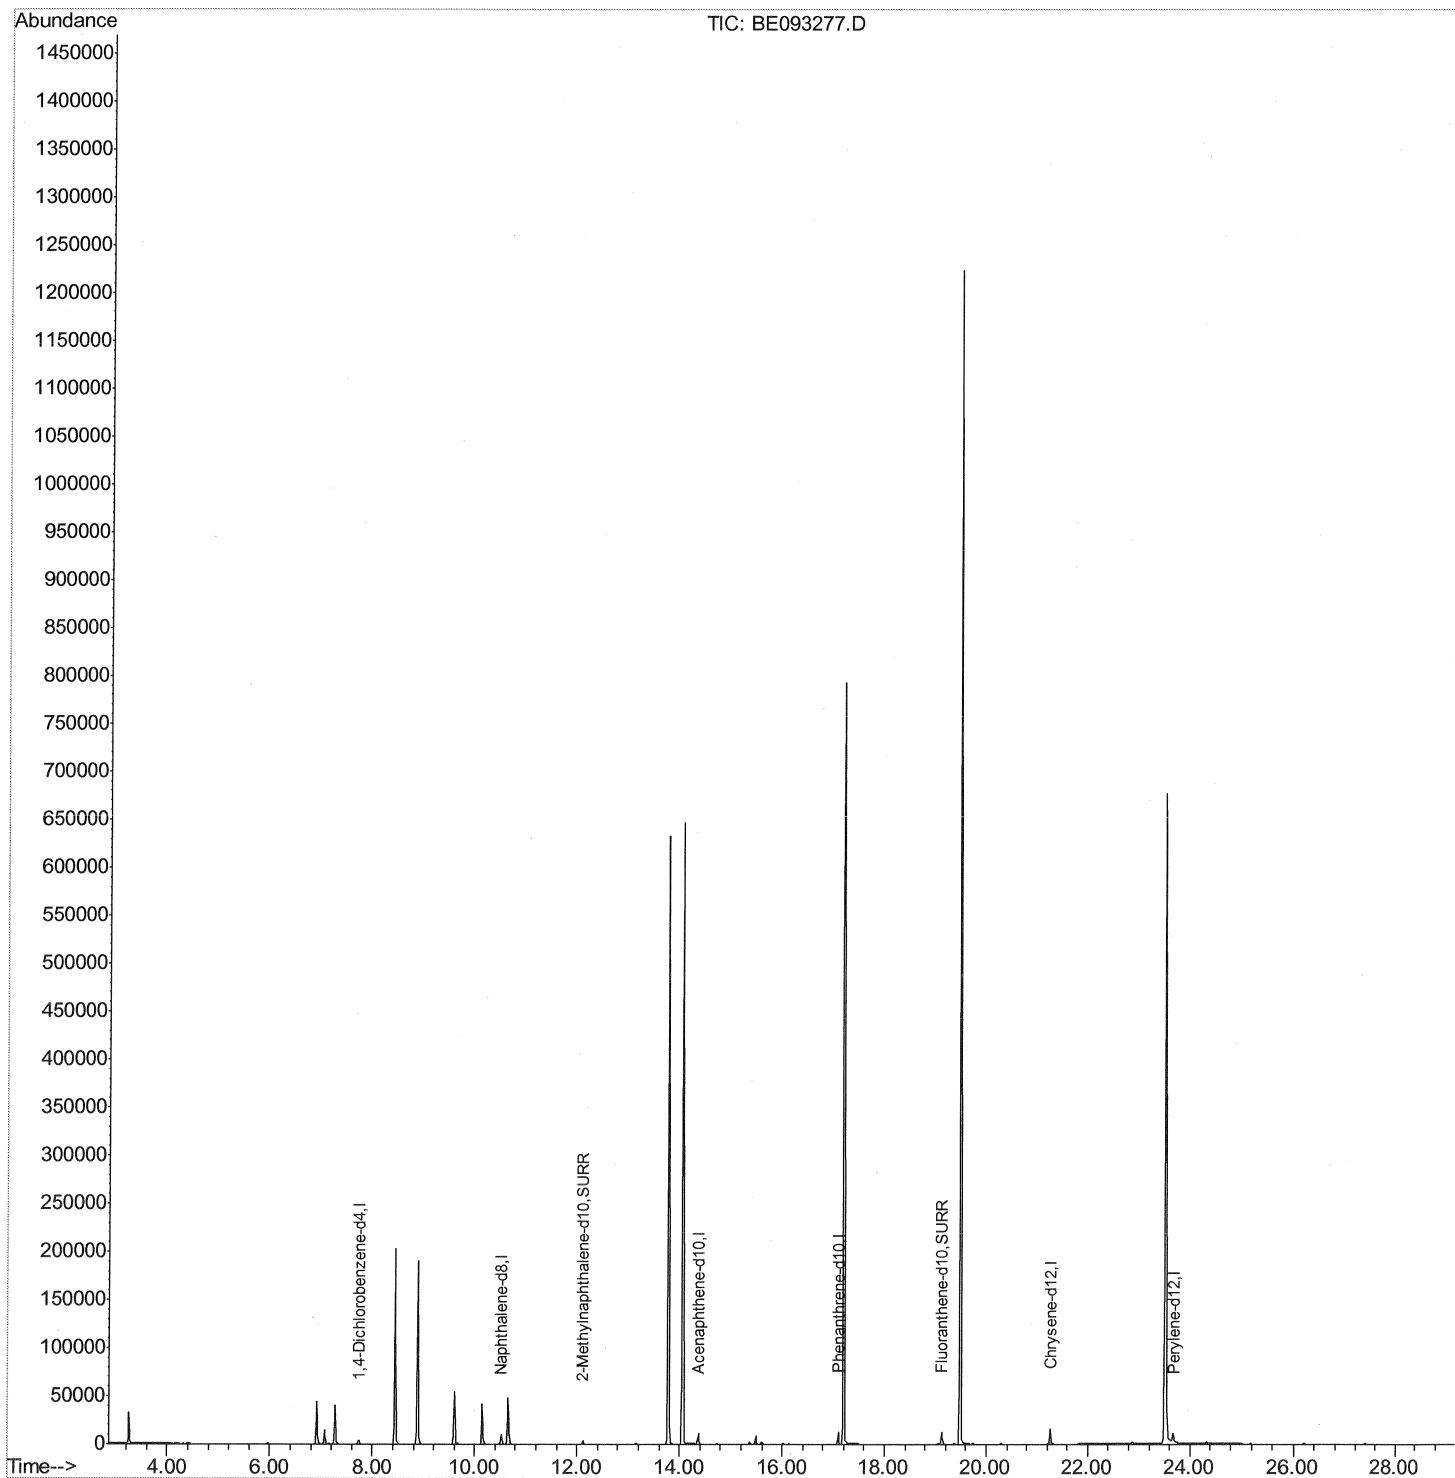

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\

Quantitation Report (Qedit)

Data File : BE093277.D

Acq On : 20 Jun 2017 12:18

Operator : SJ/JU

Sample : PB99755BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 21 01:50:05 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :


SBLK55

Manual Integrations

APPROVED

mohammad

6/21/2017 12:18:01 PM

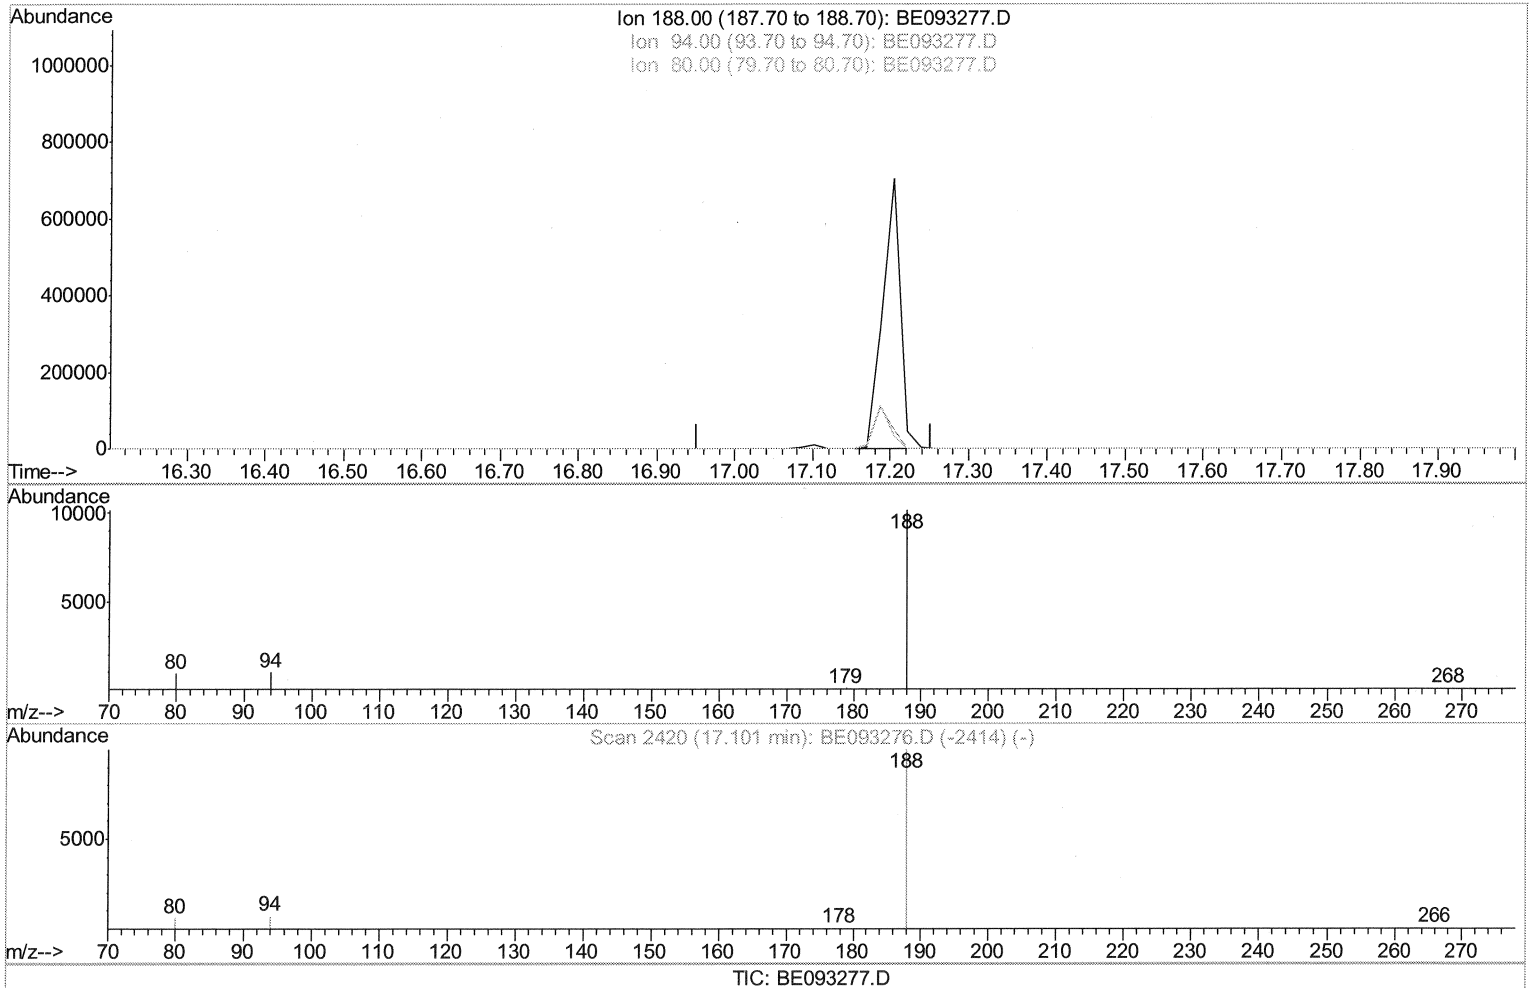

(10) Phenanthrene-d10 (I)

17.101min (-17.101) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\

Quantitation Report (Qedit)

Data File : BE093277.D

Acq On : 20 Jun 2017 12:18

Operator : SJ/JU

Sample : PB99755BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 21 01:50:05 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

Instrument :




BNA_E

ClientSampleId :

SBLK55

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:01 PM

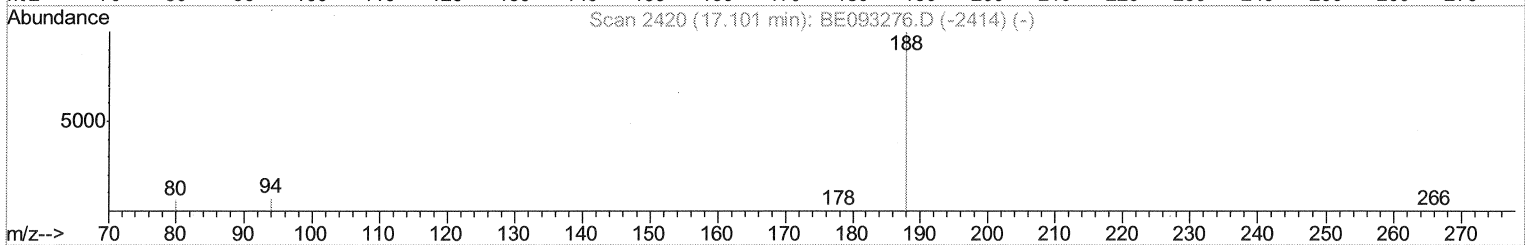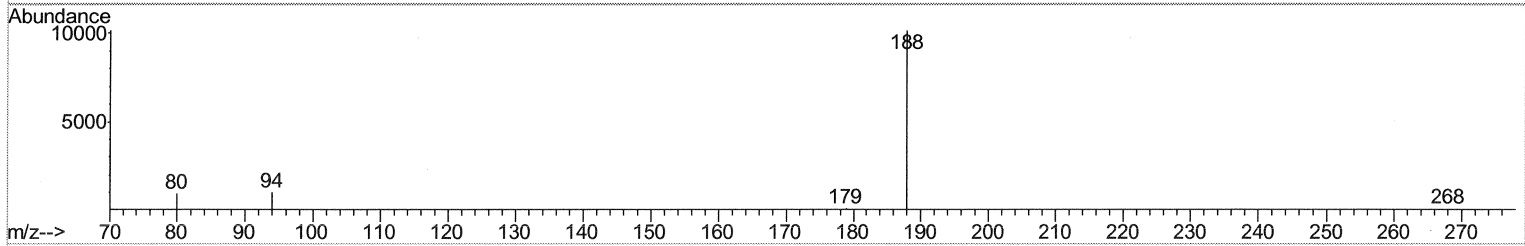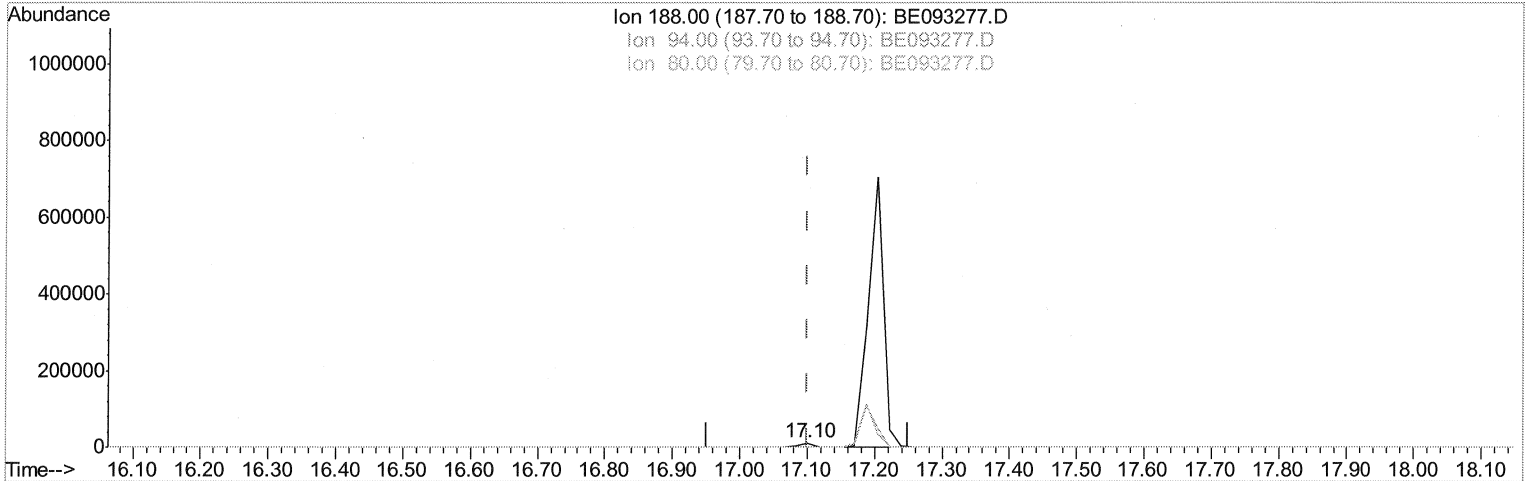

TIC: BE093277.D

(10) Phenanthrene-d10 (I)

17.101min (-0.000) 0.40ng/ul m

response 14057

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.75
80.00	11.80	9.20#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\

Quantitation Report (Qedit)

Data File : BE093277.D

Acq On : 20 Jun 2017 12:18

Operator : SJ/JU

Sample : PB99755BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 21 01:50:05 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




SBLK55

Manual Integrations

APPROVED

mohammad

6/21/2017 12:18:01 PM

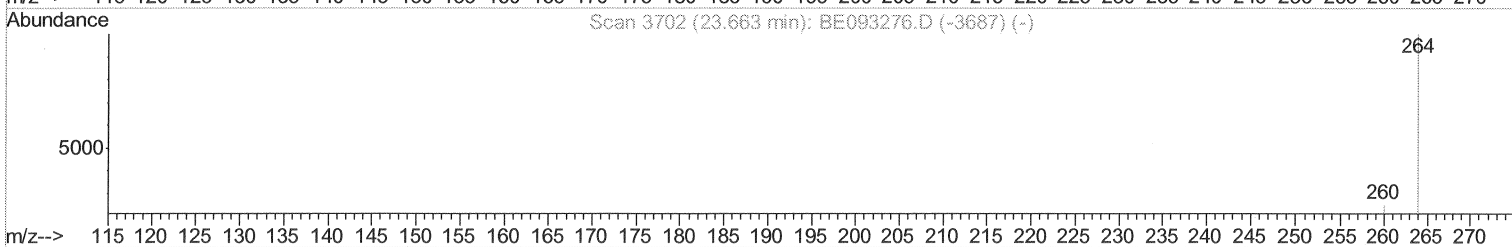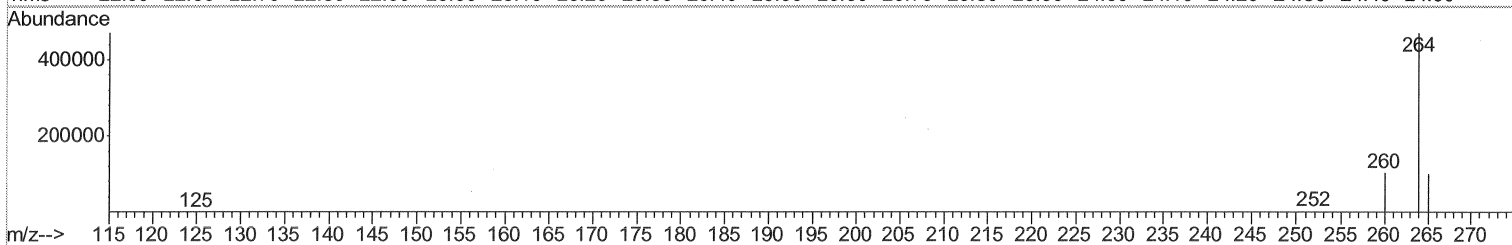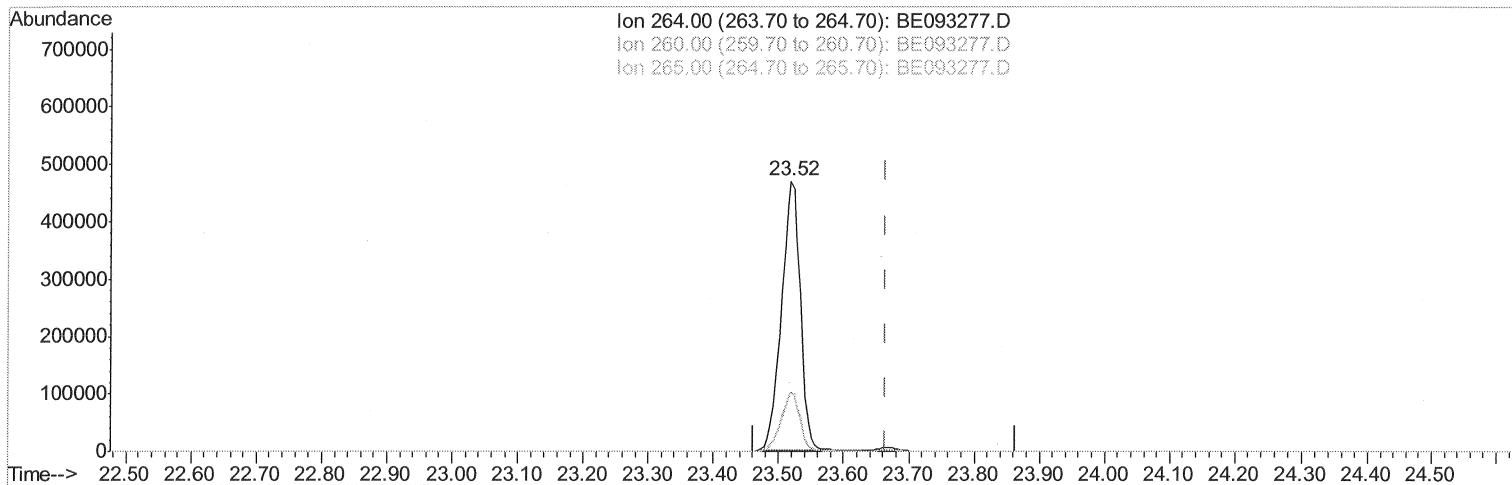

TIC: BE093277.D

(20) Perylene-d12 (I)

23.519min (-0.144) 0.40ng/ul

response 947620

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.99#
265.00	103.50	21.37#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\

Quantitation Report (Qedit)

Data File : BE093277.D

Acq On : 20 Jun 2017 12:18

Operator : SJ/JU

Sample : PB99755BL

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Jun 21 01:50:05 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

Instrument :




BNA_E

ClientSampled :

SBLK55

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:01 PM

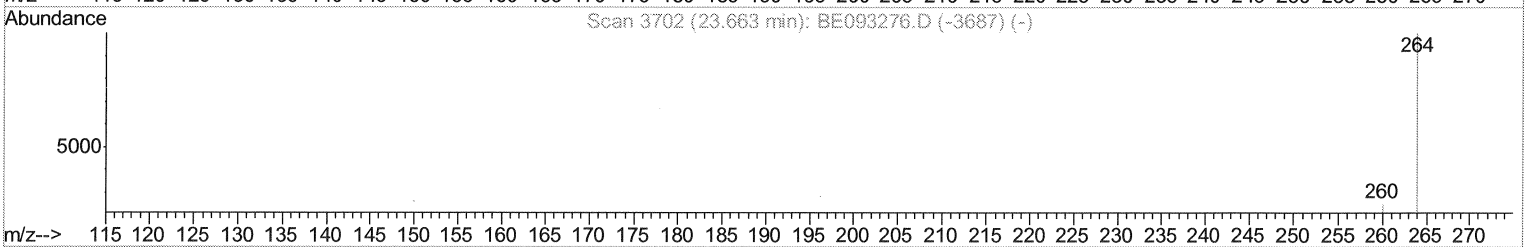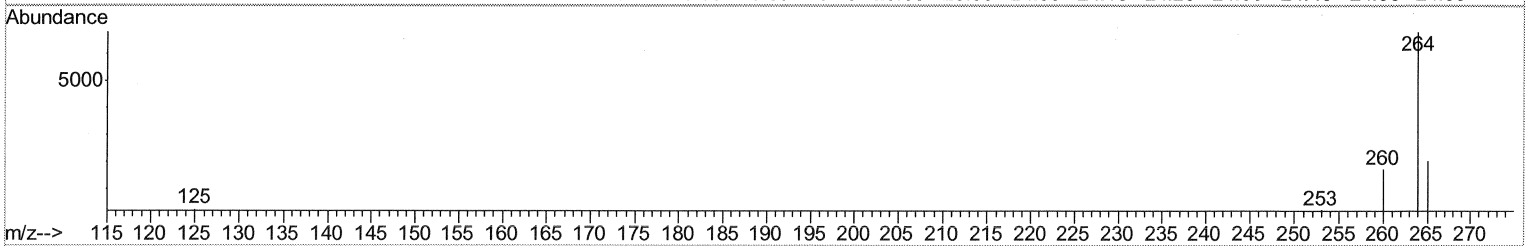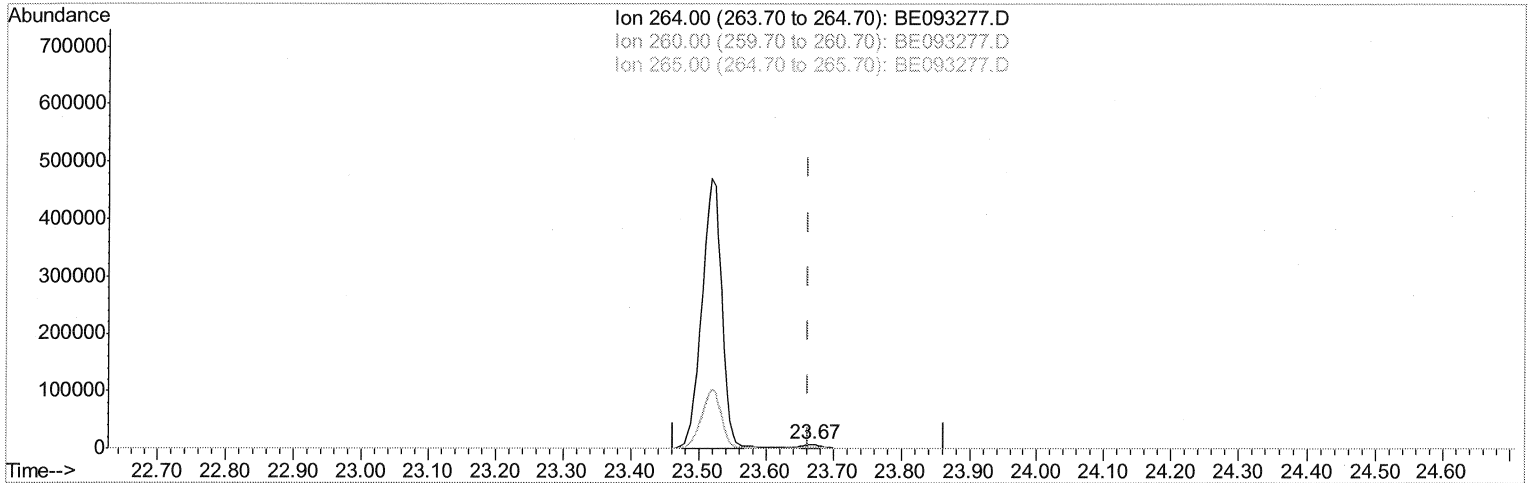

TIC: BE093277.D

(20) Perylene-d12 (I)

23.669min (+0.006) 0.40ng/ul m

response 11751

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.97
265.00	103.50	29.77#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\
Quantitation Report (QT Reviewed)

Data File : BE093277.D
Acq On : 20 Jun 2017 12:18
Operator : SJ/JU
Sample : PB99755BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK55

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:01 PM

Quant Time: Jun 21 01:56:51 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	1878	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	9794	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.37	164	6103	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	14057m	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	14177	0.40	ng/ul	0.00
20) Perylene-d12	23.67	264	11751m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	4942	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	12949	0.34	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed