

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\
Quantitation Report (QT Reviewed)


Data File : BE093287.D
Acq On : 20 Jun 2017 18:34
Operator : SJ/JU
Sample : I3627-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A44

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:30 PM

Quant Time: Jun 21 03:16:02 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

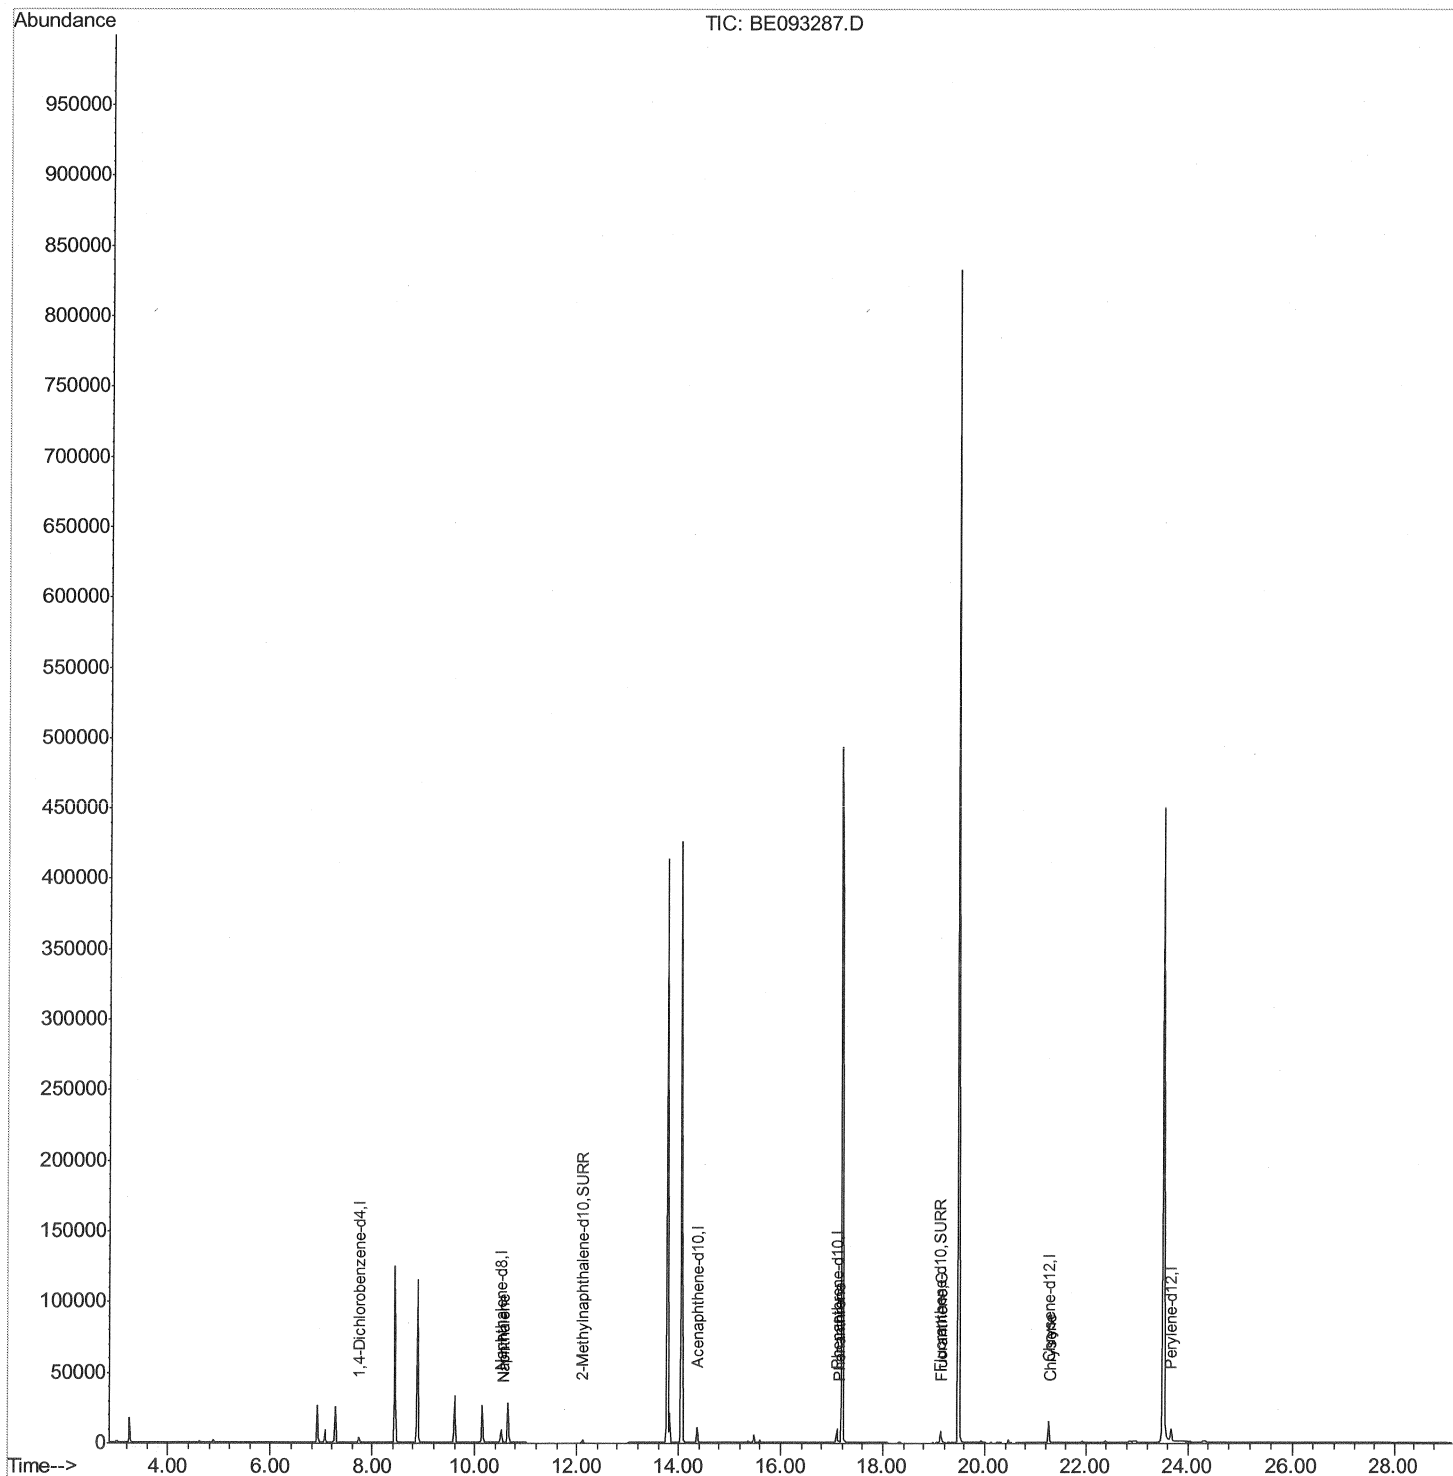

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\
Quantitation Report (Qedit)




Data File : BE093287.D
Acq On : 20 Jun 2017 18:34
Operator : SJ/JU
Sample : I3627-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A44

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:30 PM

Quant Time: Jun 21 01:51:19 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

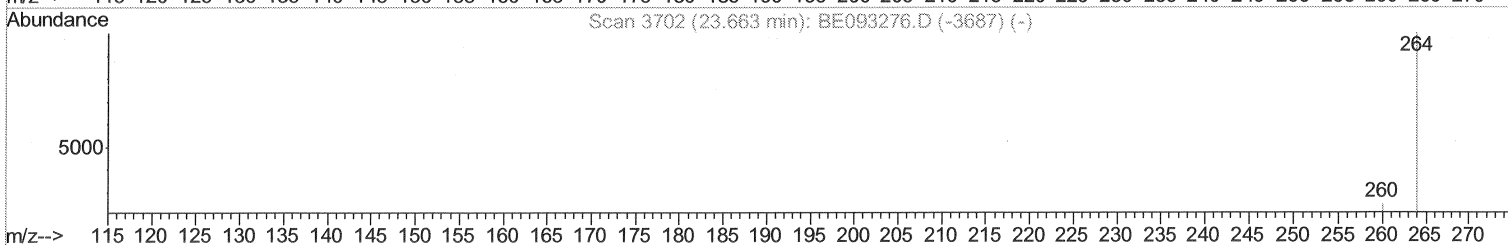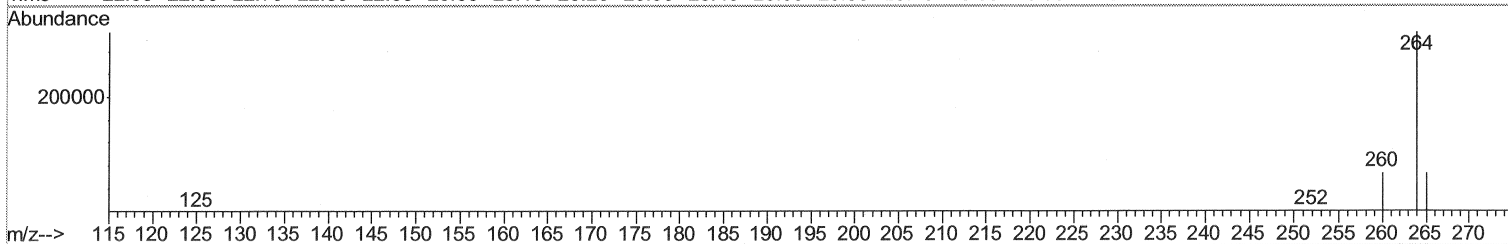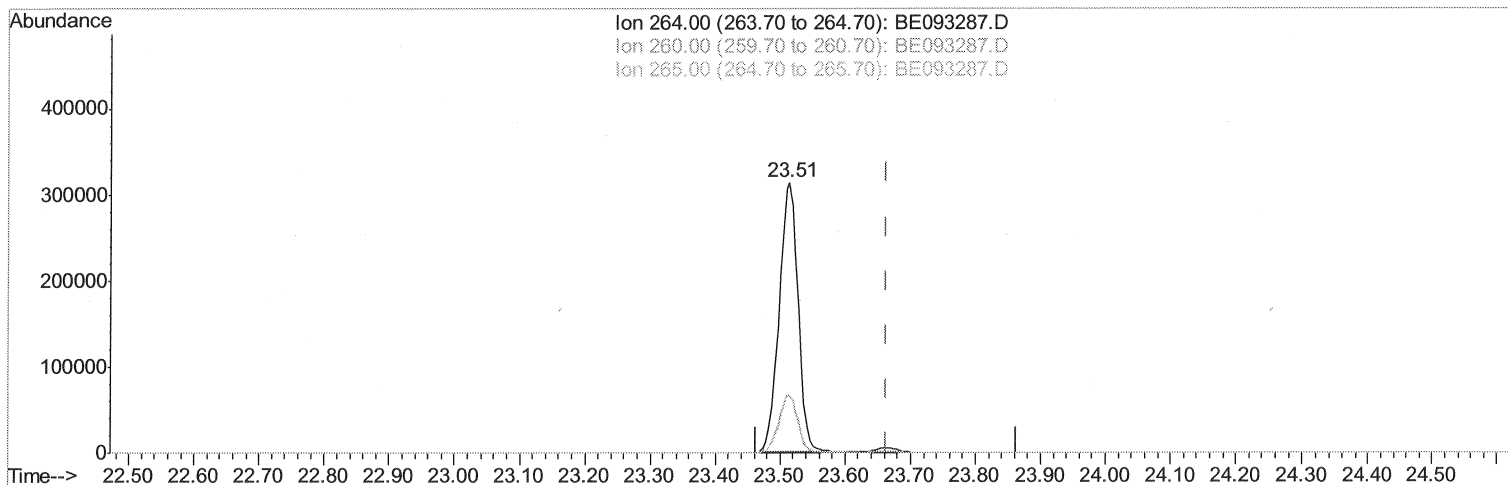

TIC: BE093287.D

(20) Perylene-d12 (I)

23.514min (-0.149) 0.40ng/ul

response 636935

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.53#
265.00	103.50	21.44#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\

Quantitation Report (Qedit)

Data File : BE093287.D

Acq On : 20 Jun 2017 18:34

Operator : SJ/JU

Sample : I3627-05

Misc :

ALS Vial : 13 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F5A44

Manual Integrations
APPROVED

mohammad

6/21/2017 12:18:30 PM




Quant Time: Jun 21 01:51:19 2017

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jun 21 01:49:50 2017

Response via : Initial Calibration

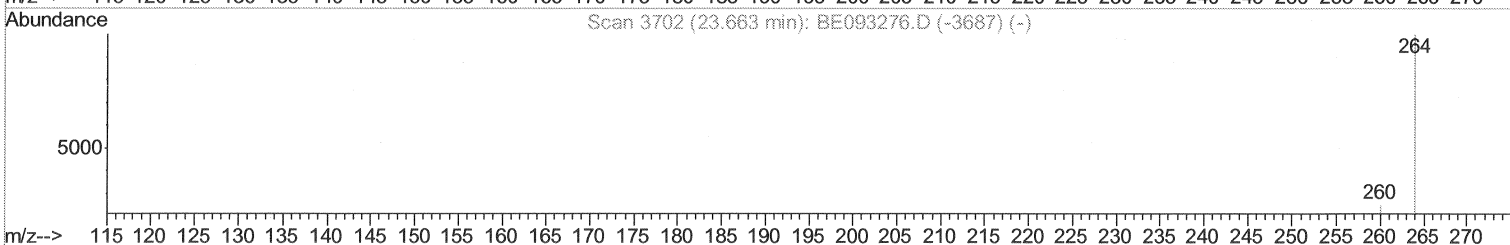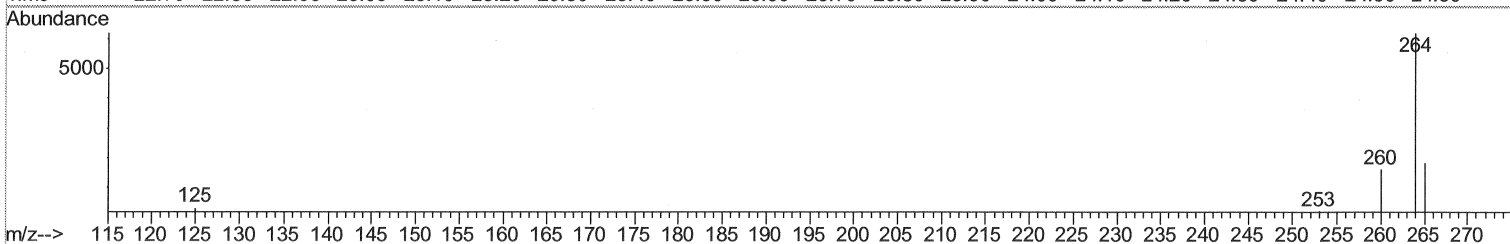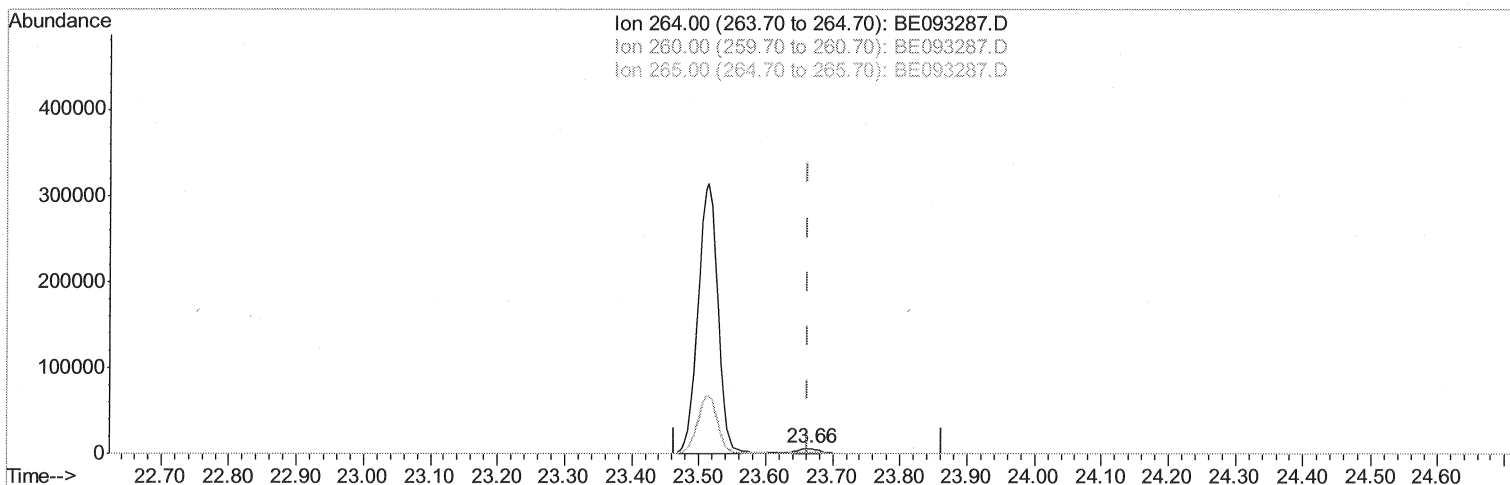

TIC: BE093287.D

(20) Perylene-d12 (I)

23.665min (+0.001) 0.40ng/ul m

response 10926

Ion Exp% Act%

264.00 100 100

260.00 30.10 25.73

265.00 103.50 29.09#

0.00 0.00 0.00

57
6/26/17

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062017\
Quantitation Report (QT Reviewed)

Data File : BE093287.D
Acq On : 20 Jun 2017 18:34
Operator : SJ/JU
Sample : I3627-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5A44

Manual Integrations
APPROVED

mohammad
6/21/2017 12:18:30 PM

Quant Time: Jun 21 03:16:02 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 01:49:50 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	1726	0.40	ng/ul	0.00
2) Naphthalene-d8	10.52	136	9046	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	5644	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.10	188	13406	0.40	ng/ul	0.00
16) Chrysene-d12	21.26	240	13386	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	10926m)	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.11	152	3154	0.24	ng/ul	0.00
14) Fluoranthene-d10	19.13	212	8970	0.25	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.56	128	561	0.02	ng/ul#	79
12) Phenanthrene	17.14	178	1016	0.03	ng/ul#	90
15) Fluoranthene	19.15	202	1559	0.03	ng/ul	86
19) Chrysene	21.29	228	986	0.03	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed