


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062118\
 Data File : BE096835.D
 Acq On : 21 Jun 2018 8:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 20 15:45:14 2018

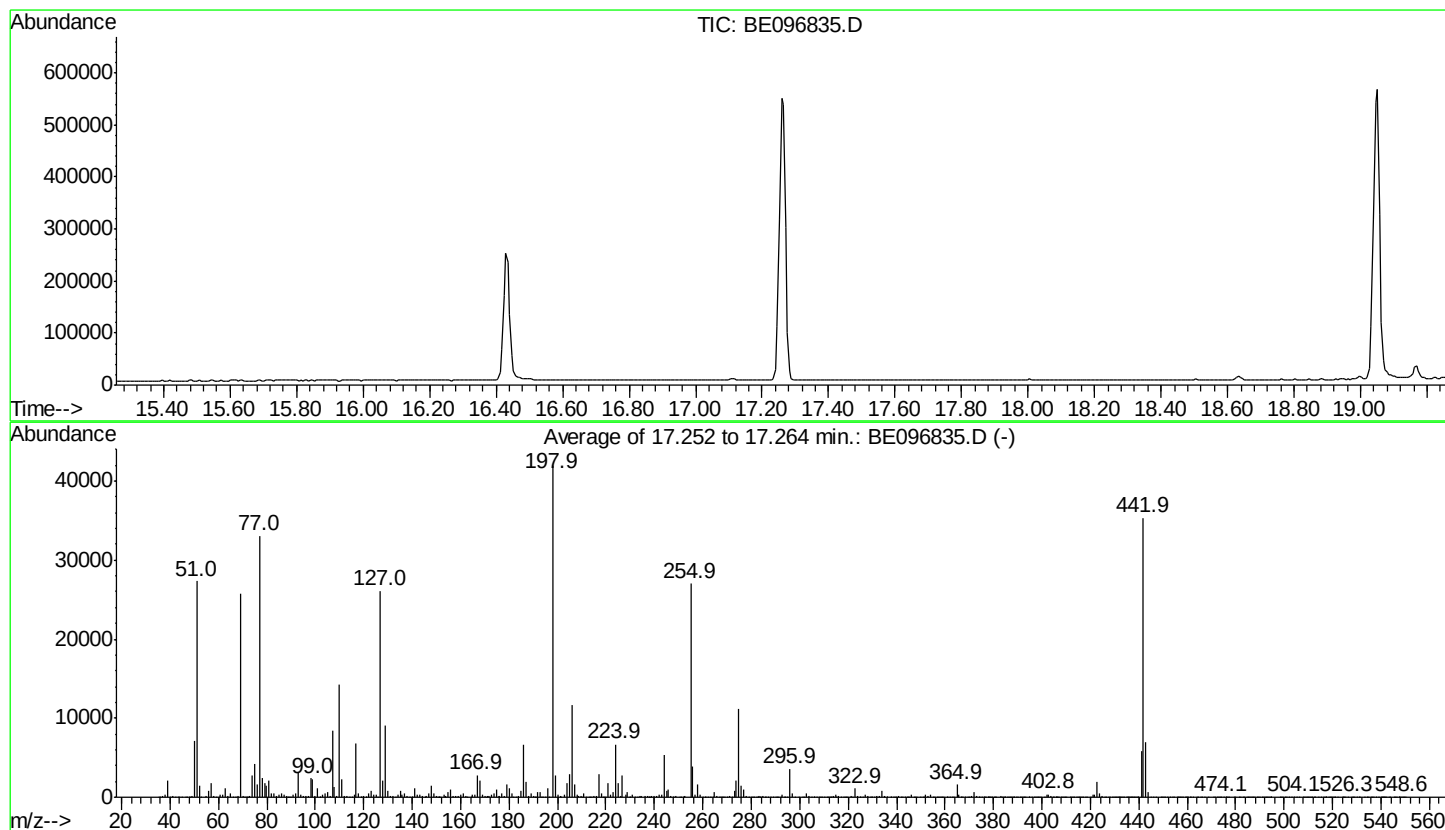

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.1	27307	PASS
68	69	0.00	2	0.5	134	PASS
69	198	0.00	100	61.4	25741	PASS
70	69	0.00	2	0.6	160	PASS
127	198	10	80	62.2	26103	PASS
197	198	0.00	2	0.1	59	PASS
198	198	100	100	100.0	41954	PASS
199	198	5	9	6.7	2828	PASS
275	198	10	60	26.7	11203	PASS
365	198	1	100	3.7	1570	PASS
441	443	0.01	100	83.0	5785	PASS
442	198	50	100	84.2	35322	PASS
443	442	15	24	19.7	6968	PASS