


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062118\  
 Data File : BE096835.D  
 Acq On : 21 Jun 2018 8:49  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE062018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jun 20 15:45:14 2018

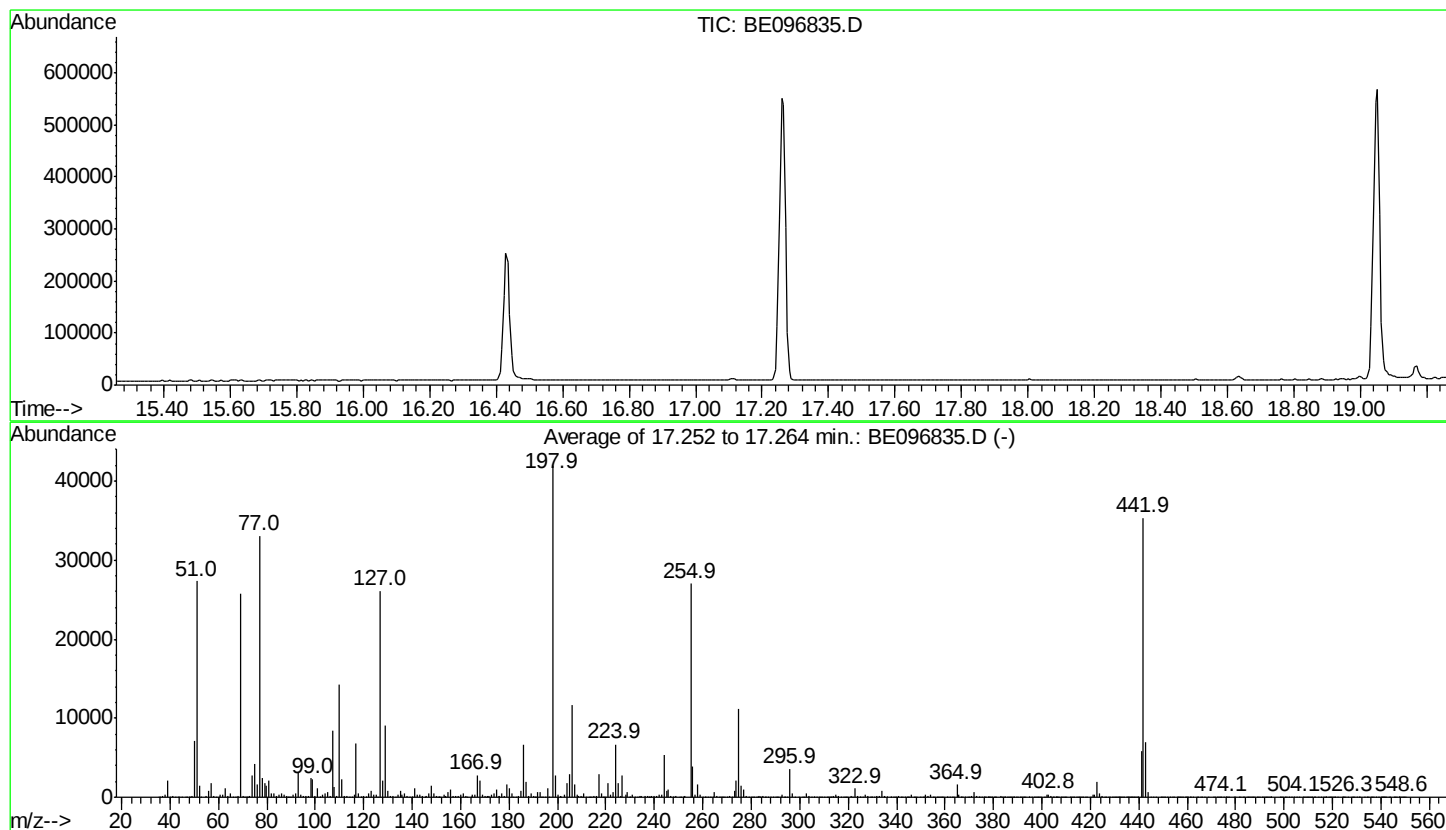

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2488

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 65.1      | 27307   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.5       | 134     | PASS             |
| 69          | 198          | 0.00         | 100          | 61.4      | 25741   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 160     | PASS             |
| 127         | 198          | 10           | 80           | 62.2      | 26103   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.1       | 59      | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 41954   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 2828    | PASS             |
| 275         | 198          | 10           | 60           | 26.7      | 11203   | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 1570    | PASS             |
| 441         | 443          | 0.01         | 100          | 83.0      | 5785    | PASS             |
| 442         | 198          | 50           | 100          | 84.2      | 35322   | PASS             |
| 443         | 442          | 15           | 24           | 19.7      | 6968    | PASS             |