

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062217\
 Data File : BE093330.D
 Acq On : 22 Jun 2017 16:10
 Operator : SJ/JU
 Sample : I3687-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS033-170613

Manual Integrations
 APPROVED

mohammad
 6/26/2017 11:29:28 AM

Quant Time: Jun 23 08:05:22 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 12 14:07:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	195	0.40	ng	-0.02
7) Naphthalene-d8	10.51	136	950	0.40	ng	-0.02
13) Acenaphthene-d10	14.37	164	573	0.40	ng	0.00
19) Phenanthrene-d10	17.10	188	1208	0.40	ng	-0.03
27) Chrysene-d12	21.25	240	1499	0.40	ng	-0.02
34) Perylene-d12	23.65	264	1240	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	92	0.16	ng	0.00
5) Phenol-d6	6.90	99	87m	0.10	ng	0.00
8) Nitrobenzene-d5	8.86	82	278	0.37	ng	-0.02
11) 2-Methylnaphthalene-d10	12.10	152	498	0.35	ng	-0.01
14) 2,4,6-Tribromophenol	15.85	330	71	0.54	ng	0.00
15) 2-Fluorobiphenyl	12.99	172	840	0.34	ng	0.00
25) Fluoranthene-d10	19.11	212	1385m	0.35	ng	0.00
29) Terphenyl-d14	19.72	244	1078	0.37	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.16	149	194	0.092	ng	Qvalue # 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062217\
Data File : BE093330.D
Acq On : 22 Jun 2017 16:10
Operator : SJ/JU
Sample : I3687-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
KY038PS033-170613

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:28 AM

Quant Time: Jun 23 08:05:22 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 12 14:07:54 2017
Response via : Initial Calibration

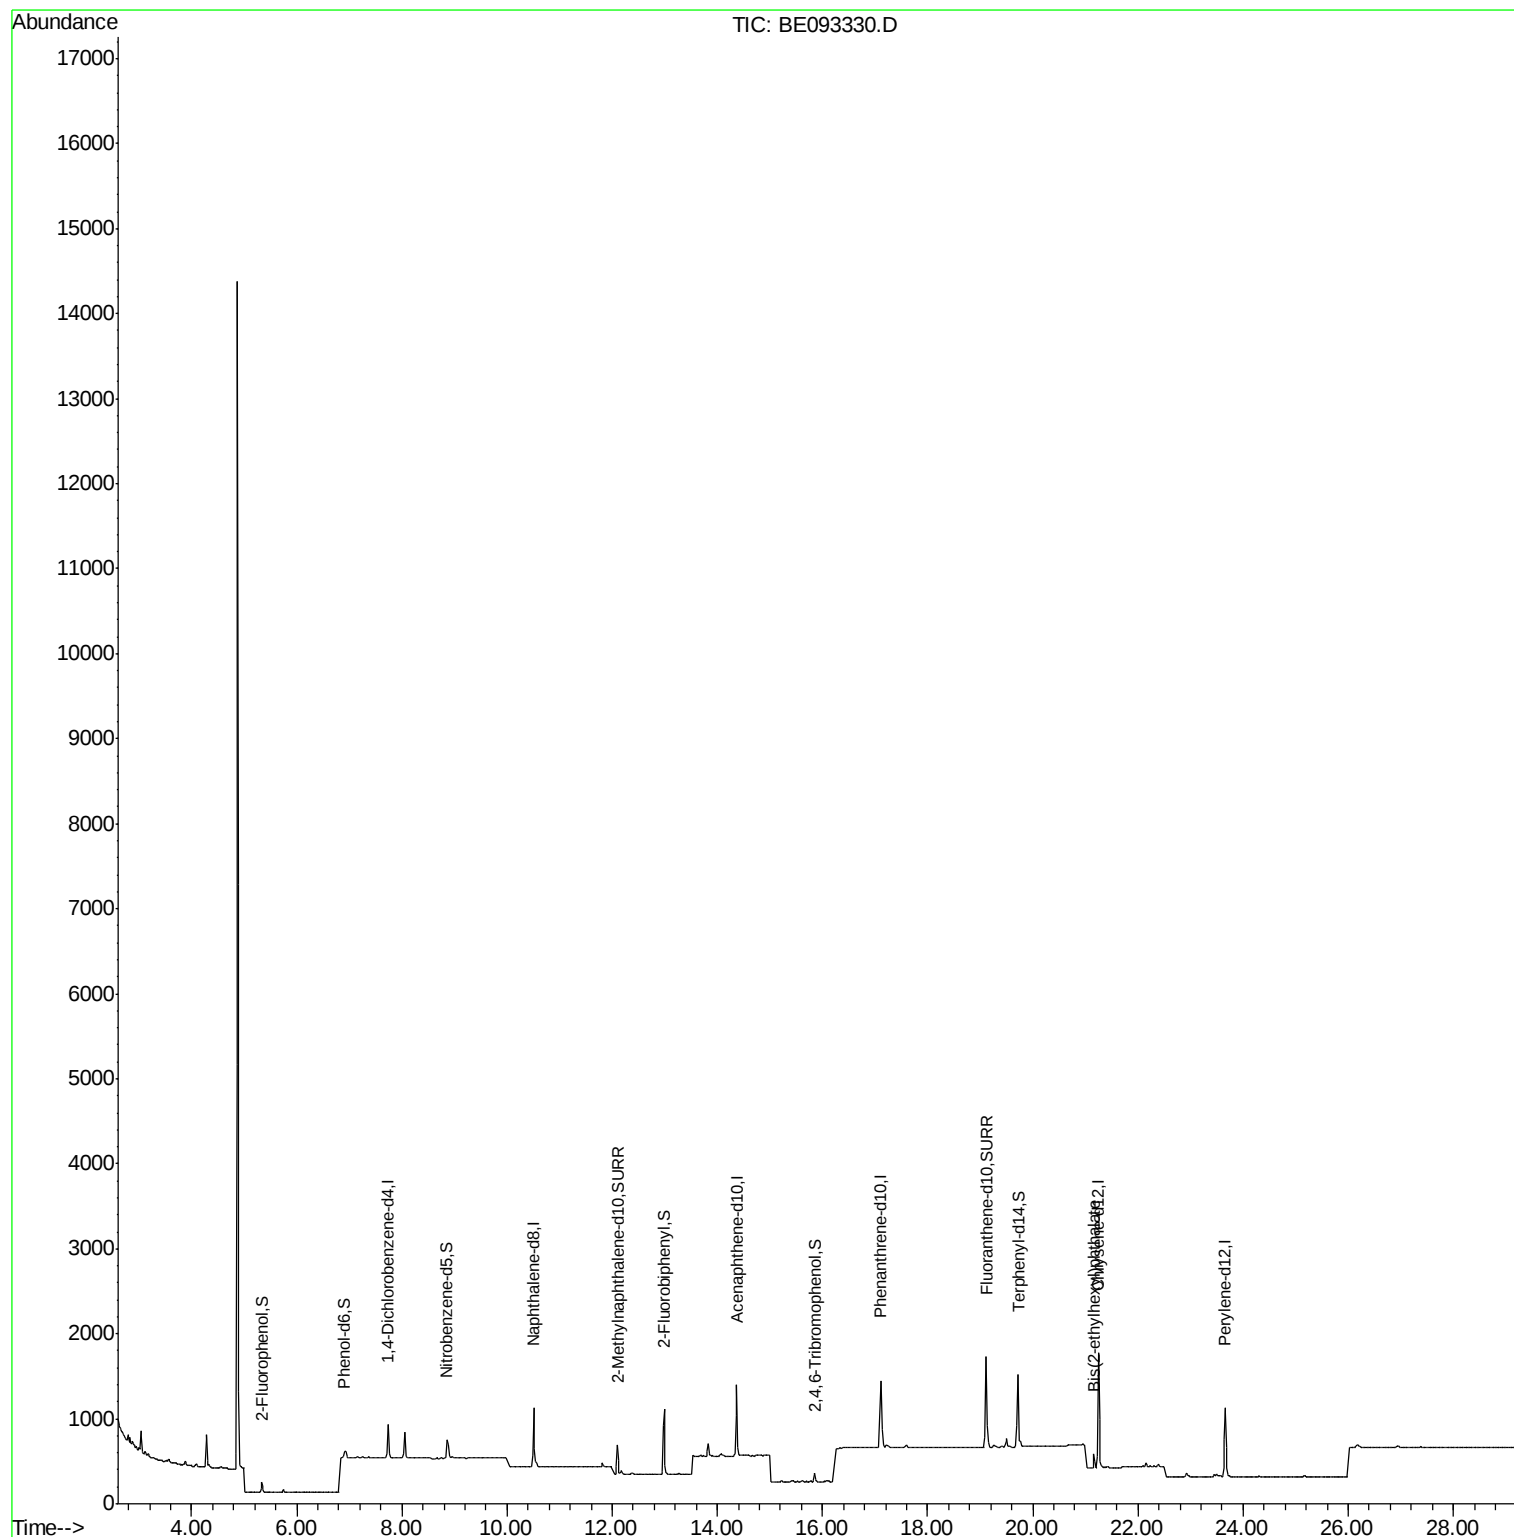




#1

1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.73 min Scan# 554
Delta R.T. -0.02 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10




Instrument :
BNA_E
ClientSampleId :
KY038PS033-170613

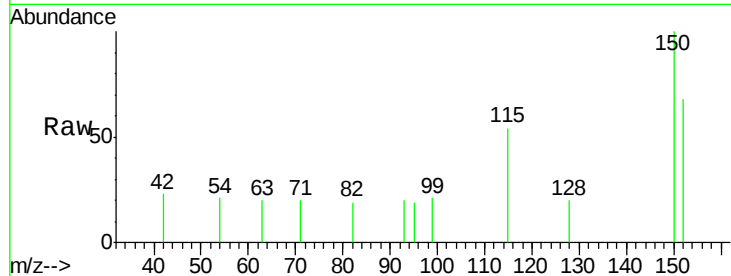

Tgt Ion	Ratio	Lower	Upper
152	100		
150	146.5	125.1	187.7
115	79.6	55.7	83.5

Manual Integrations
APPROVED




mohammad
6/26/2017 11:29:28 AM

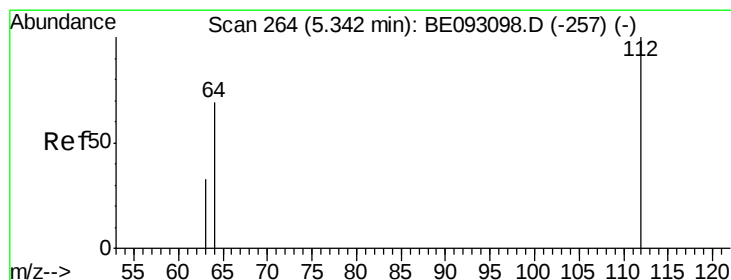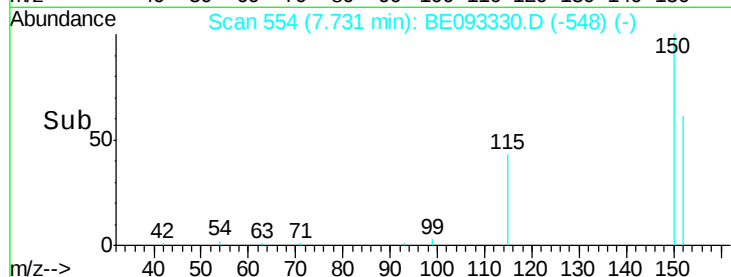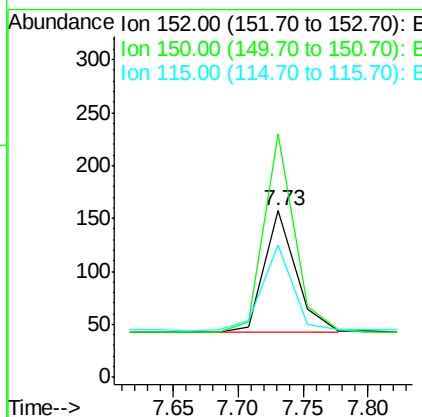


#4

2-Fluorophenol
Concen: 0.160 ng
RT: 5.34 min Scan# 264
Delta R.T. 0.00 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.7	56.4	84.6
63	39.1	29.3	43.9

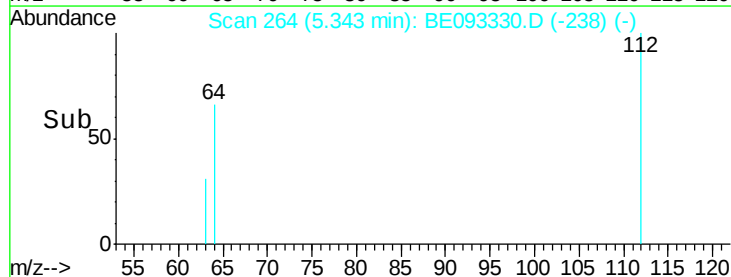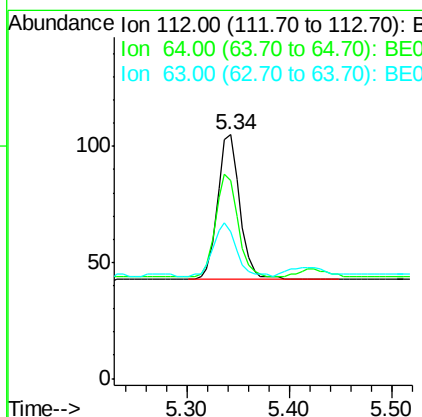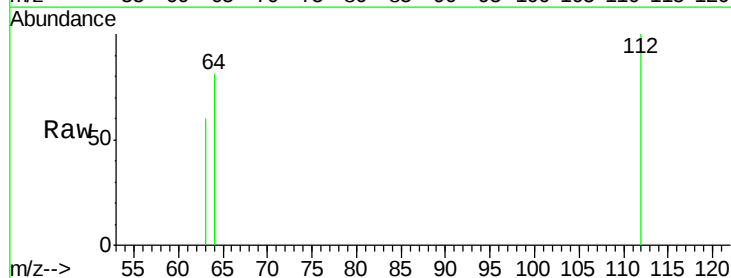



#5

Phenol-d6

Concen: 0.103 ng m

RT: 6.90 min Scan# 518

Delta R.T. 0.00 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Instrument :

BNA_E





ClientSampleId :

KY038PS033-170613

Tgt Ion	Ratio	Lower	Upper
99	100		
42	639.1	0.0	0.0#
71	589.7	0.0	0.0#

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:28 AM

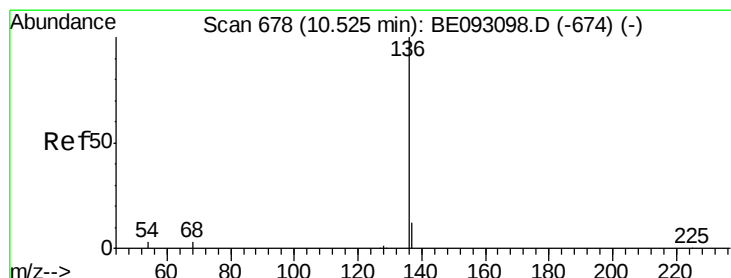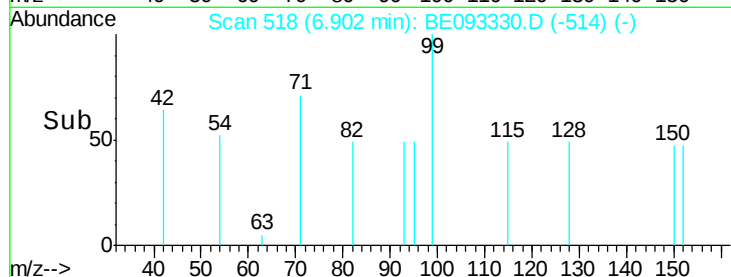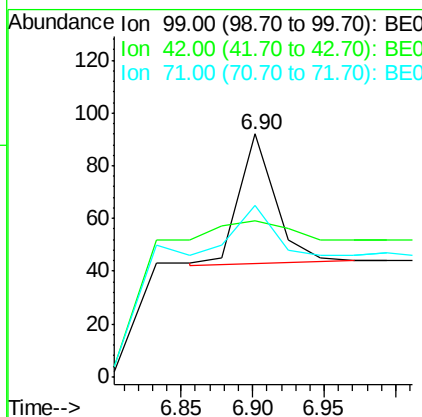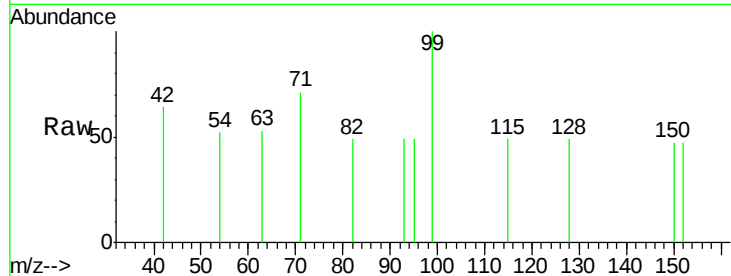

#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.51 min Scan# 677


Delta R.T. -0.02 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Tgt Ion	Ratio	Lower	Upper
136	100		
137	16.9	9.8	14.8#
54	15.2	10.3	15.5
68	14.9	9.0	13.4#

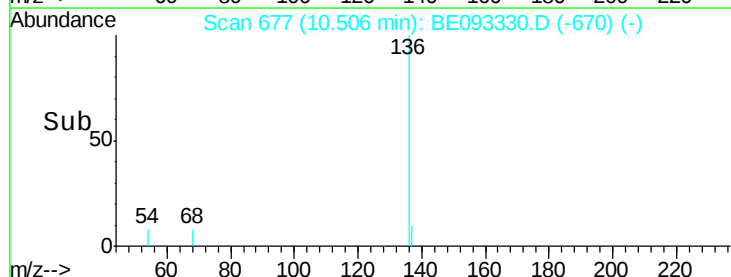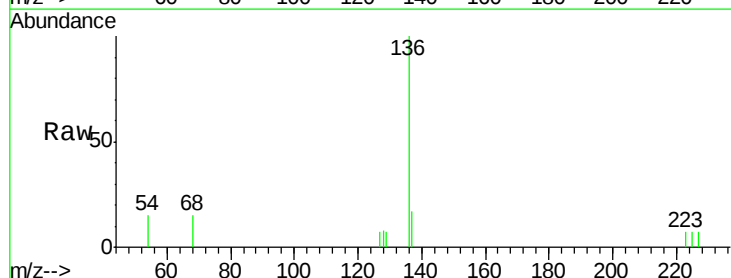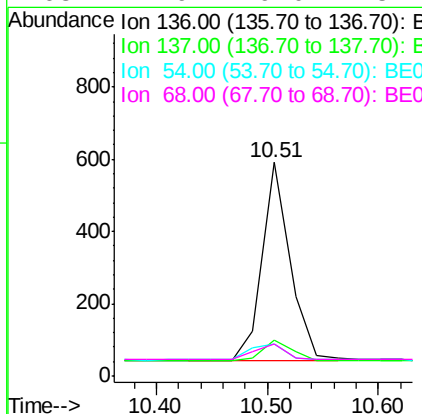

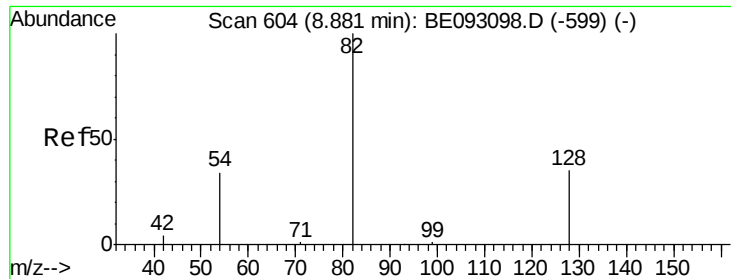





#8
 Nitrobenzene-d5
 Concen: 0.367 ng
 RT: 8.86 min Scan# 603
 Delta R.T. -0.02 min
 Lab File: BE093330.D
 Acq: 22 Jun 2017 16:10

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS033-170613

Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.6	17.0	25.4#
54	81.0	53.8	80.6#




Manual Integrations
 APPROVED


mohammad
 6/26/2017 11:29:28 AM

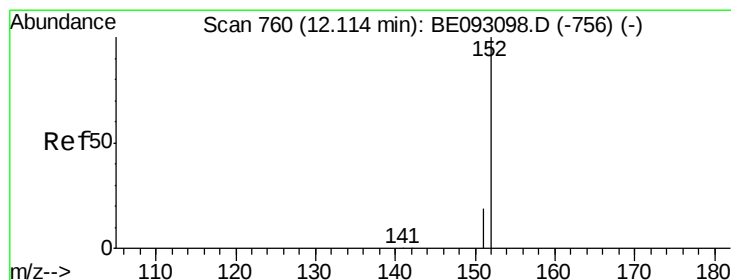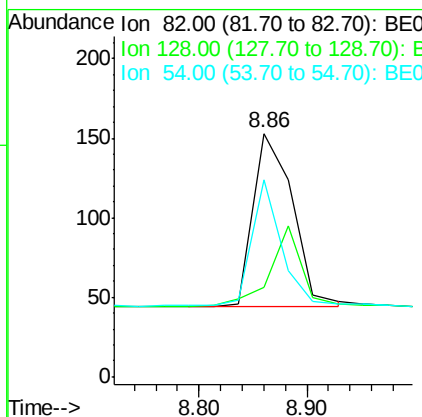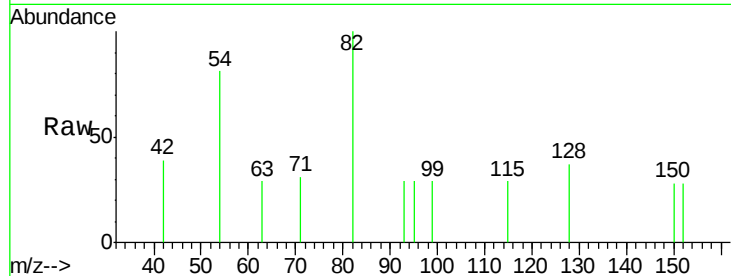

#11
 2-Methylnaphthalene-d10
 Concen: 0.349 ng
 RT: 12.10 min Scan# 759
 Delta R.T. -0.01 min
 Lab File: BE093330.D
 Acq: 22 Jun 2017 16:10

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.3	15.1	22.7

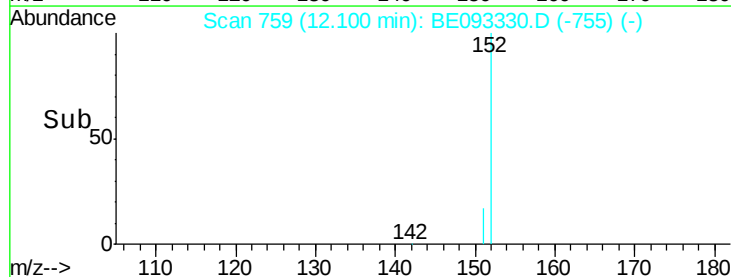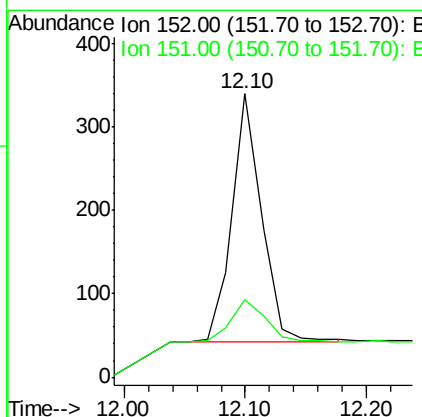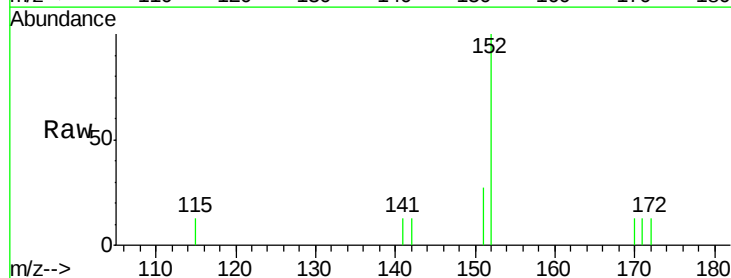

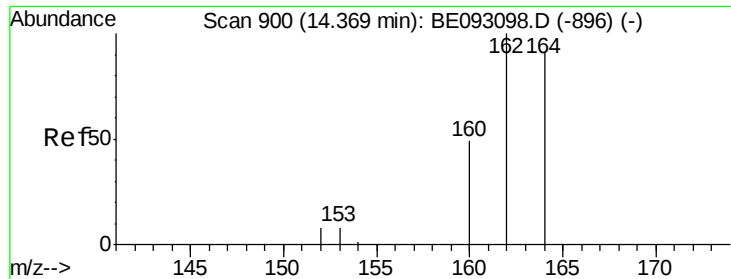





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.37 min Scan# 900
Delta R.T. 0.00 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10

Instrument :
BNA_E
ClientSampleId :
KY038PS033-170613

Tgt Ion:164 Resp: 573
Ion Ratio Lower Upper
164 100
162 94.8 84.6 127.0
160 45.5 41.8 62.6




Manual Integrations
APPROVED


mohammad
6/26/2017 11:29:28 AM

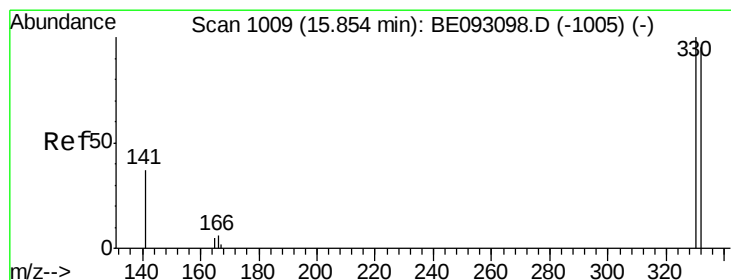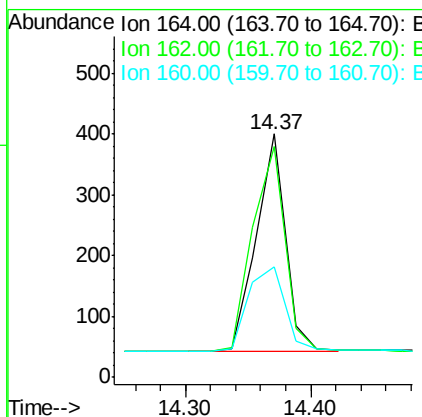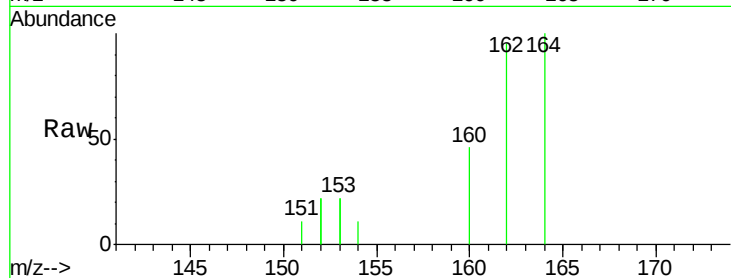

#14
2,4,6-Tribromophenol
Concen: 0.544 ng
RT: 15.85 min Scan# 1008
Delta R.T. -0.00 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10

Tgt Ion:330 Resp: 71
Ion Ratio Lower Upper
330 100
332 94.4 77.7 116.5
141 46.5 56.2 84.4#

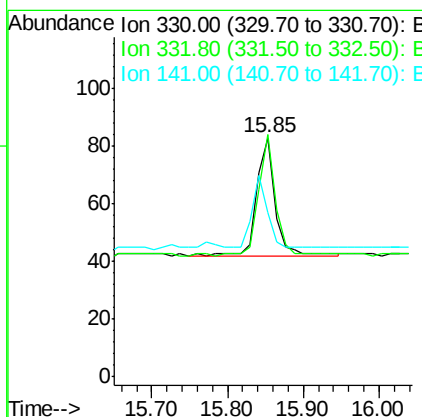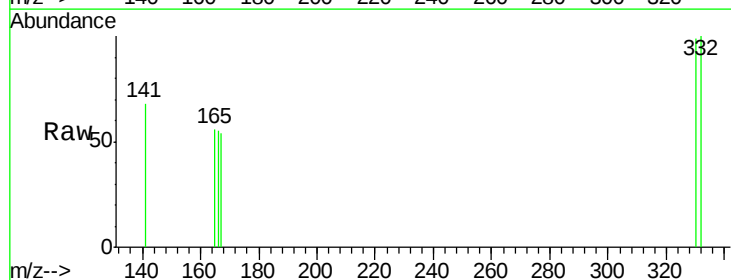

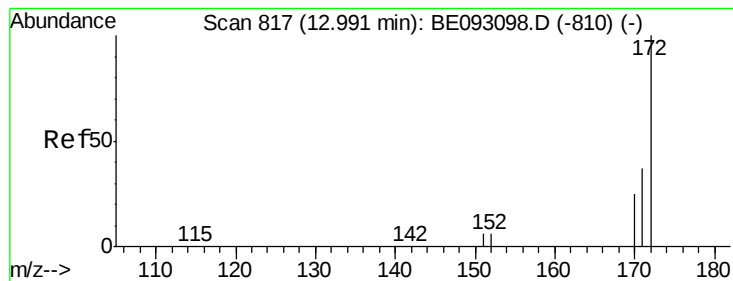


#15
2-Fluorobiphenyl
Concen: 0.343 ng
RT: 12.99 min Scan# 817
Delta R.T. 0.00 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10

Instrument :
BNA_E
ClientSampleId :
KY038PS033-170613


Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.8	44.6
170	24.3	20.7	31.1

Manual Integrations
APPROVED



mohammad
6/26/2017 11:29:28 AM

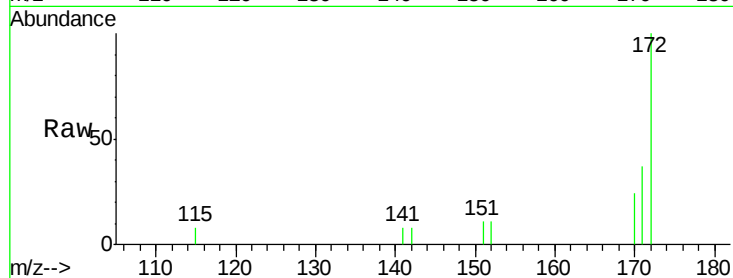

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

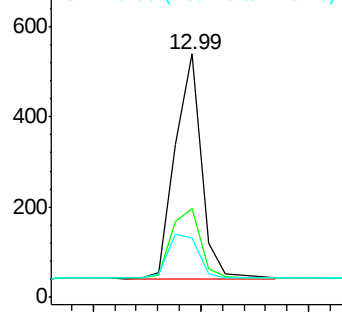


Time-->

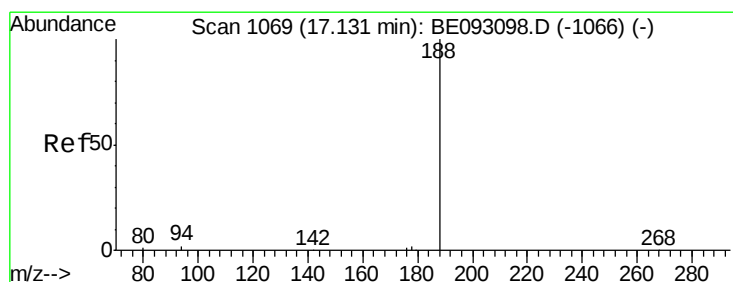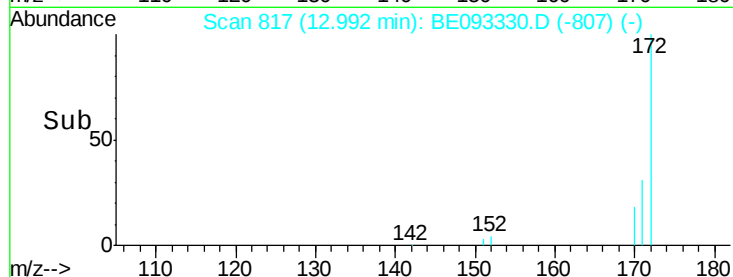


#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.10 min Scan# 1068
Delta R.T. -0.03 min
Lab File: BE093330.D
Acq: 22 Jun 2017 16:10


Tgt Ion	Ratio	Lower	Upper
188	100		
94	35.0	11.3	16.9#
80	40.0	11.7	17.5#

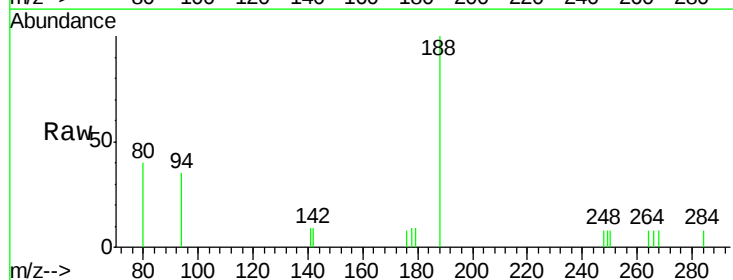


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

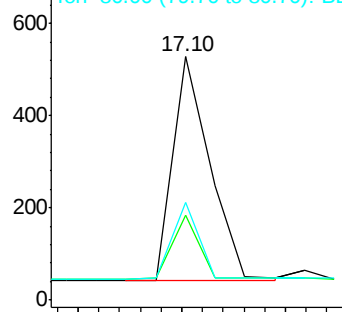

Time-->

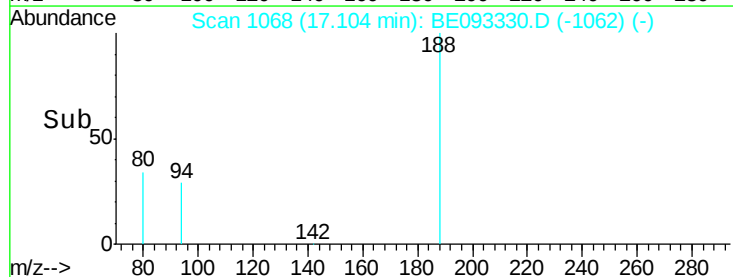

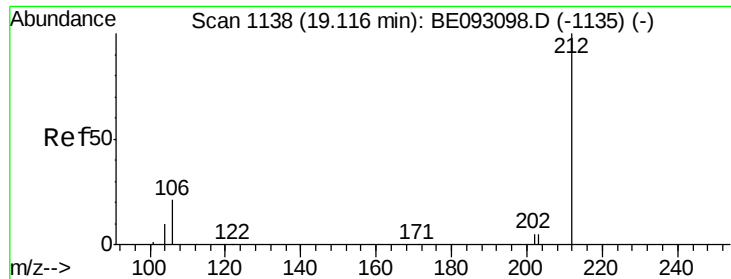

#25

Fluoranthene-d10

Concen: 0.348 ng m

RT: 19.11 min Scan# 1138

Delta R.T. -0.00 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Instrument :

BNA_E


ClientSampleId :

KY038PS033-170613




Tgt Ion	Ratio	Resp	Lower	Upper
212	100	1385		
106	49.1	0.0	0.0	0.0#
104	0.0	0.0	0.0	0.0

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:28 AM

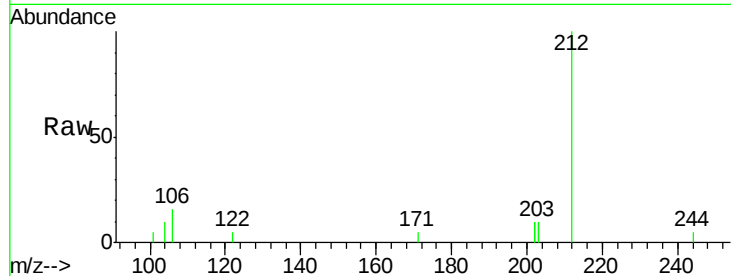

Abundance Ion 212.00 (211.70 to 212.70): E
Ion 106.00 (105.70 to 106.70): E
Ion 104.00 (103.70 to 104.70): E

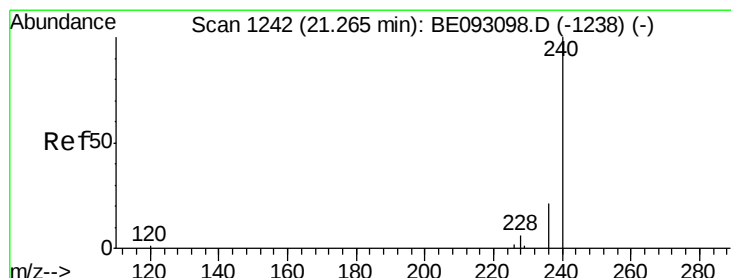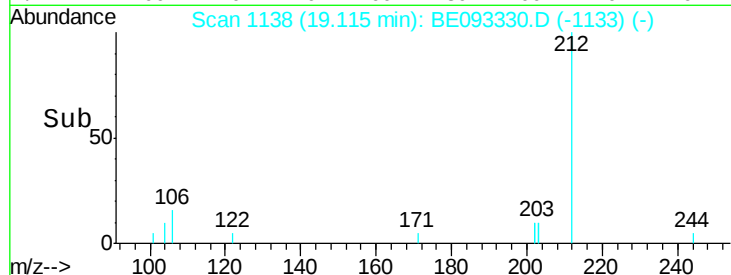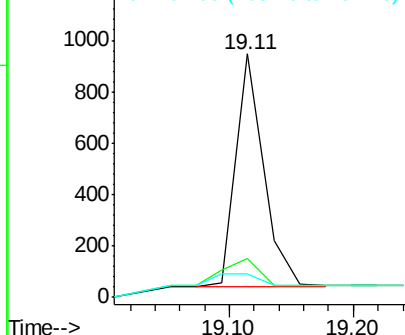

#27

Chrysene-d12

Concen: 0.400 ng


RT: 21.25 min Scan# 1241

Delta R.T. -0.02 min



Lab File: BE093330.D


Acq: 22 Jun 2017 16:10

Tgt Ion	Ratio	Resp	Lower	Upper
240	100	1499		
120	17.1	4.6	7.0	#
236	33.5	20.8	31.2	#

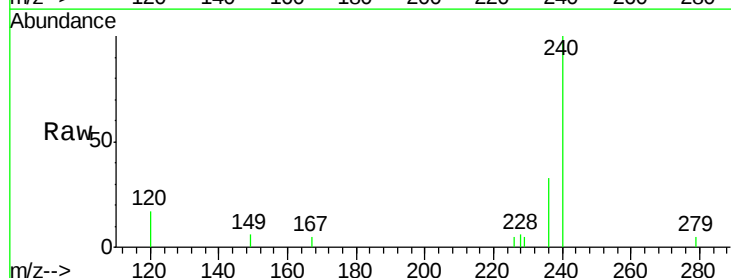

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

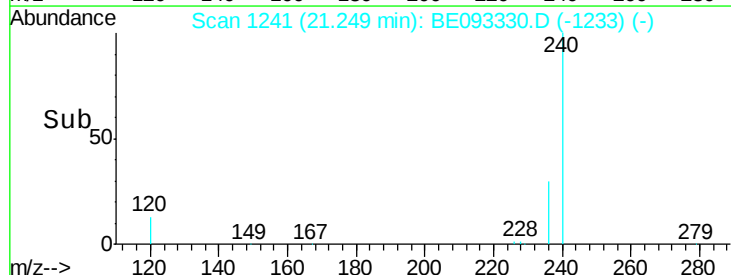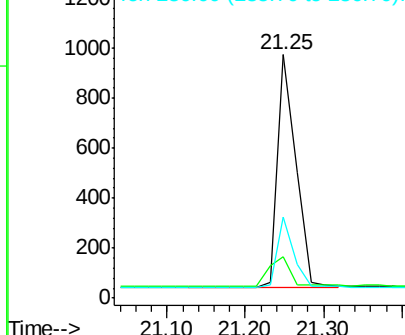



#29

Terphenyl-d14

Concen: 0.373 ng

RT: 19.72 min Scan# 1167

Delta R.T. -0.00 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Instrument :

BNA_E





ClientSampleId :

KY038PS033-170613

Tgt Ion:	244	Resp:	1078
Ion Ratio	Lower	Upper	
244	100		
212	12.4	10.6	16.0
122	7.5	15.4	23.0#

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:28 AM

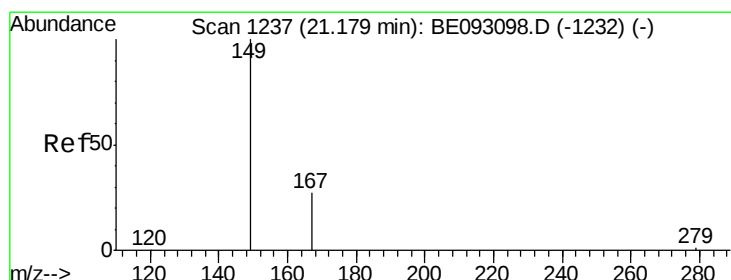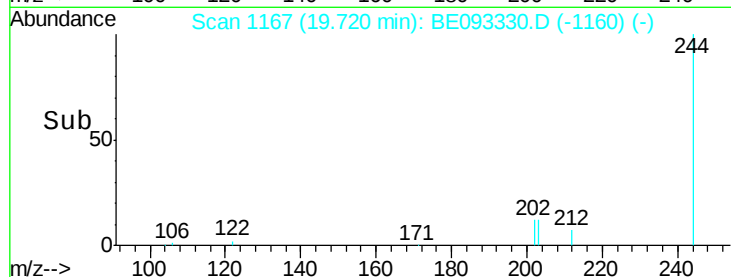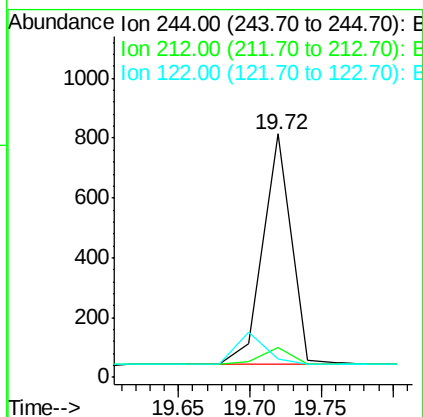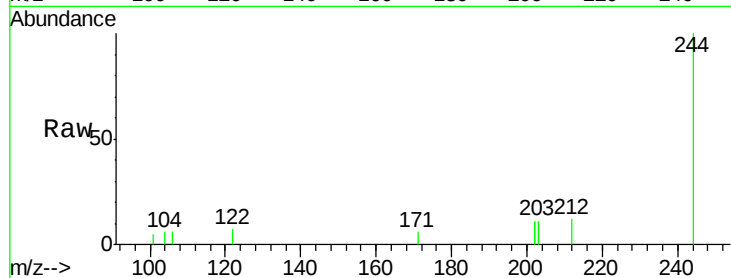

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.092 ng




RT: 21.16 min Scan# 1236




Delta R.T. -0.02 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Tgt Ion:	149	Resp:	194
Ion Ratio	Lower	Upper	
149	100		
167	23.2	20.1	30.1
279	0.0	2.2	3.4#

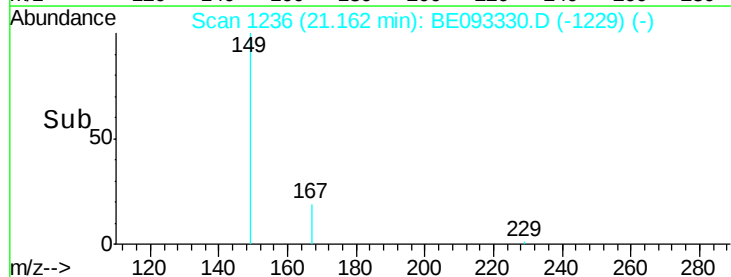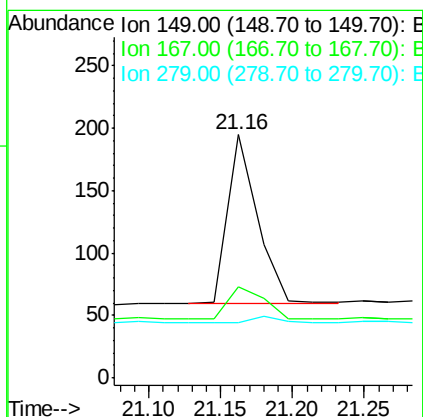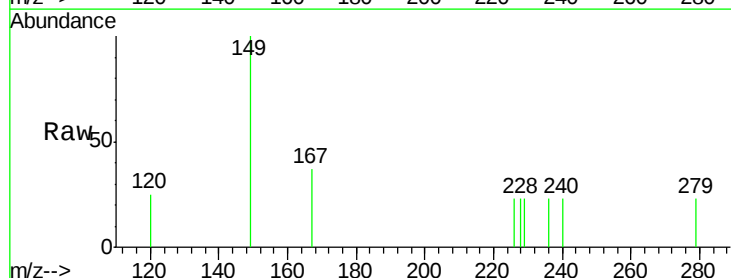

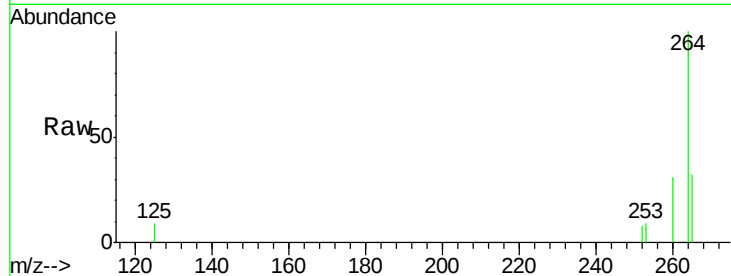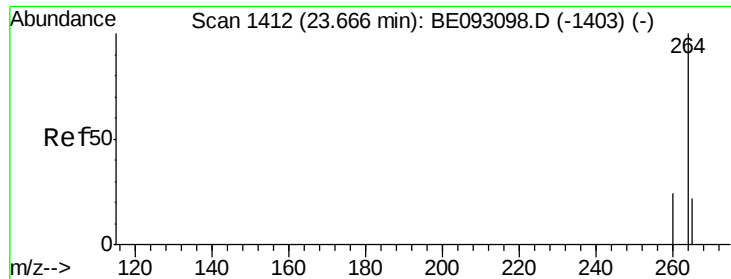

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.65 min Scan# 1411

Delta R.T. -0.01 min

Lab File: BE093330.D

Acq: 22 Jun 2017 16:10

Tgt Ion	Ratio	Lower	Upper
264	100		
260	30.8	21.0	31.4
265	31.7	24.6	36.8

Instrument :

BNA_E

ClientSampleId :

KY038PS033-170613

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:28 AM

