

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062217\
 Data File : BE093331.D
 Acq On : 22 Jun 2017 16:46
 Operator : SJ/JU
 Sample : I3687-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS034-170613

Manual Integrations
 APPROVED

mohammad
 6/26/2017 11:29:31 AM

Quant Time: Jun 23 08:06:56 2017
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 12 14:07:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	185	0.40	ng	-0.02
7) Naphthalene-d8	10.51	136	897	0.40	ng	-0.02
13) Acenaphthene-d10	14.37	164	554	0.40	ng	0.00
19) Phenanthrene-d10	17.10	188	1177	0.40	ng	-0.03
27) Chrysene-d12	21.25	240	1411	0.40	ng	-0.02
34) Perylene-d12	23.67	264	1166	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	33	0.06	ng	0.00
5) Phenol-d6	6.90	99	51m	0.06	ng	0.00
8) Nitrobenzene-d5	8.86	82	221	0.31	ng	-0.02
11) 2-Methylnaphthalene-d10	12.10	152	401	0.30	ng	-0.01
14) 2,4,6-Tribromophenol	15.85	330	19	0.15	ng	0.00
15) 2-Fluorobiphenyl	12.99	172	723	0.31	ng	0.00
25) Fluoranthene-d10	19.11	212	1139m	0.29	ng	0.00
29) Terphenyl-d14	19.72	244	895	0.33	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.16	149	423	0.265	ng	Qvalue # 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062217\
Data File : BE093331.D
Acq On : 22 Jun 2017 16:46
Operator : SJ/JU
Sample : I3687-05
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
KY038PS034-170613

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:31 AM

Quant Time: Jun 23 08:06:56 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 12 14:07:54 2017
Response via : Initial Calibration

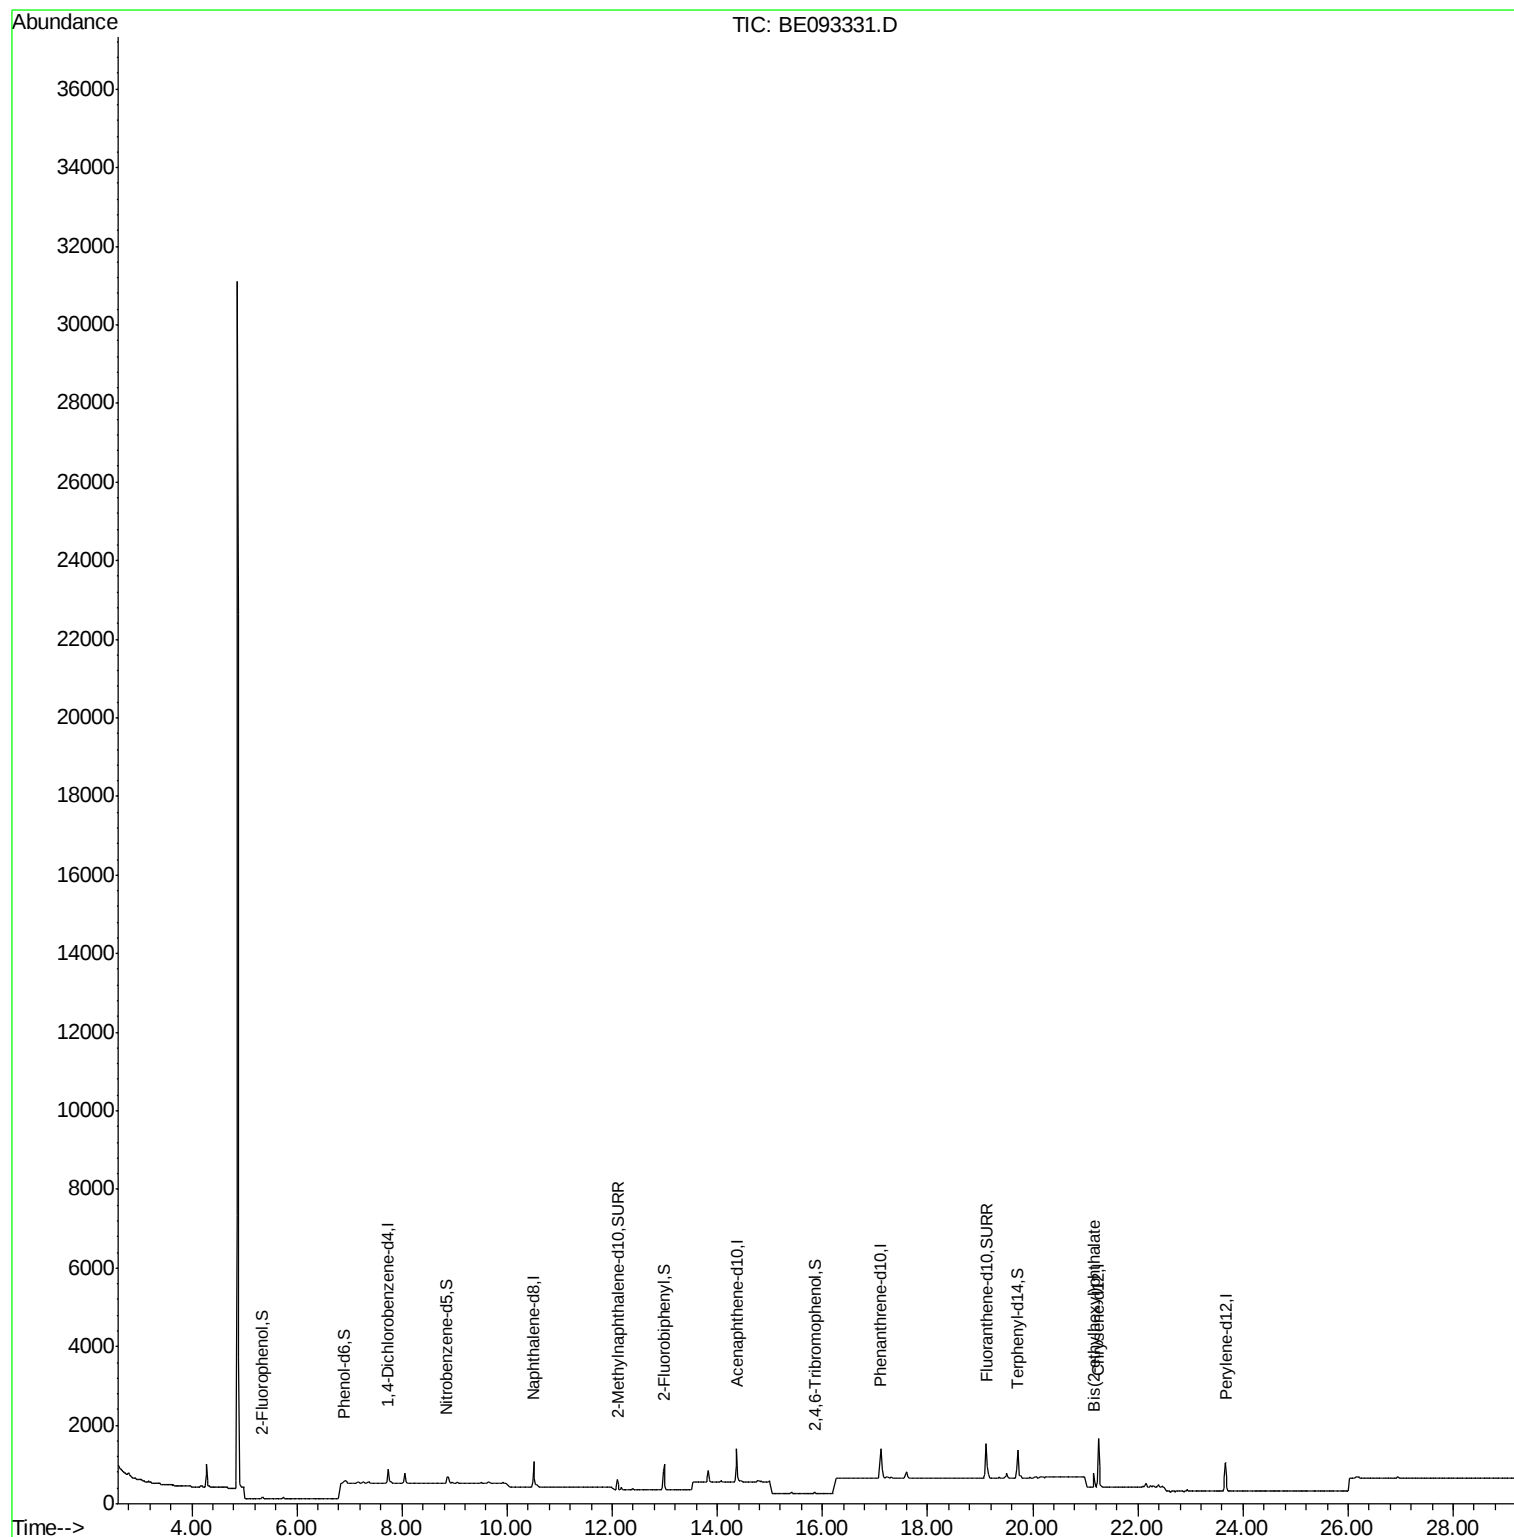

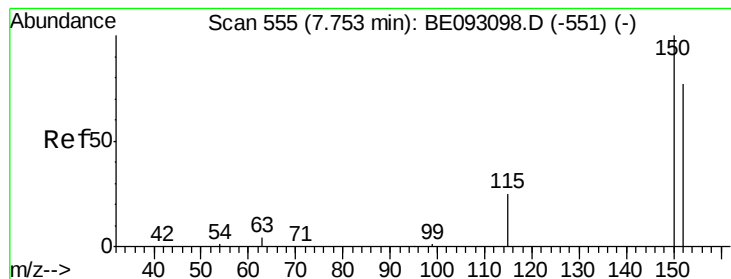





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.73 min Scan# 554
 Delta R.T. -0.02 min
 Lab File: BE093331.D
 Acq: 22 Jun 2017 16:46

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS034-170613

Tgt Ion	Ratio	Lower	Upper
152	100		
150	147.6	125.1	187.7
115	82.8	55.7	83.5




Manual Integrations
 APPROVED


mohammad
 6/26/2017 11:29:31 AM

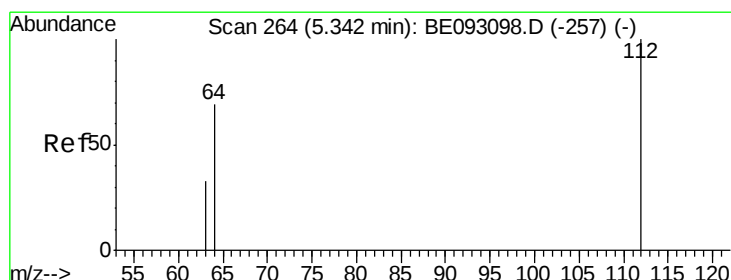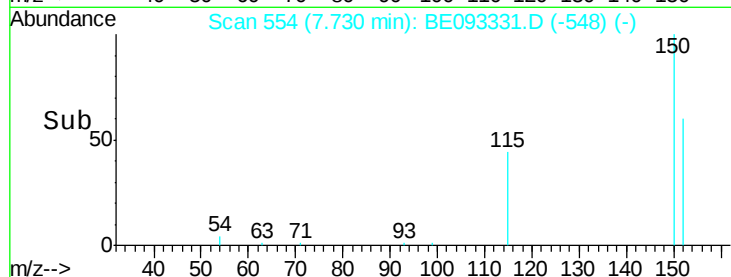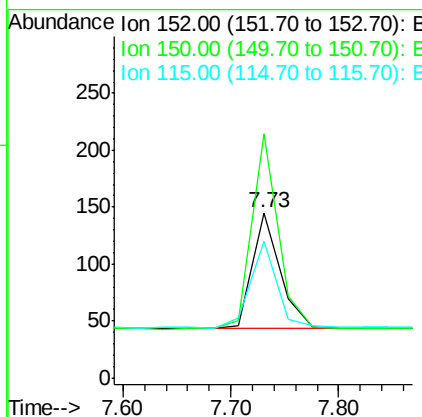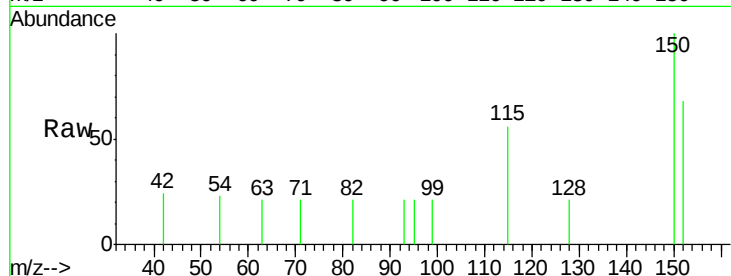

#4
 2-Fluorophenol
 Concen: 0.060 ng
 RT: 5.34 min Scan# 264
 Delta R.T. 0.00 min
 Lab File: BE093331.D
 Acq: 22 Jun 2017 16:46

Tgt Ion	Ratio	Lower	Upper
112	100		
64	72.7	56.4	84.6
63	42.4	29.3	43.9

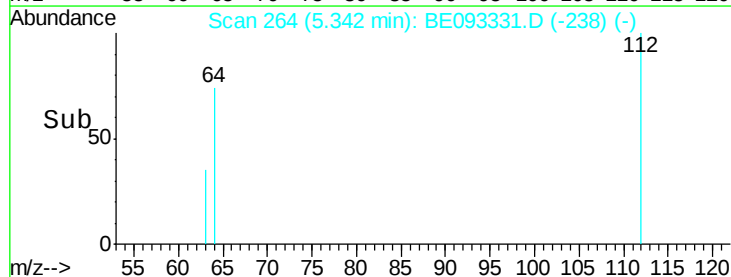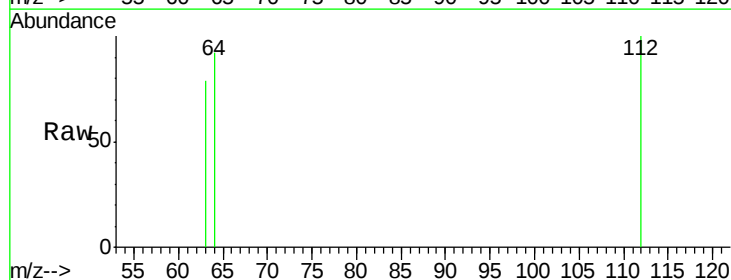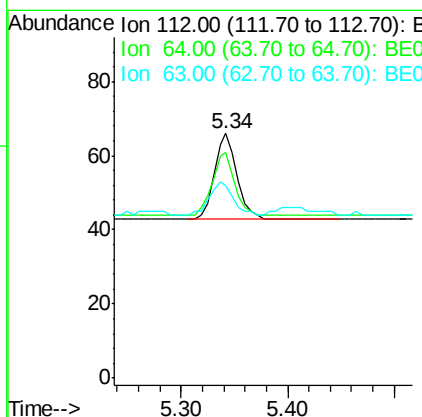

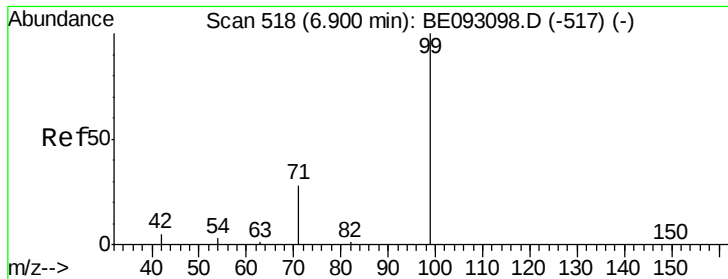

#5

Phenol-d6

Concen: 0.064 ng m

RT: 6.90 min Scan# 518

Delta R.T. 0.00 min

Lab File: BE093331.D

Acq: 22 Jun 2017 16:46

Instrument :

BNA_E

ClientSampleId :

KY038PS034-170613

Tgt Ion: 99 Resp: 51

Ion Ratio Lower Upper

99 100

42 1180.4 0.0 0.0


71 962.7 0.0 0.0

Manual Integrations

APPROVED

mohammad


6/26/2017 11:29:31 AM

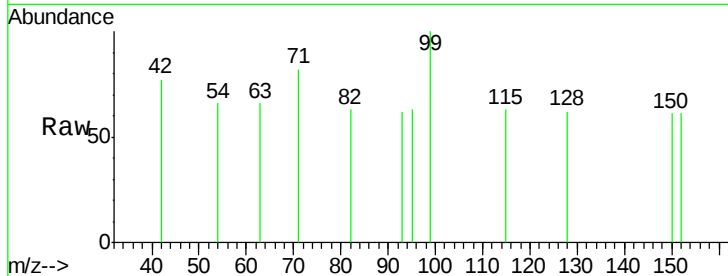


Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

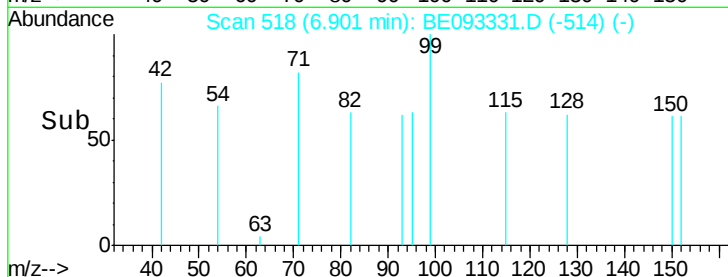

Time-->

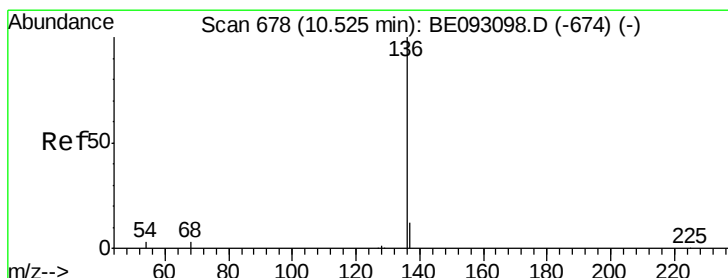

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.51 min Scan# 677

Delta R.T. -0.02 min

Lab File: BE093331.D

Acq: 22 Jun 2017 16:46

Tgt Ion: 136 Resp: 897


Ion Ratio Lower Upper

136 100

137 17.3 9.8 14.8#

54 15.8 10.3 15.5#

68 15.1 9.0 13.4#

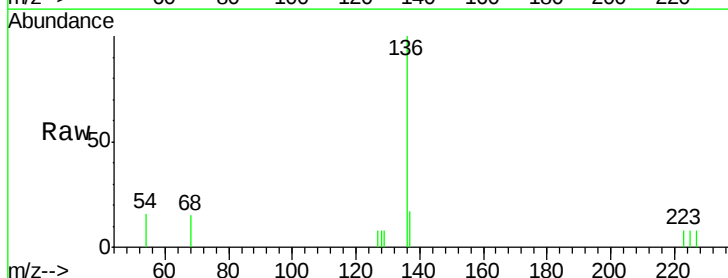


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

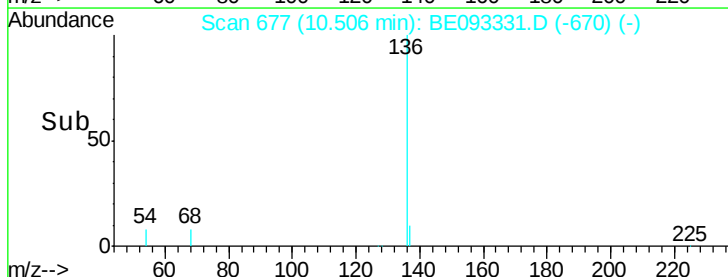

Time-->

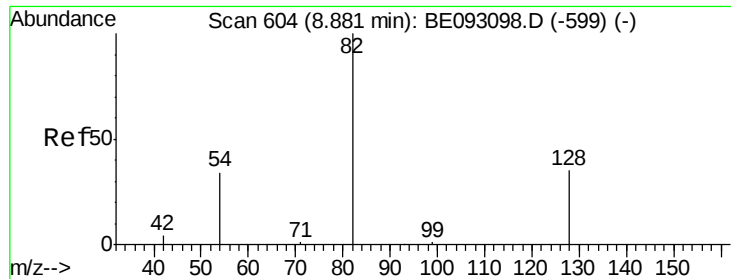





#8
 Nitrobenzene-d5
 Concen: 0.309 ng
 RT: 8.86 min Scan# 603
 Delta R.T. -0.02 min
 Lab File: BE093331.D
 Acq: 22 Jun 2017 16:46

Instrument :
 BNA_E
 ClientSampleId :
 KY038PS034-170613

Tgt Ion	Ratio	Lower	Upper
82	100		
128	42.1	17.0	25.4#
54	86.0	53.8	80.6#




Manual Integrations
 APPROVED


mohammad
 6/26/2017 11:29:31 AM

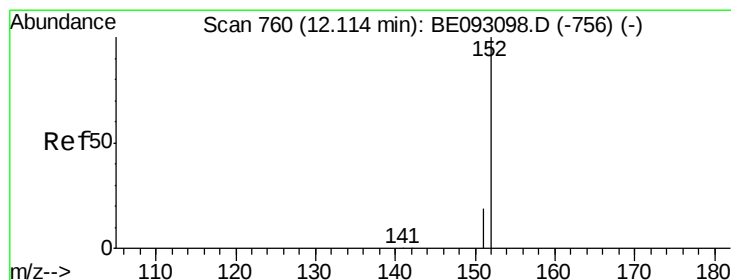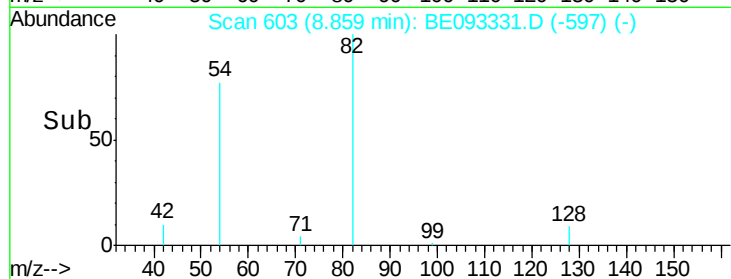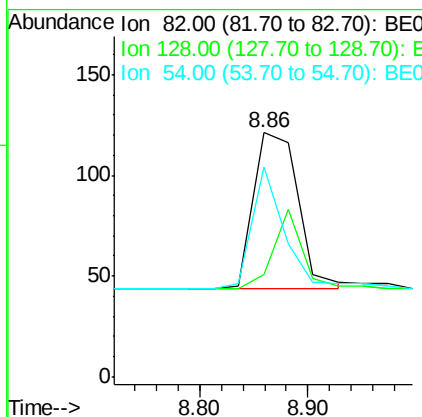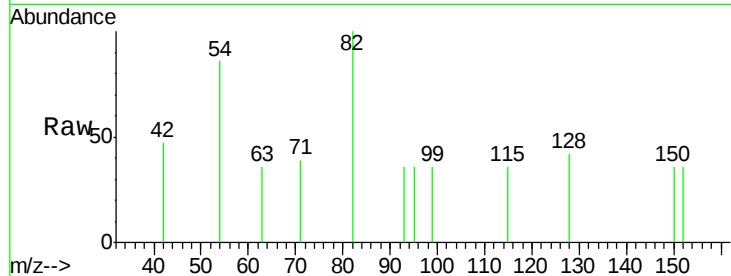

#11
 2-Methylnaphthalene-d10
 Concen: 0.297 ng
 RT: 12.10 min Scan# 759
 Delta R.T. -0.01 min
 Lab File: BE093331.D
 Acq: 22 Jun 2017 16:46

Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.0	15.1	22.7

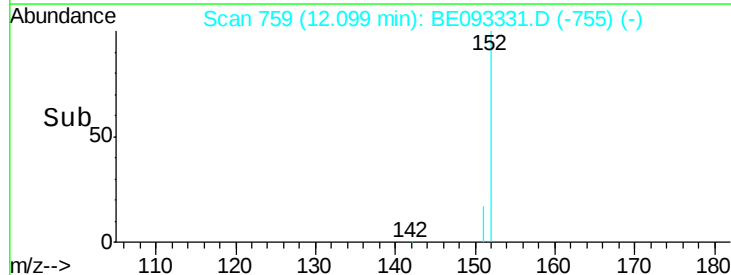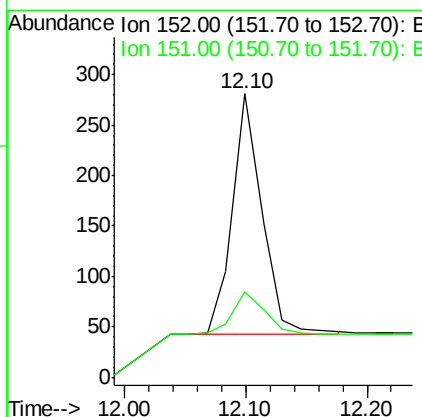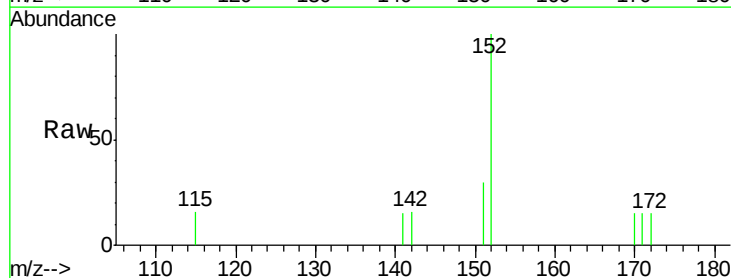

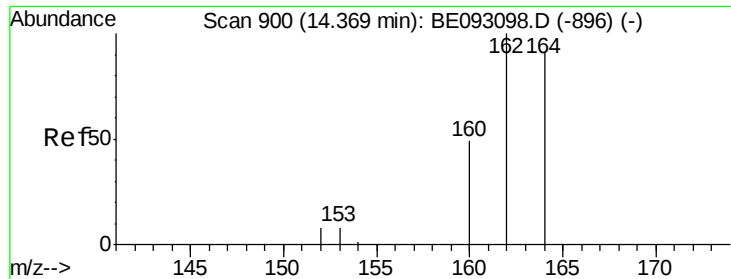





#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.37 min Scan# 900
Delta R.T. 0.00 min
Lab File: BE093331.D
Acq: 22 Jun 2017 16:46

Instrument :
BNA_E
ClientSampleId :
KY038PS034-170613

Tgt Ion:164 Resp: 554
Ion Ratio Lower Upper
164 100
162 96.6 84.6 127.0
160 48.3 41.8 62.6




Manual Integrations
APPROVED


mohammad
6/26/2017 11:29:31 AM

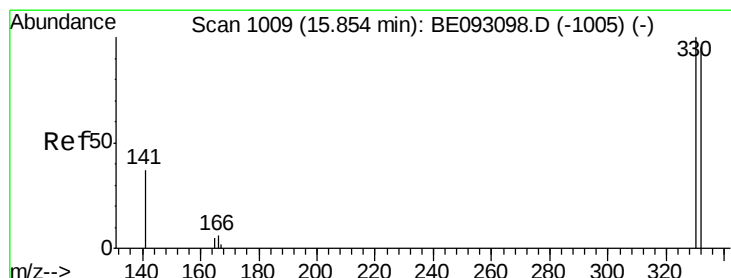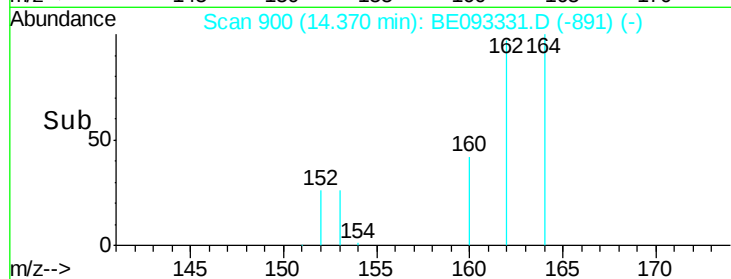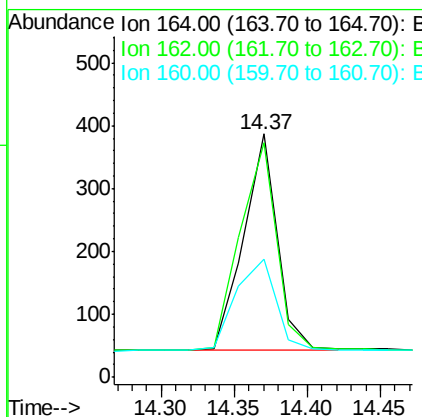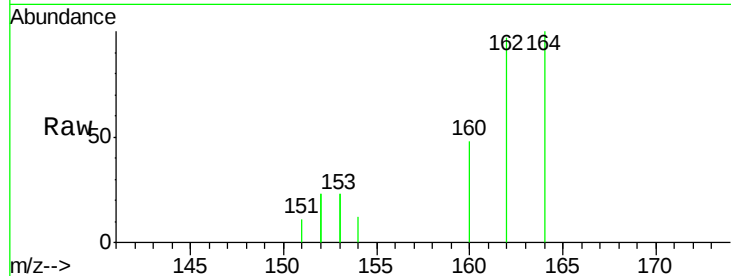

#14
2,4,6-Tribromophenol
Concen: 0.151 ng
RT: 15.85 min Scan# 1009
Delta R.T. 0.00 min
Lab File: BE093331.D
Acq: 22 Jun 2017 16:46

Tgt Ion:330 Resp: 19
Ion Ratio Lower Upper
330 100
332 52.6 77.7 116.5#
141 47.4 56.2 84.4#

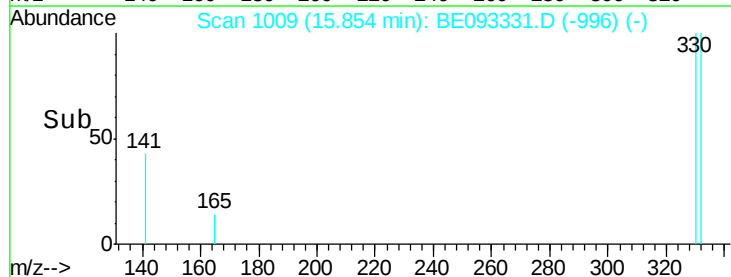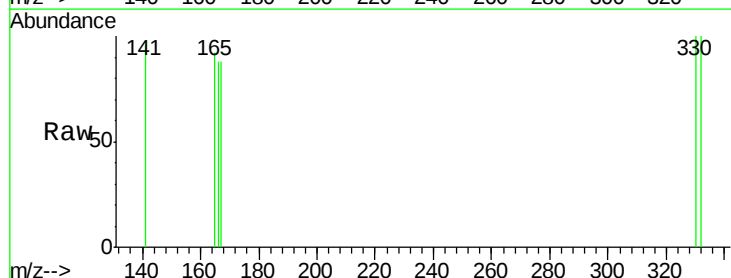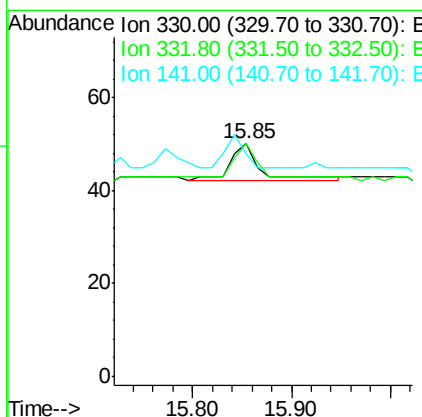

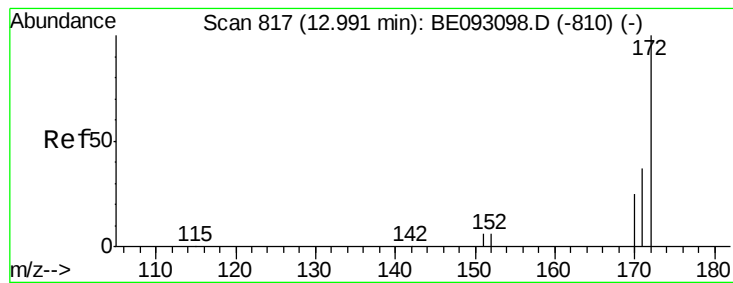





#15
2-Fluorobiphenyl
Concen: 0.306 ng
RT: 12.99 min Scan# 817
Delta R.T. 0.00 min
Lab File: BE093331.D
Acq: 22 Jun 2017 16:46

Instrument :
BNA_E
ClientSampleId :
KY038PS034-170613

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	29.8	44.6
170	25.9	20.7	31.1




Manual Integrations
APPROVED


mohammad
6/26/2017 11:29:31 AM

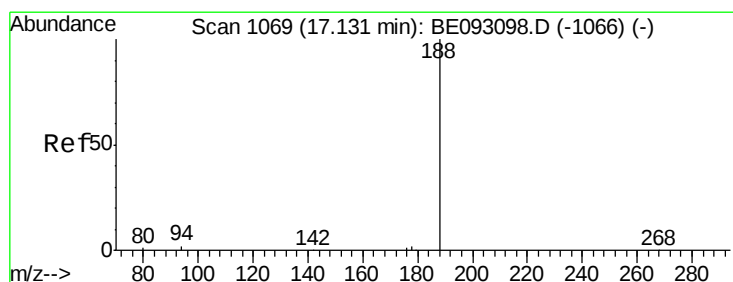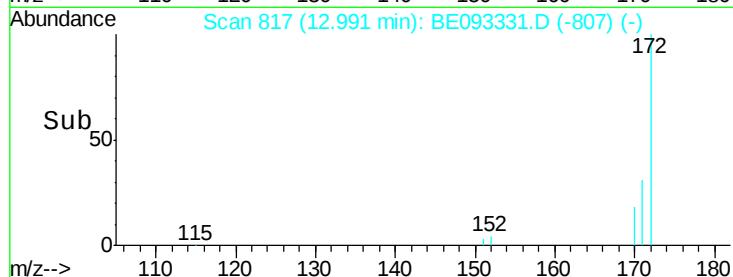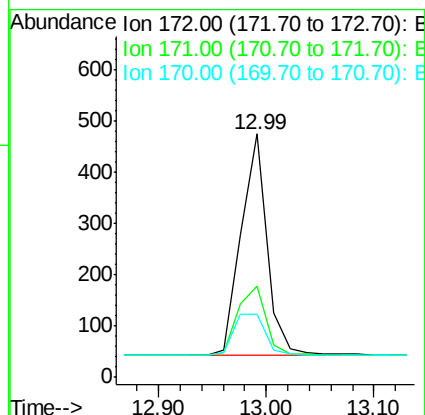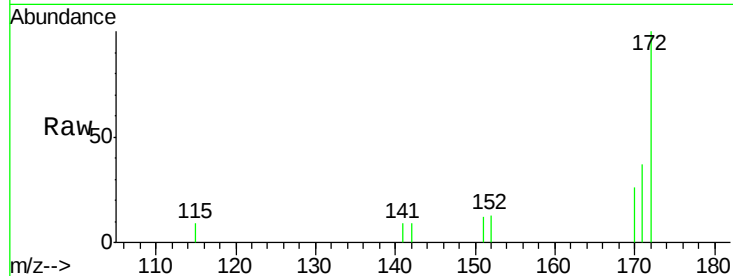

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.10 min Scan# 1068
Delta R.T. -0.03 min
Lab File: BE093331.D
Acq: 22 Jun 2017 16:46

Tgt Ion	Ratio	Lower	Upper
188	100		
94	34.6	11.3	16.9#
80	37.3	11.7	17.5#

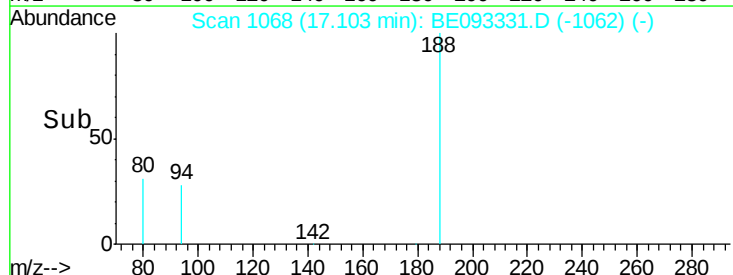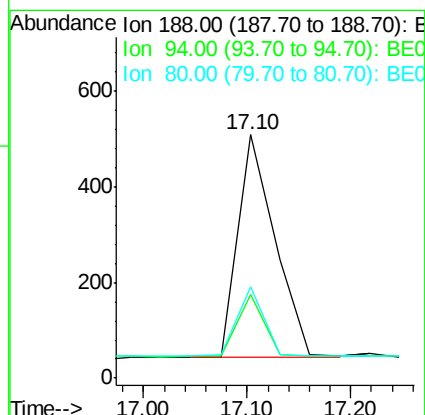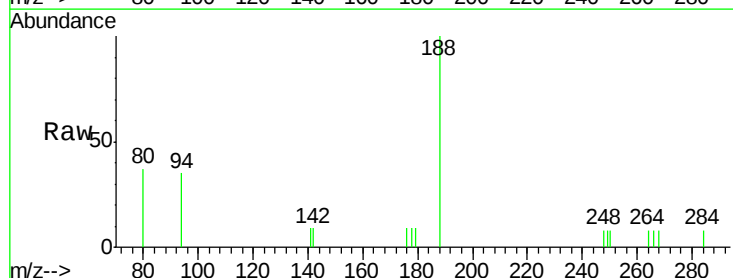

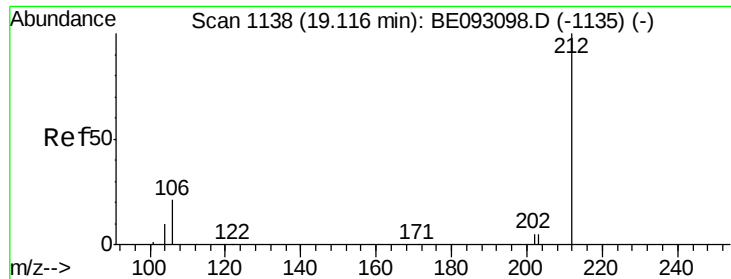

#25

Fluoranthene-d10

Concen: 0.294 ng m

RT: 19.11 min Scan# 1138

Delta R.T. -0.00 min

Lab File: BE093331.D

Acq: 22 Jun 2017 16:46

Instrument :

BNA_E


ClientSampleId :

KY038PS034-170613


Tgt Ion:	212	Resp:	1139
Ion Ratio	Lower	Upper	
212	100		
106	54.9	0.0	0.0#
104	0.0	0.0	0.0

Manual Integrations
APPROVED



mohammad
6/26/2017 11:29:31 AM

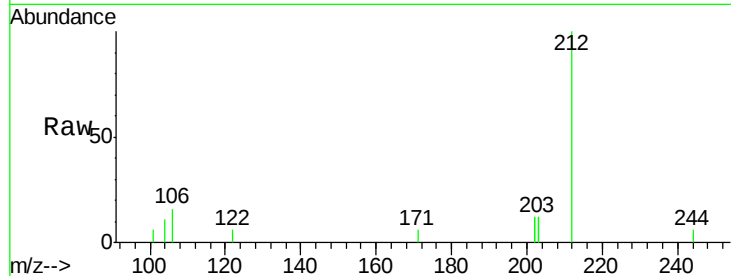

Abundance Ion 212.00 (211.70 to 212.70): E
Ion 106.00 (105.70 to 106.70): E
Ion 104.00 (103.70 to 104.70): E

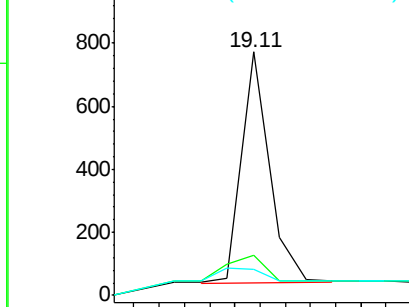

Time-->

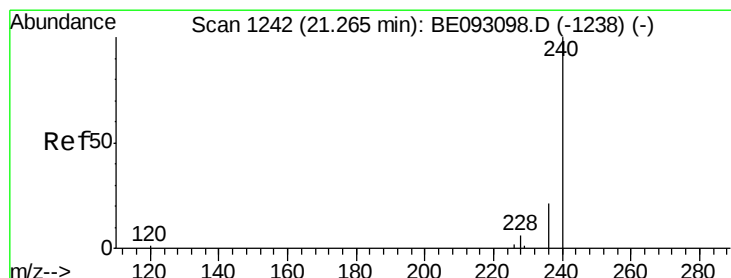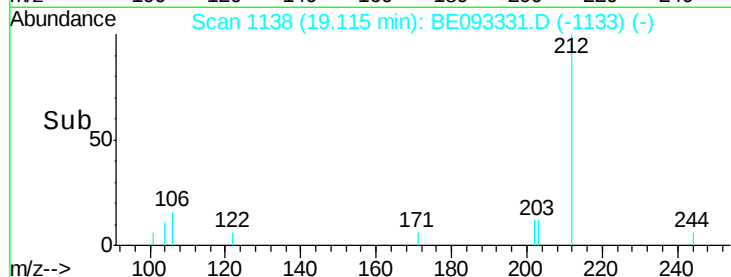

#27

Chrysene-d12

Concen: 0.400 ng


RT: 21.25 min Scan# 1241

Delta R.T. -0.02 min


Lab File: BE093331.D

Acq: 22 Jun 2017 16:46


Tgt Ion:	240	Resp:	1411
Ion Ratio	Lower	Upper	
240	100		
120	17.1	4.6	7.0#
236	33.4	20.8	31.2#

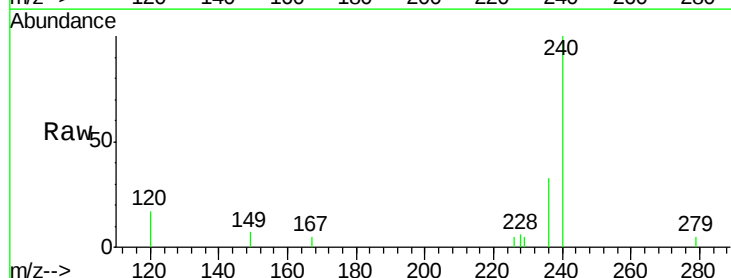


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

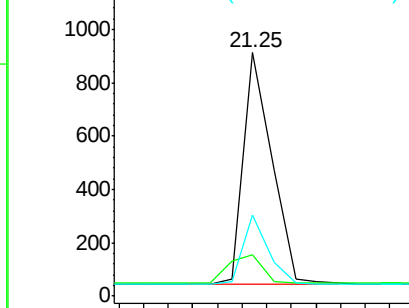

Time-->

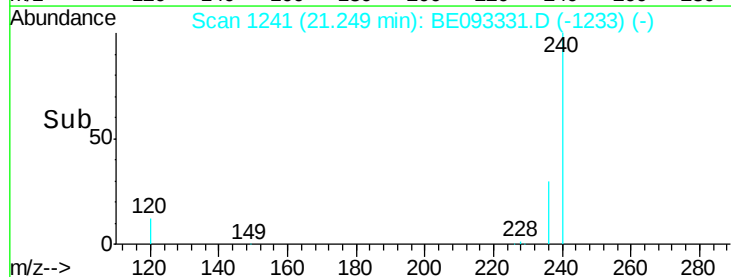

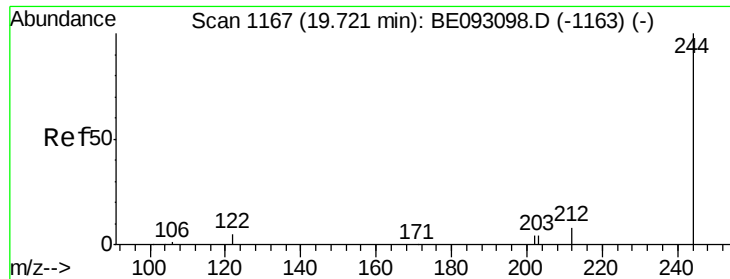

#29

Terphenyl-d14

Concen: 0.329 ng

RT: 19.72 min Scan# 1167

Delta R.T. -0.00 min

Lab File: BE093331.D


Acq: 22 Jun 2017 16:46

Instrument :

BNA_E

ClientSampleId :




KY038PS034-170613

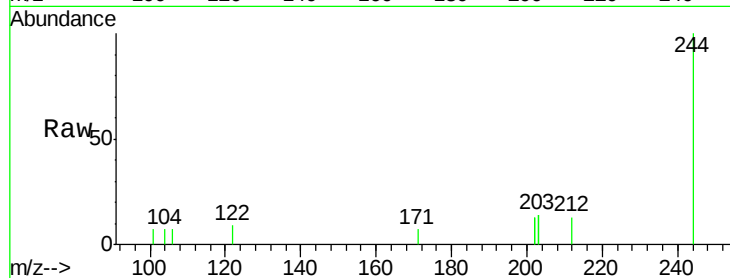

Tgt Ion	Ratio	Lower	Upper
244	100		
212	13.3	10.6	16.0
122	8.5	15.4	23.0#

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:31 AM

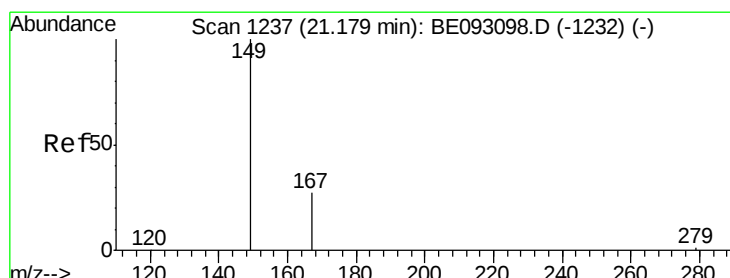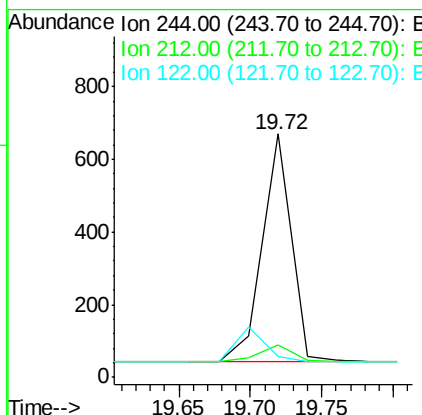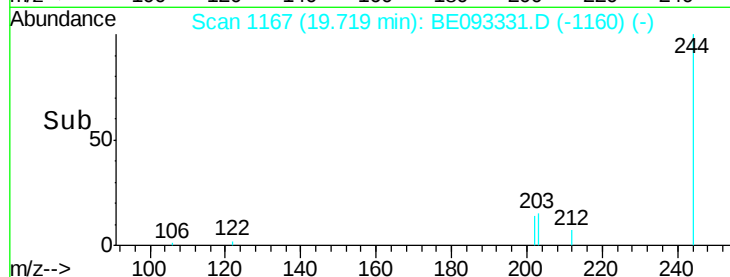

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.265 ng




RT: 21.16 min Scan# 1236




Delta R.T. -0.02 min

Lab File: BE093331.D

Acq: 22 Jun 2017 16:46

Tgt Ion	Ratio	Lower	Upper
149	100		
167	24.8	20.1	30.1
279	0.0	2.2	3.4#

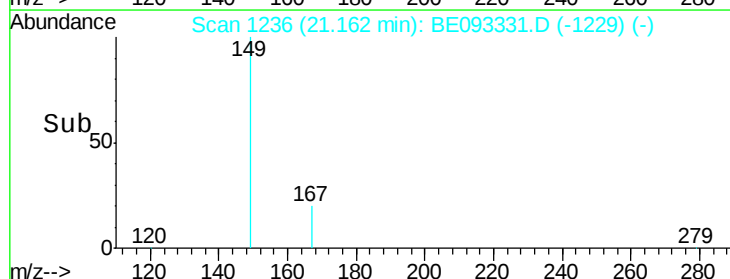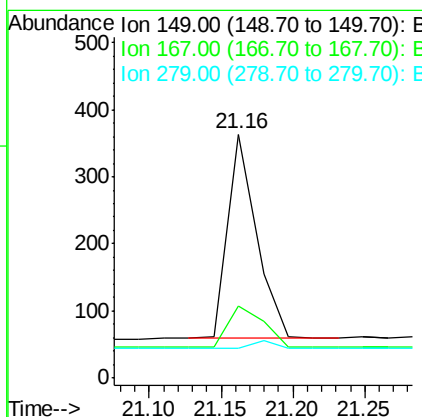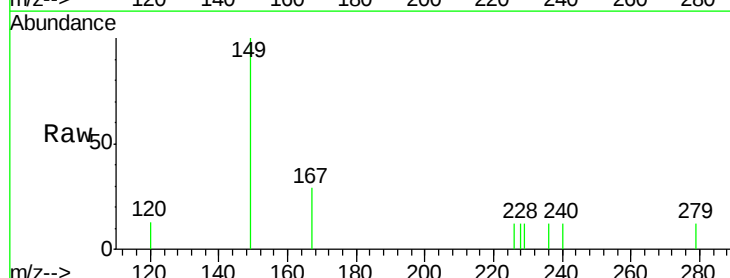

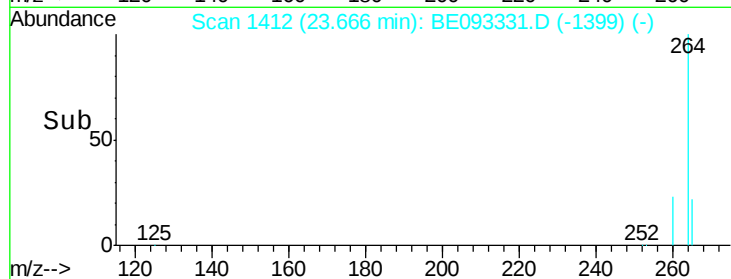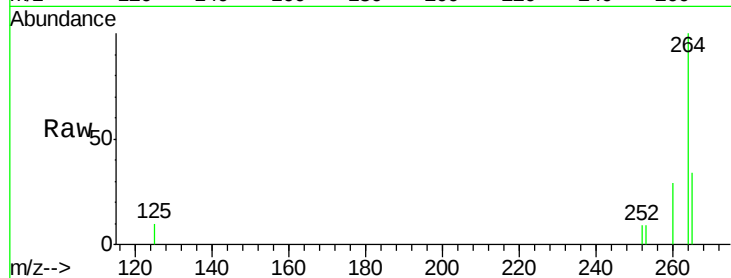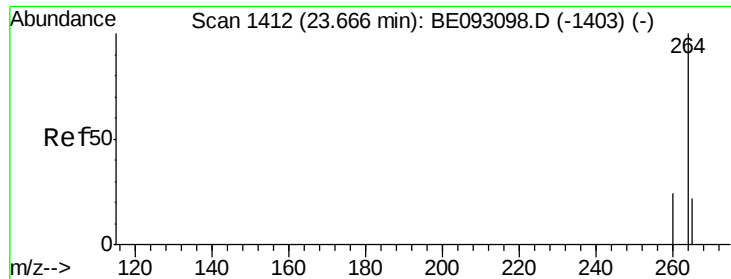

#34
Perylene-d12
Concen: 0.400 ng
RT: 23.67 min Scan# 1412
Delta R.T. 0.00 min
Lab File: BE093331.D
Acq: 22 Jun 2017 16:46

Tgt Ion	Ratio	Lower	Upper
264	100		
260	28.7	21.0	31.4
265	34.1	24.6	36.8

Instrument :
BNA_E
ClientSampleId :
KY038PS034-170613

Manual Integrations
APPROVED

mohammad
6/26/2017 11:29:31 AM

