



1,4-Dioxane

Response Ratio

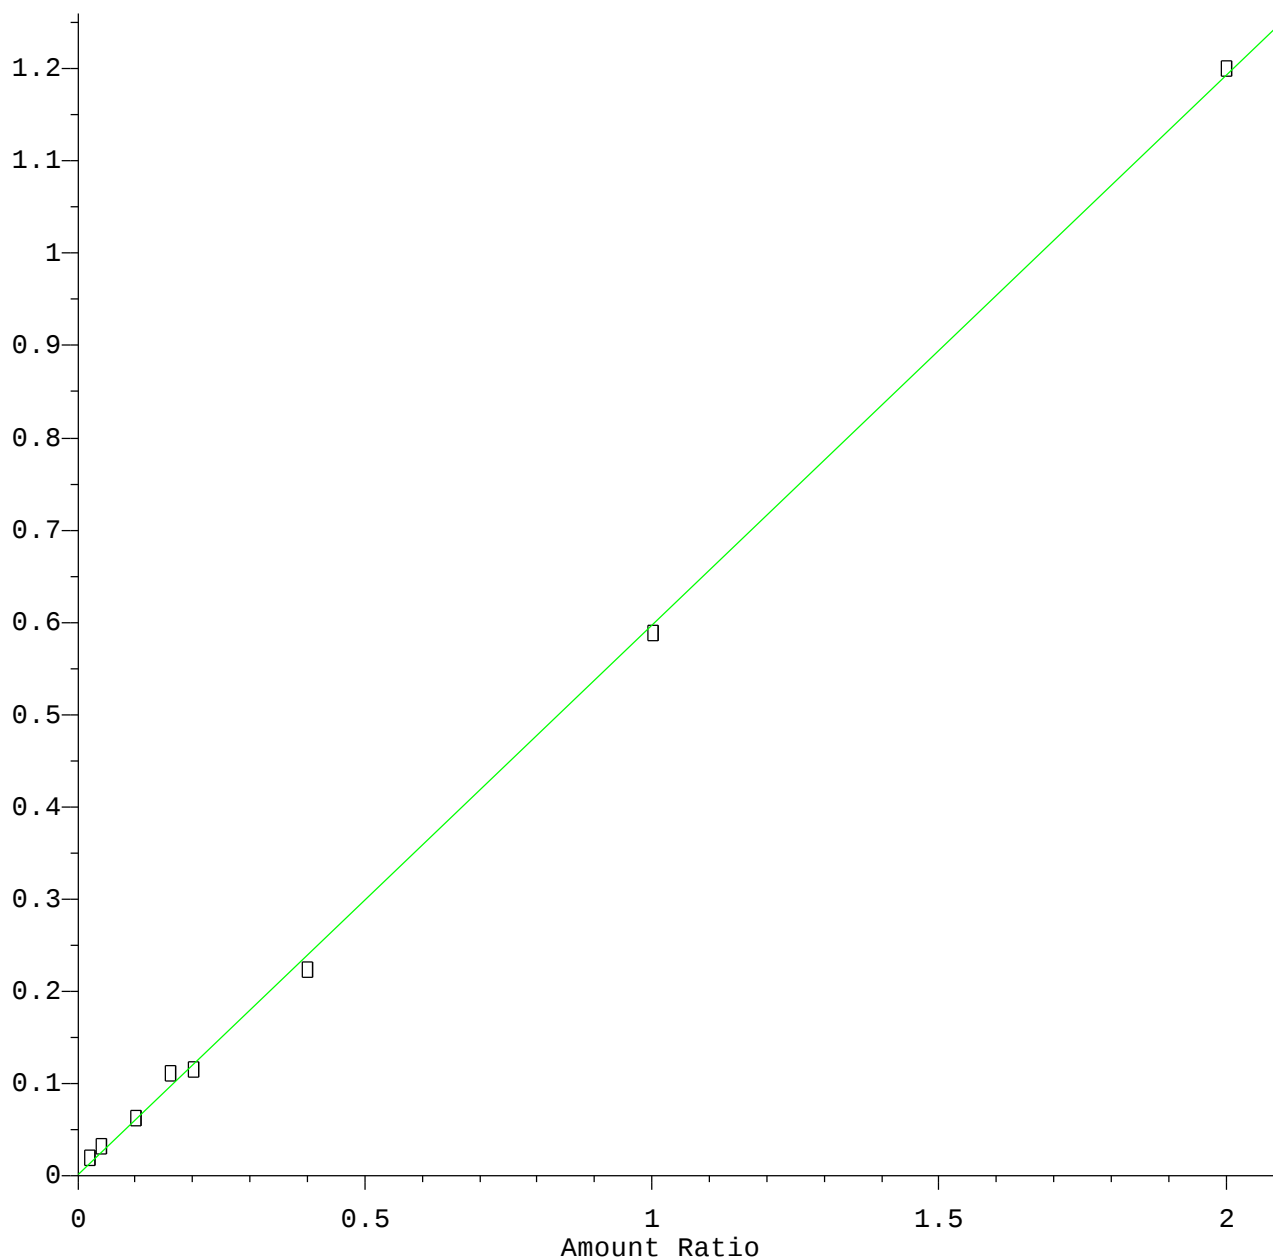


Resp Ratio = $5.95 \times 10^{-1} \times \text{Amt} + 2.24 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
Calibration Table Last Updated: Wed Jun 24 09:27:42 2015

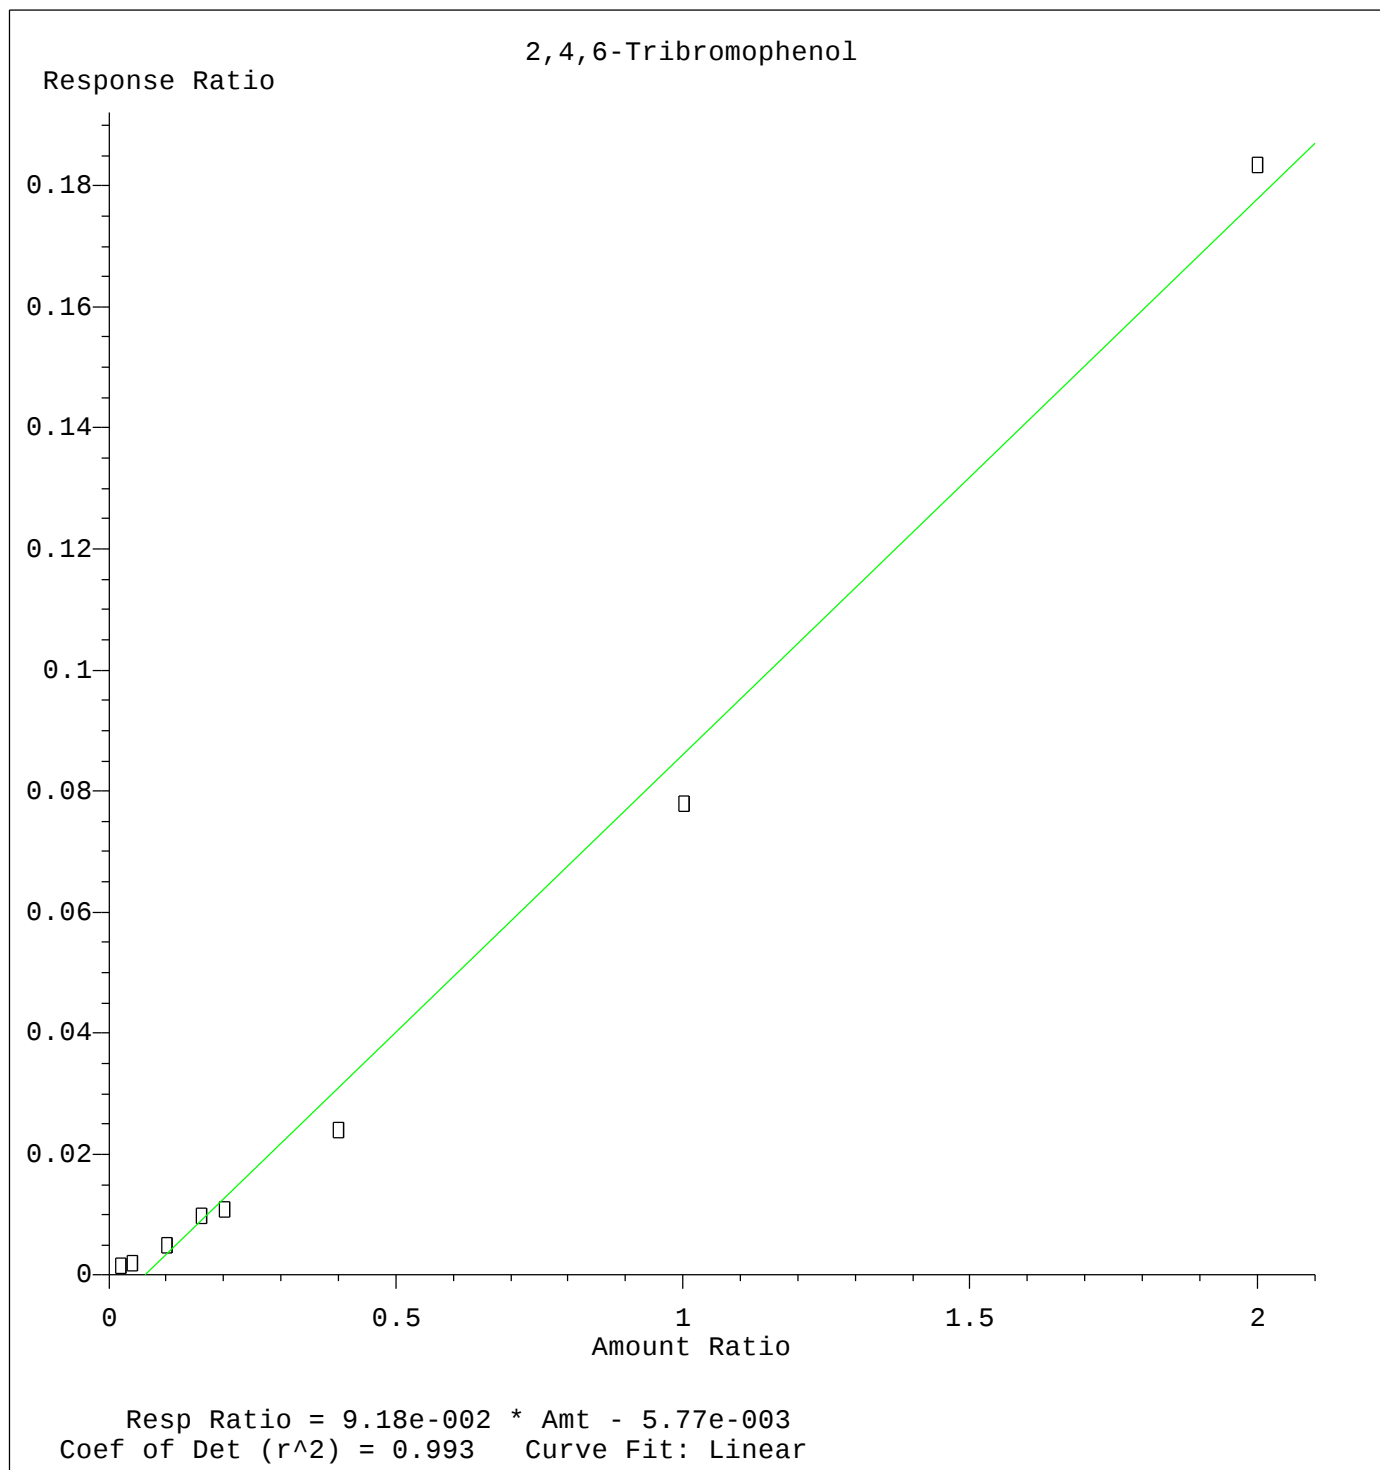

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
Calibration Table Last Updated: Wed Jun 24 09:27:42 2015

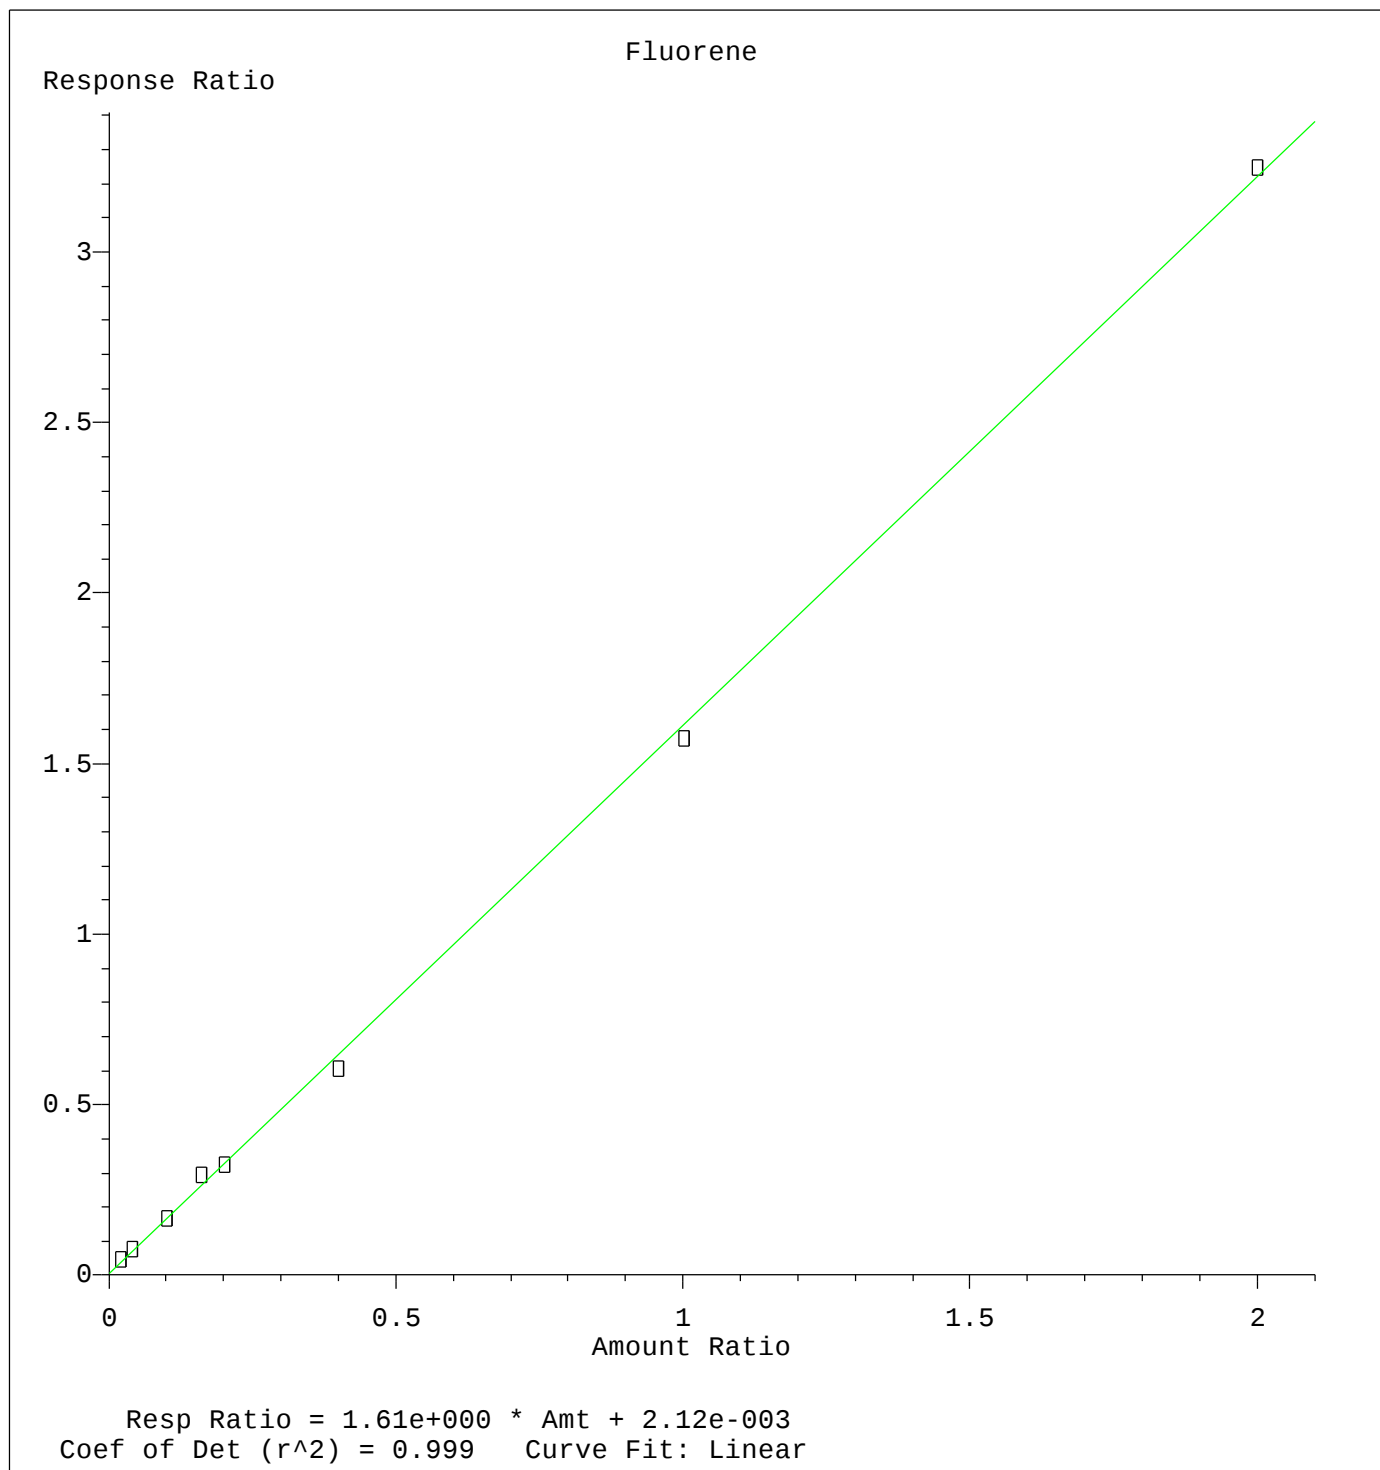

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
Calibration Table Last Updated: Wed Jun 24 09:27:42 2015

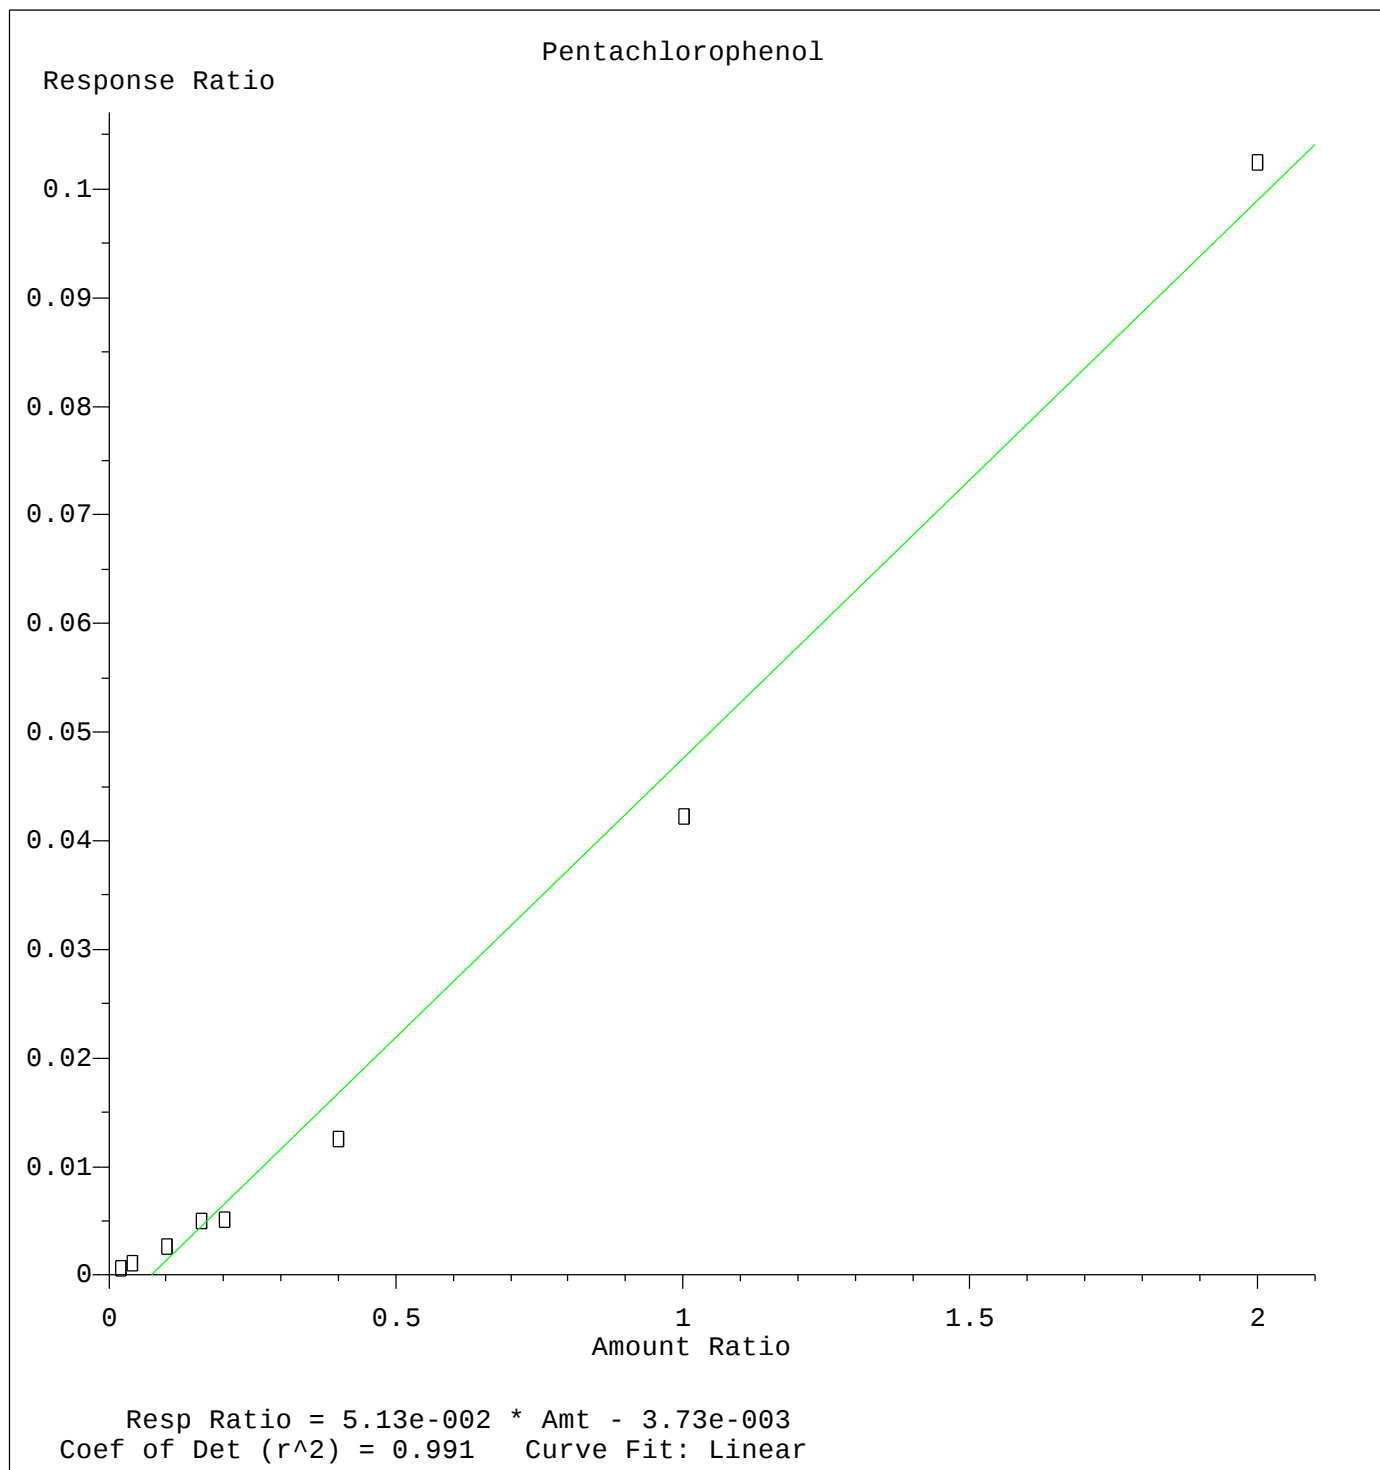

Method Name: Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
Calibration Table Last Updated: Wed Jun 24 09:27:42 2015