


Data Path : Z:\HPCHEM1\BNA_E\Data\BE062315\
 Data File : BE089922.D
 Acq On : 23 Jun 2015 20:09
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 25 16:51:27 2015

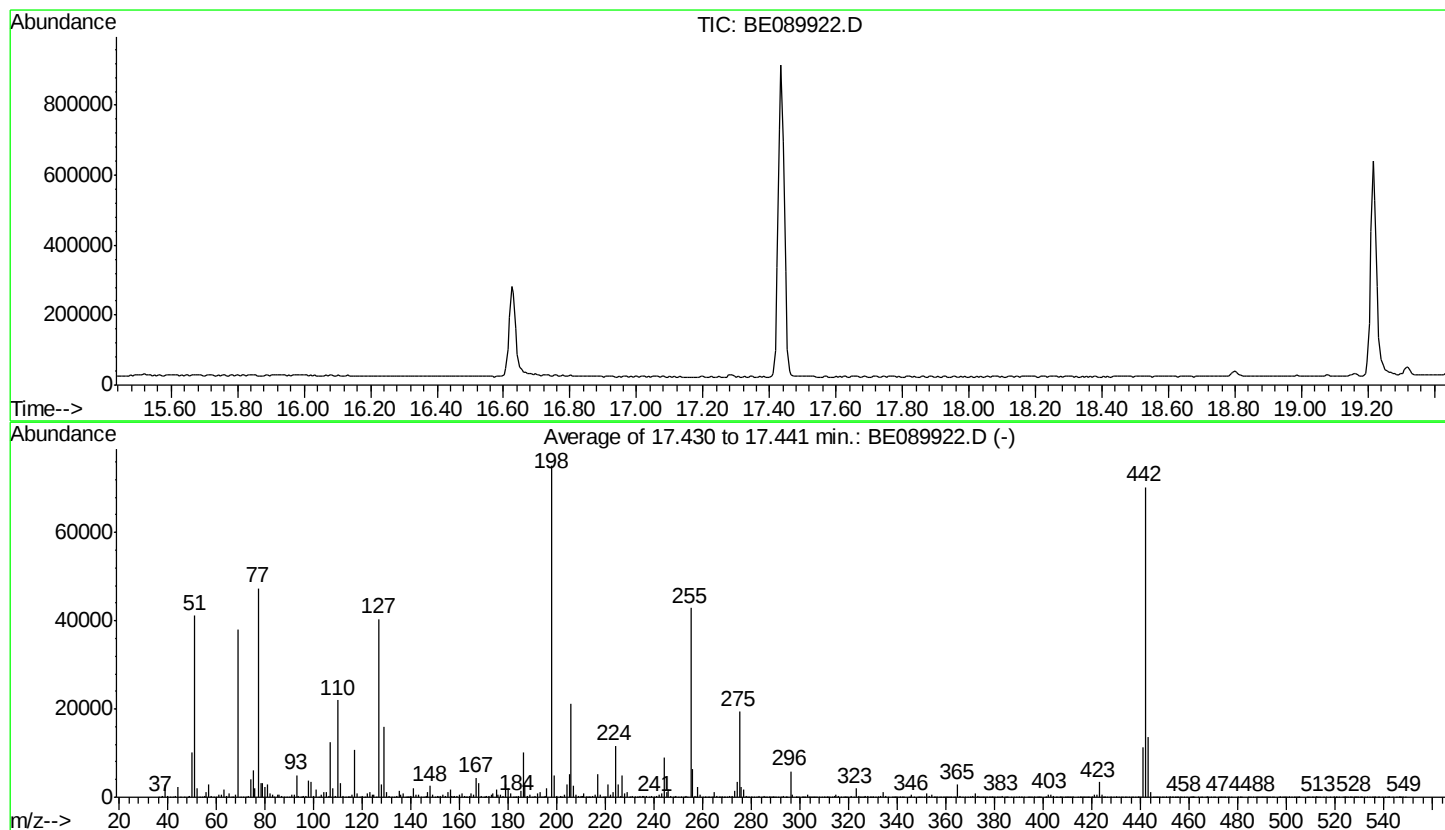

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	41113	PASS
68	69	0.00	2	1.9	711	PASS
69	198	0.00	100	50.5	37939	PASS
70	69	0.00	2	0.3	122	PASS
127	198	10	80	53.8	40452	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75157	PASS
199	198	5	9	6.5	4906	PASS
275	198	10	60	25.7	19333	PASS
365	198	1	100	3.8	2882	PASS
441	442	0.01	24	16.2	11386	PASS
442	198	50	100	93.5	70274	PASS
443	442	15	24	19.3	13541	PASS